
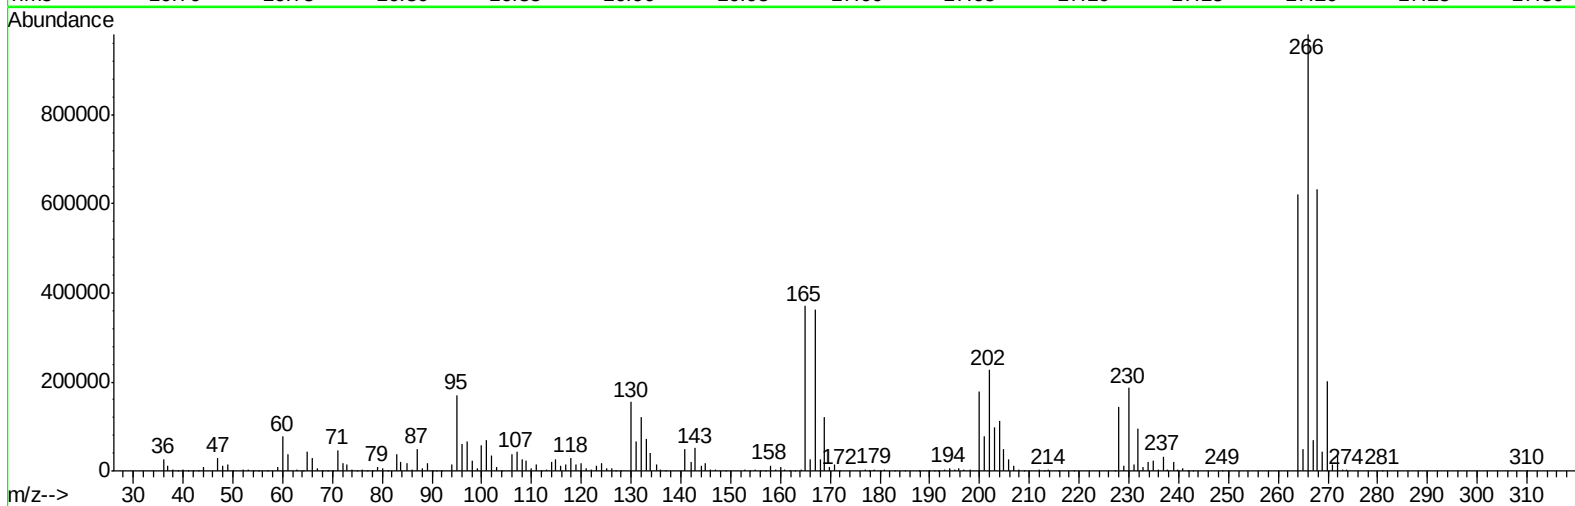


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM062219\
Data File : BM021089.D
Acq On : 22 Jun 2019 07:17
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 24 08:20:22 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM062019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 20 15:39:58 2019
Response via : Initial Calibration

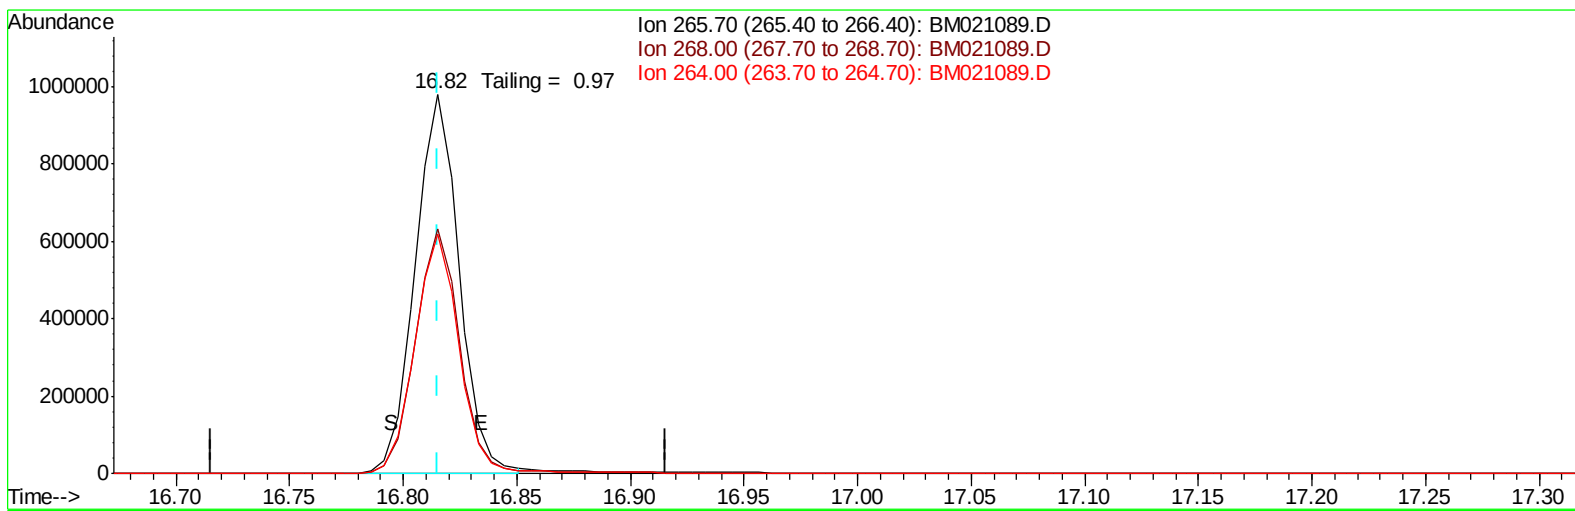

TIC: BM021089.D

(70) Pentachlorophenol (C)



16.815min (-0.000) 125015.37ng

response 1328296

Ion	Exp%	Act%
265.70	100	100
268.00	63.70	64.58
264.00	62.40	63.21
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM062219\
Data File : BM021089.D
Acq On : 22 Jun 2019 07:17
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 24 08:20:22 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM062019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 20 15:39:58 2019
Response via : Initial Calibration

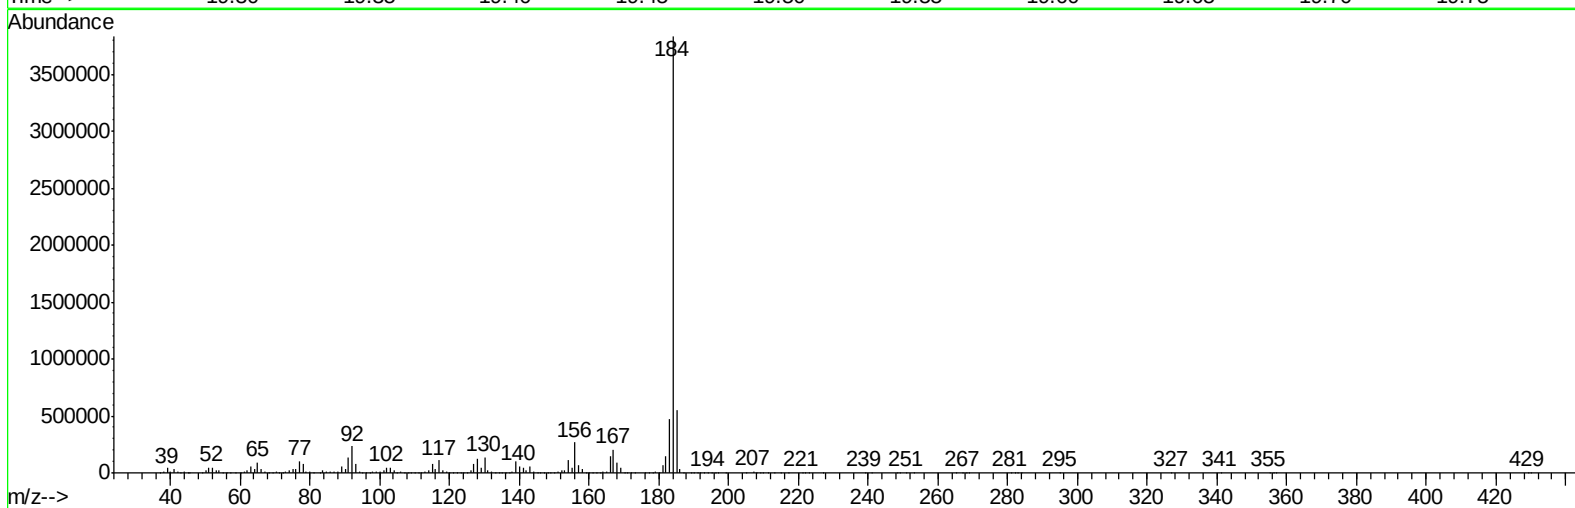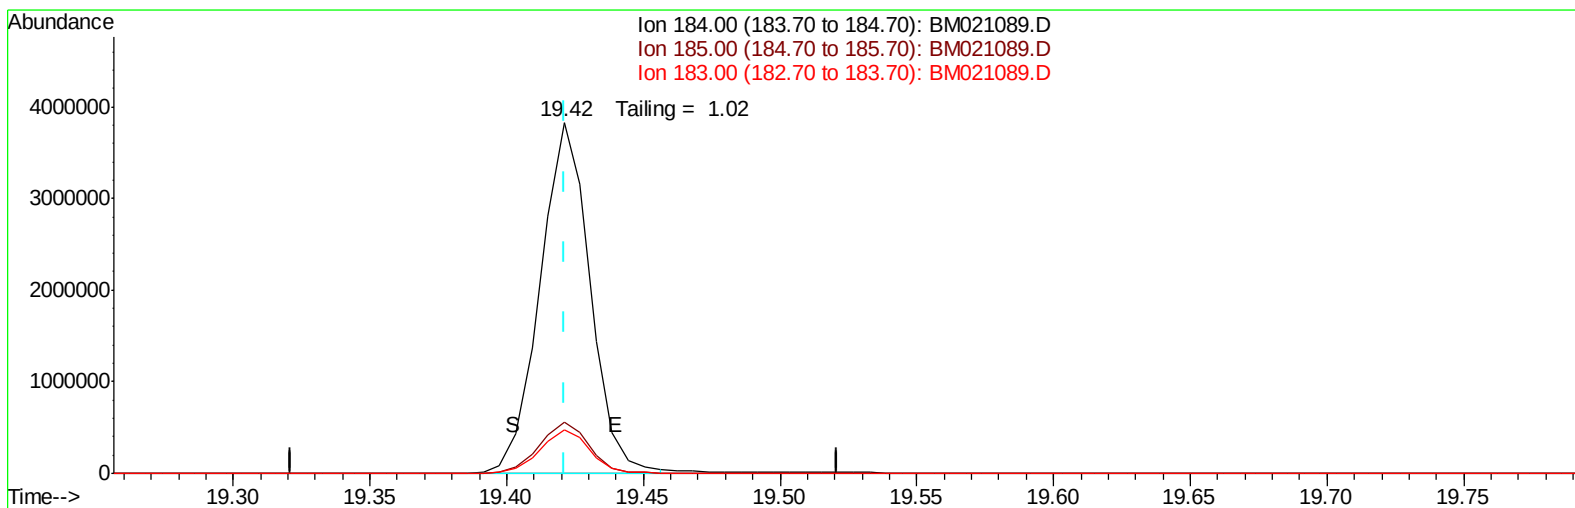

TIC: BM021089.D

(77) Benzidine

19.421min (-0.000) 8199.24ng

response 4927053

Ion	Exp%	Act%
184.00	100	100
185.00	14.30	14.46
183.00	12.00	12.41
0.00	0.00	0.00