


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM062219\
 Data File : BM021089.D
 Acq On : 22 Jun 2019 07:17
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM062019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jun 20 15:39:58 2019

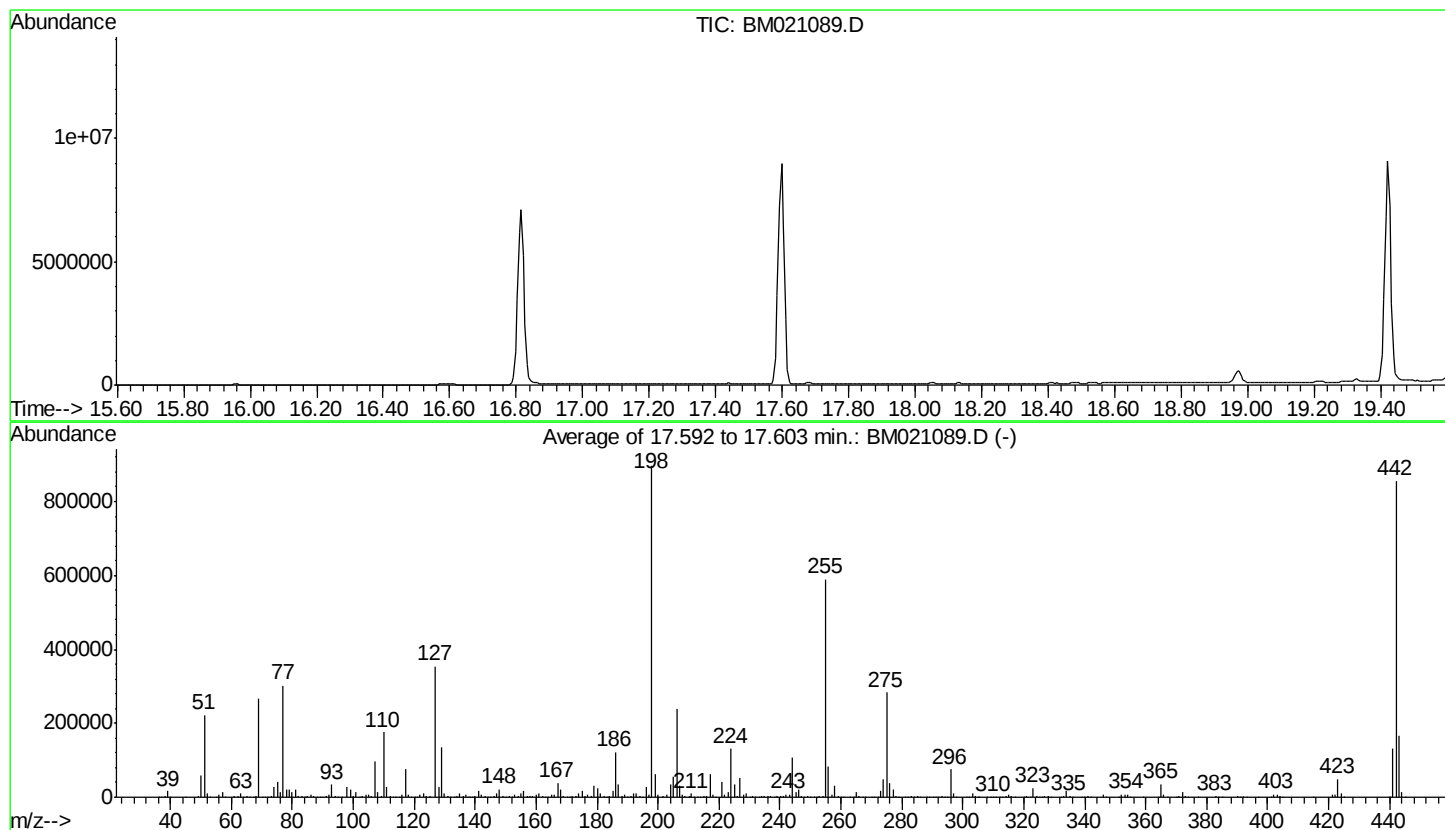

AutoFind: Scans 2483, 2484, 2485; Background Corrected with Scan 2476

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	24.9	223509	PASS
68	69	0.00	2	1.7	4572	PASS
69	198	0.00	100	29.8	267008	PASS
70	69	0.00	2	0.5	1297	PASS
127	198	10	80	39.4	353429	PASS
197	198	0.00	2	0.7	6600	PASS
198	198	100	100	100.0	897173	PASS
199	198	5	9	6.8	60800	PASS
275	198	10	60	31.5	282538	PASS
365	198	1	100	3.9	35226	PASS
441	198	0.01	100	14.6	131008	PASS
442	198	50	100	95.5	856938	PASS
443	442	15	24	19.3	164989	PASS