

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062223\
 Data File : BM040360.D
 Acq On : 22 Jun 2023 22:10
 Operator : MA/JU
 Sample : 03084-17
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DCFN4

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 06/23/2023
 Supervised By :mohammad ahmed 06/23/2023

Quant Time: Jun 23 02:28:02 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 23 00:44:24 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.953	152	9639	0.400	ng/ul	0.00
4) Naphthalene-d8	10.760	136	38774	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.590	164	22371	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.335	188	40648	0.400	ng/ul	0.00
17) Chrysene-d12	21.512	240	22719	0.400	ng/ul	0.00
23) Perylene-d12	23.929	264	23254	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.333	96	42609	2.814	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.349	152	12284	0.226	ng/ul	0.00
18) Fluoranthene-d10	19.360	212	21041	0.289	ng/ul	0.00
Target Compounds						
					Qvalue	
5) Naphthalene	10.810	128	177356	1.658	ng/ul	99
7) 2-Methylnaphthalene	12.421	142	78211	1.245	ng/ul	98
8) 1-Methylnaphthalene	12.641	142	50127	0.799	ng/ul	100
10) Acenaphthylene	14.312	152	100179	1.002	ng/ul	99
11) Acenaphthene	14.654	153	11542	0.137	ng/ul	96
12) Fluorene	15.640	166	14005	0.155	ng/ul#	93
15) Phenanthrene	17.377	178	471377	3.733	ng/ul	99
16) Anthracene	17.466	178	95113	0.896	ng/ul	100
19) Fluoranthene	19.392	202	1321782	13.696	ng/ul#	94
20) Pyrene	19.755	202	1032131	9.976	ng/ul	96
21) Benzo(a)anthracene	21.498	228	547897	7.130	ng/ul	97
22) Chrysene	21.550	228	585882	6.684	ng/ul	97
24) Benzo(b)fluoranthene	23.193	252	858747	9.542	ng/ul	89
25) Benzo(k)fluoranthene	23.237	252	296562m	3.344	ng/ul	
26) Benzo(a)pyrene	23.824	252	511694	6.312	ng/ul#	84
27) Indeno(1,2,3-cd)pyrene	26.437	276	438977	3.888	ng/ul#	86
28) Dibenzo(a,h)anthracene	26.448	278	111594	1.262	ng/ul	96
29) Benzo(g,h,i)perylene	27.216	276	431275	4.358	ng/ul	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062223\
Data File : BM040360.D
Acq On : 22 Jun 2023 22:10
Operator : MA/JU
Sample : 03084-17
Misc :
ALS Vial : 9 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
DCFN4

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/23/2023
Supervised By :mohammad ahmed 06/23/2023


Quant Time: Jun 23 02:28:02 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 23 00:44:24 2023
Response via : Initial Calibration

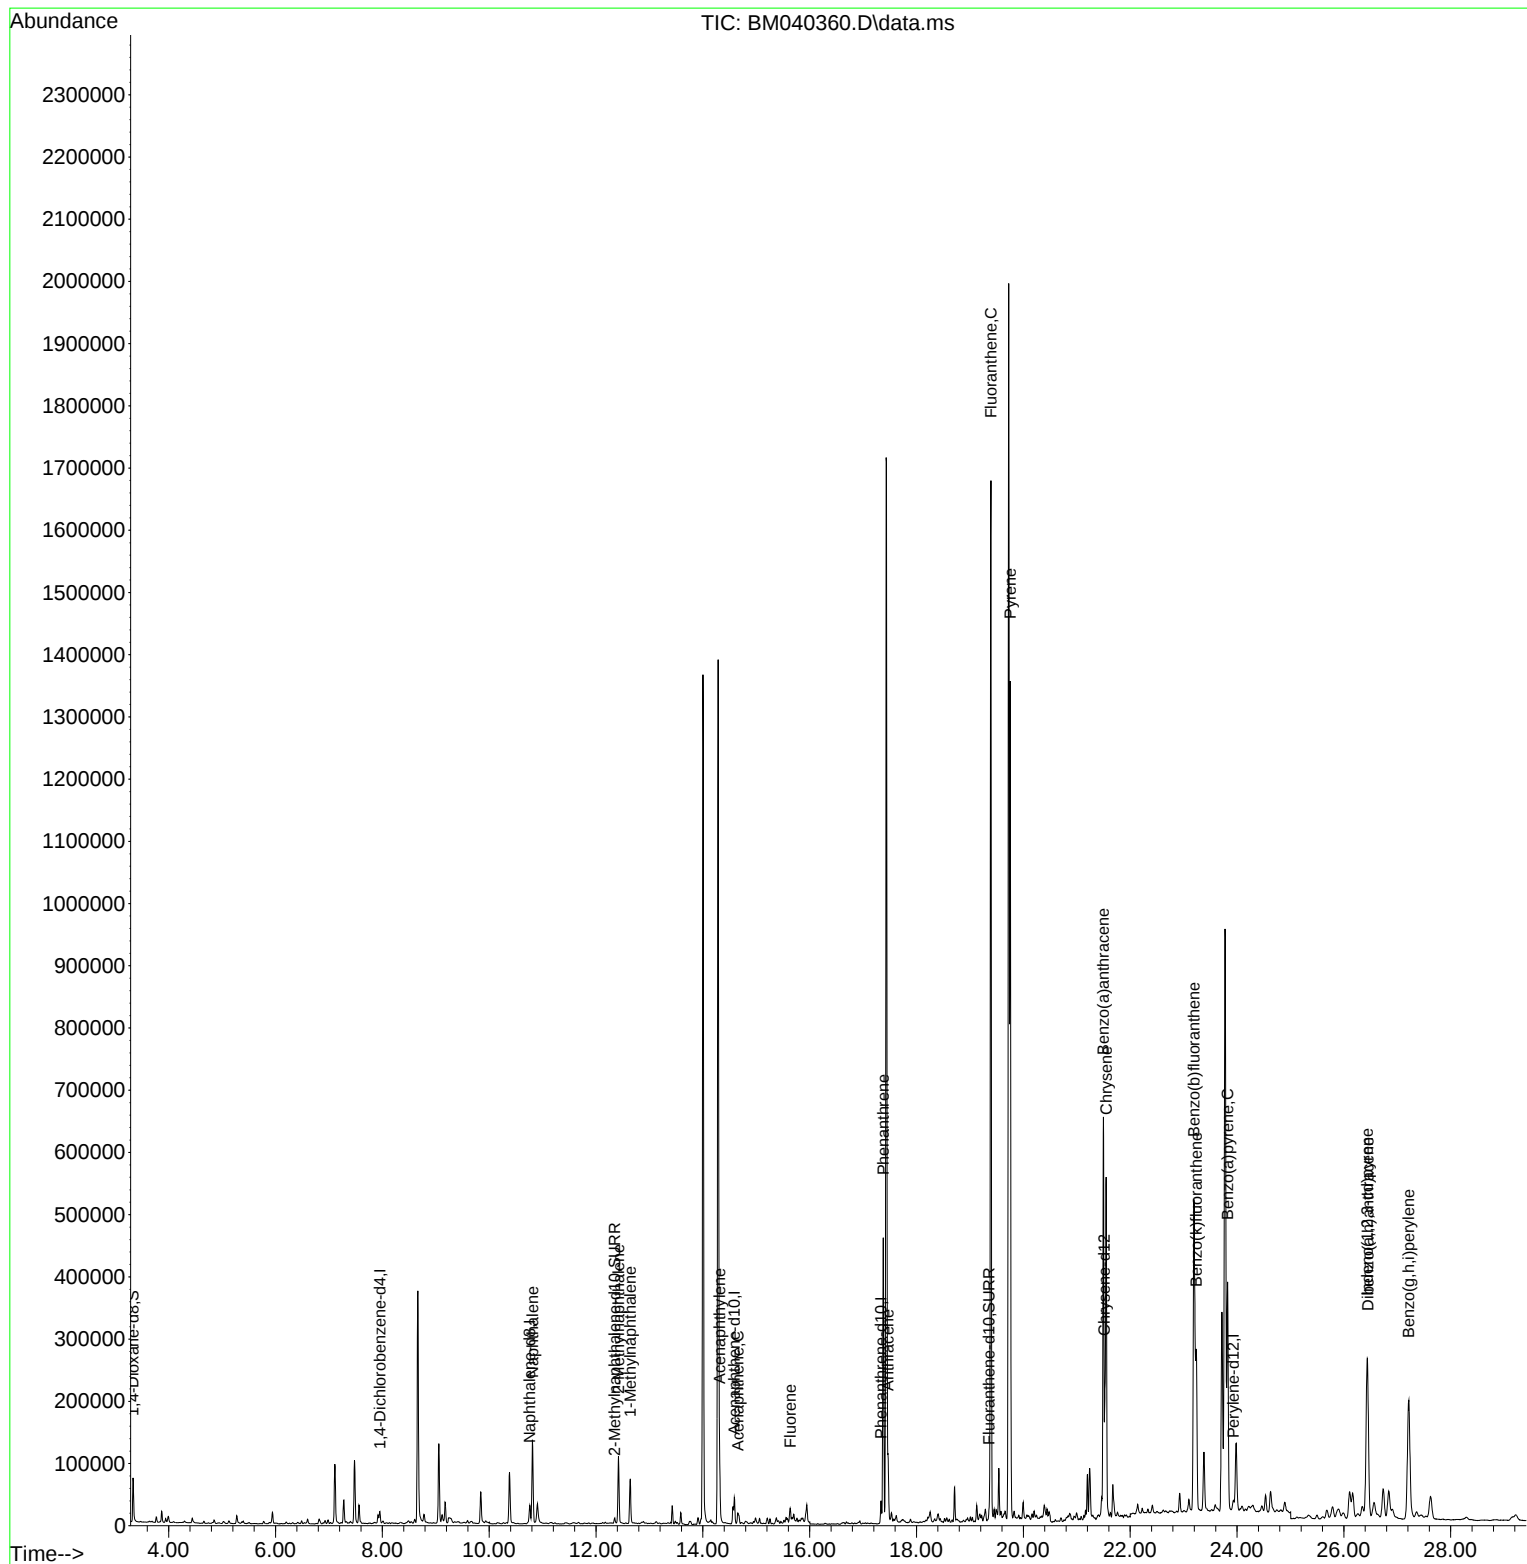

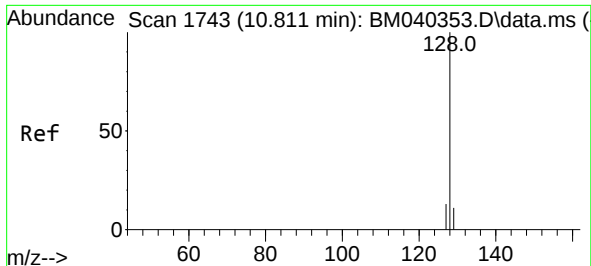

#5
Naphthalene
Concen: 1.658 ng/ul
RT: 10.810 min Scan# 1743
Delta R.T. -0.001 min
Lab File: BM040360.D
Acq: 22 Jun 2023 22:10




Instrument :
BNA_M
ClientSampleId :
DCFN4



Tgt Ion:128 Resp: 177350
Ion Ratio Lower Upper
128 100
129 11.3 9.2 13.8
127 13.0 10.6 15.8




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 06/23/2023
Supervised By :mohammad ahmed 06/23/2023

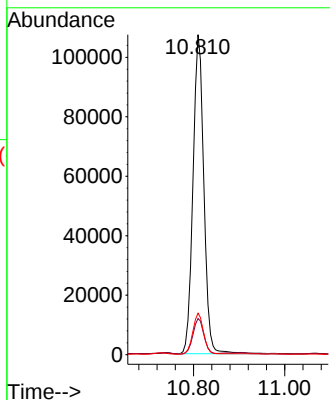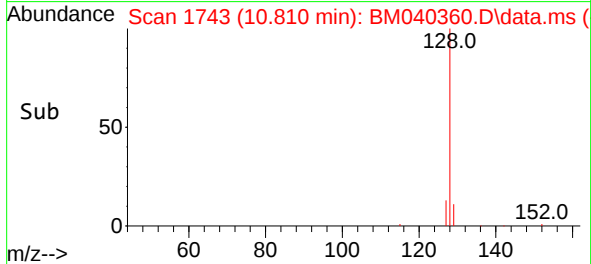

#7
2-Methylnaphthalene
Concen: 1.245 ng/ul
RT: 12.421 min Scan# 2036
Delta R.T. -0.001 min
Lab File: BM040360.D
Acq: 22 Jun 2023 22:10


Tgt Ion:142 Resp: 78211
Ion Ratio Lower Upper
142 100
141 87.7 71.9 107.9

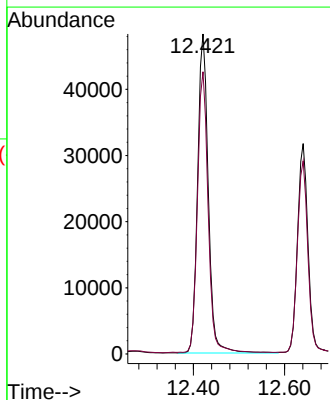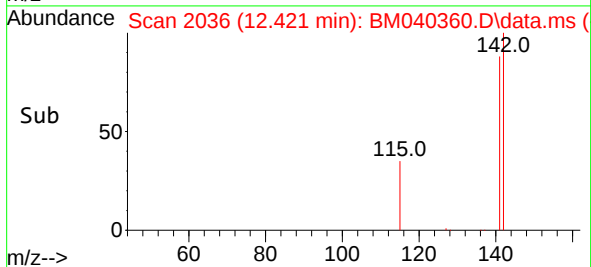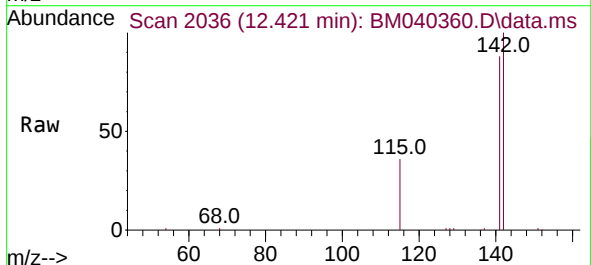

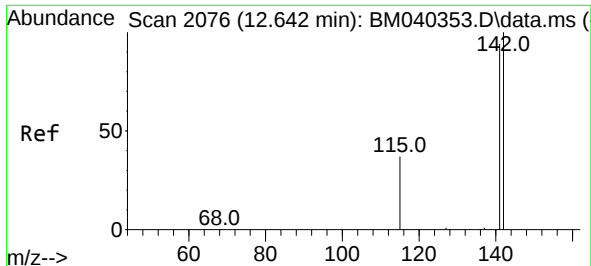

#8
1-Methylnaphthalene
Concen: 0.799 ng/ul
RT: 12.641 min Scan# 2076
Delta R.T. -0.001 min
Lab File: BM040360.D
Acq: 22 Jun 2023 22:10




Instrument :
BNA_M
ClientSampleId :
DCFN4

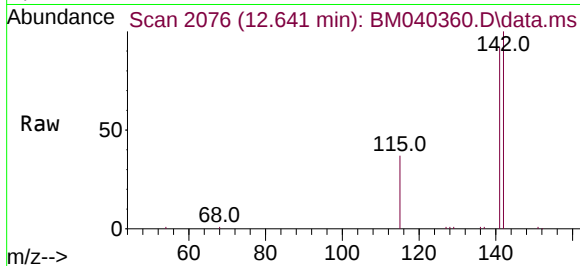

Tgt Ion:142 Resp: 5012
Ion Ratio Lower Upper
142 100
141 92.1 73.7 110.5




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 06/23/2023
Supervised By :mohammad ahmed 06/23/2023

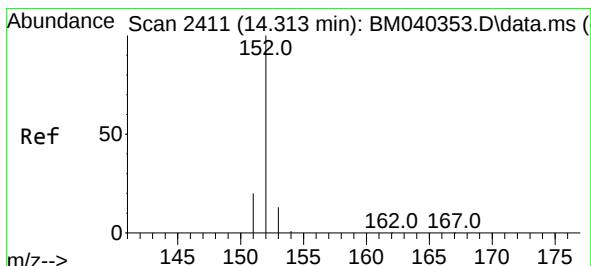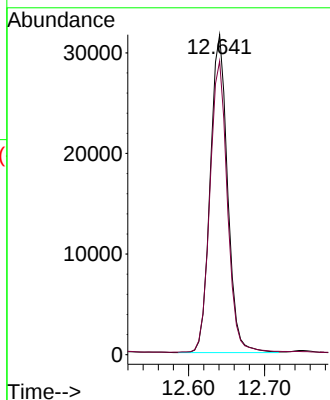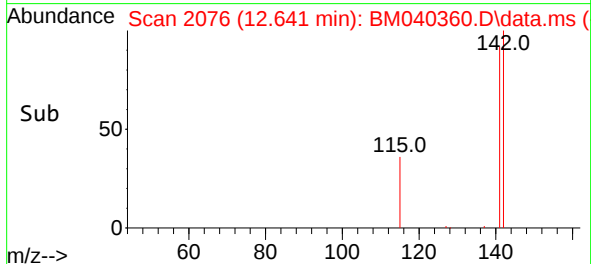

#10
Acenaphthylene
Concen: 1.002 ng/ul
RT: 14.312 min Scan# 2411
Delta R.T. -0.001 min
Lab File: BM040360.D
Acq: 22 Jun 2023 22:10


Tgt Ion:152 Resp: 100179
Ion Ratio Lower Upper
152 100
151 20.5 16.2 24.2
153 14.7 10.9 16.3

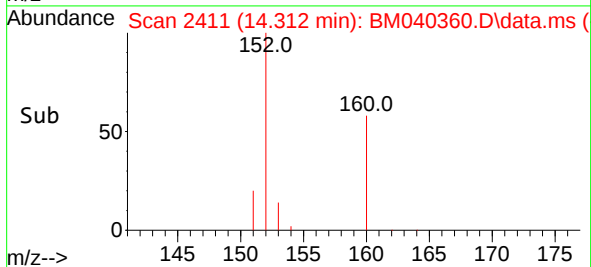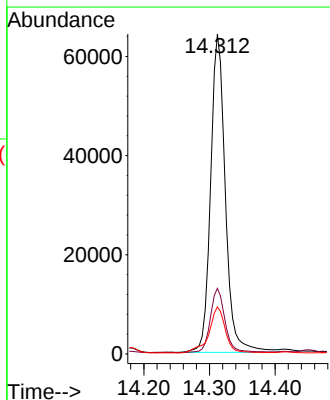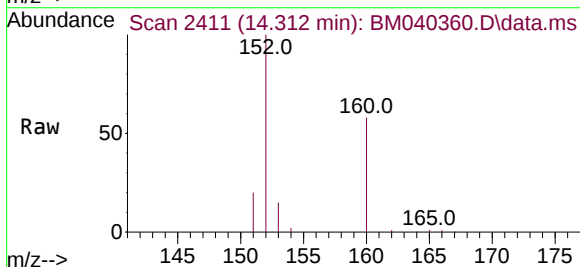

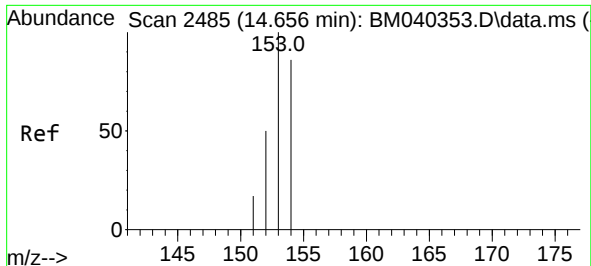

#11
Acenaphthene
Concen: 0.137 ng/ul
RT: 14.654 min Scan# 2485
Delta R.T. -0.001 min
Lab File: BM040360.D
Acq: 22 Jun 2023 22:10




Instrument :
BNA_M
ClientSampleId :
DCFN4

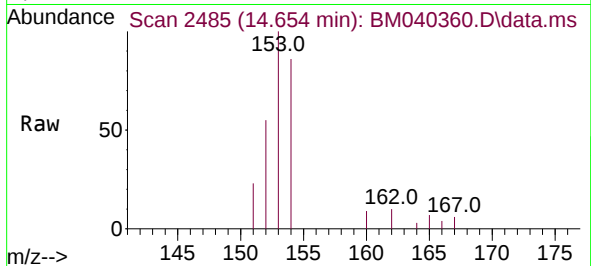

Tgt Ion:153 Resp: 1154
Ion Ratio Lower Upper
153 100
152 55.4 41.0 61.4
154 86.1 70.8 106.2




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 06/23/2023
Supervised By :mohammad ahmed 06/23/2023

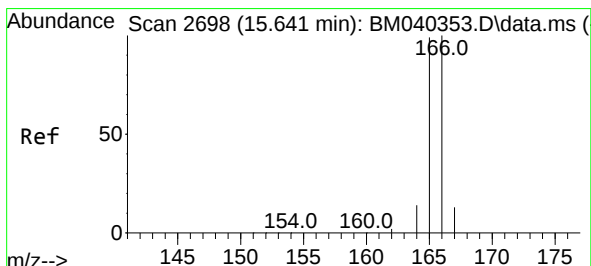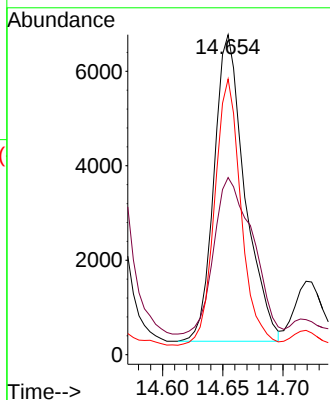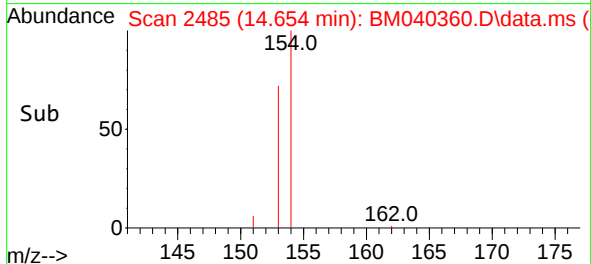

#12
Fluorene
Concen: 0.155 ng/ul
RT: 15.640 min Scan# 2698
Delta R.T. -0.001 min
Lab File: BM040360.D
Acq: 22 Jun 2023 22:10

Tgt Ion:166 Resp: 14005
Ion Ratio Lower Upper
166 100
165 103.6 79.6 119.4
167 26.8 11.4 17.0#

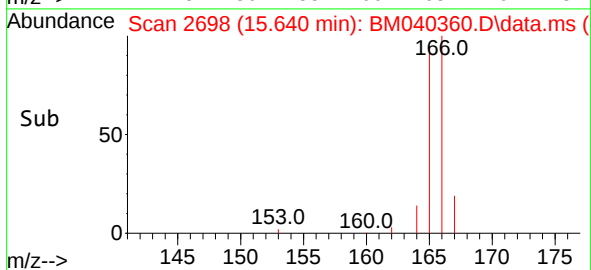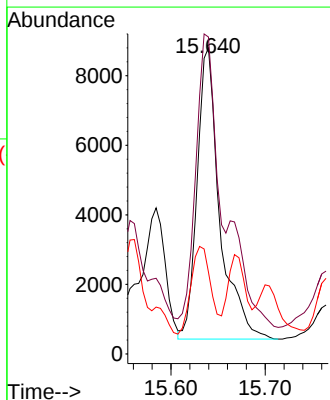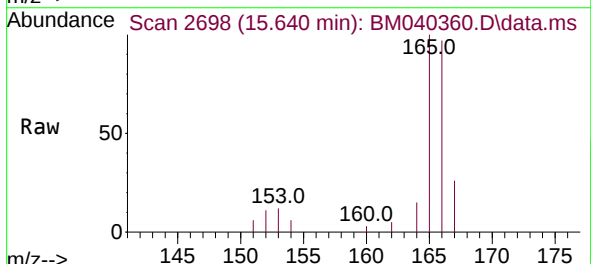

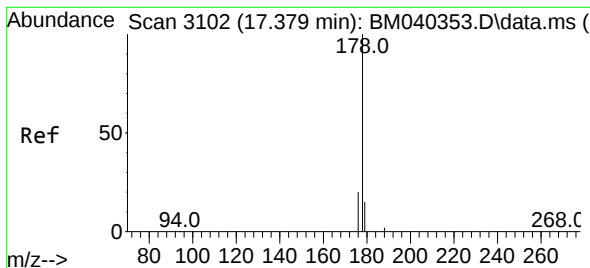

#15

Phenanthrene

Concen: 3.733 ng/u1

RT: 17.377 min Scan# 3102

Delta R.T. -0.001 min

Lab File: BM040360.D

Acq: 22 Jun 2023 22:10

Instrument :

BNA_M

ClientSampleId :

DCFN4

Tgt Ion:178 Resp: 47137





Ion	Ratio	Lower	Upper
178	100		
179	15.5	12.8	19.2
176	19.7	16.4	24.6

Manual Integrations

APPROVED

Reviewed By :Yogesh Patel 06/23/2023

Supervised By :mohammad ahmed 06/23/2023

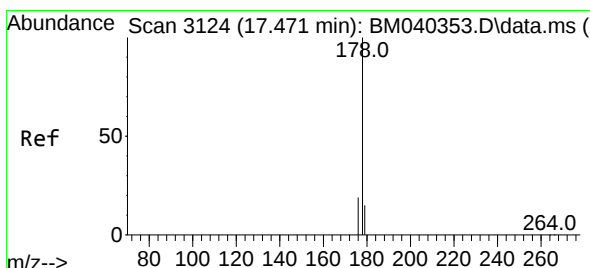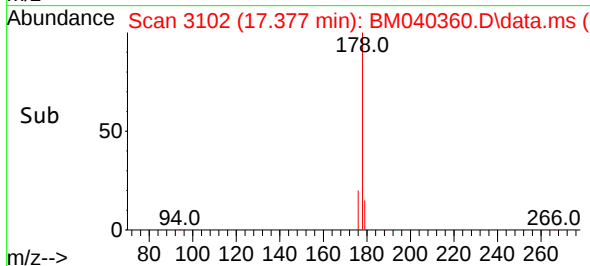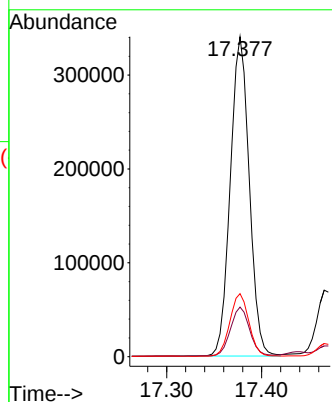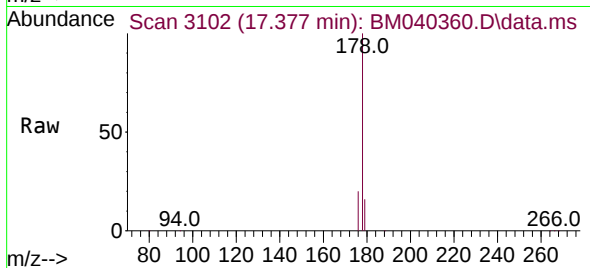

#16

Anthracene

Concen: 0.896 ng/u1

RT: 17.466 min Scan# 3123




Delta R.T. -0.006 min


Lab File: BM040360.D

Acq: 22 Jun 2023 22:10

Tgt Ion:178 Resp: 95113


Ion	Ratio	Lower	Upper
178	100		
179	16.2	12.9	19.3
176	19.6	15.8	23.6

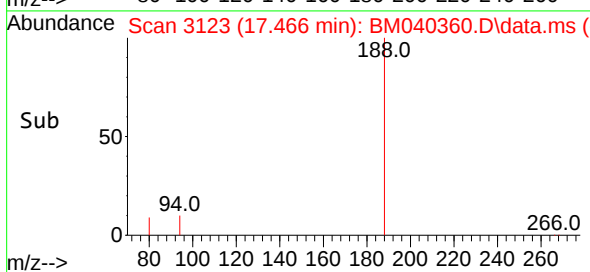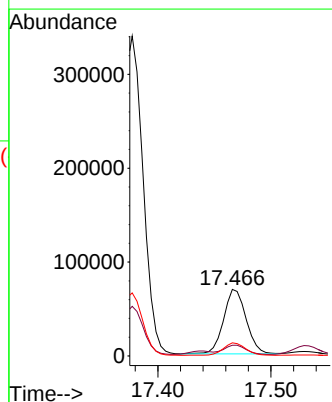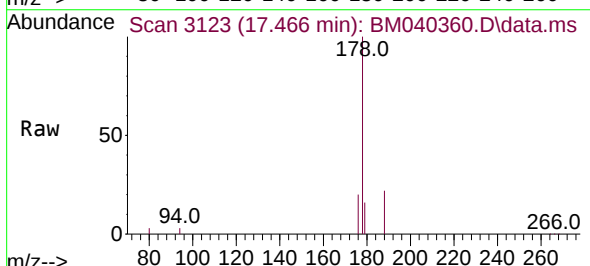



#19
Fluoranthene
Concen: 13.696 ng/u1
RT: 19.392 min Scan# 3560
Delta R.T. 0.003 min
Lab File: BM040360.D
Acq: 22 Jun 2023 22:10




Instrument :
BNA_M
ClientSampleId :
DCFN4

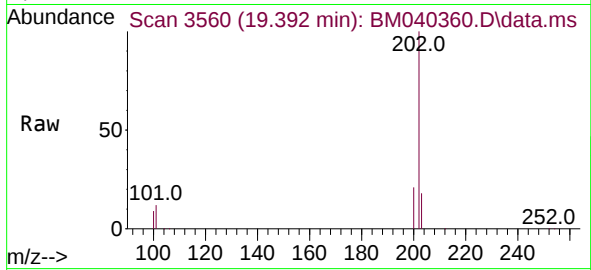


Tgt Ion:202 Resp: 132178
Ion Ratio Lower Upper
202 100
101 11.7 11.4 17.0
100 8.5 8.7 13.1

Manual Integrations
APPROVED



Reviewed By :Yogesh Patel 06/23/2023
Supervised By :mohammad ahmed 06/23/2023

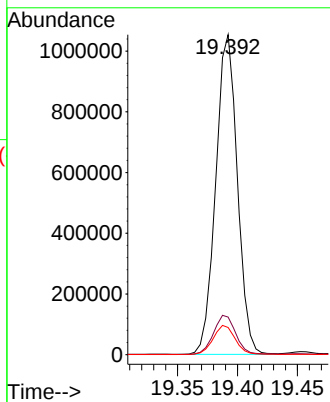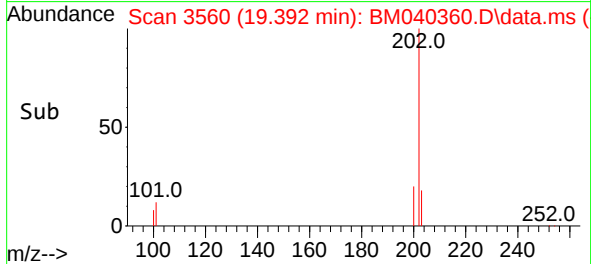


#20
Pyrene
Concen: 9.976 ng/u1
RT: 19.755 min Scan# 3638
Delta R.T. -0.001 min
Lab File: BM040360.D
Acq: 22 Jun 2023 22:10

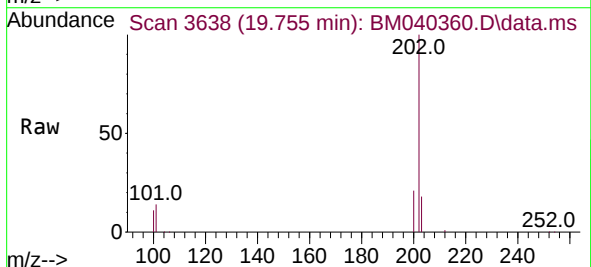


Tgt Ion:202 Resp: 1032131
Ion Ratio Lower Upper
202 100
101 13.9 12.6 18.8
100 10.8 9.8 14.6

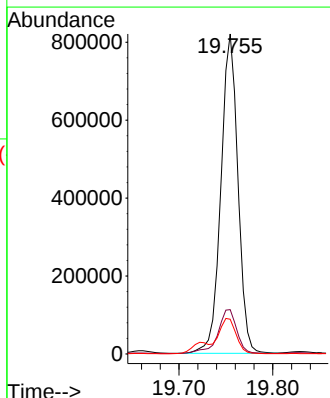

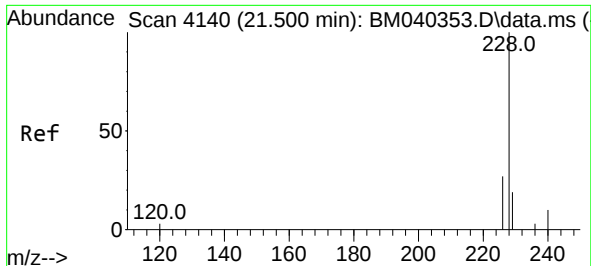

#21
Benzo(a)anthracene
Concen: 7.130 ng/ul
RT: 21.498 min Scan# 4139
Delta R.T. -0.003 min
Lab File: BM040360.D
Acq: 22 Jun 2023 22:10




Instrument :
BNA_M
ClientSampleId :
DCFN4



Tgt Ion:228 Resp: 54789
Ion Ratio Lower Upper
228 100
229 21.6 16.0 24.0
226 29.3 22.3 33.5




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 06/23/2023
Supervised By :mohammad ahmed 06/23/2023

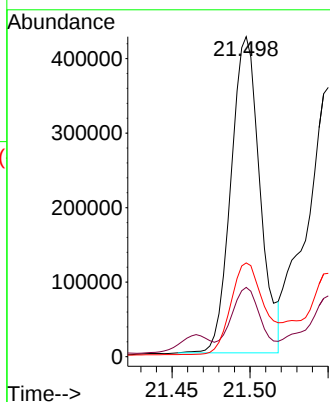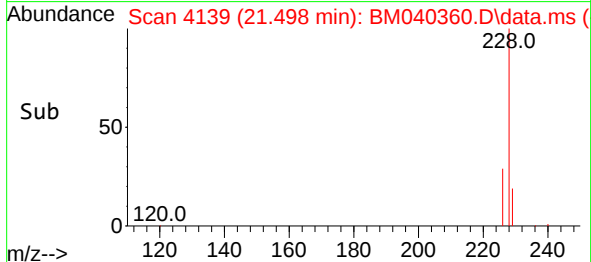

#22
Chrysene
Concen: 6.684 ng/ul
RT: 21.550 min Scan# 4157
Delta R.T. -0.003 min
Lab File: BM040360.D
Acq: 22 Jun 2023 22:10


Tgt Ion:228 Resp: 585882
Ion Ratio Lower Upper
228 100
226 31.0 24.9 37.3
229 22.6 15.8 23.6

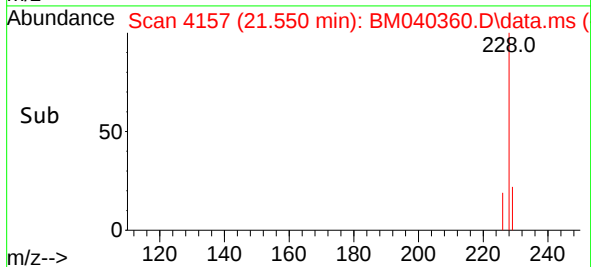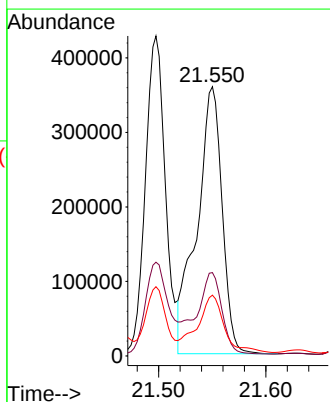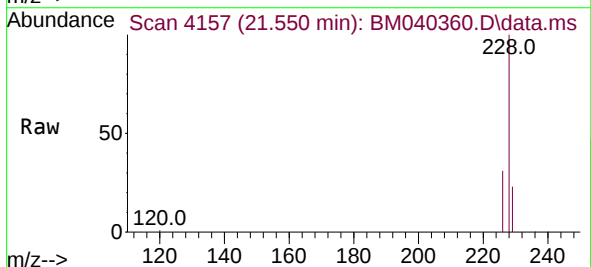

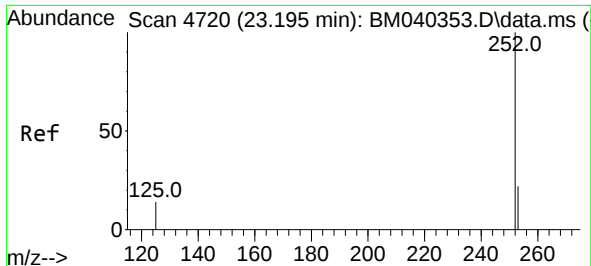

#24
Benzo(b)fluoranthene
Concen: 9.542 ng/ul
RT: 23.193 min Scan# 4719
Delta R.T. 0.000 min
Lab File: BM040360.D
Acq: 22 Jun 2023 22:10




Instrument :
BNA_M
ClientSampleId :
DCFN4




Tgt Ion:252 Resp: 85874
Ion Ratio Lower Upper
252 100
253 23.4 0.0 52.8
125 13.8 0.0 43.0

Manual Integrations
APPROVED



Reviewed By :Yogesh Patel 06/23/2023
Supervised By :mohammad ahmed 06/23/2023

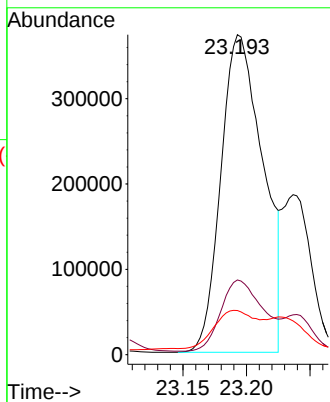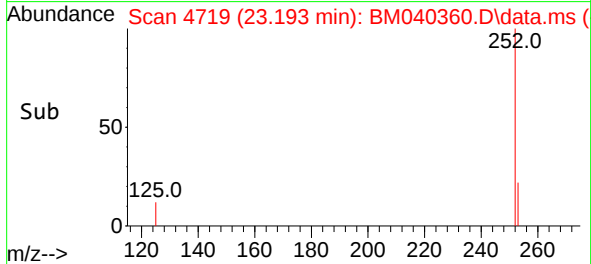


#25
Benzo(k)fluoranthene
Concen: 3.344 ng/ul m
RT: 23.237 min Scan# 4734
Delta R.T. -0.006 min
Lab File: BM040360.D
Acq: 22 Jun 2023 22:10

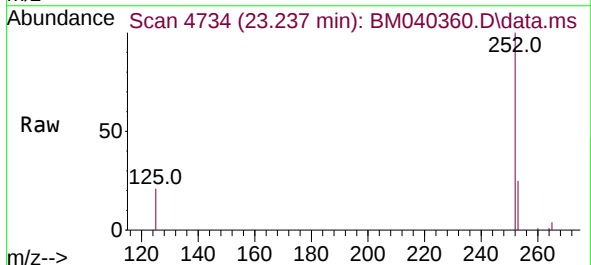


Tgt Ion:252 Resp: 296562
Ion Ratio Lower Upper
252 100
253 25.0 21.2 31.8
125 21.1 16.4 24.6

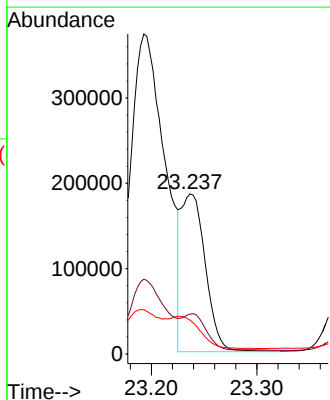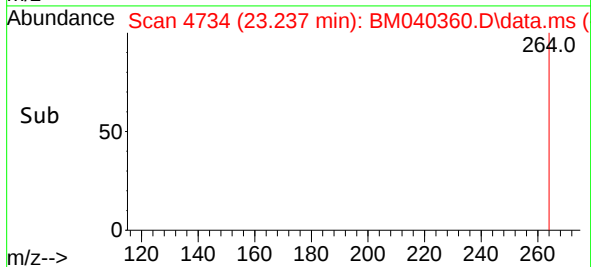

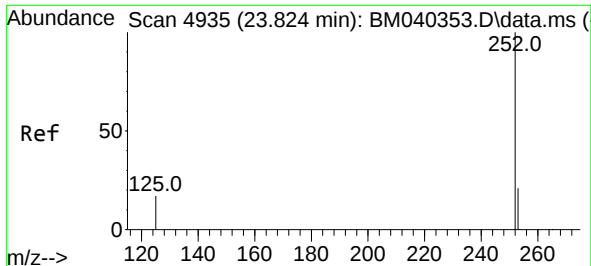

#26
Benzo(a)pyrene
Concen: 6.312 ng/ul
RT: 23.824 min Scan# 4935
Delta R.T. 0.000 min
Lab File: BM040360.D
Acq: 22 Jun 2023 22:10




Instrument :
BNA_M
ClientSampleId :
DCFN4



Tgt Ion:252 Resp: 511694
Ion Ratio Lower Upper
252 100
253 23.8 22.9 34.3
125 14.0 21.0 31.4




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 06/23/2023
Supervised By :mohammad ahmed 06/23/2023

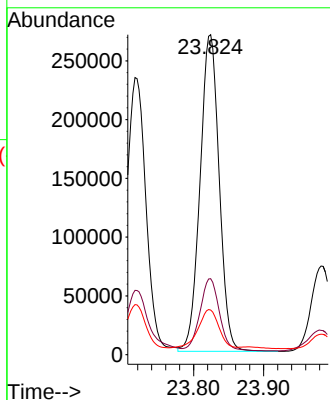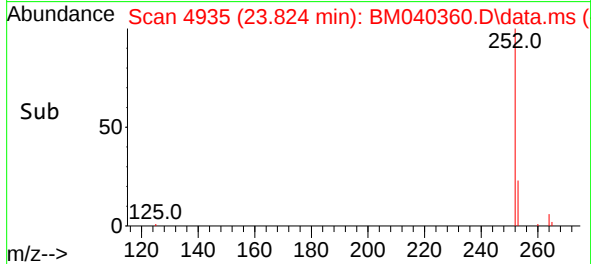

#27
Indeno(1,2,3-cd)pyrene
Concen: 3.888 ng/ul
RT: 26.437 min Scan# 5766
Delta R.T. 0.004 min
Lab File: BM040360.D
Acq: 22 Jun 2023 22:10

Tgt Ion:276 Resp: 438977
Ion Ratio Lower Upper
276 100
138 22.8 24.5 36.7#
227 0.0 0.1 0.1#

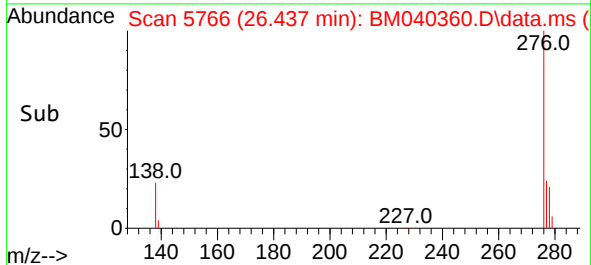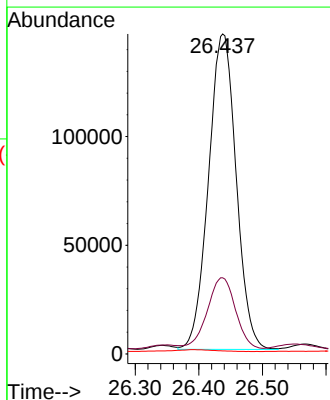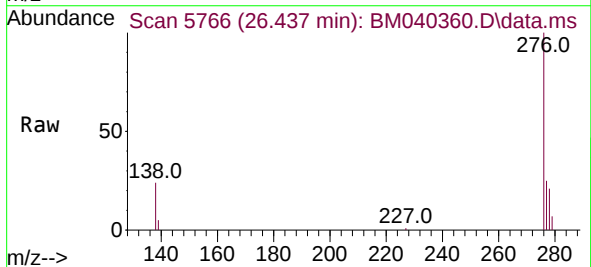



#28

Dibenzo(a,h)anthracene

Concen: 1.262 ng/ul

RT: 26.448 min Scan# 51

Delta R.T. -0.006 min

Lab File: BM040360.D

Acq: 22 Jun 2023 22:10

Instrument :

BNA_M

ClientSampleId :

DCFN4

Tgt Ion:278 Resp: 111594

Ion Ratio Lower Upper

278 100

139 22.4 17.9 26.9





279 31.1 22.0 33.0

Manual Integrations

APPROVED

Reviewed By :Yogesh Patel 06/23/2023

Supervised By :mohammad ahmed 06/23/2023

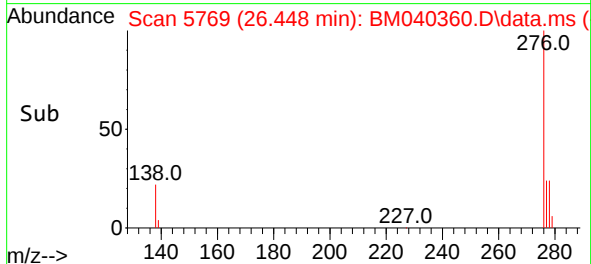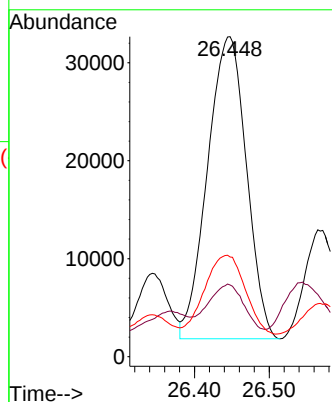

#29

Benzo(g,h,i)perylene

Concen: 4.358 ng/ul

RT: 27.216 min Scan# 5998

Delta R.T. 0.010 min

Lab File: BM040360.D

Acq: 22 Jun 2023 22:10

Tgt Ion:276 Resp: 431275

Ion Ratio Lower Upper

276 100

138 24.2 23.0 34.6

277 24.6 20.3 30.5

