

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062322\
 Data File : BM035633.D
 Acq On : 23 Jun 2022 19:53
 Operator : CG/JU
 Sample : N3358-03
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Jun 24 01:36:10 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM061822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 20 01:56:13 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.820	152	5644	0.400	ng/ul	-0.04
4) Naphthalene-d8	10.605	136	22079	0.400	ng/ul	-0.04
9) Acenaphthene-d10	14.446	164	12696	0.400	ng/ul	-0.02
13) Phenanthrene-d10	17.196	188	24839	0.400	ng/ul	-0.03
17) Chrysene-d12	21.405	240	15857	0.400	ng/ul	0.00
23) Perylene-d12	23.726	264	20238	0.400	ng/ul	#-0.04
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.264	96	26630	3.353	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.217	152	9254	0.282	ng/ul	-0.03
18) Fluoranthene-d10	19.234	212	19921	0.374	ng/ul	-0.02
Target Compounds						
					Qvalue	
14) Pentachlorophenol	16.900	266	156	0.033	ng/ul	97
20) Pyrene	19.620	202	3620	0.043	ng/ul#	51
26) Benzo(a)pyrene	23.562	252	5264	0.057	ng/ul#	47


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062322\
Data File : BM035633.D
Acq On : 23 Jun 2022 19:53
Operator : CG/JU
Sample : N3358-03
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :


Quant Time: Jun 24 01:36:10 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM061822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 20 01:56:13 2022
Response via : Initial Calibration

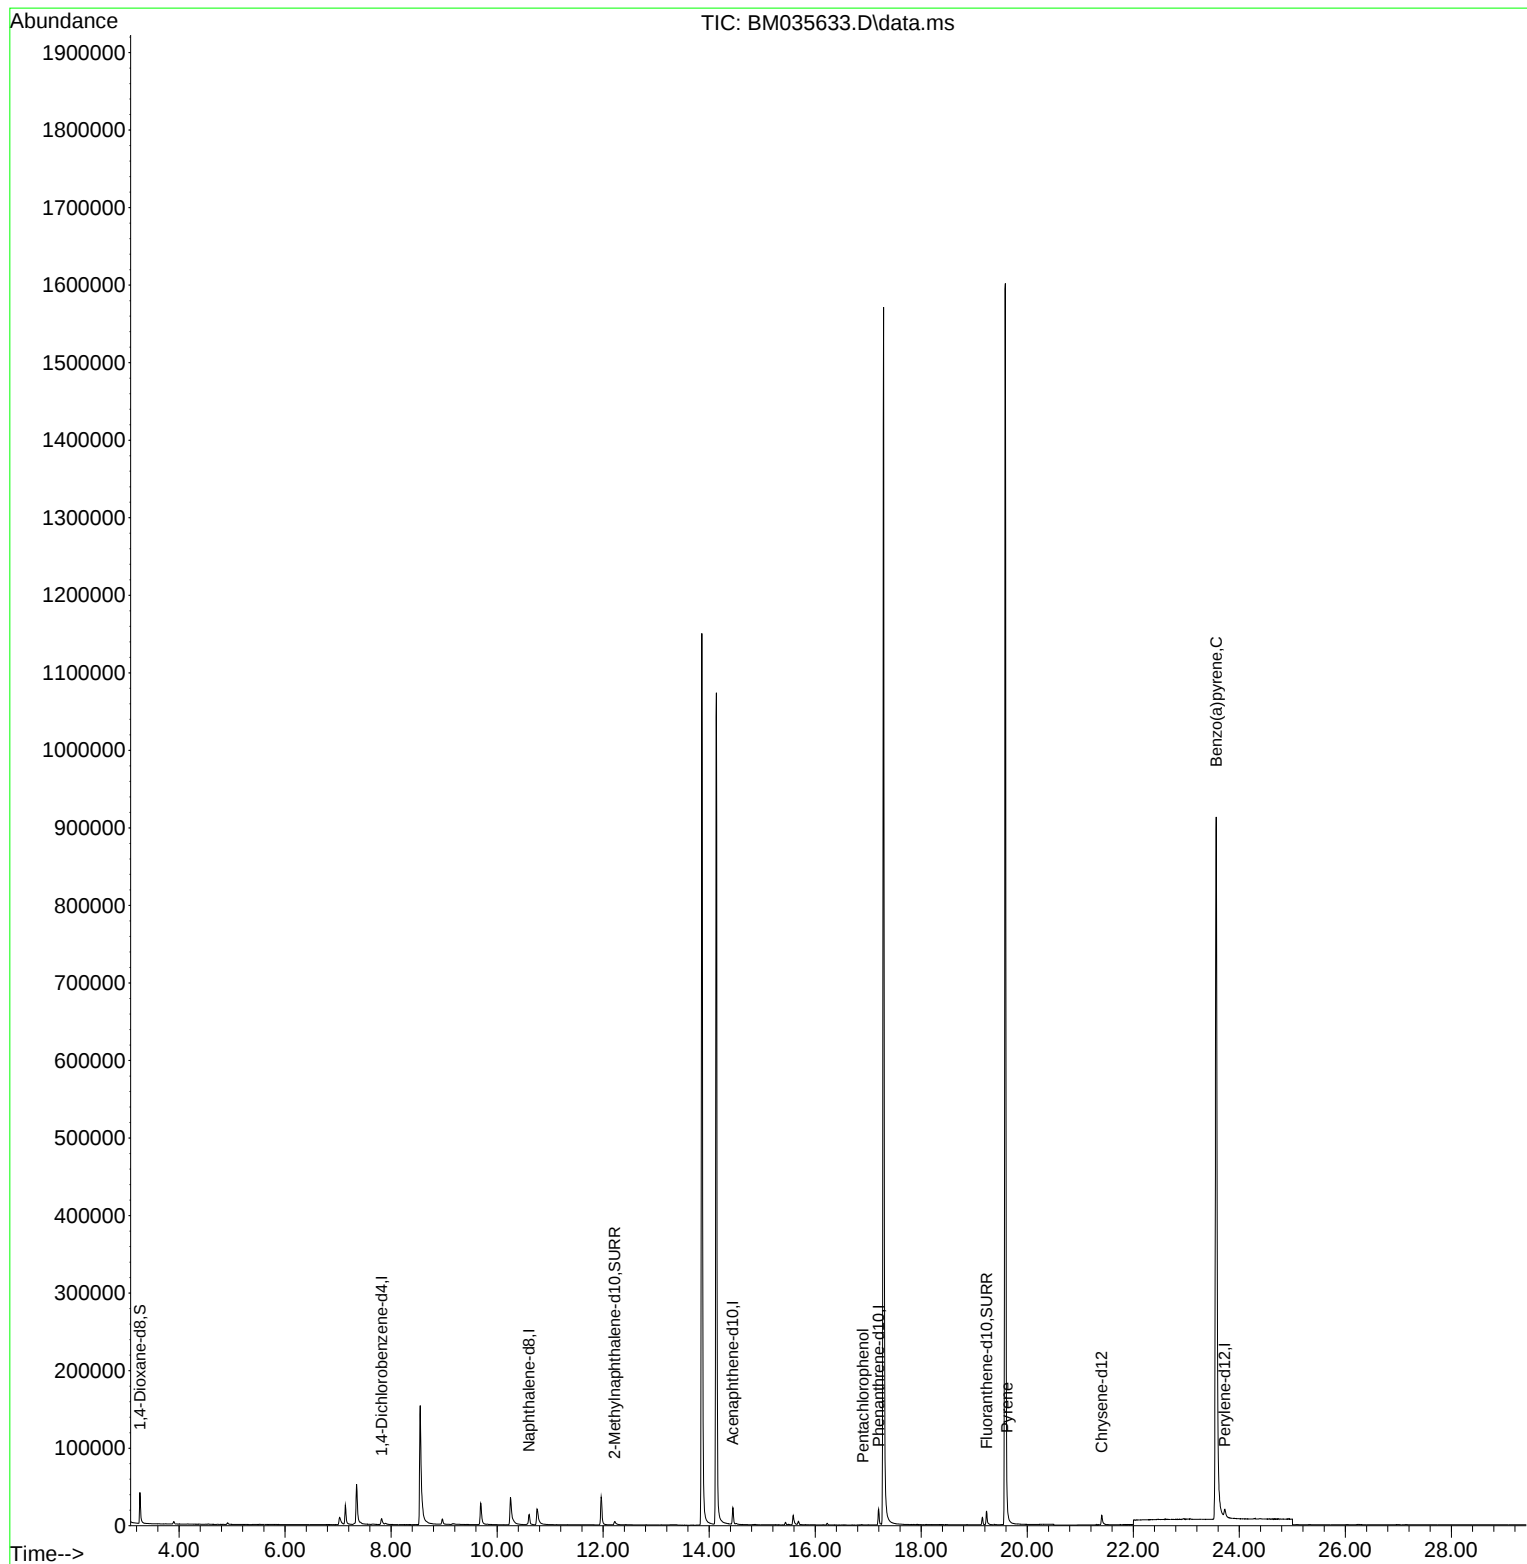



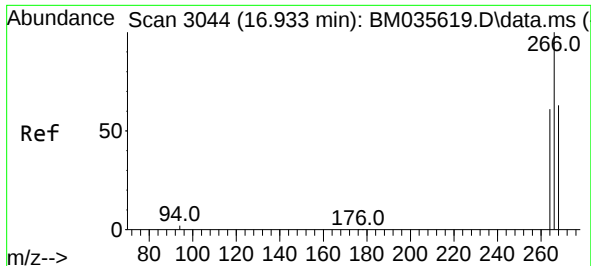


#14
 Pentachlorophenol
 Concen: 0.033 ng/ul
 RT: 16.900 min Scan# 3044
 Delta R.T. -0.030 min
 Lab File: BM035633.D
 Acq: 23 Jun 2022 19:53

Instrument :
 BNA_M
 ClientSampleId :



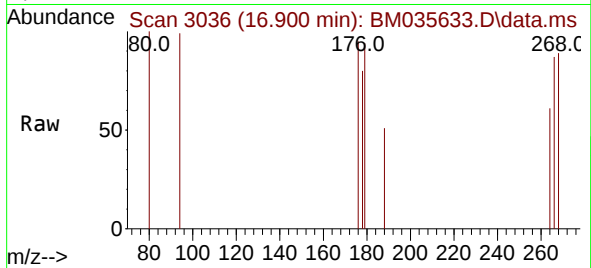



Tgt Ion:266 Resp: 156
 Ion Ratio Lower Upper
 266 100
 264 66.0 51.0 76.4
 268 62.8 51.7 77.5

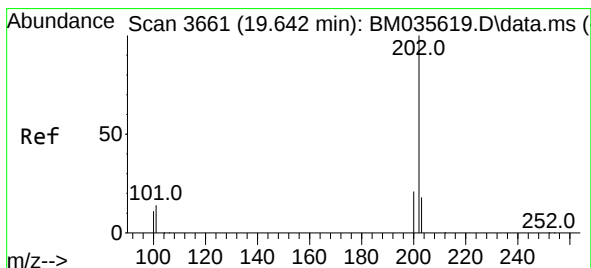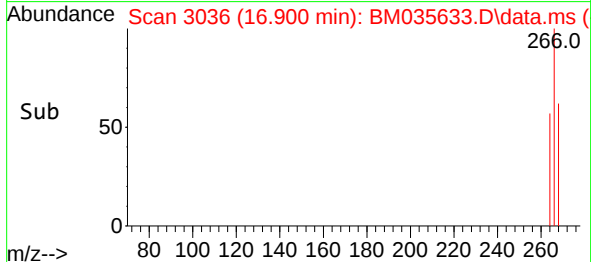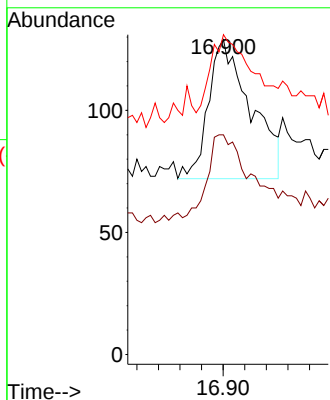

#20
 Pyrene
 Concen: 0.043 ng/ul
 RT: 19.620 min Scan# 3656
 Delta R.T. -0.028 min
 Lab File: BM035633.D
 Acq: 23 Jun 2022 19:53


Tgt Ion:202 Resp: 3620
 Ion Ratio Lower Upper
 202 100
 101 25.6 11.6 17.4#
 100 41.3 9.3 13.9#

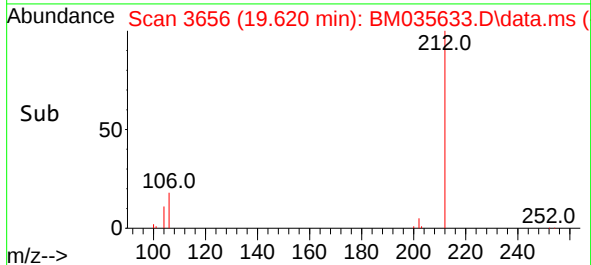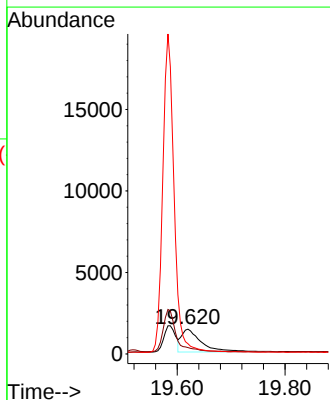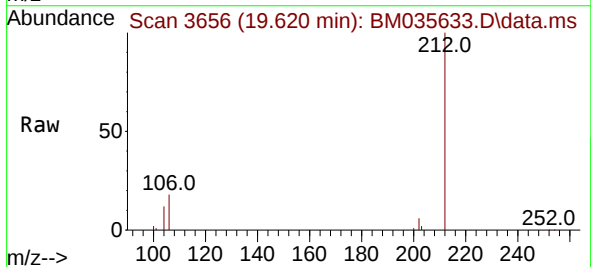

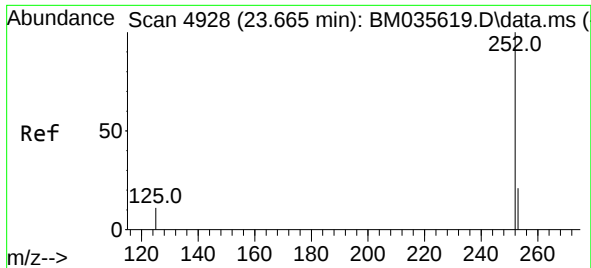

#26
 Benzo(a)pyrene
 Concen: 0.057 ng/ul
 RT: 23.562 min Scan# 41
 Delta R.T. -0.105 min
 Lab File: BM035633.D
 Acq: 23 Jun 2022 19:53

Instrument :
 BNA_M
 ClientSampleId :

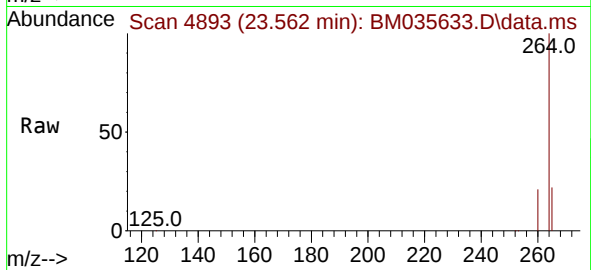

Tgt Ion:252 Resp: 5264
 Ion Ratio Lower Upper
 252 100
 253 62.9 27.8 41.6#
 125 59.6 23.3 34.9#

