

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062322\
 Data File : BM035637.D
 Acq On : 23 Jun 2022 22:54
 Operator : CG/JU
 Sample : PB145602BL
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Jun 24 01:36:28 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM061822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 20 01:56:13 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.820	152	5656	0.400	ng/ul	-0.04
4) Naphthalene-d8	10.606	136	20888	0.400	ng/ul	#-0.04
9) Acenaphthene-d10	14.446	164	12831	0.400	ng/ul	#-0.02
13) Phenanthrene-d10	17.195	188	27967	0.400	ng/ul	-0.03
17) Chrysene-d12	21.415	240	19352	0.400	ng/ul	0.00
23) Perylene-d12	23.727	264	22577	0.400	ng/ul	#-0.04
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.260	96	34900	4.385	ng/ul	-0.01
6) 2-Methylnaphthalene-d10	12.250	152	8022	0.258	ng/ul	0.00
18) Fluoranthene-d10	19.233	212	19066	0.293	ng/ul	-0.02
Target Compounds						
					Qvalue	
20) Pyrene	19.615	202	2650	0.026	ng/ul#	1
26) Benzo(a)pyrene	23.560	252	4810	0.047	ng/ul#	56


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062322\
Data File : BM035637.D
Acq On : 23 Jun 2022 22:54
Operator : CG/JU
Sample : PB145602BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :


Quant Time: Jun 24 01:36:28 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM061822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 20 01:56:13 2022
Response via : Initial Calibration

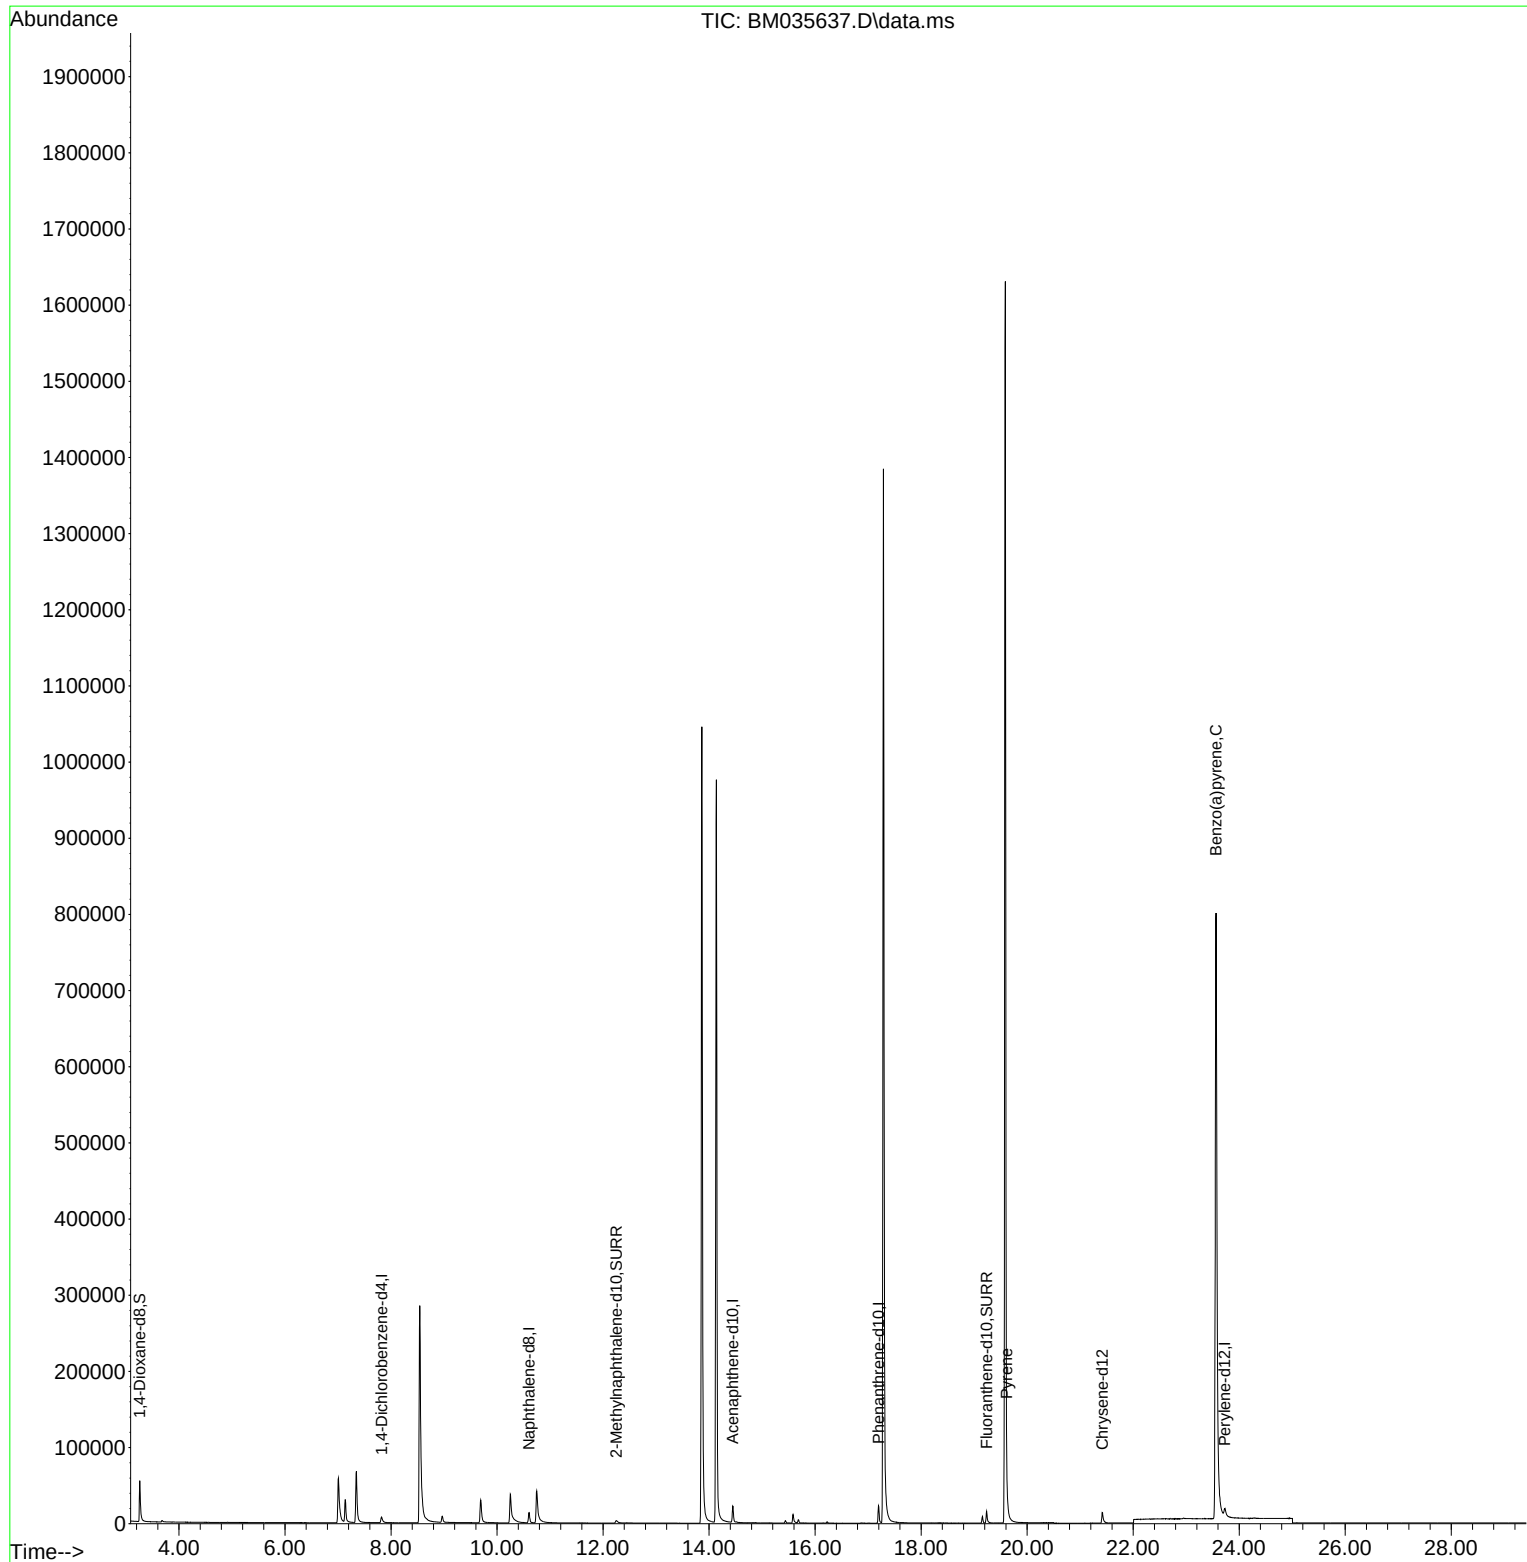



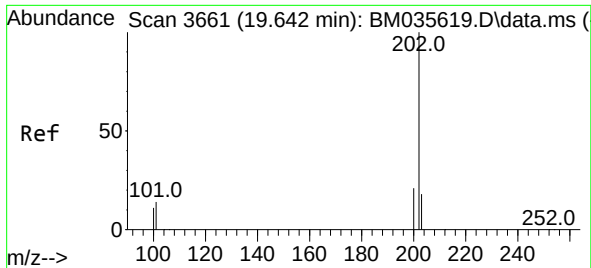


#20
Pyrene
Concen: 0.026 ng/ul
RT: 19.615 min Scan# 3655
Delta R.T. -0.033 min
Lab File: BM035637.D
Acq: 23 Jun 2022 22:54

Instrument :
BNA_M
ClientSampleId :

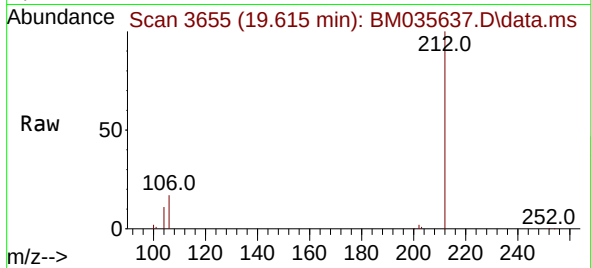

Tgt Ion:202 Resp: 2650
Ion Ratio Lower Upper
202 100
101 35.2 11.6 17.4#
100 115.5 9.3 13.9#

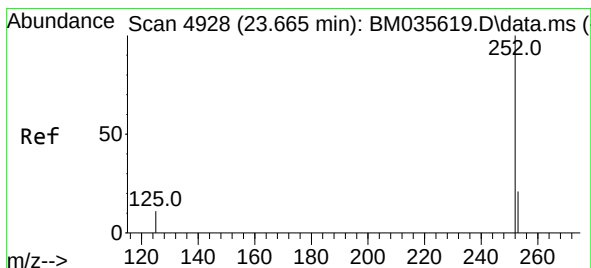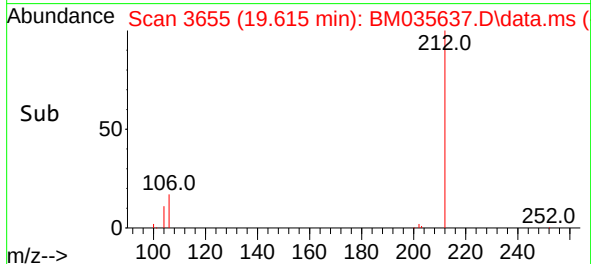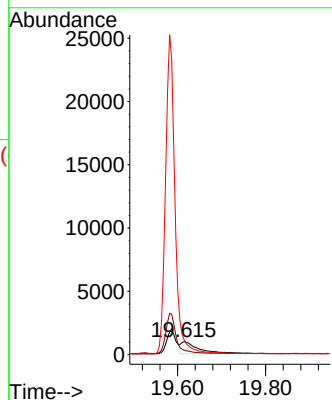

#26
Benzo(a)pyrene
Concen: 0.047 ng/ul
RT: 23.560 min Scan# 4892
Delta R.T. -0.107 min
Lab File: BM035637.D
Acq: 23 Jun 2022 22:54

Tgt Ion:252 Resp: 4810
Ion Ratio Lower Upper
252 100
253 58.1 27.8 41.6#
125 54.5 23.3 34.9#

