

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062322\
 Data File : BM035640.D
 Acq On : 24 Jun 2022 00:43
 Operator : CG/JU
 Sample : N3358-01
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Jun 24 01:36:39 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM061822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 20 01:56:13 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.816	152	5370	0.400	ng/ul	-0.04
4) Naphthalene-d8	10.600	136	21658	0.400	ng/ul	-0.04
9) Acenaphthene-d10	14.445	164	12433	0.400	ng/ul	-0.02
13) Phenanthrene-d10	17.195	188	28442	0.400	ng/ul	-0.03
17) Chrysene-d12	21.400	240	24052	0.400	ng/ul	-0.01
23) Perylene-d12	23.727	264	25375	0.400	ng/ul	#-0.04
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.260	96	27702	3.666	ng/ul	-0.01
6) 2-Methylnaphthalene-d10	12.217	152	8452	0.263	ng/ul	-0.03
18) Fluoranthene-d10	19.229	212	25658	0.318	ng/ul	-0.02
Target Compounds						
					Qvalue	
14) Pentachlorophenol	16.904	266	185	0.034	ng/ul	89
20) Pyrene	19.619	202	2916	0.023	ng/ul#	44
26) Benzo(a)pyrene	23.563	252	5921	0.051	ng/ul#	49


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062322\
Data File : BM035640.D
Acq On : 24 Jun 2022 00:43
Operator : CG/JU
Sample : N3358-01
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :


Quant Time: Jun 24 01:36:39 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM061822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 20 01:56:13 2022
Response via : Initial Calibration

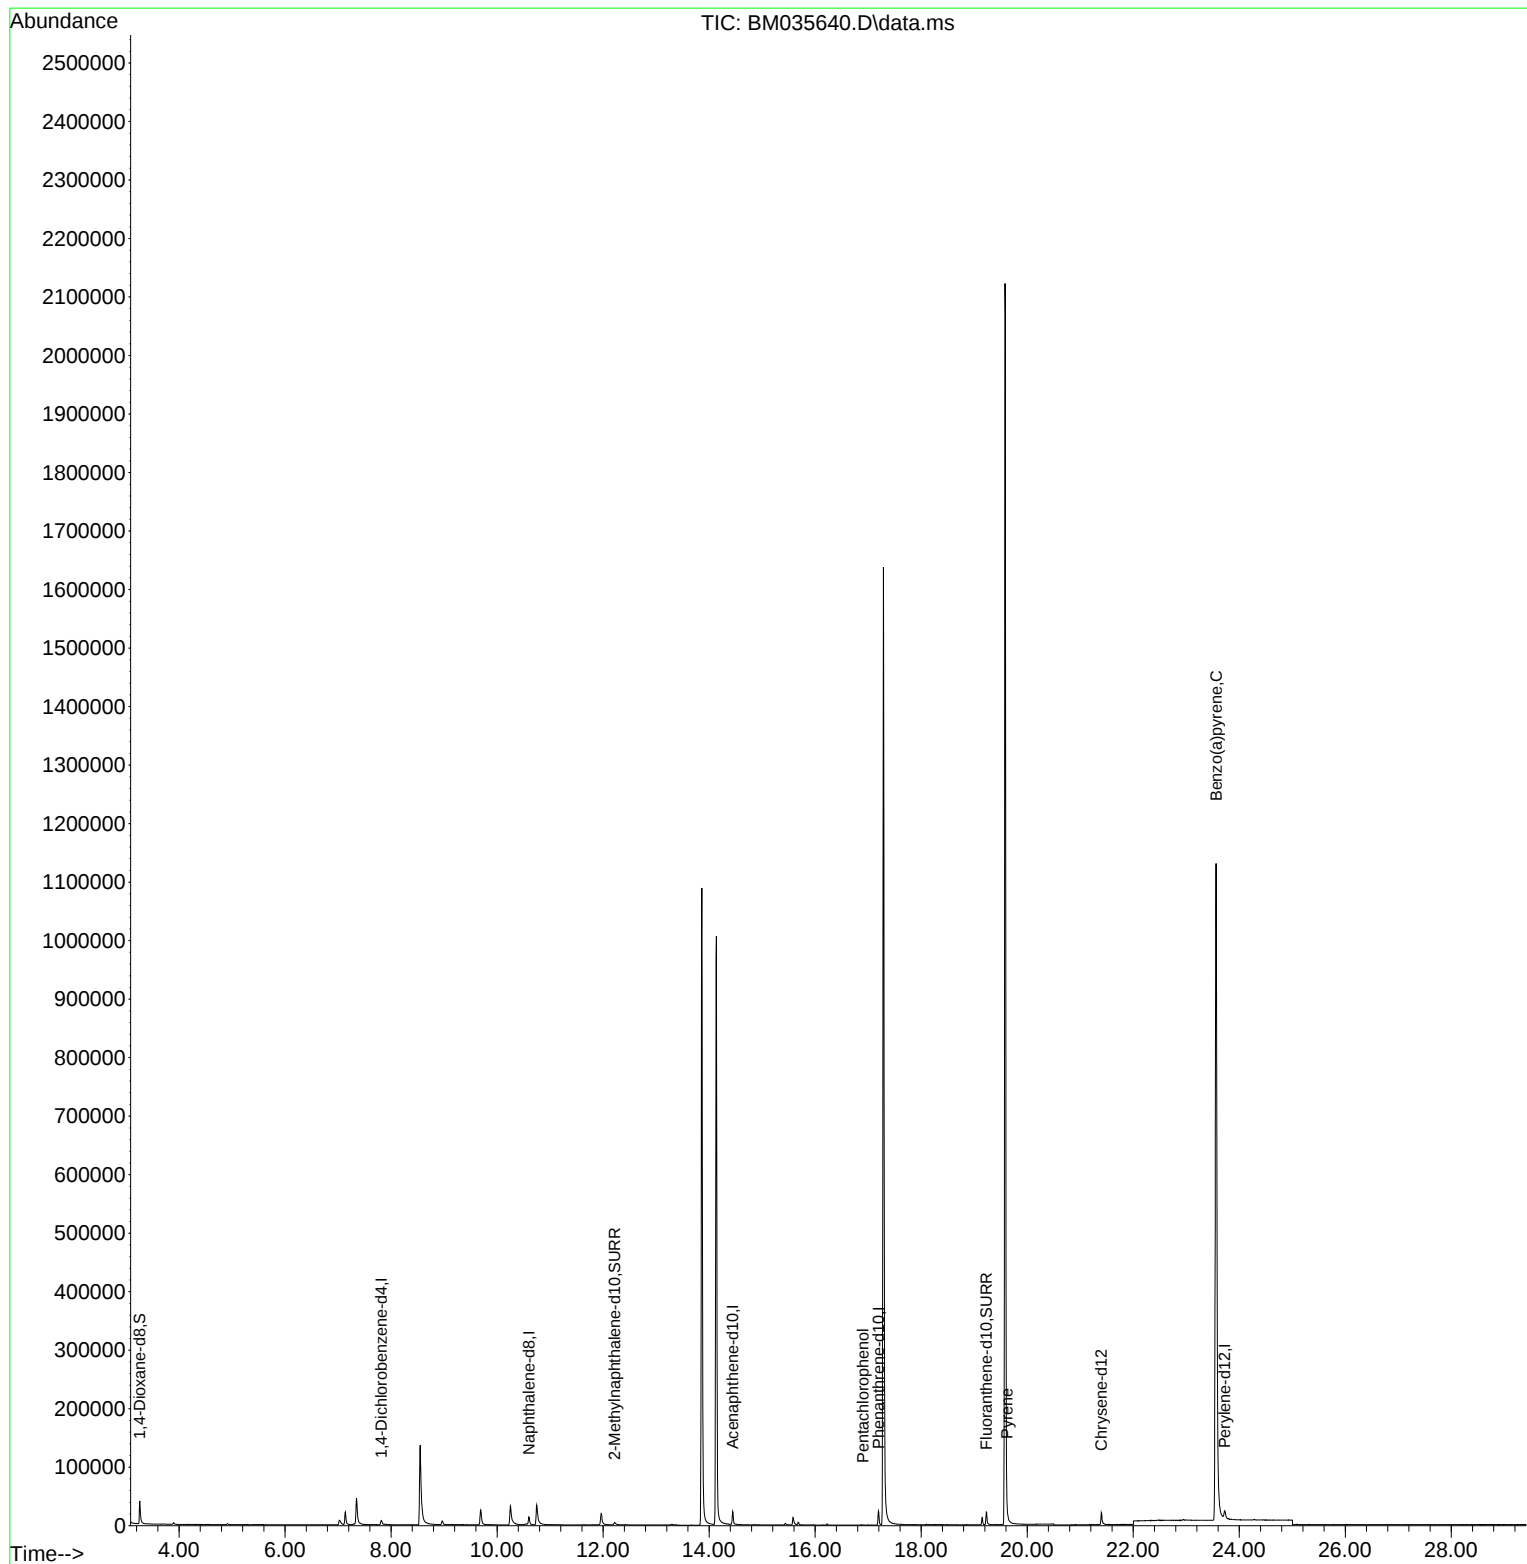



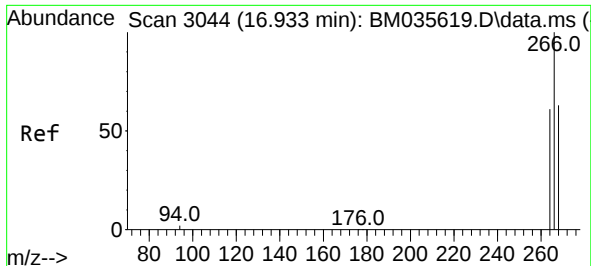


#14
 Pentachlorophenol
 Concen: 0.034 ng/ul
 RT: 16.904 min Scan# 3044
 Delta R.T. -0.026 min
 Lab File: BM035640.D
 Acq: 24 Jun 2022 00:43

Instrument :
 BNA_M
 ClientSampleId :



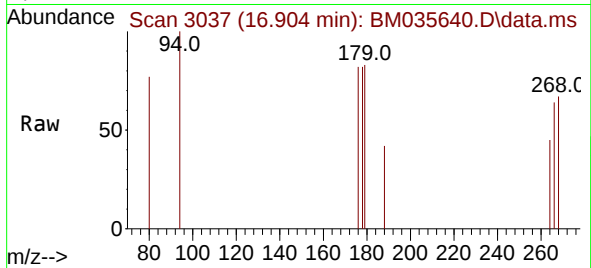



Tgt Ion:266 Resp: 185
 Ion Ratio Lower Upper
 266 100
 264 55.7 51.0 76.4
 268 55.1 51.7 77.5

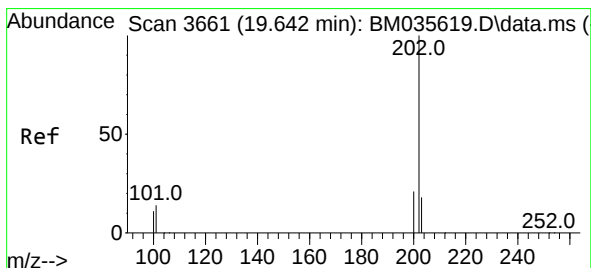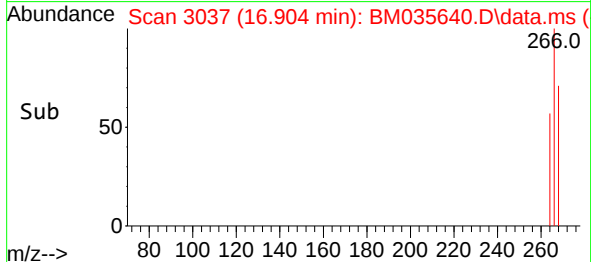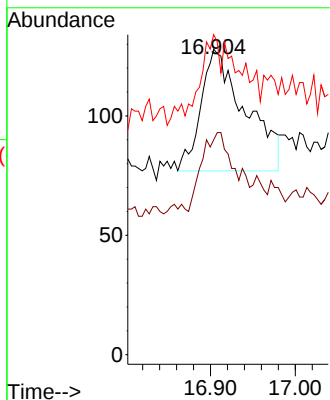

#20
 Pyrene
 Concen: 0.023 ng/ul
 RT: 19.619 min Scan# 3656
 Delta R.T. -0.029 min
 Lab File: BM035640.D
 Acq: 24 Jun 2022 00:43


Tgt Ion:202 Resp: 2916
 Ion Ratio Lower Upper
 202 100
 101 30.3 11.6 17.4#
 100 41.7 9.3 13.9#

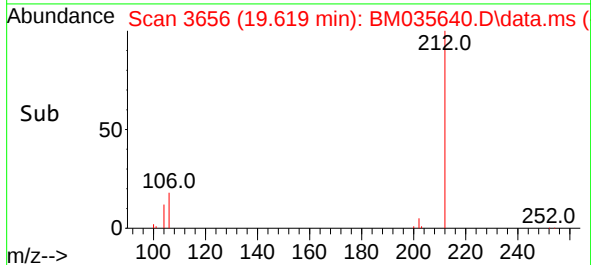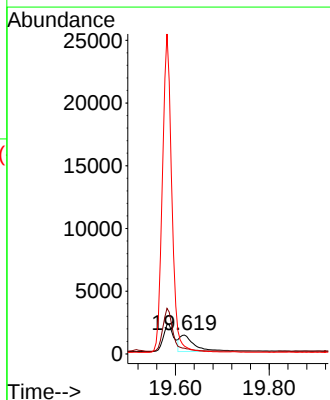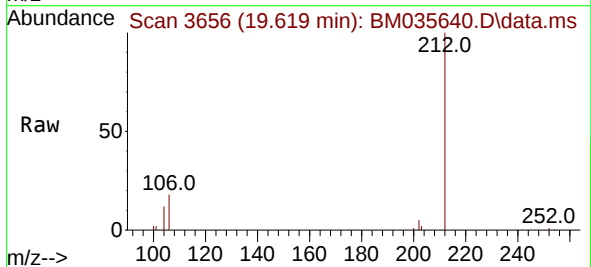

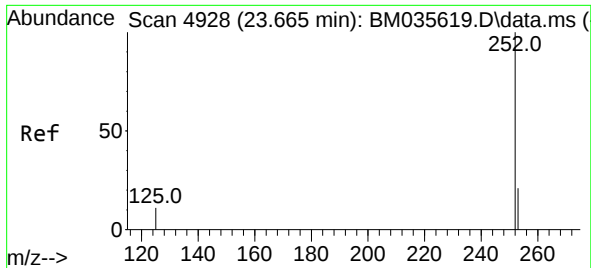

#26
 Benzo(a)pyrene
 Concen: 0.051 ng/ul
 RT: 23.563 min Scan# 41
 Delta R.T. -0.104 min
 Lab File: BM035640.D
 Acq: 24 Jun 2022 00:43

Instrument :
 BNA_M
 ClientSampleId :

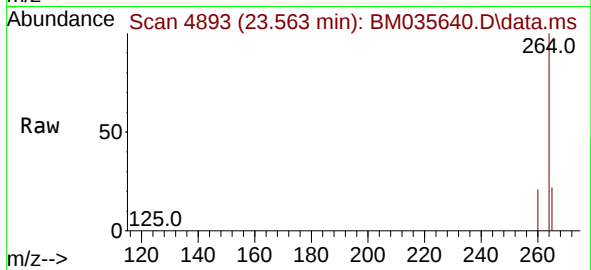

Tgt Ion:252 Resp: 5921
 Ion Ratio Lower Upper
 252 100
 253 61.2 27.8 41.6#
 125 59.2 23.3 34.9#

