

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062322\
 Data File : BM035655.D
 Acq On : 24 Jun 2022 10:21
 Operator : CG/JU
 Sample : PB145605BL
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Jun 25 04:05:25 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM061822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 20 01:56:13 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.820	152	4853	0.400	ng/ul	-0.04
4) Naphthalene-d8	10.604	136	17971	0.400	ng/ul	-0.04
9) Acenaphthene-d10	14.449	164	10838	0.400	ng/ul	#-0.02
13) Phenanthrene-d10	0.000	188	0	0.000	ng/ul	-17.23
17) Chrysene-d12	21.422	240	12867	0.400	ng/ul	0.01
23) Perylene-d12	23.728	264	16349	0.400	ng/ul	#-0.04
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.259	96	33543	4.912	ng/ul	-0.01
6) 2-Methylnaphthalene-d10	12.248	152	7764	0.291	ng/ul	0.00
18) Fluoranthene-d10	19.236	212	15138	0.350	ng/ul	-0.02
Target Compounds						
					Qvalue	
20) Pyrene	19.617	202	2662	0.039	ng/ul#	1
26) Benzo(a)pyrene	23.564	252	3832	0.052	ng/ul#	40


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062322\
Data File : BM035655.D
Acq On : 24 Jun 2022 10:21
Operator : CG/JU
Sample : PB145605BL
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Jun 25 04:05:25 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM061822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 20 01:56:13 2022
Response via : Initial Calibration




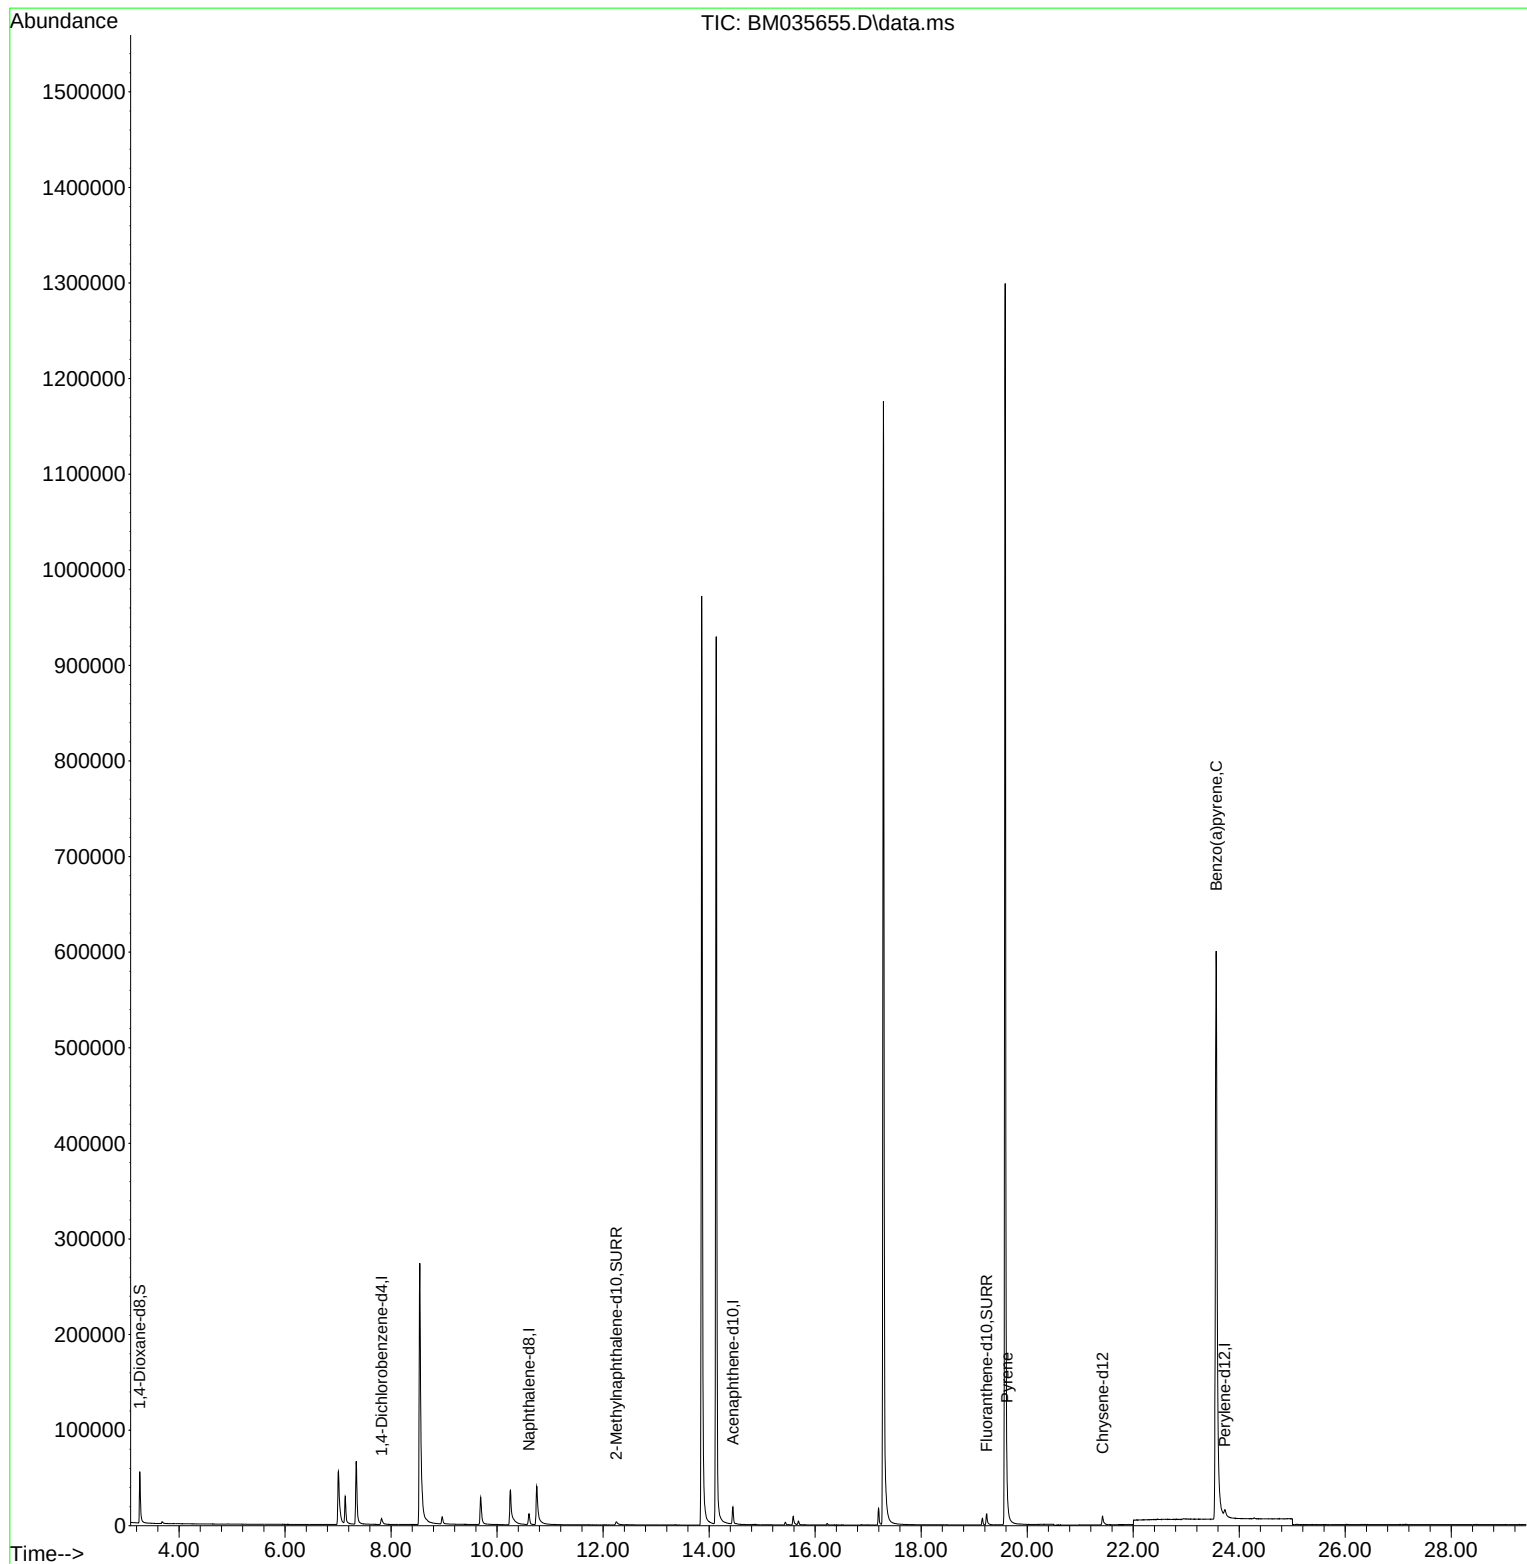


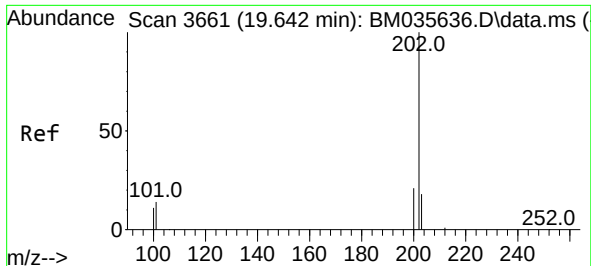

#20
Pyrene
Concen: 0.039 ng/ul
RT: 19.617 min Scan# 30
Delta R.T. -0.031 min
Lab File: BM035655.D
Acq: 24 Jun 2022 10:21

Instrument :
BNA_M
ClientSampleId :

Tgt Ion:202 Resp: 2662
Ion Ratio Lower Upper
202 100
101 32.4 11.6 17.4#
100 100.0 9.3 13.9#

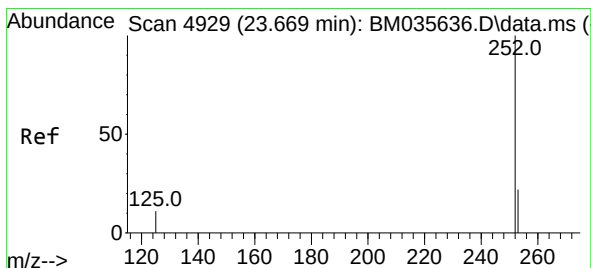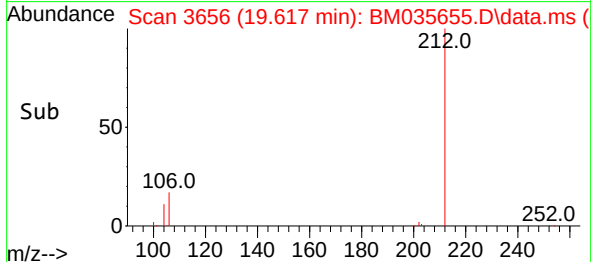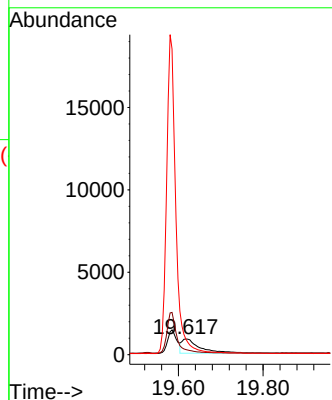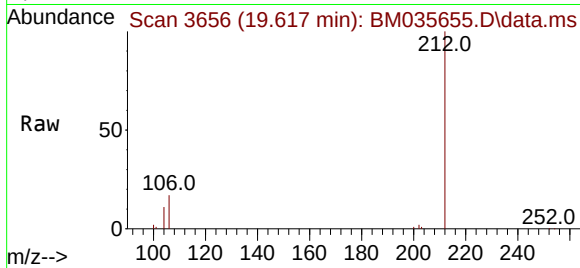

#26
Benzo(a)pyrene
Concen: 0.052 ng/ul
RT: 23.564 min Scan# 4894
Delta R.T. -0.103 min
Lab File: BM035655.D
Acq: 24 Jun 2022 10:21

Tgt Ion:252 Resp: 3832
Ion Ratio Lower Upper
252 100
253 67.0 27.8 41.6#
125 63.9 23.3 34.9#

