

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062322\
 Data File : BM035665.D
 Acq On : 24 Jun 2022 17:20
 Operator : CG/JU
 Sample : PB145602BL
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Jun 25 04:06:04 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM061822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 20 01:56:13 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.825	152	4817	0.400	ng/ul	-0.03
4) Naphthalene-d8	10.605	136	18025	0.400	ng/ul	-0.04
9) Acenaphthene-d10	14.450	164	10907	0.400	ng/ul	#-0.02
13) Phenanthrene-d10	0.000	188	0	0.000	ng/ul	-17.23
17) Chrysene-d12	21.427	240	14738	0.400	ng/ul	0.02
23) Perylene-d12	0.000	264	0	0.000	ng/ul	-23.76
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.260	96	30132	4.446	ng/ul	-0.01
6) 2-Methylnaphthalene-d10	12.261	152	6780	0.253	ng/ul	0.02
18) Fluoranthene-d10	19.238	212	15705	0.317	ng/ul	-0.01
Target Compounds						
20) Pyrene	19.619	202	2542	0.032	ng/ul#	Qvalue 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062322\
Data File : BM035665.D
Acq On : 24 Jun 2022 17:20
Operator : CG/JU
Sample : PB145602BL
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Jun 25 04:06:04 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM061822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 20 01:56:13 2022
Response via : Initial Calibration

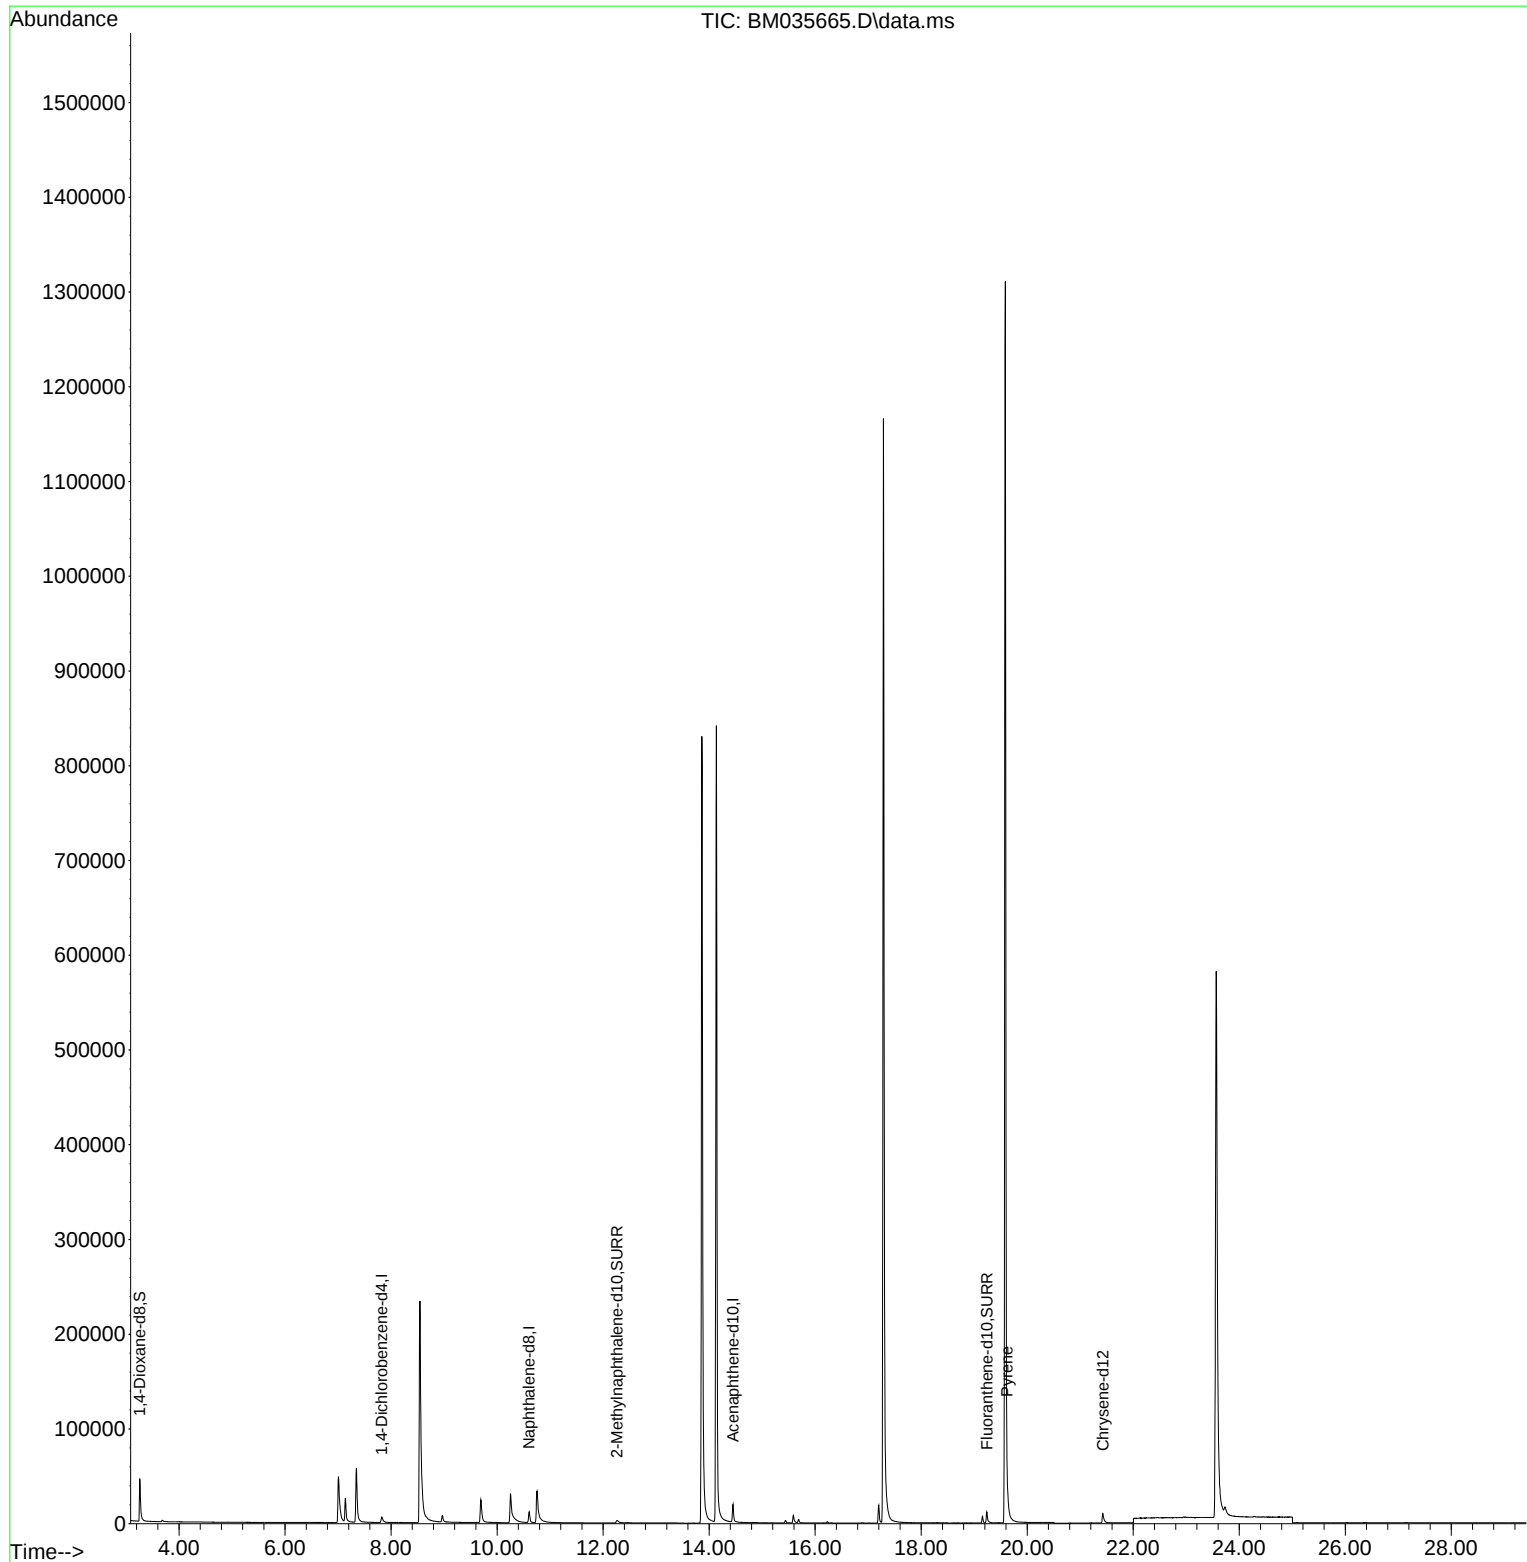

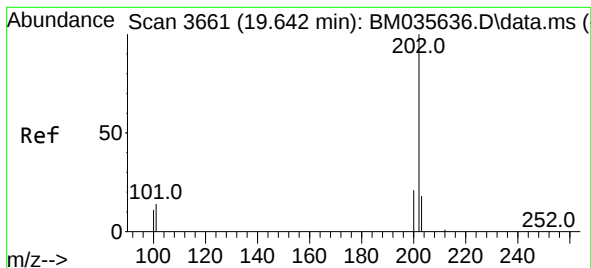

#20

Pyrene

Concen: 0.032 ng/ul

RT: 19.619 min Scan# 30

Delta R.T. -0.029 min


Lab File: BM035665.D

Acq: 24 Jun 2022 17:20

Instrument :

BNA_M

ClientSampleId :

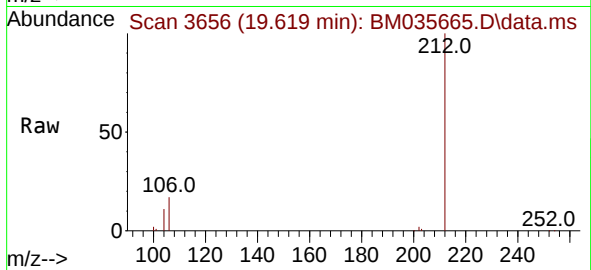

Tgt Ion:202 Resp: 2542

Ion Ratio Lower Upper

202 100

101 33.8 11.6 17.4#

100 109.5 9.3 13.9#

