

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062322\
 Data File : BM035666.D
 Acq On : 24 Jun 2022 17:57
 Operator : CG/JU
 Sample : PB145603BL
 Misc :
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Jun 25 04:06:08 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM061822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 20 01:56:13 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.829	152	4035	0.400	ng/ul	-0.03
4) Naphthalene-d8	10.605	136	15175	0.400	ng/ul	-0.04
9) Acenaphthene-d10	14.450	164	9144	0.400	ng/ul	#-0.02
13) Phenanthrene-d10	0.000	188	0	0.000	ng/ul	-17.23
17) Chrysene-d12	21.430	240	10746	0.400	ng/ul	0.02
23) Perylene-d12	0.000	264	0	0.000	ng/ul	-23.76
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.264	96	31252	5.505	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.261	152	6916	0.307	ng/ul	0.02
18) Fluoranthene-d10	19.238	212	14044	0.389	ng/ul	-0.01
Target Compounds						
20) Pyrene	19.619	202	2531	0.044	ng/ul#	Qvalue 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062322\
Data File : BM035666.D
Acq On : 24 Jun 2022 17:57
Operator : CG/JU
Sample : PB145603BL
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :


Quant Time: Jun 25 04:06:08 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM061822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 20 01:56:13 2022
Response via : Initial Calibration

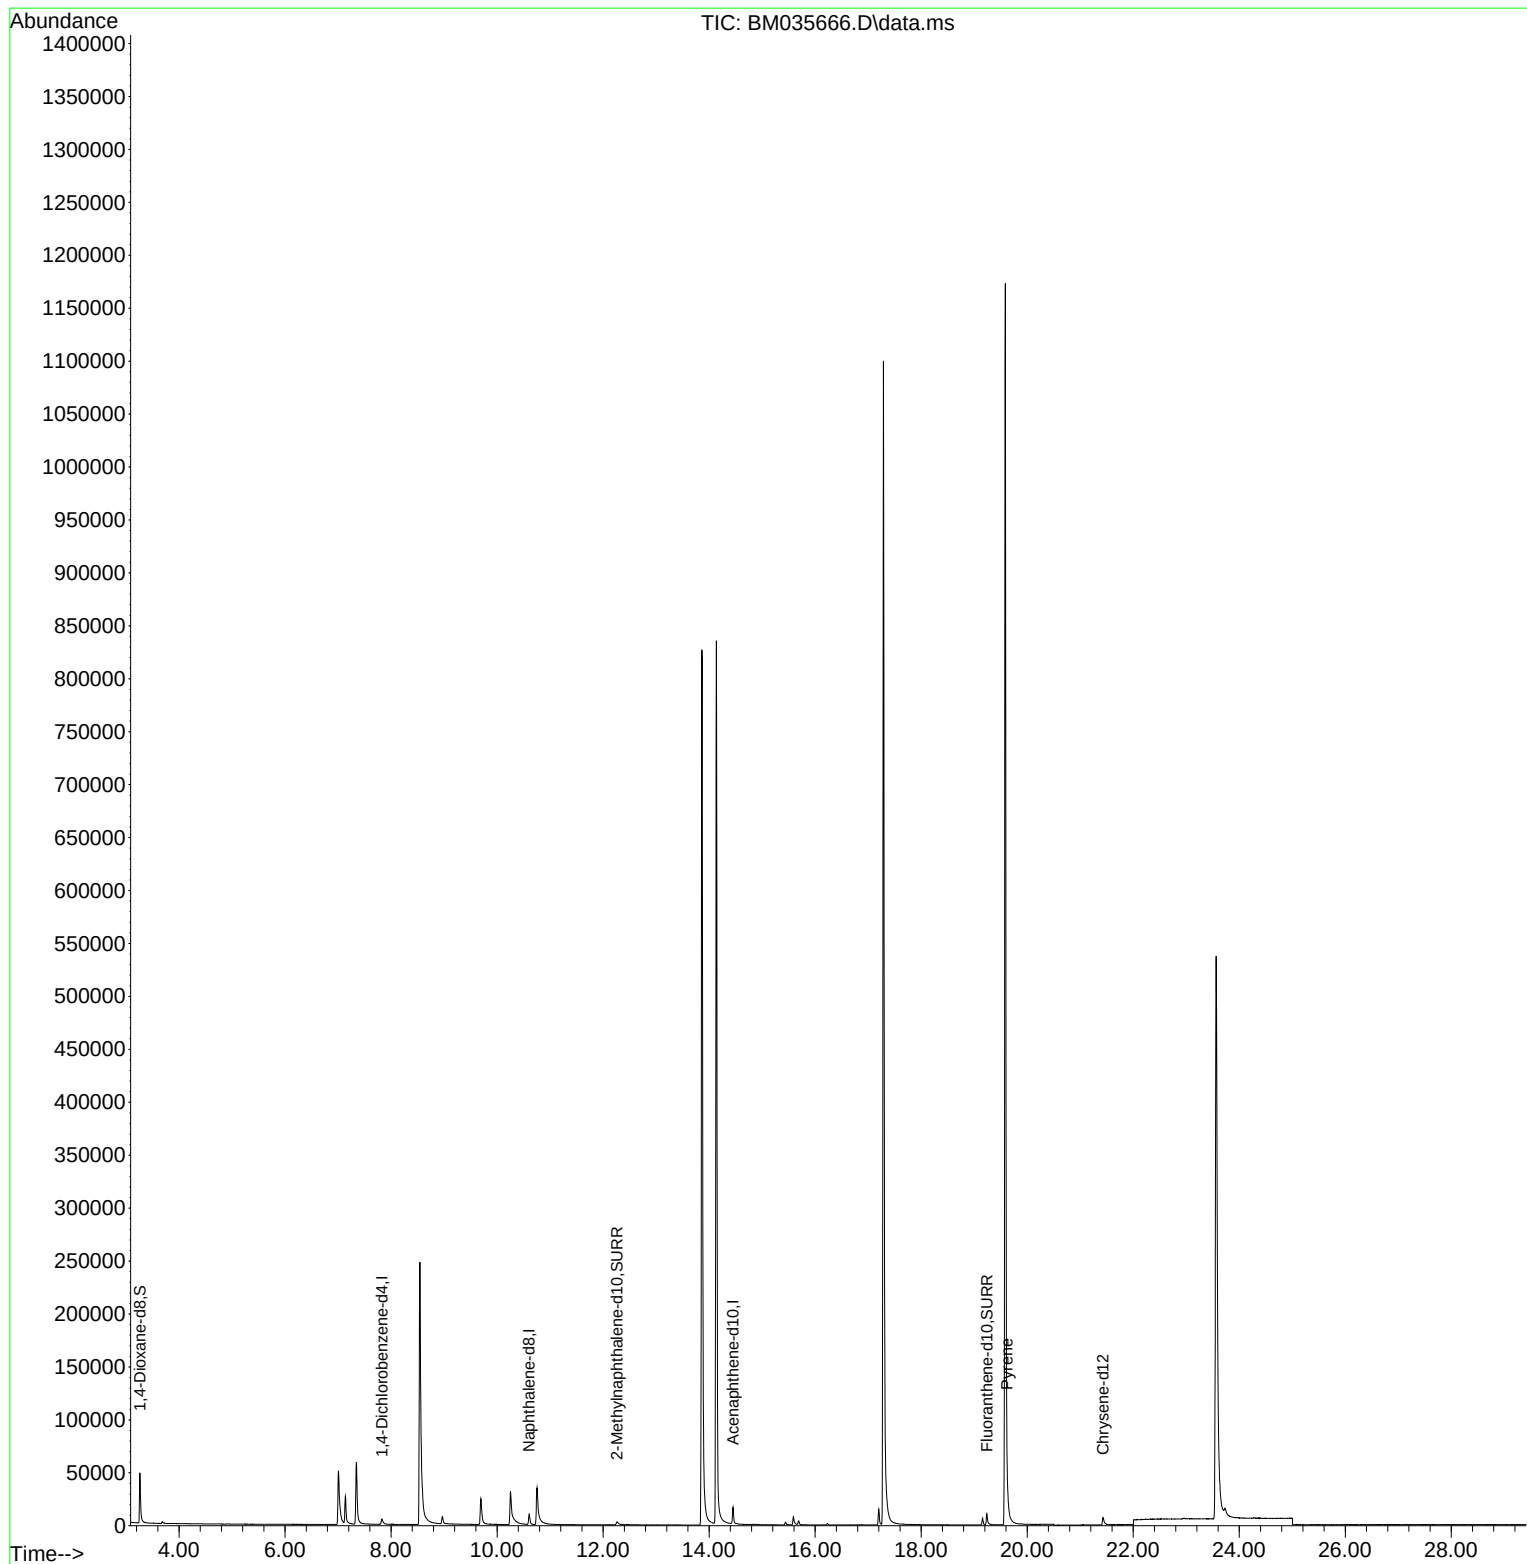

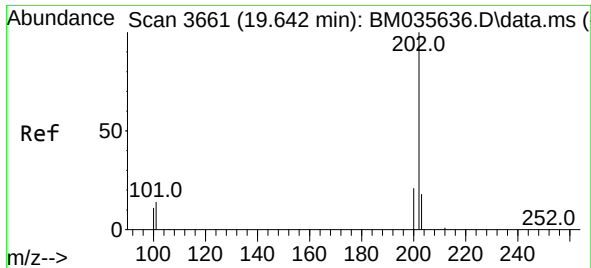

#20
 Pyrene
 Concen: 0.044 ng/ul
 RT: 19.619 min Scan# 30
 Delta R.T. -0.029 min
 Lab File: BM035666.D
 Acq: 24 Jun 2022 17:57

Instrument :
 BNA_M
 ClientSampleId :

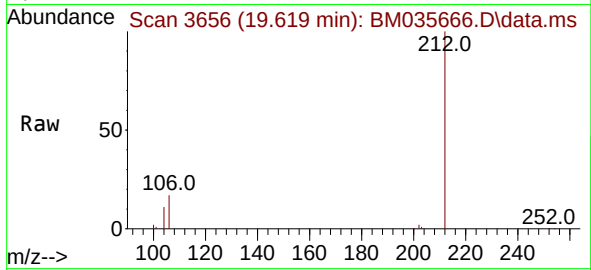

Tgt Ion:202 Resp: 2531
 Ion Ratio Lower Upper
 202 100
 101 36.2 11.6 17.4#
 100 117.8 9.3 13.9#

