

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062322\
 Data File : BM035667.D
 Acq On : 24 Jun 2022 18:34
 Operator : CG/JU
 Sample : N3285-19RE
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Jun 25 04:06:11 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM061822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 20 01:56:13 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.829	152	4446	0.400	ng/ul	-0.03
4) Naphthalene-d8	10.611	136	16760	0.400	ng/ul	-0.03
9) Acenaphthene-d10	14.450	164	10274	0.400	ng/ul	#-0.02
13) Phenanthrene-d10	0.000	188	0	0.000	ng/ul	-17.23
17) Chrysene-d12	21.415	240	12222	0.400	ng/ul	0.00
23) Perylene-d12	23.730	264	14769	0.400	ng/ul	#-0.03
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.264	96	25451	4.068	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.250	152	7113	0.286	ng/ul	0.00
18) Fluoranthene-d10	19.233	212	17593	0.429	ng/ul	-0.02
Target Compounds						
					Qvalue	
20) Pyrene	19.619	202	2302	0.035	ng/ul#	5
26) Benzo(a)pyrene	23.563	252	3584	0.053	ng/ul#	39


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062322\
Data File : BM035667.D
Acq On : 24 Jun 2022 18:34
Operator : CG/JU
Sample : N3285-19RE
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Jun 25 04:06:11 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM061822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 20 01:56:13 2022
Response via : Initial Calibration




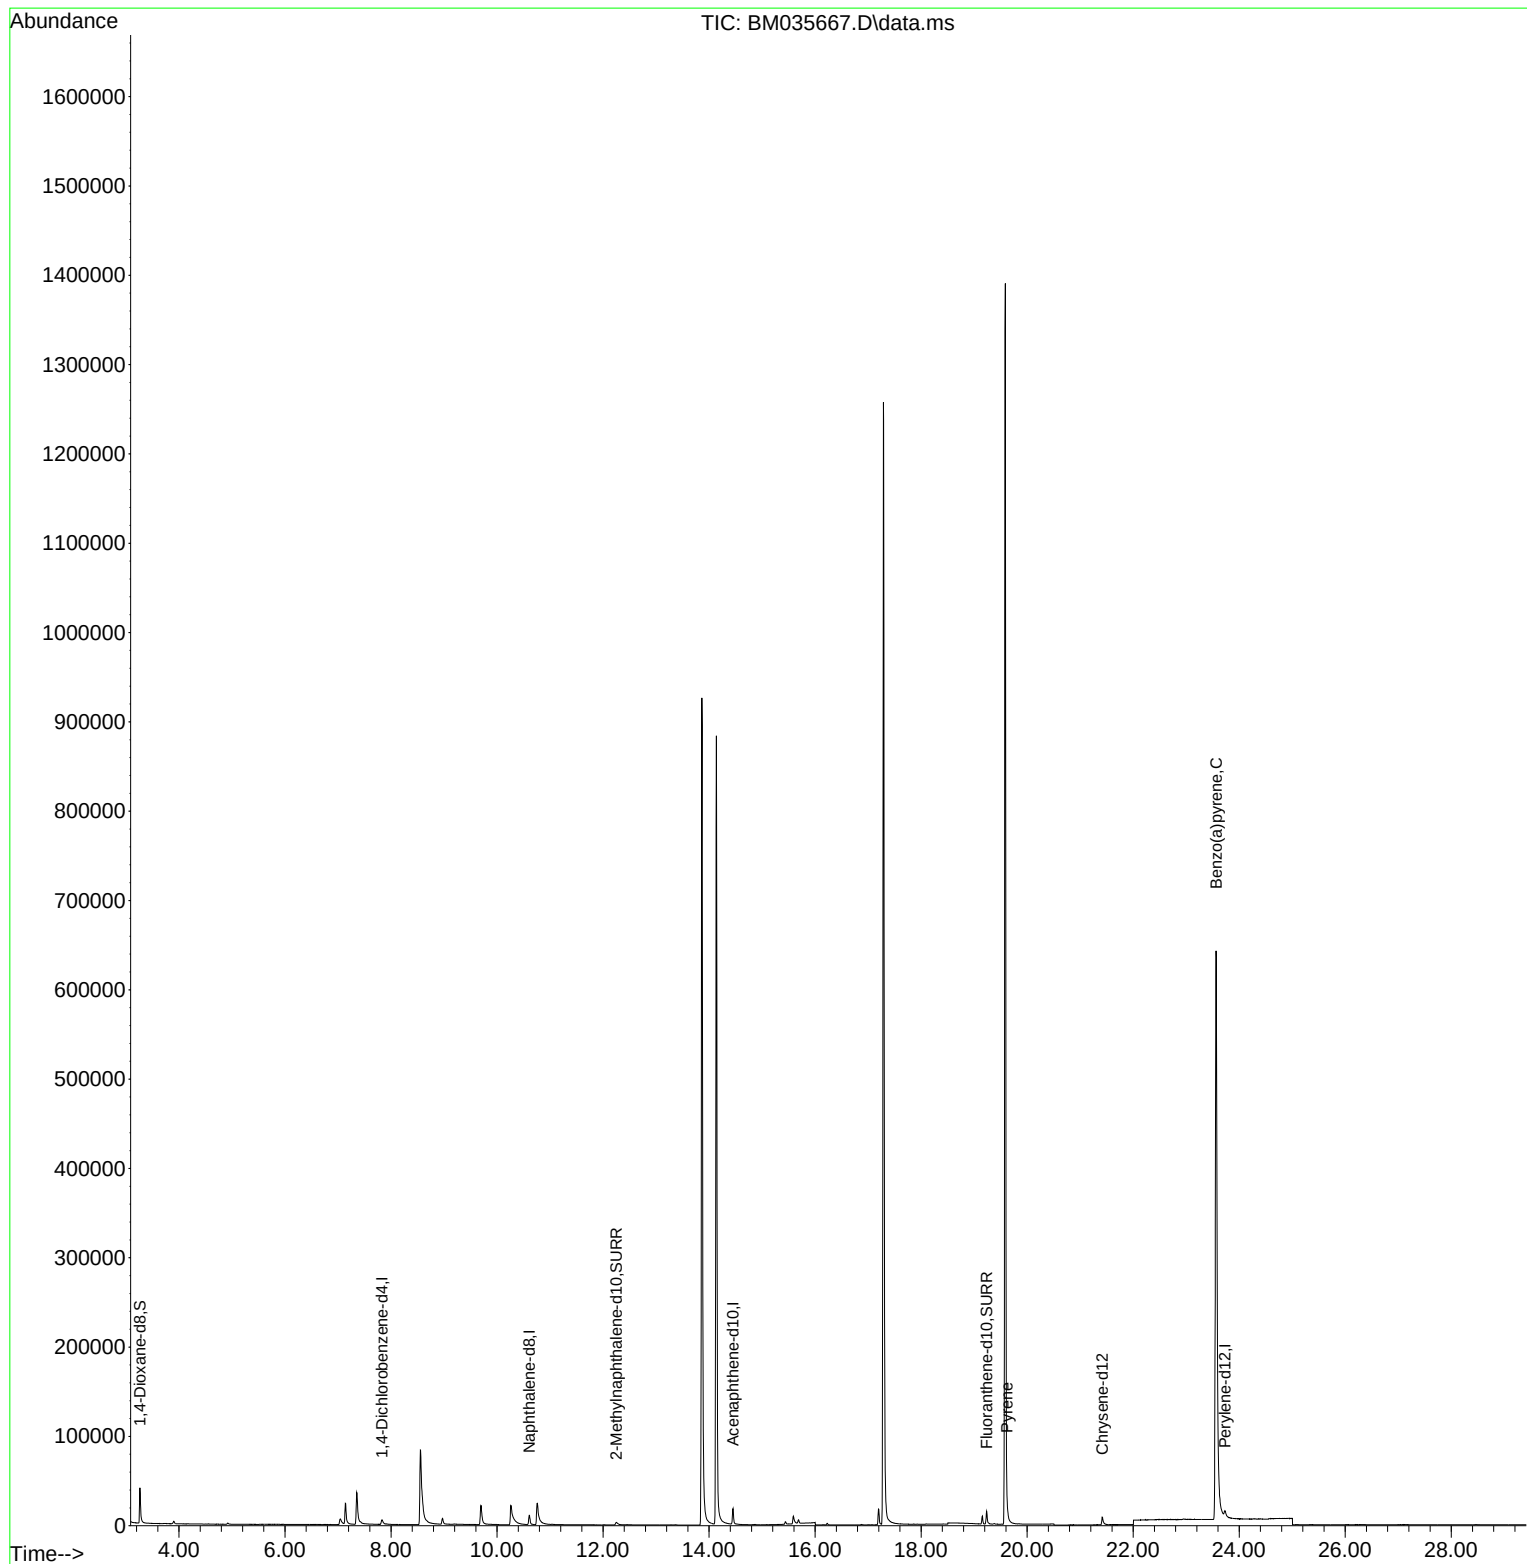


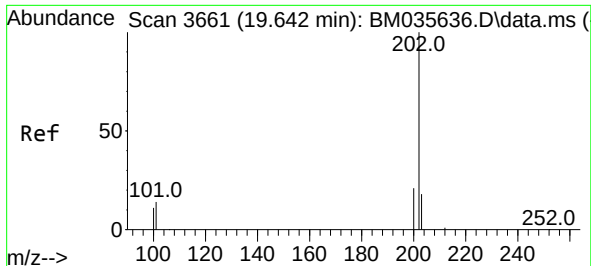

#20
Pyrene
Concen: 0.035 ng/ul
RT: 19.619 min Scan# 30
Delta R.T. -0.029 min
Lab File: BM035667.D
Acq: 24 Jun 2022 18:34

Instrument :
BNA_M
ClientSampleId :

Tgt Ion:202 Resp: 2302
Ion Ratio Lower Upper
202 100
101 36.0 11.6 17.4#
100 68.4 9.3 13.9#

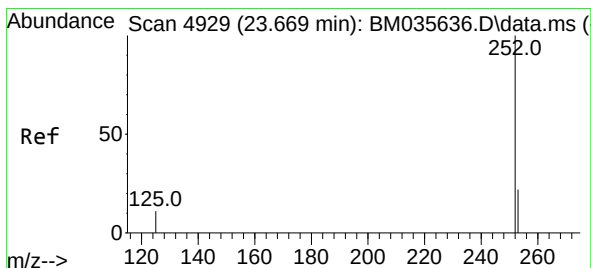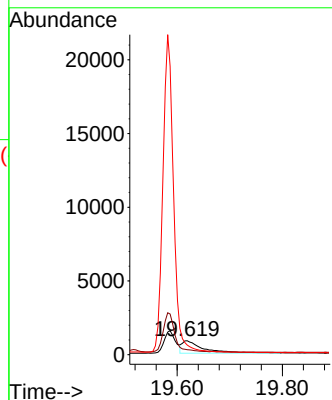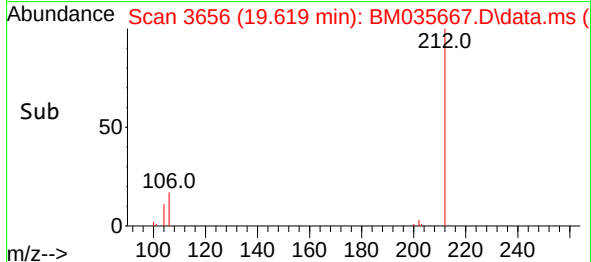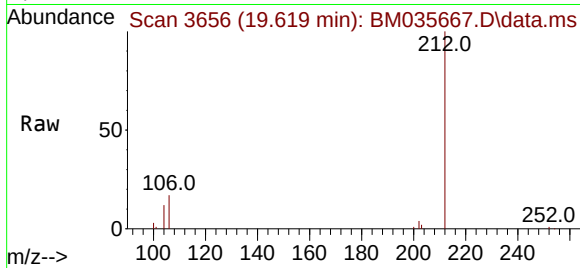

#26
Benzo(a)pyrene
Concen: 0.053 ng/ul
RT: 23.563 min Scan# 4893
Delta R.T. -0.104 min
Lab File: BM035667.D
Acq: 24 Jun 2022 18:34

Tgt Ion:252 Resp: 3584
Ion Ratio Lower Upper
252 100
253 70.2 27.8 41.6#
125 62.0 23.3 34.9#

