

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062322\
 Data File : BM035673.D
 Acq On : 24 Jun 2022 22:16
 Operator : CG/JU
 Sample : N3358-01
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Jun 25 04:06:31 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM061822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 20 01:56:13 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.825	152	6171	0.400	ng/ul	-0.03
4) Naphthalene-d8	10.606	136	22243	0.400	ng/ul	-0.04
9) Acenaphthene-d10	14.450	164	11478	0.400	ng/ul	#-0.02
13) Phenanthrene-d10	0.000	188	0	0.000	ng/ul	-17.23
17) Chrysene-d12	21.409	240	13970	0.400	ng/ul	0.00
23) Perylene-d12	23.724	264	17265	0.400	ng/ul	#-0.04
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.264	96	32458	3.738	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.233	152	9475	0.287	ng/ul	-0.01
18) Fluoranthene-d10	19.233	212	18705	0.399	ng/ul	-0.02
Target Compounds						
					Qvalue	
20) Pyrene	19.615	202	2138	0.029	ng/ul#	1
26) Benzo(a)pyrene	23.552	252	4649	0.059	ng/ul#	46


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062322\
Data File : BM035673.D
Acq On : 24 Jun 2022 22:16
Operator : CG/JU
Sample : N3358-01
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :


Quant Time: Jun 25 04:06:31 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM061822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 20 01:56:13 2022
Response via : Initial Calibration

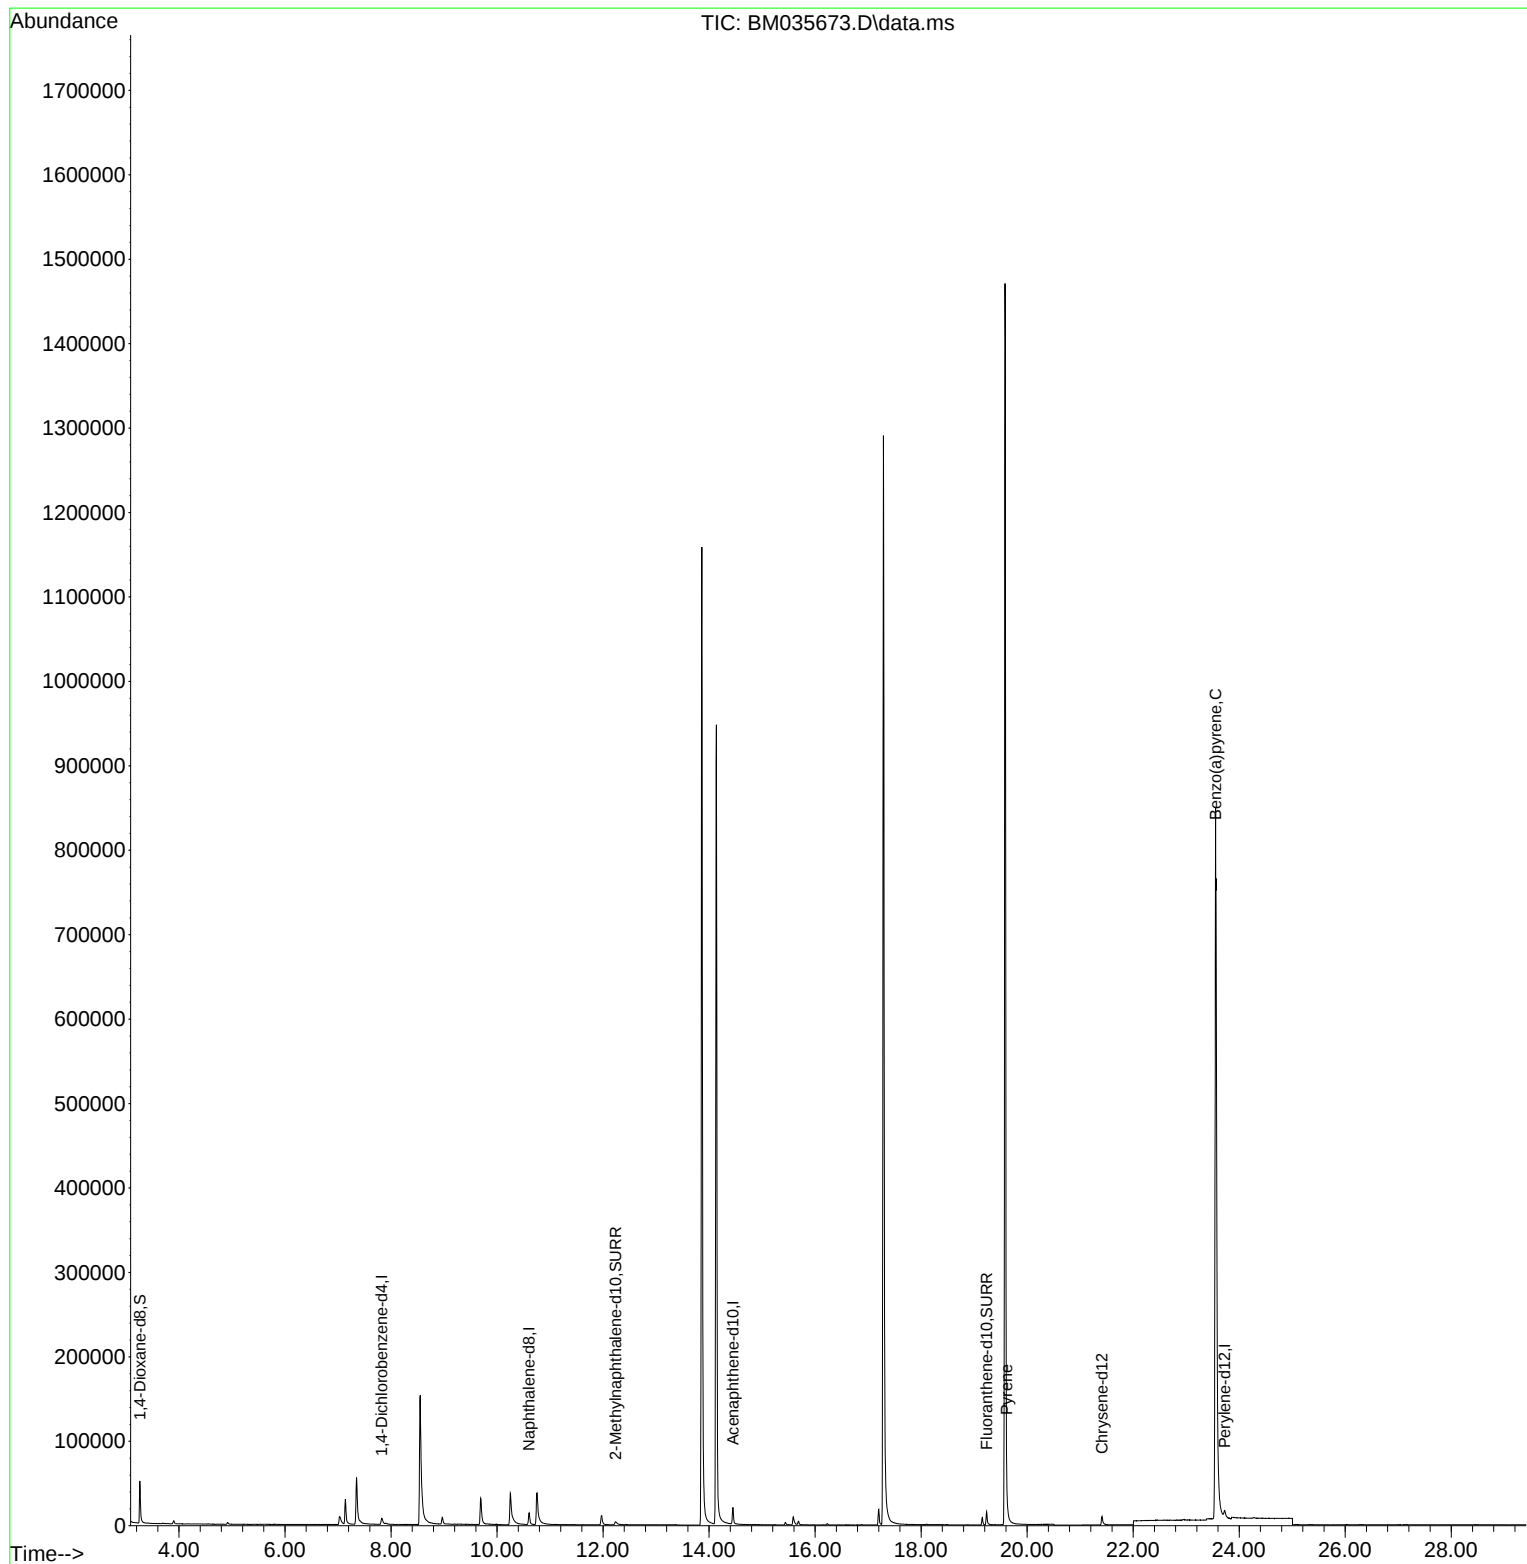



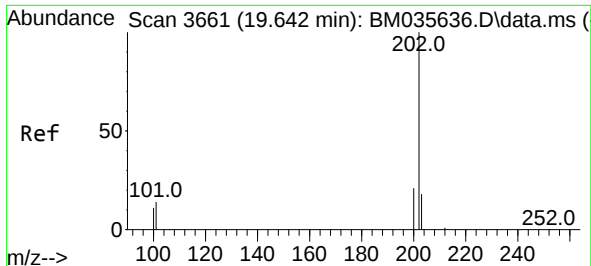


#20
Pyrene
Concen: 0.029 ng/ul
RT: 19.615 min Scan# 3
Delta R.T. -0.033 min
Lab File: BM035673.D
Acq: 24 Jun 2022 22:16

Instrument :
BNA_M
ClientSampleId :

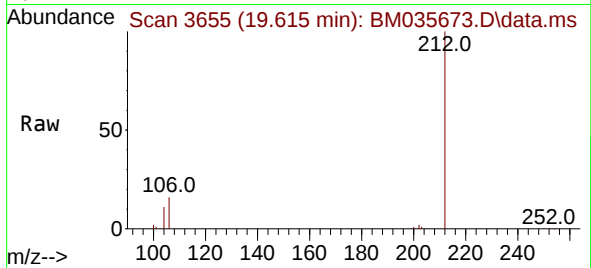

Tgt Ion:202 Resp: 2138
Ion Ratio Lower Upper
202 100
101 34.4 11.6 17.4#
100 93.9 9.3 13.9#

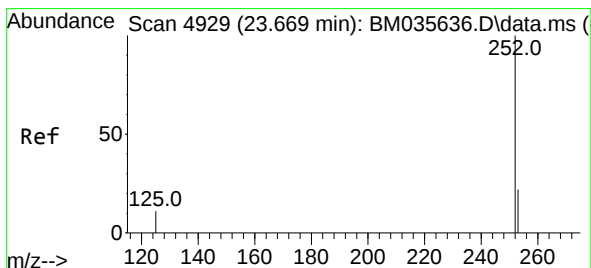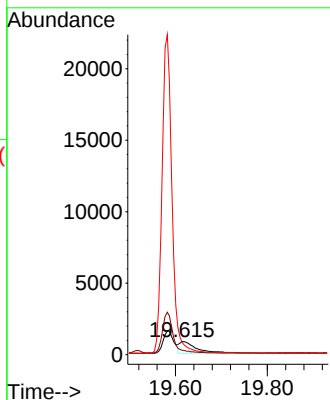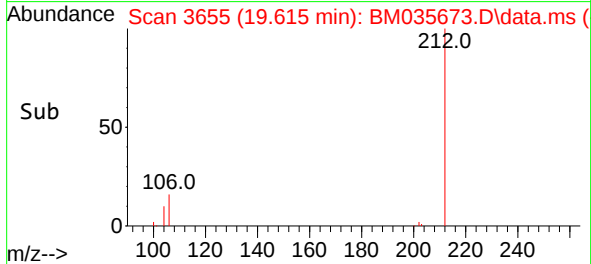

#26
Benzo(a)pyrene
Concen: 0.059 ng/ul
RT: 23.552 min Scan# 4889
Delta R.T. -0.116 min
Lab File: BM035673.D
Acq: 24 Jun 2022 22:16

Tgt Ion:252 Resp: 4649
Ion Ratio Lower Upper
252 100
253 62.9 27.8 41.6#
125 61.3 23.3 34.9#

