

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062322\
 Data File : BM035676.D
 Acq On : 25 Jun 2022 00:06
 Operator : CG/JU
 Sample : N3358-17
 Misc :
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Jun 25 04:06:41 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM061822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 20 01:56:13 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.829	152	4837	0.400	ng/ul	-0.03
4) Naphthalene-d8	10.605	136	17765	0.400	ng/ul	-0.04
9) Acenaphthene-d10	14.450	164	11087	0.400	ng/ul	#-0.02
13) Phenanthrene-d10	0.000	188	0	0.000	ng/ul	-17.23
17) Chrysene-d12	21.406	240	21882	0.400	ng/ul	0.00
23) Perylene-d12	23.724	264	26458	0.400	ng/ul	#-0.04
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.259	96	24667	3.624	ng/ul	-0.01
6) 2-Methylnaphthalene-d10	12.222	152	10832	0.410	ng/ul	-0.02
18) Fluoranthene-d10	19.233	212	30726	0.418	ng/ul	-0.02
Target Compounds						
					Qvalue	
20) Pyrene	19.614	202	2798	0.024	ng/ul#	6
26) Benzo(a)pyrene	23.557	252	7762	0.065	ng/ul#	66


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062322\
Data File : BM035676.D
Acq On : 25 Jun 2022 00:06
Operator : CG/JU
Sample : N3358-17
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :


Quant Time: Jun 25 04:06:41 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM061822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 20 01:56:13 2022
Response via : Initial Calibration

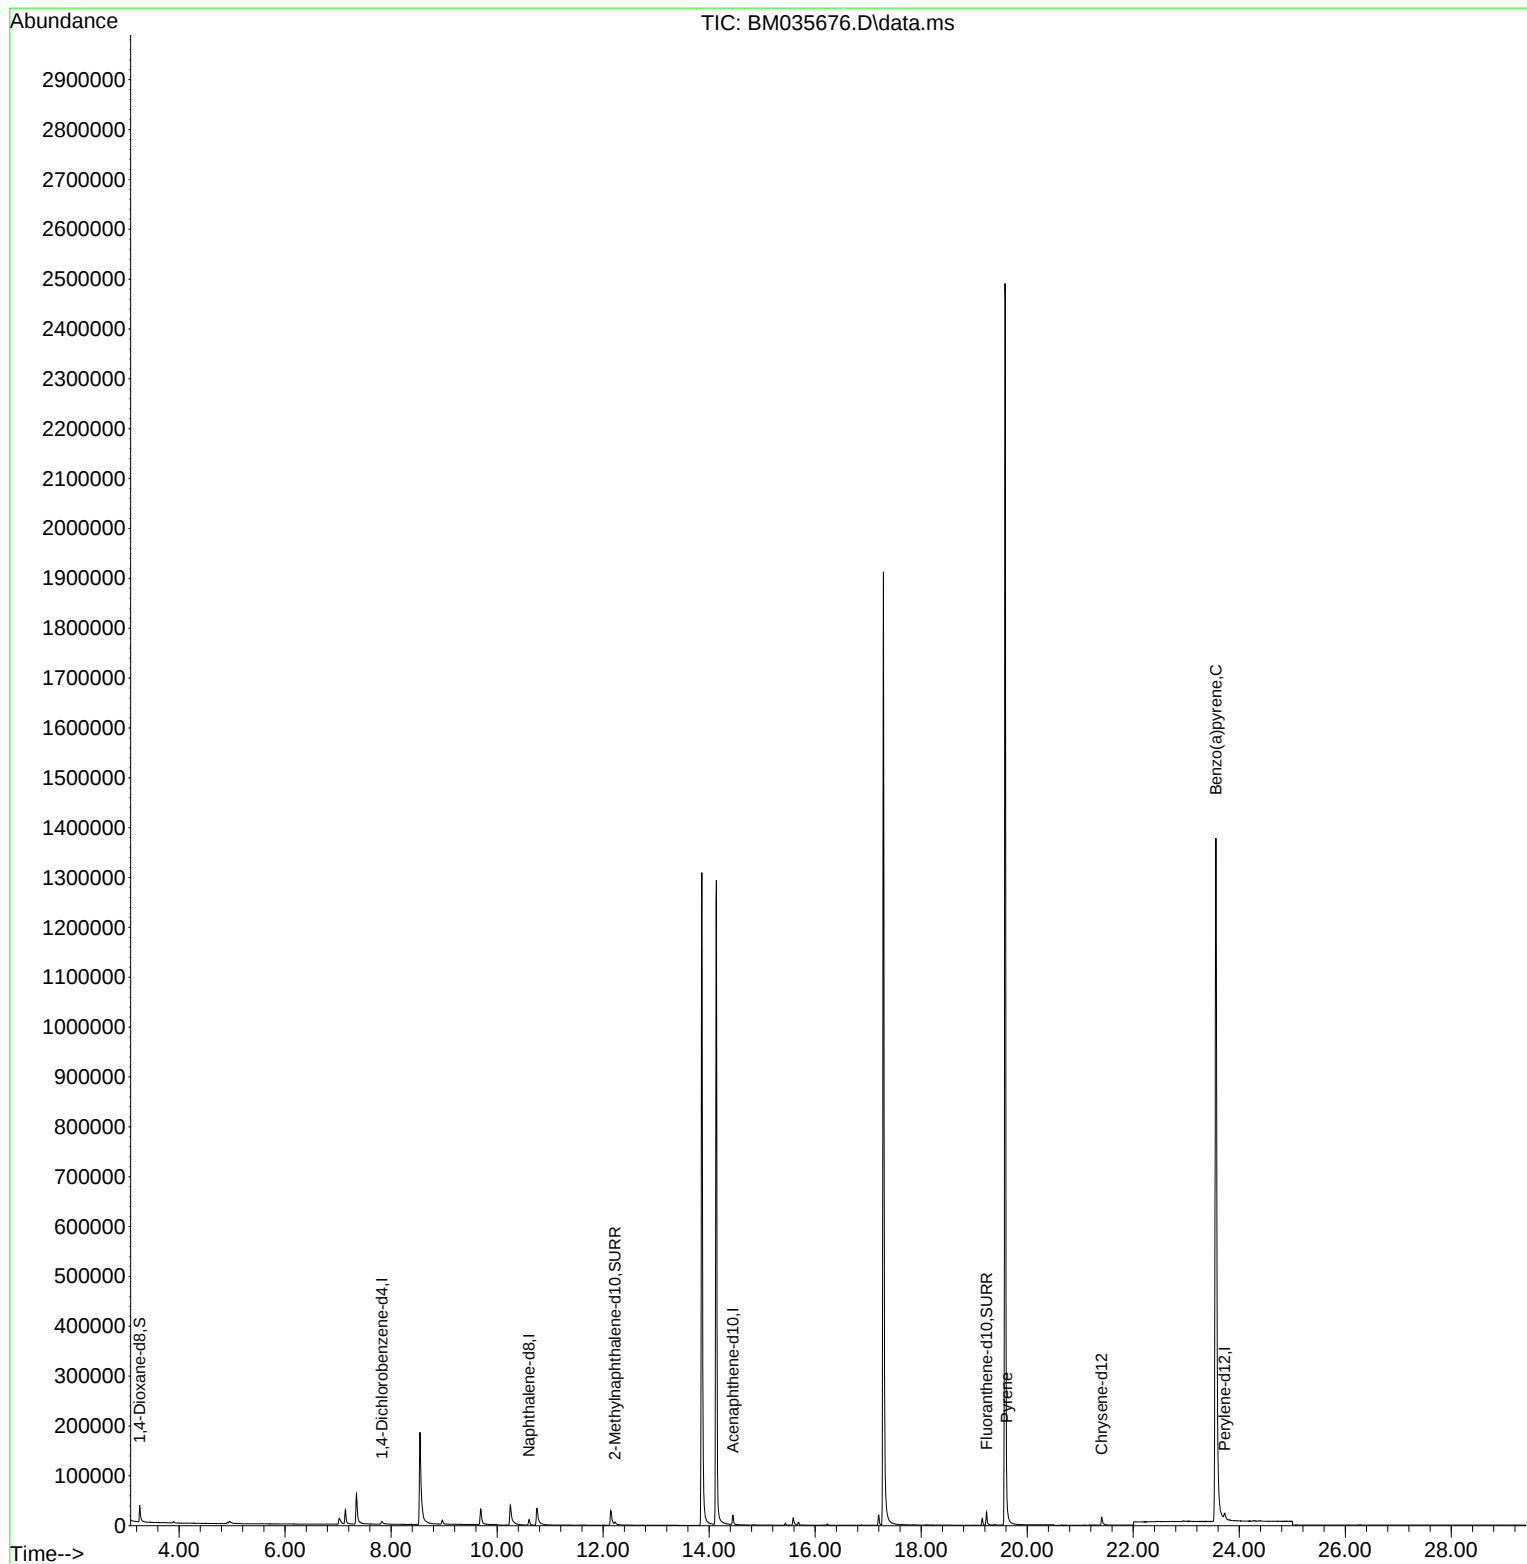



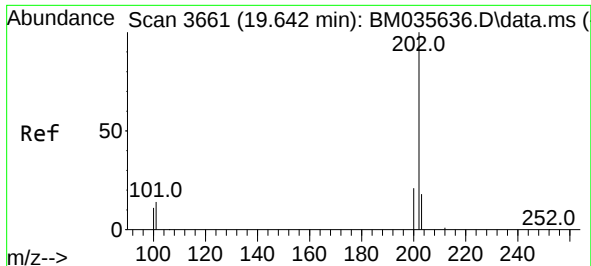


#20
Pyrene
Concen: 0.024 ng/ul
RT: 19.614 min Scan# 30
Delta R.T. -0.034 min
Lab File: BM035676.D
Acq: 25 Jun 2022 00:06

Instrument :
BNA_M
ClientSampleId :

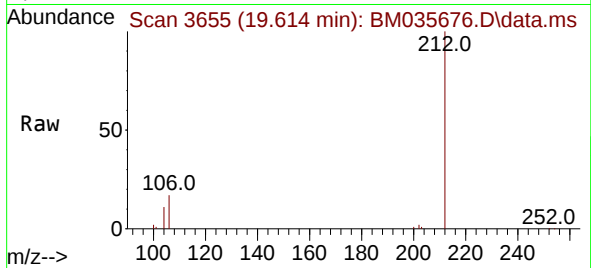

Tgt Ion:202 Resp: 2798
Ion Ratio Lower Upper
202 100
101 30.3 11.6 17.4#
100 74.4 9.3 13.9#

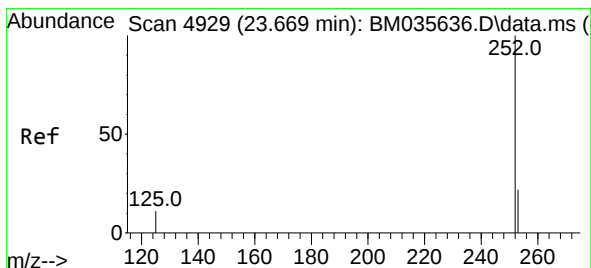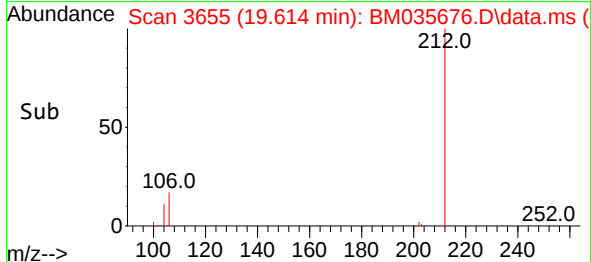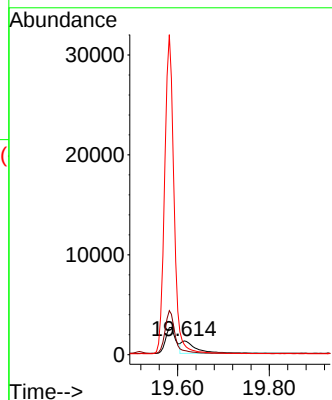

#26
Benzo(a)pyrene
Concen: 0.065 ng/ul
RT: 23.557 min Scan# 4891
Delta R.T. -0.110 min
Lab File: BM035676.D
Acq: 25 Jun 2022 00:06

Tgt Ion:252 Resp: 7762
Ion Ratio Lower Upper
252 100
253 52.4 27.8 41.6#
125 49.4 23.3 34.9#

