




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062322\
 Data File : BM035626.D
 Acq On : 23 Jun 2022 15:27
 Operator : CG/JU
 Sample : N3358-07
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4R7

Manual IntegrationsAPPROVED

Quant Time: Jun 24 01:35:41 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM061822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 20 01:56:13 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/24/2022
 Supervised By :Yogesh Patel 06/28/2022

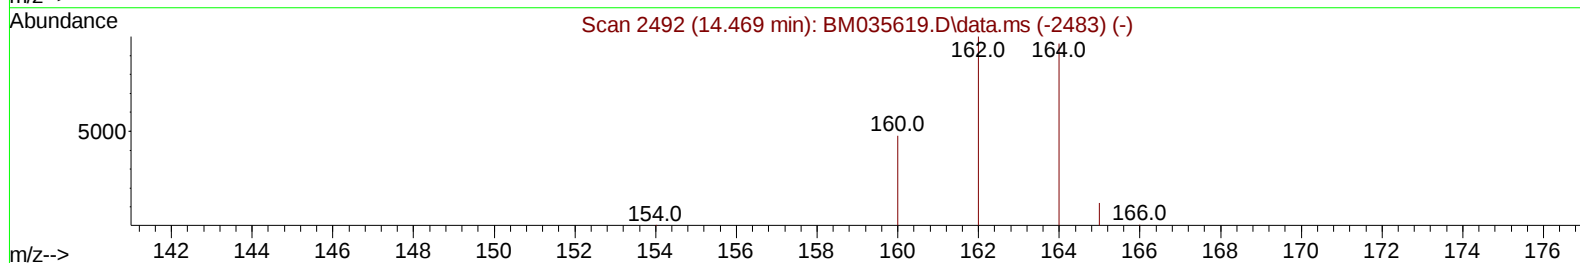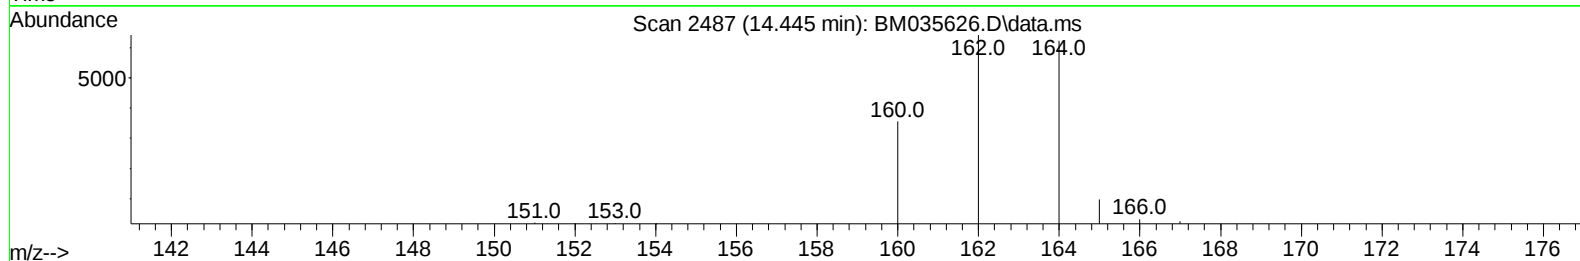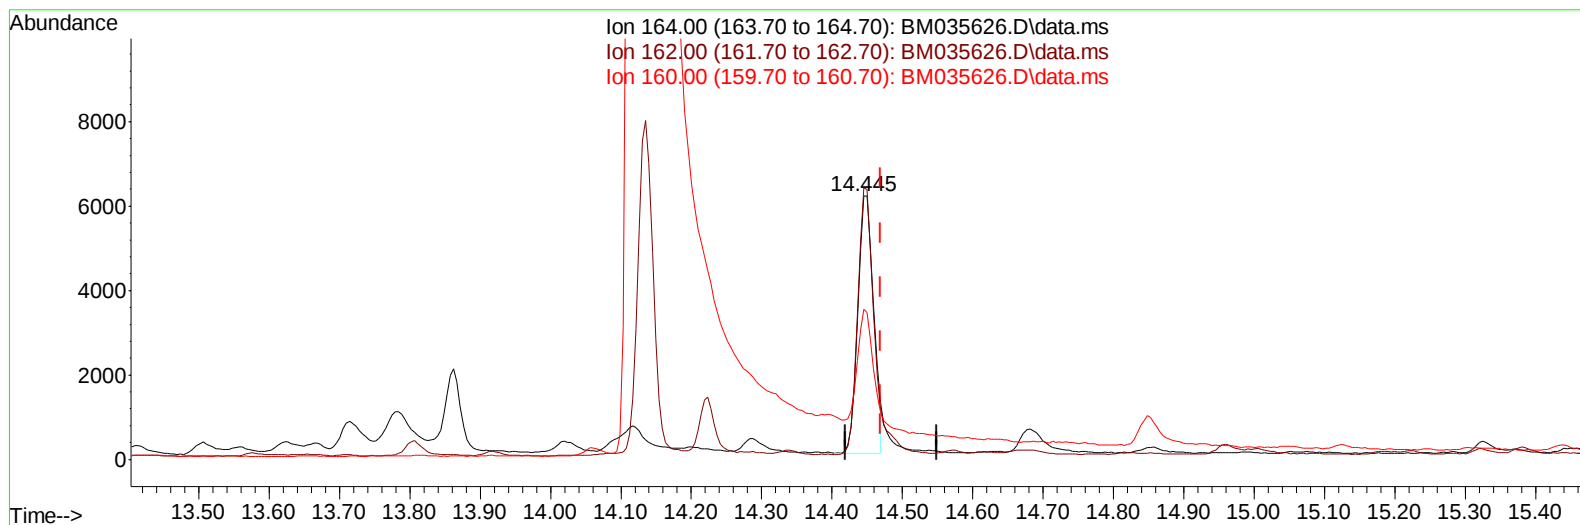

TIC: BM035626.D\data.ms

(9) Acenaphthene-d10 (I)

14.445min (-0.024) 0.40 ng/u1

response 9515

Ion	Exp%	Act%
164.00	100.00	100.00
162.00	106.40	103.06
160.00	49.90	56.99
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062322\
Data File : BM035626.D
Acq On : 23 Jun 2022 15:27
Operator : CG/JU
Sample : N3358-07
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4R7

Manual IntegrationsAPPROVED

Quant Time: Jun 24 01:35:41 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM061822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 20 01:56:13 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/24/2022
Supervised By :Yogesh Patel 06/28/2022

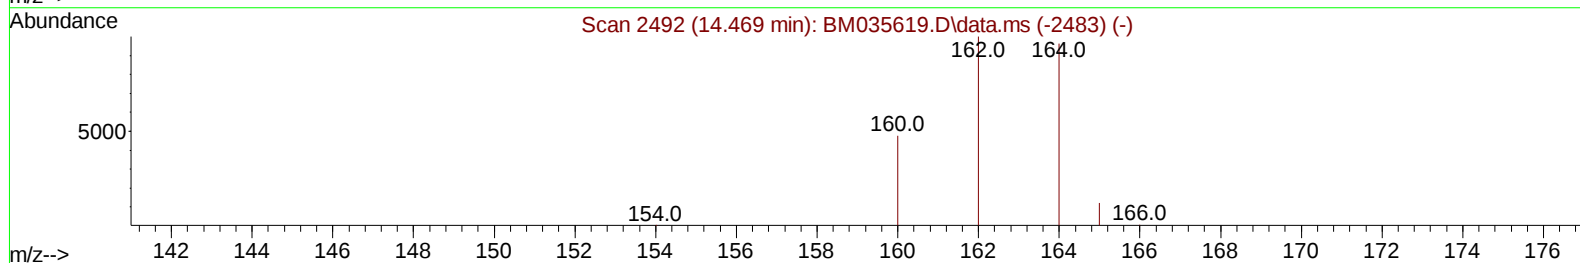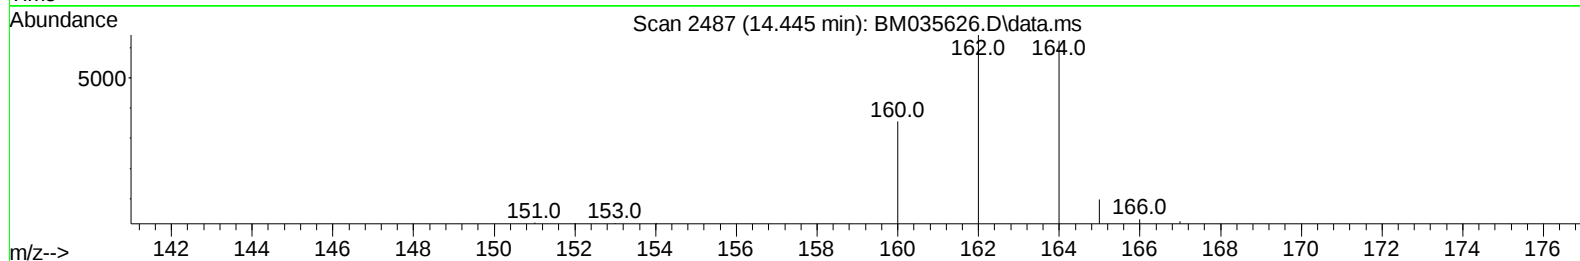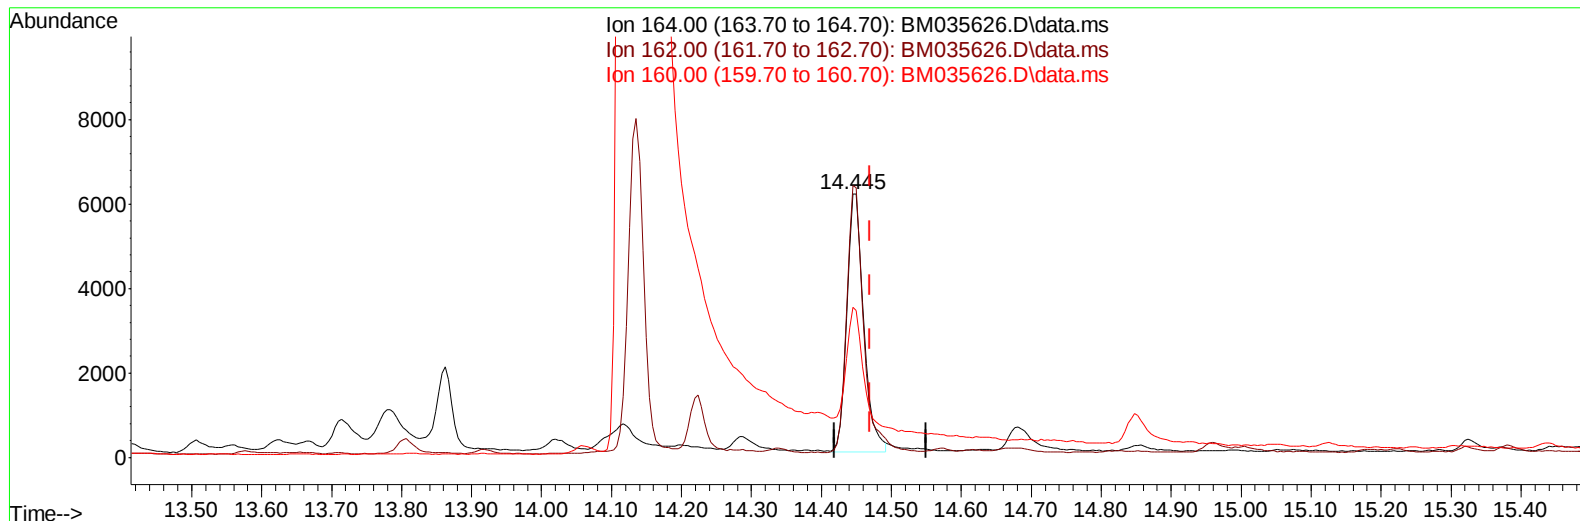

TIC: BM035626.D\data.ms

(9) Acenaphthene-d10 (I)

14.445min (-0.024) 0.40 ng/u1 m

response 10106

Ion	Exp%	Act%
164.00	100.00	100.00
162.00	106.40	103.06
160.00	49.90	56.99
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062322\
 Data File : BM035626.D
 Acq On : 23 Jun 2022 15:27
 Operator : CG/JU
 Sample : N3358-07
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4R7

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 06/24/2022
 Supervised By :Yogesh Patel 06/28/2022

Quant Time: Jun 24 01:35:41 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM061822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 20 01:56:13 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.820	152		4882	0.400	ng/ul	-0.04
4) Naphthalene-d8	10.600	136		20889	0.400	ng/ul	-0.04
9) Acenaphthene-d10	14.445	164		10106m	0.400	ng/ul	-0.02
13) Phenanthrene-d10	17.195	188		17076	0.400	ng/ul	#-0.03
17) Chrysene-d12	21.395	240		14165	0.400	ng/ul	-0.02
23) Perylene-d12	23.724	264		17157	0.400	ng/ul	#-0.04
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.264	96		31310	4.558	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.206	152		9987	0.322	ng/ul	-0.04
18) Fluoranthene-d10	19.229	212		17476	0.367	ng/ul	-0.02
Target Compounds							Qvalue
11) Acenaphthene	14.510	153		1214	0.029	ng/ul	90

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062322\
Data File : BM035626.D
Acq On : 23 Jun 2022 15:27
Operator : CG/JU
Sample : N3358-07
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4R7

Manual IntegrationsAPPROVED

Quant Time: Jun 24 01:35:41 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM061822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 20 01:56:13 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/24/2022
Supervised By :Yogesh Patel 06/28/2022

