




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062322\
Data File : BM035633.D
Acq On : 23 Jun 2022 19:53
Operator : CG/JU
Sample : N3358-03
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4R9

Manual IntegrationsAPPROVED

Quant Time: Jun 24 01:36:10 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM061822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 20 01:56:13 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/27/2022
Supervised By :Yogesh Patel 06/28/2022

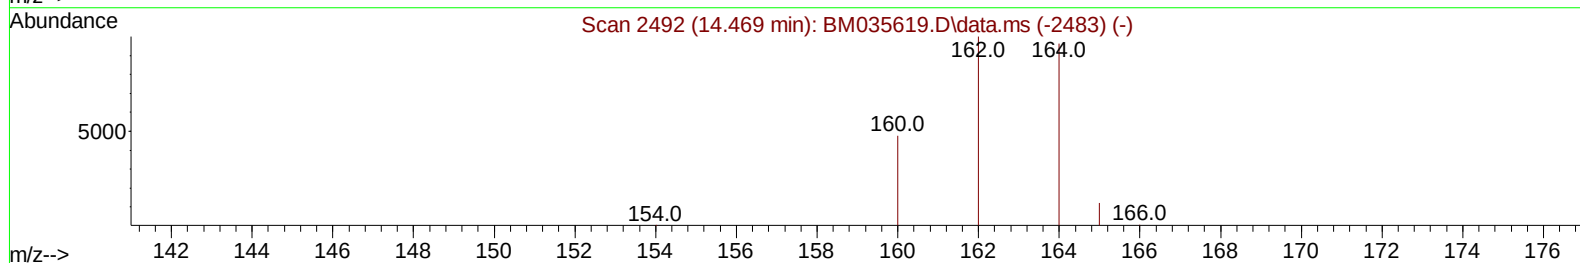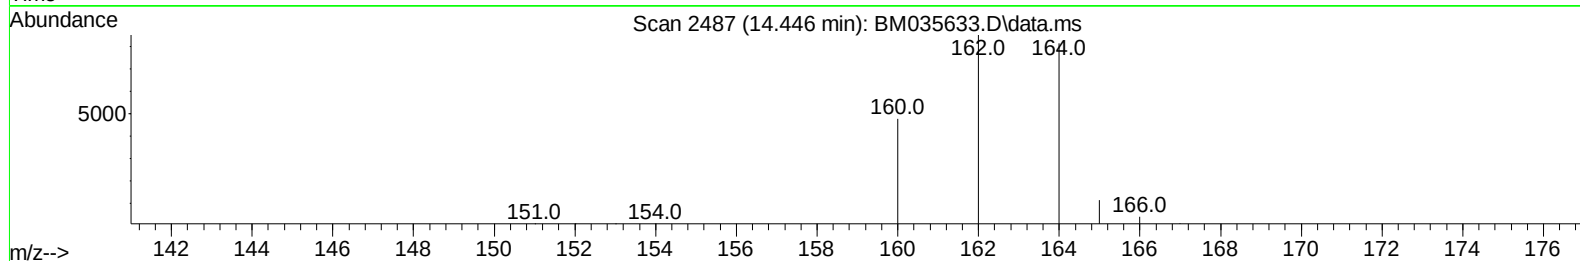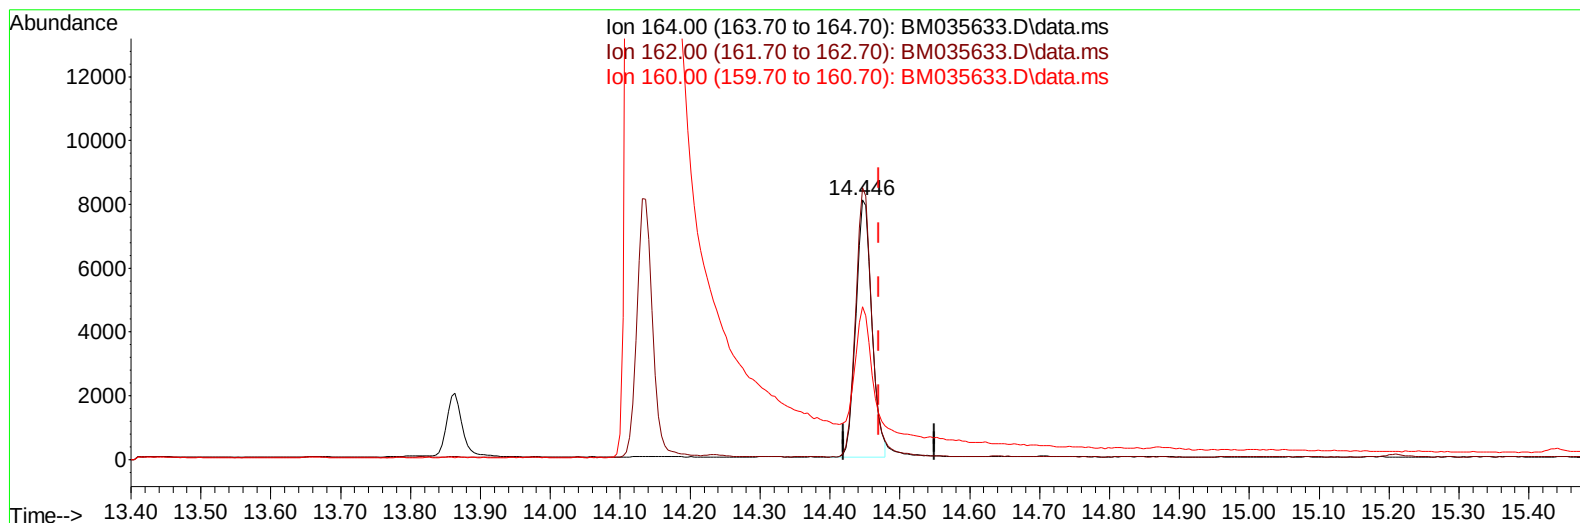

TIC: BM035633.D\data.ms

(9) Acenaphthene-d10 (I)

14.446min (-0.023) 0.40 ng/u1

response 12696

Ion	Exp%	Act%
164.00	100.00	100.00
162.00	106.40	104.66
160.00	49.90	58.75
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062322\
 Data File : BM035633.D
 Acq On : 23 Jun 2022 19:53
 Operator : CG/JU
 Sample : N3358-03
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4R9

Manual IntegrationsAPPROVED

Quant Time: Jun 24 01:36:10 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM061822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 20 01:56:13 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/27/2022
 Supervised By :Yogesh Patel 06/28/2022

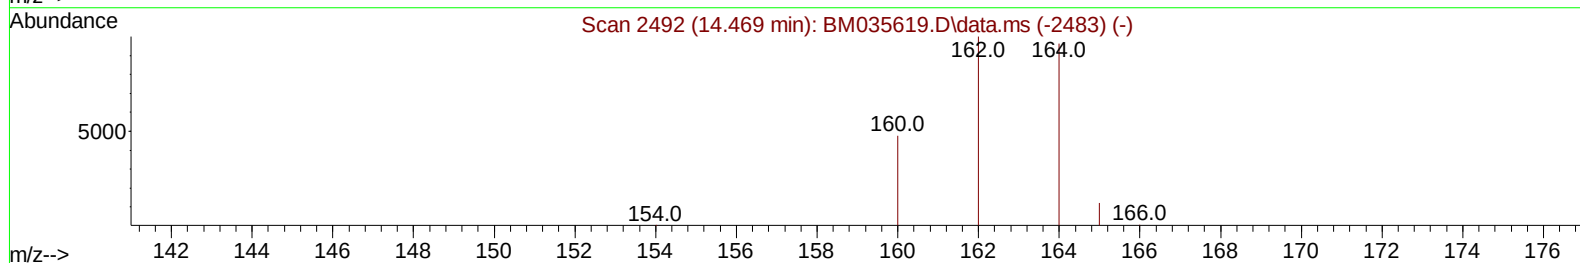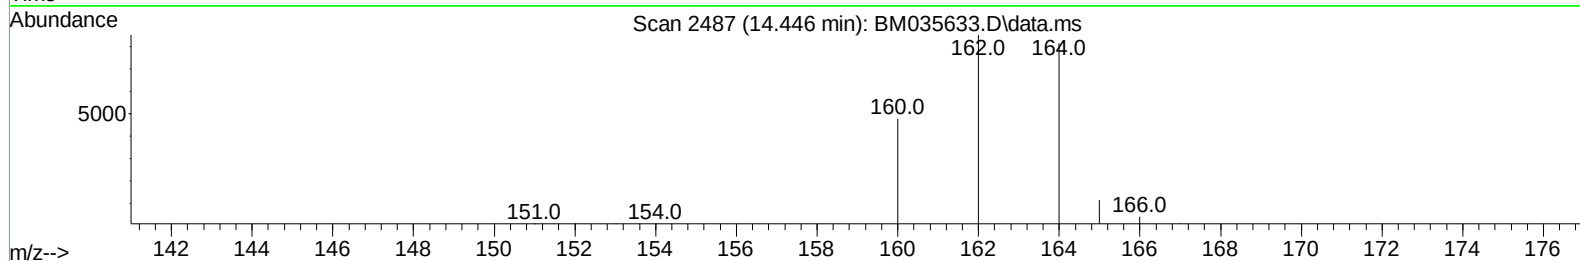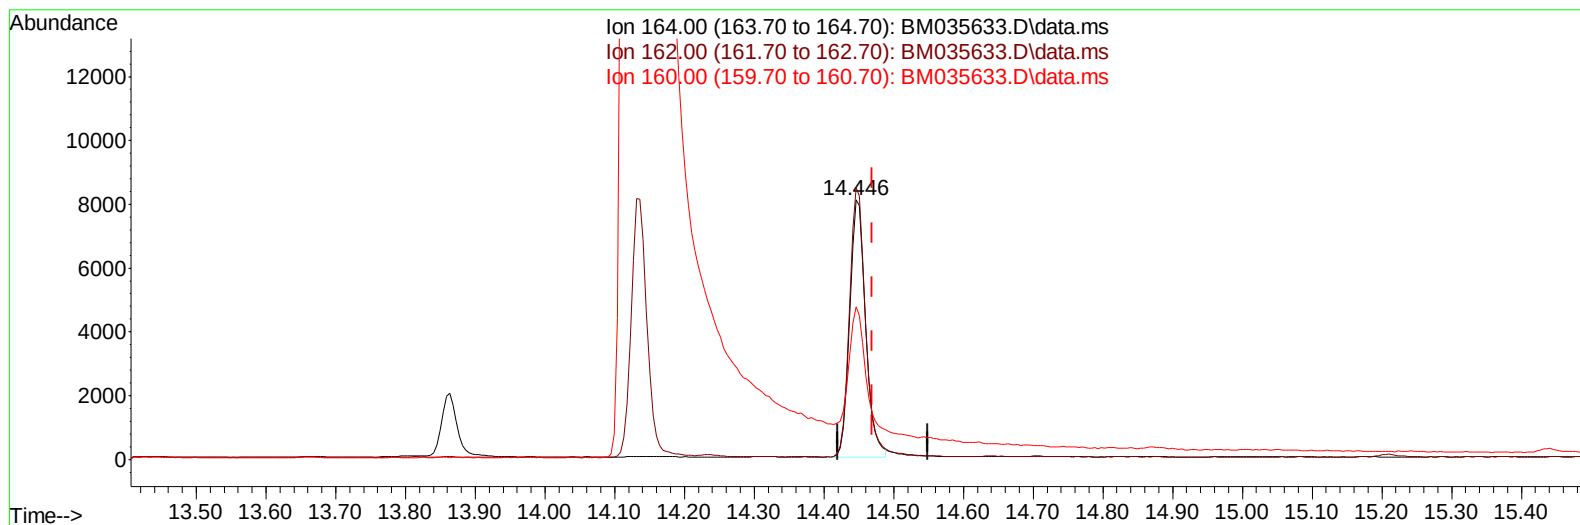

TIC: BM035633.D\data.ms

(9) Acenaphthene-d10 (I)

14.446min (-0.023) 0.40 ng/ul m

response 12900

Ion	Exp%	Act%
164.00	100.00	100.00
162.00	106.40	104.66
160.00	49.90	58.75
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062322\
 Data File : BM035633.D
 Acq On : 23 Jun 2022 19:53
 Operator : CG/JU
 Sample : N3358-03
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4R9

Manual IntegrationsAPPROVED

Quant Time: Jun 24 01:36:10 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM061822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 20 01:56:13 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/27/2022
 Supervised By :Yogesh Patel 06/28/2022

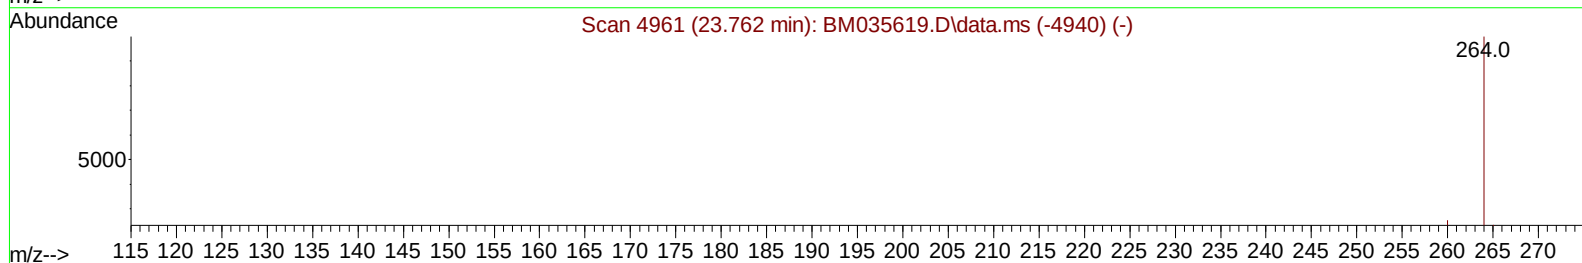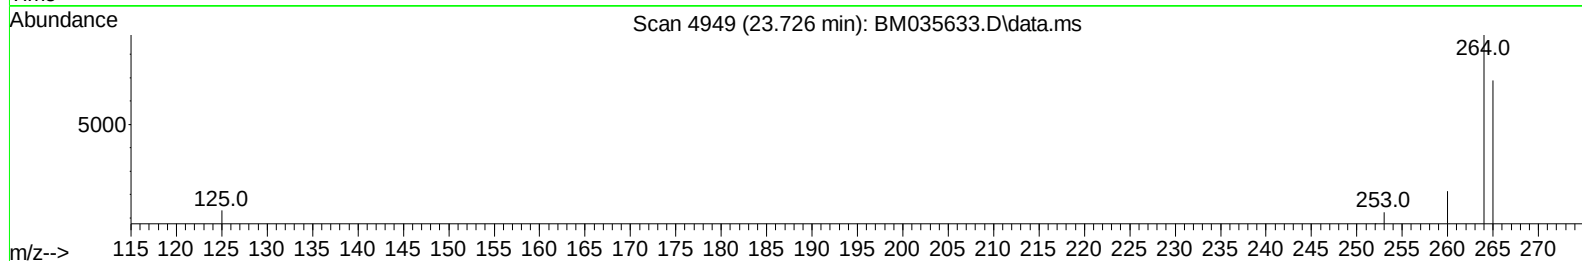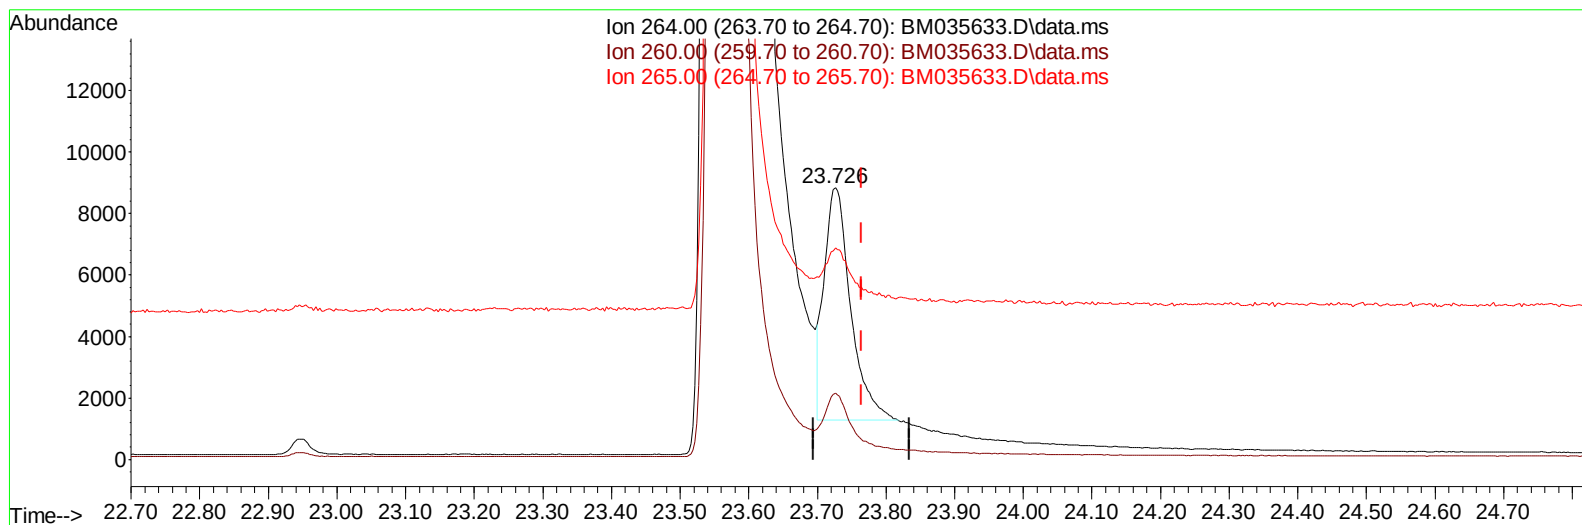

TIC: BM035633.D\data.ms

(23) Perylene-d12 (I)

23.726min (-0.038) 0.40 ng/u1

response 20238

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.30	24.33
265.00	123.50	77.95#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062322\
Data File : BM035633.D
Acq On : 23 Jun 2022 19:53
Operator : CG/JU
Sample : N3358-03
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4R9

Manual IntegrationsAPPROVED

Quant Time: Jun 24 01:36:10 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM061822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 20 01:56:13 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/27/2022
Supervised By :Yogesh Patel 06/28/2022

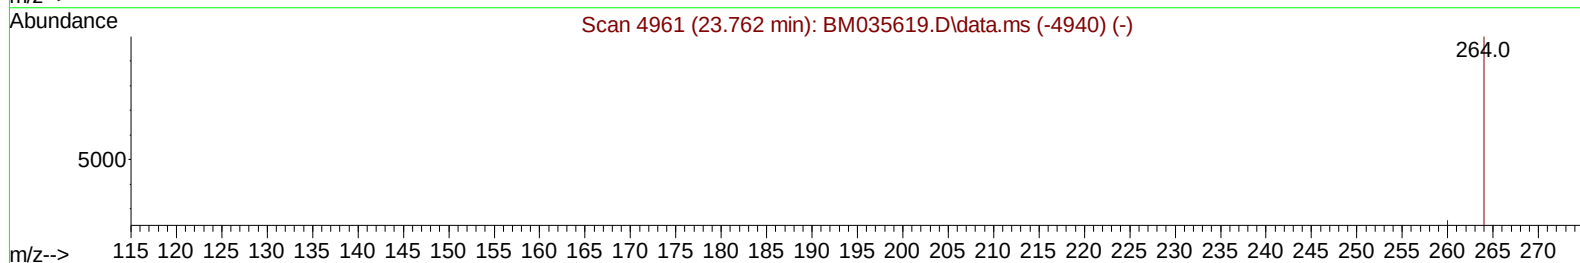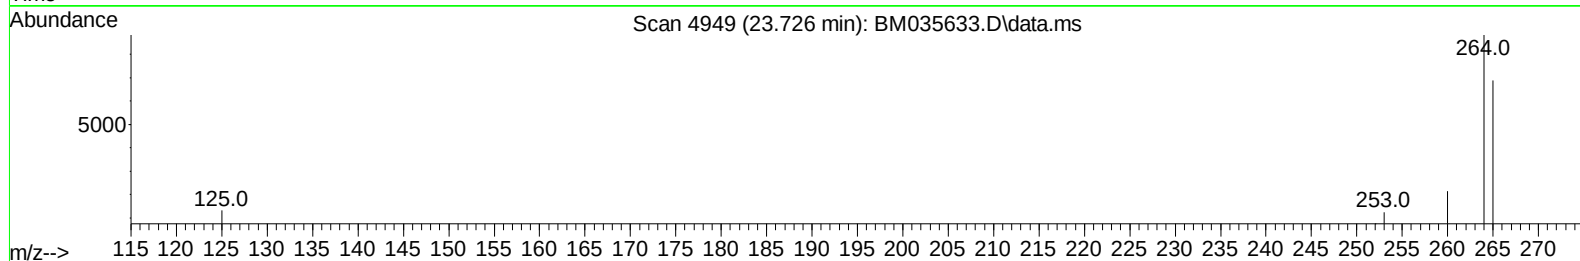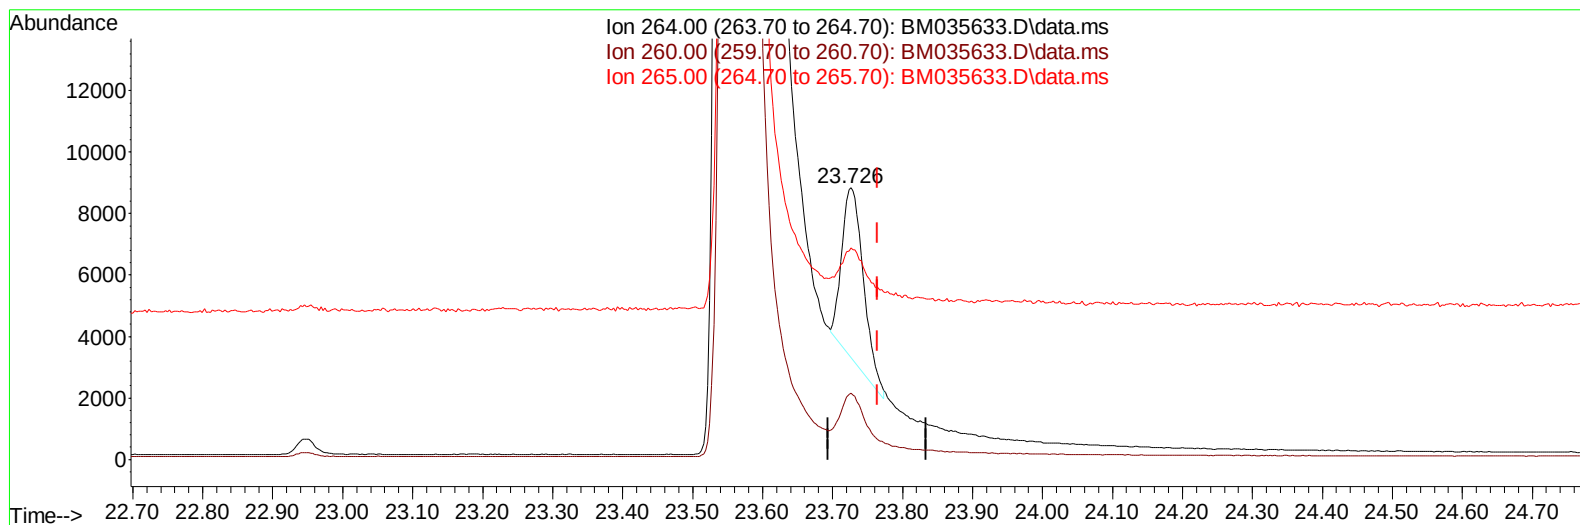

TIC: BM035633.D\data.ms

(23) Perylene-d12 (I)

23.726min (-0.038) 0.40 ng/ul m

response 11766

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.30	24.33
265.00	123.50	77.95#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062322\
 Data File : BM035633.D
 Acq On : 23 Jun 2022 19:53
 Operator : CG/JU
 Sample : N3358-03
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4R9

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 06/27/2022
 Supervised By :Yogesh Patel 06/28/2022

Quant Time: Jun 24 01:36:10 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM061822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 20 01:56:13 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.820	152		5644	0.400	ng/ul	-0.04
4) Naphthalene-d8	10.605	136		22079	0.400	ng/ul	-0.04
9) Acenaphthene-d10	14.446	164		12900m	0.400	ng/ul	-0.02
13) Phenanthrene-d10	17.196	188		24839	0.400	ng/ul	-0.03
17) Chrysene-d12	21.405	240		15857	0.400	ng/ul	0.00
23) Perylene-d12	23.726	264		11766m	0.400	ng/ul	-0.04
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.264	96		26630	3.353	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.217	152		9254	0.282	ng/ul	-0.03
18) Fluoranthene-d10	19.234	212		19921	0.374	ng/ul	-0.02

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062322\
Data File : BM035633.D
Acq On : 23 Jun 2022 19:53
Operator : CG/JU
Sample : N3358-03
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4R9

Manual IntegrationsAPPROVED

Quant Time: Jun 24 01:36:10 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM061822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 20 01:56:13 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/27/2022
Supervised By :Yogesh Patel 06/28/2022

