




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062322\
Data File : BM035642.D
Acq On : 24 Jun 2022 01:55
Operator : CG/JU
Sample : N3358-19
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4T2

Manual IntegrationsAPPROVED

Quant Time: Jun 24 02:51:11 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM061822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 20 01:56:13 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/27/2022
Supervised By :Yogesh Patel 06/28/2022

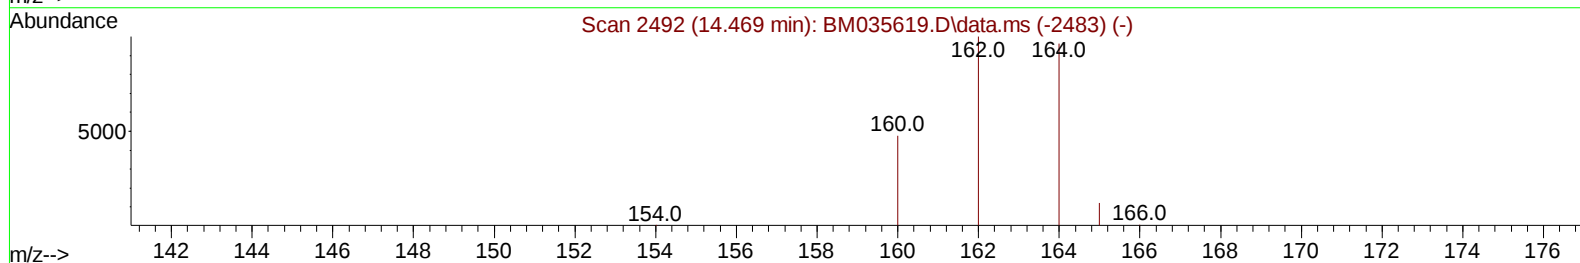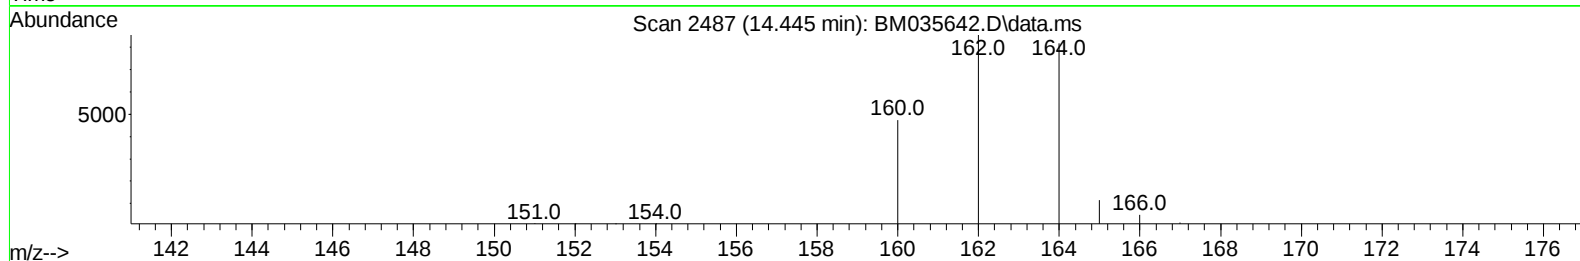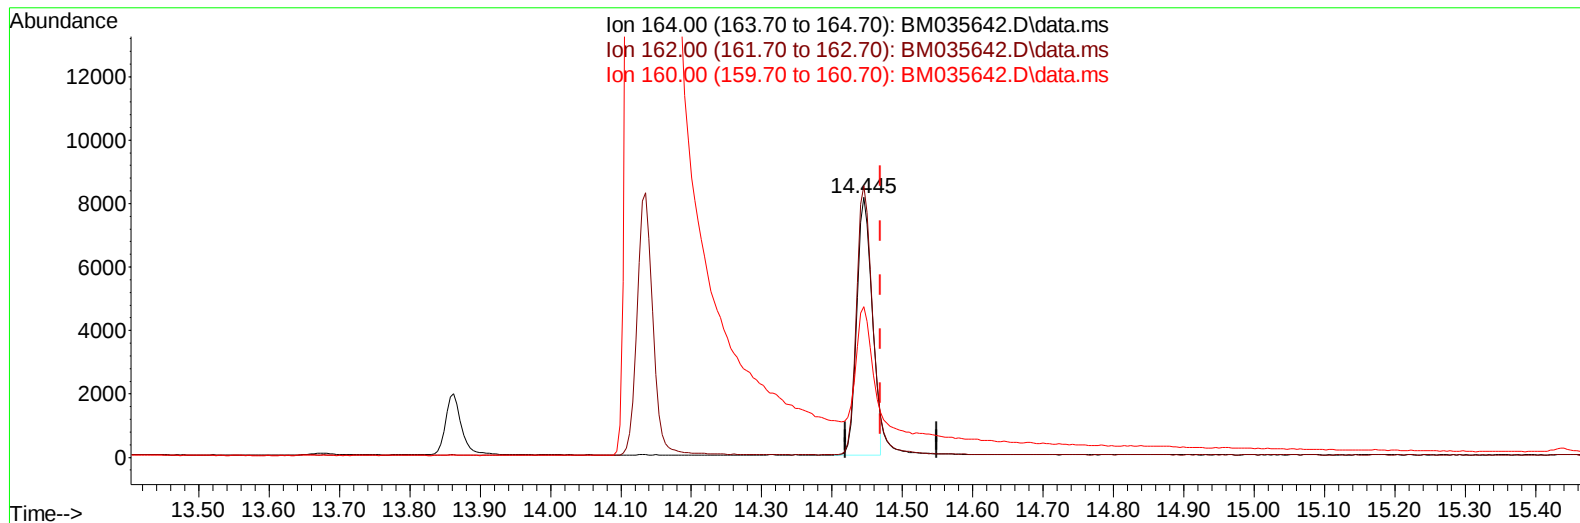

TIC: BM035642.D\data.ms

(9) Acenaphthene-d10 (I)

14.445min (-0.024) 0.40 ng/u1

response 12370

Ion	Exp%	Act%
164.00	100.00	100.00
162.00	106.40	104.38
160.00	49.90	58.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062322\
 Data File : BM035642.D
 Acq On : 24 Jun 2022 01:55
 Operator : CG/JU
 Sample : N3358-19
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4T2

Manual IntegrationsAPPROVED

Quant Time: Jun 24 02:51:11 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM061822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 20 01:56:13 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/27/2022
 Supervised By :Yogesh Patel 06/28/2022

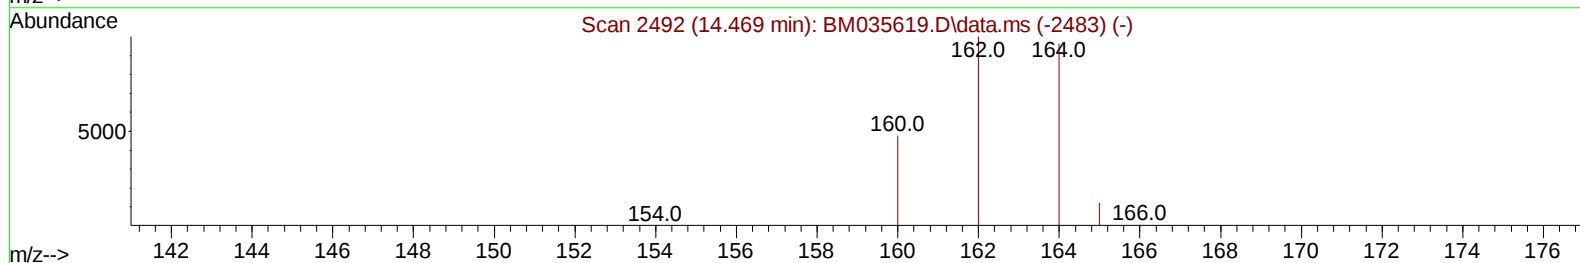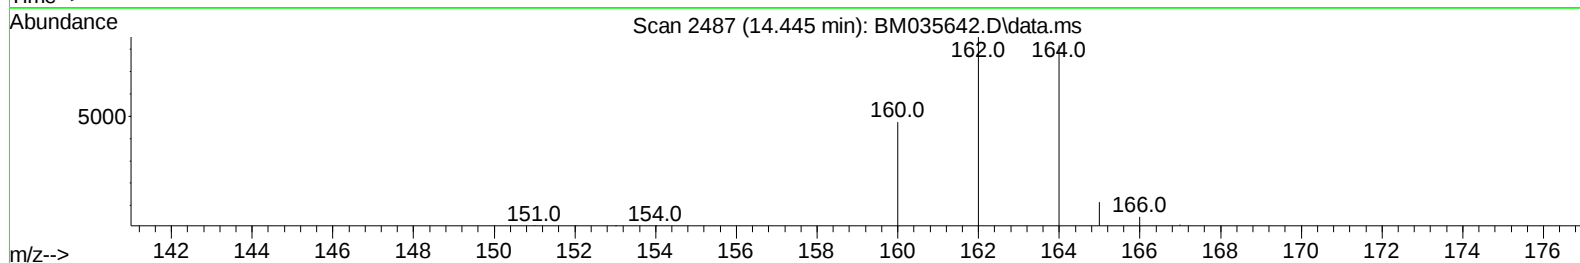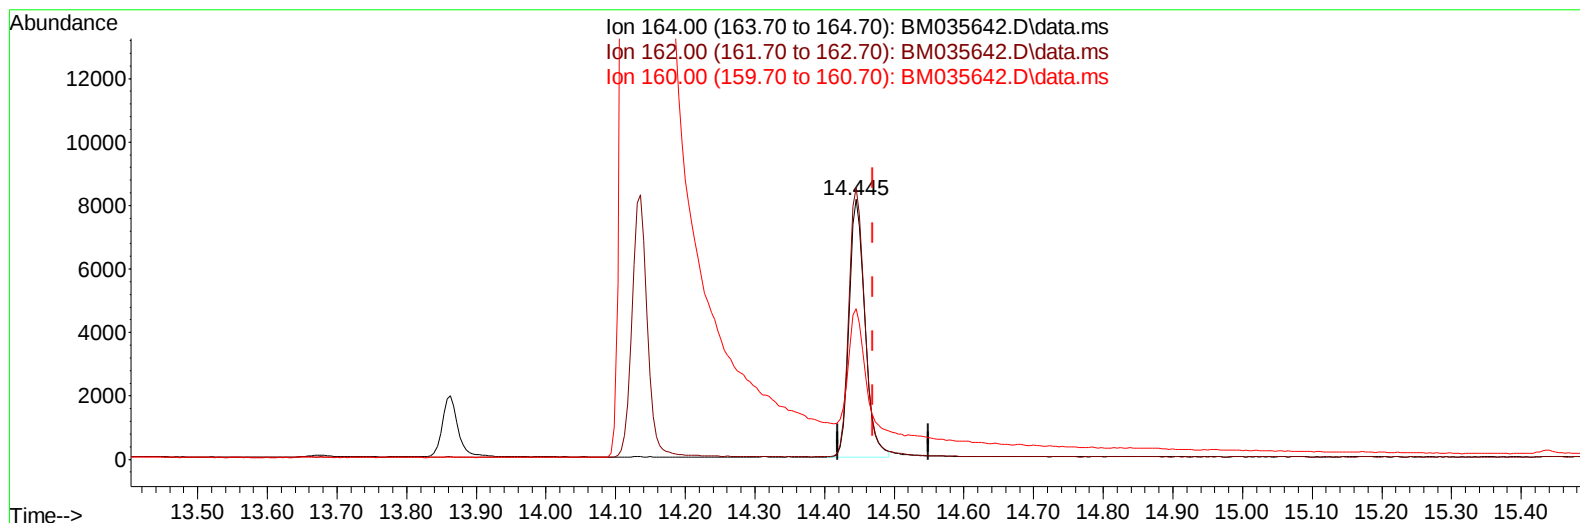

TIC: BM035642.D\data.ms

(9) Acenaphthene-d10 (I)

14.445min (-0.024) 0.40 ng/u1 m

response 12927

Ion	Exp%	Act%
164.00	100.00	100.00
162.00	106.40	104.38
160.00	49.90	58.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062322\
 Data File : BM035642.D
 Acq On : 24 Jun 2022 01:55
 Operator : CG/JU
 Sample : N3358-19
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4T2

Manual IntegrationsAPPROVED

Quant Time: Jun 24 02:51:11 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM061822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 20 01:56:13 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/27/2022
 Supervised By :Yogesh Patel 06/28/2022

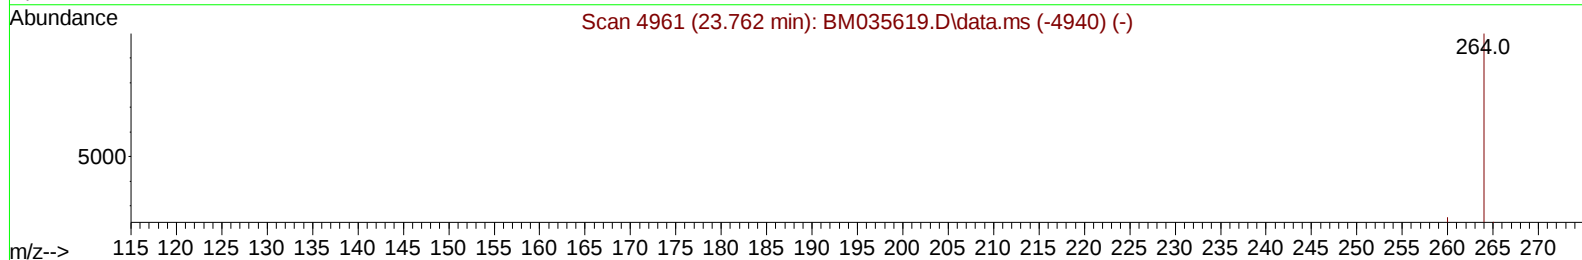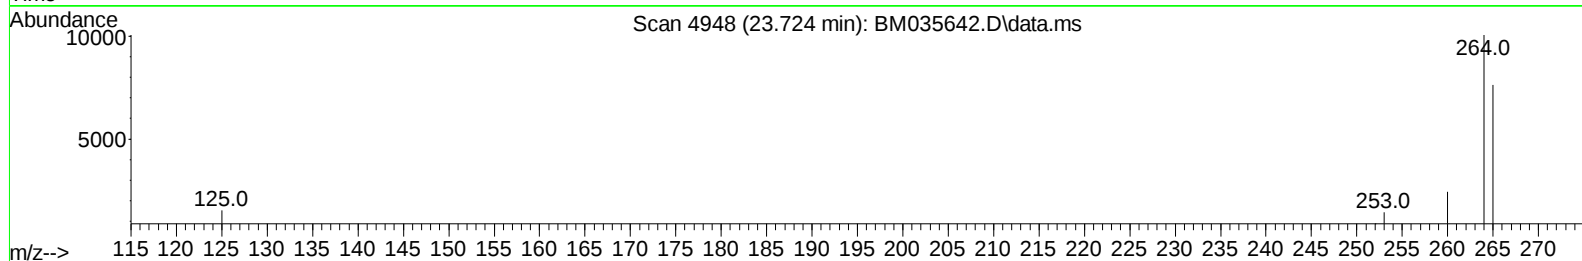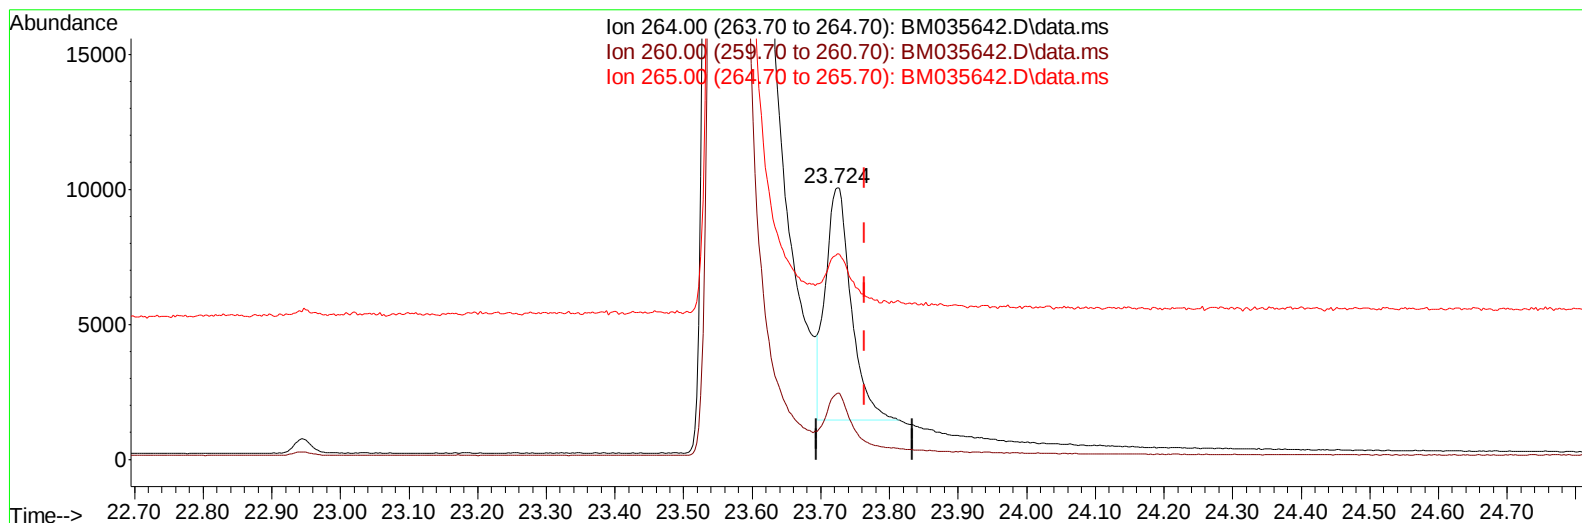

TIC: BM035642.D\data.ms

(23) Perylene-d12 (I)

23.724min (-0.040) 0.40 ng/u1

response 22328

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.30	24.38
265.00	123.50	75.79#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062322\
 Data File : BM035642.D
 Acq On : 24 Jun 2022 01:55
 Operator : CG/JU
 Sample : N3358-19
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4T2

Manual IntegrationsAPPROVED

Quant Time: Jun 24 02:51:11 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM061822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 20 01:56:13 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/27/2022
 Supervised By :Yogesh Patel 06/28/2022

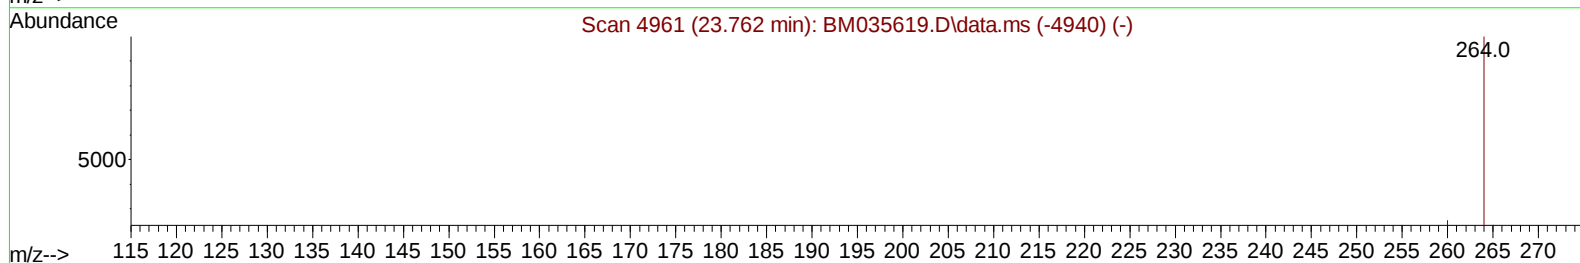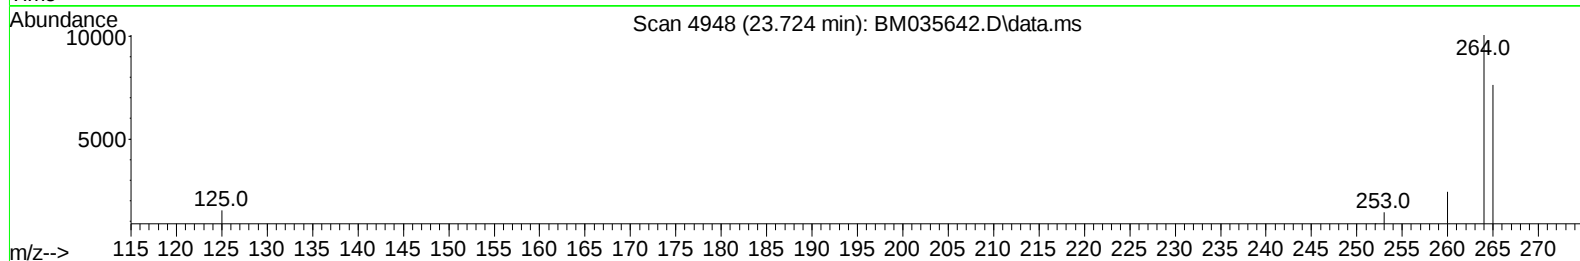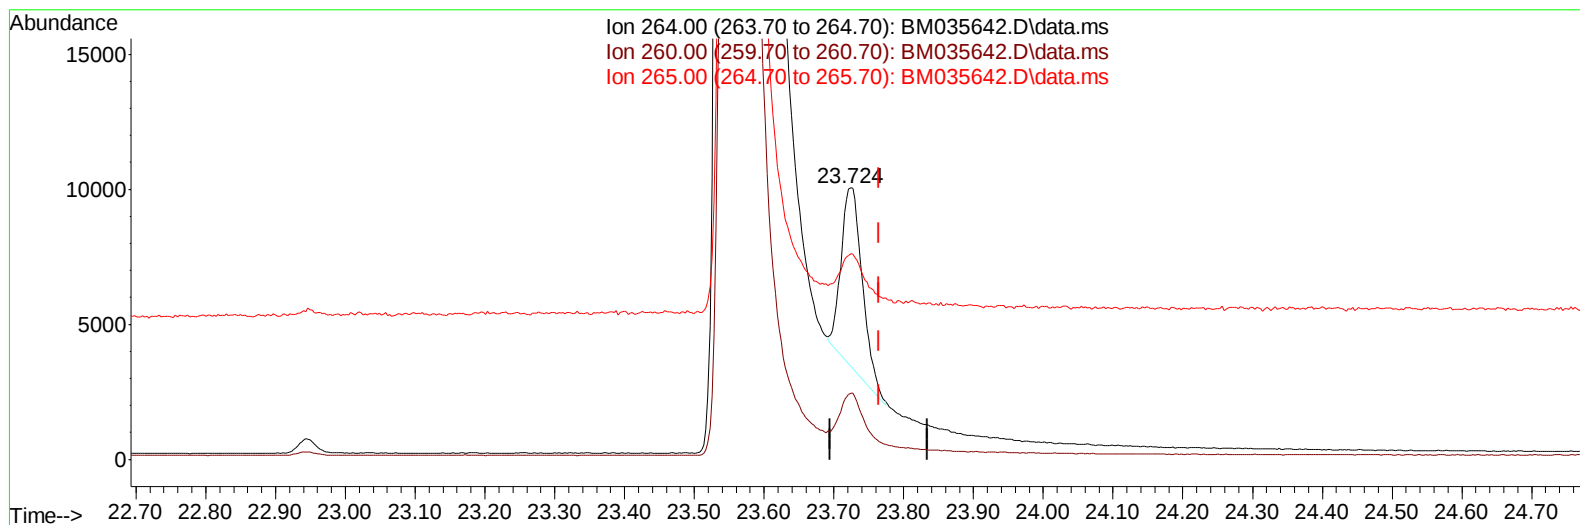

TIC: BM035642.D\data.ms

(23) Perylene-d12 (I)

23.724min (-0.040) 0.40 ng/ul m

response 13807

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.30	24.38
265.00	123.50	75.79#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062322\
 Data File : BM035642.D
 Acq On : 24 Jun 2022 01:55
 Operator : CG/JU
 Sample : N3358-19
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4T2

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 06/27/2022
 Supervised By :Yogesh Patel 06/28/2022

Quant Time: Jun 24 02:51:11 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM061822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 20 01:56:13 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.816	152		5472	0.400	ng/ul	-0.04
4) Naphthalene-d8	10.600	136		20467	0.400	ng/ul	-0.04
9) Acenaphthene-d10	14.445	164		12927m	0.400	ng/ul	-0.02
13) Phenanthrene-d10	17.195	188		27314	0.400	ng/ul	-0.03
17) Chrysene-d12	21.400	240		18480	0.400	ng/ul	-0.01
23) Perylene-d12	23.724	264		13807m	0.400	ng/ul	-0.04
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.259	96		28646	3.721	ng/ul	-0.01
6) 2-Methylnaphthalene-d10	12.211	152		8744	0.287	ng/ul	-0.03
18) Fluoranthene-d10	19.233	212		20869	0.336	ng/ul	-0.02

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062322\
Data File : BM035642.D
Acq On : 24 Jun 2022 01:55
Operator : CG/JU
Sample : N3358-19
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4T2

Manual IntegrationsAPPROVED

Quant Time: Jun 24 02:51:11 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM061822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 20 01:56:13 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/27/2022
Supervised By :Yogesh Patel 06/28/2022

