
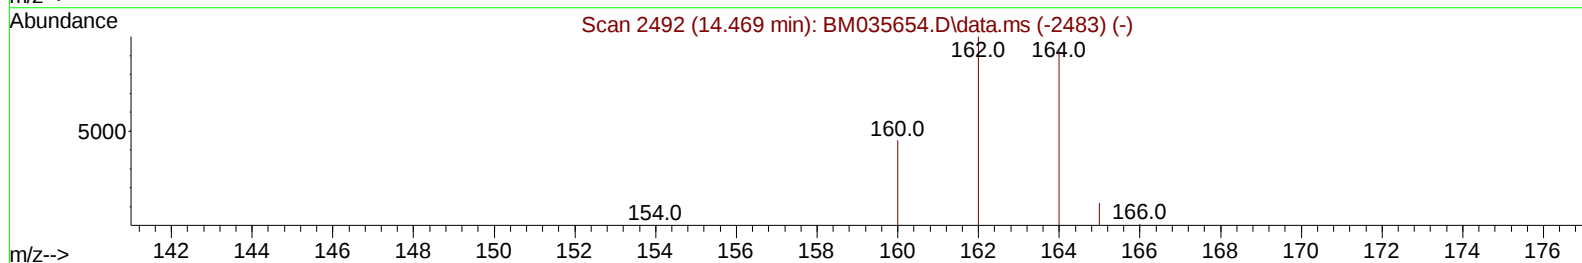
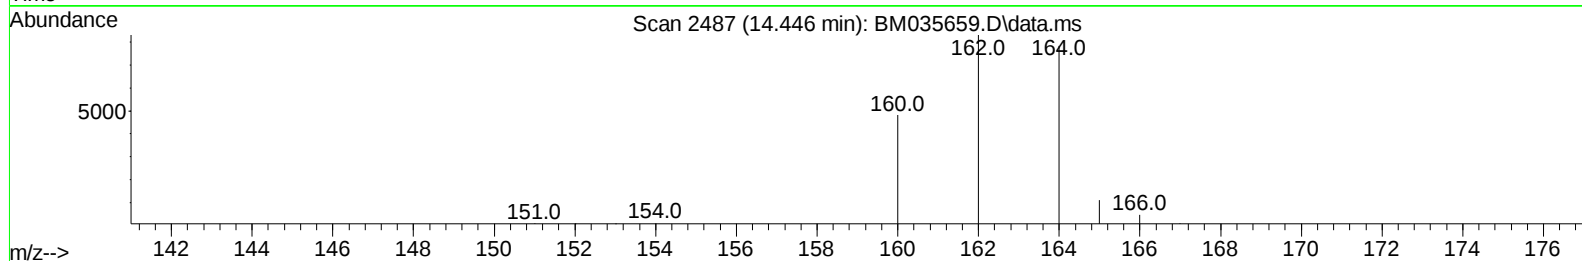


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062322\
Data File : BM035659.D
Acq On : 24 Jun 2022 12:46
Operator : CG/JU
Sample : PB145603BL
Misc :
ALS Vial : 43 Sample Multiplier: 1

Quant Time: Jun 28 09:59:25 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM061822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 20 01:56:13 2022
Response via : Initial Calibration

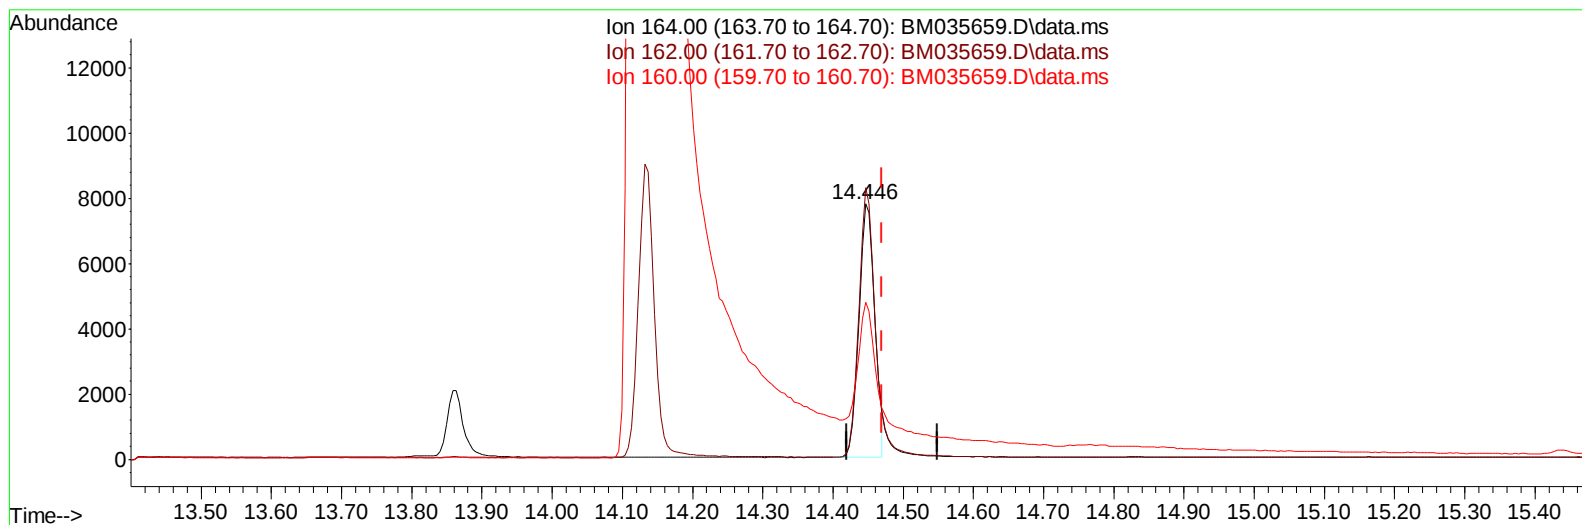

TIC: BM035659.D\data.ms

(9) Acenaphthene-d10 (I)




14.446min (-0.023) 0.40 ng/u1

response 12067

Ion	Exp%	Act%
164.00	100.00	100.00
162.00	106.40	106.20
160.00	49.90	61.51#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062322\
Data File : BM035659.D
Acq On : 24 Jun 2022 12:46
Operator : CG/JU
Sample : PB145603BL
Misc :
ALS Vial : 43 Sample Multiplier: 1

Quant Time: Jun 25 04:05:39 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM061822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 20 01:56:13 2022
Response via : Initial Calibration

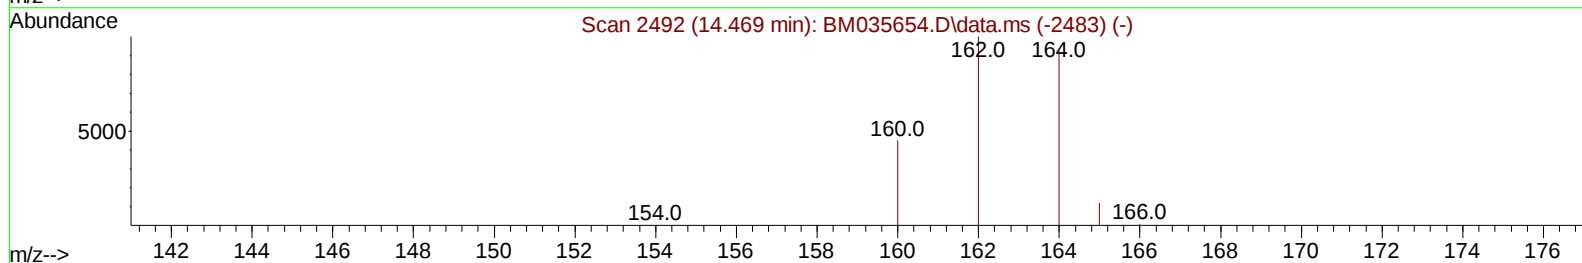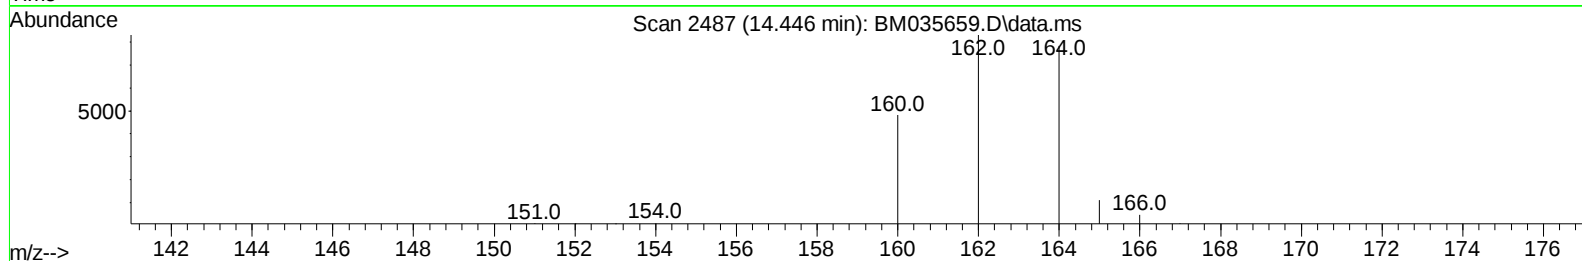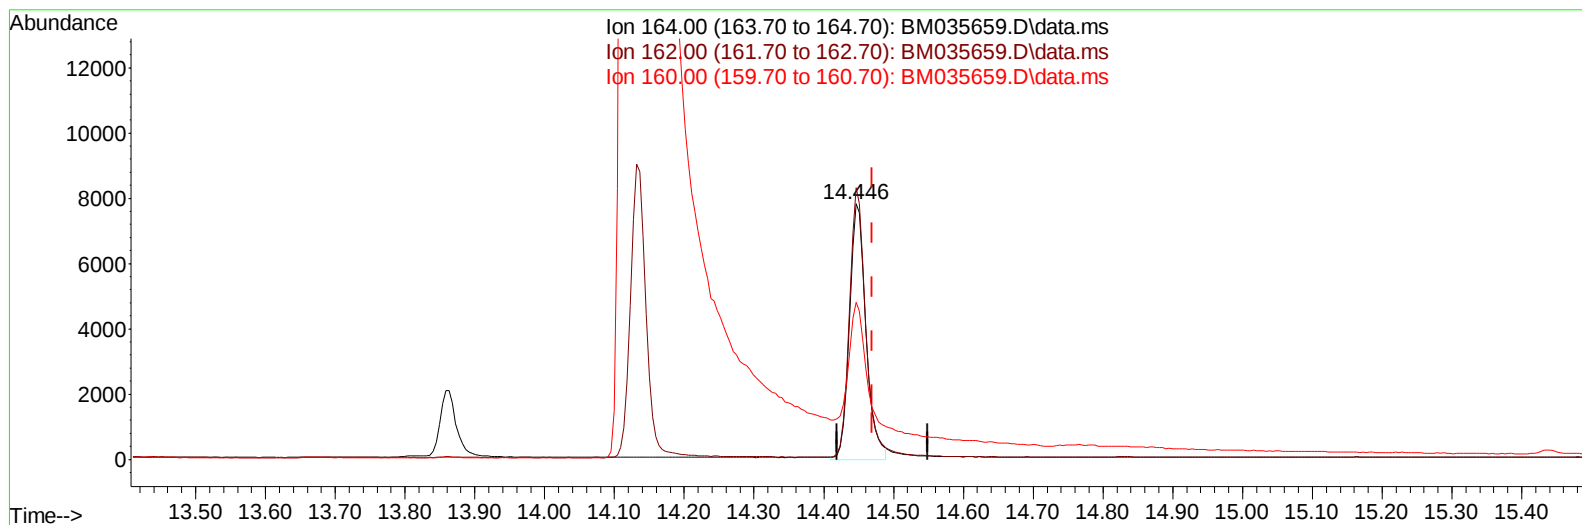

TIC: BM035659.D\data.ms

(9) Acenaphthene-d10 (I)




14.446min (-0.023) 0.40 ng/ul m

response 12930

Ion	Exp%	Act%
164.00	100.00	100.00
162.00	106.40	106.20
160.00	49.90	61.51#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062322\
 Data File : BM035659.D
 Acq On : 24 Jun 2022 12:46
 Operator : CG/JU
 Sample : PB145603BL
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Quant Time: Jun 28 09:59:25 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM061822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 20 01:56:13 2022
 Response via : Initial Calibration

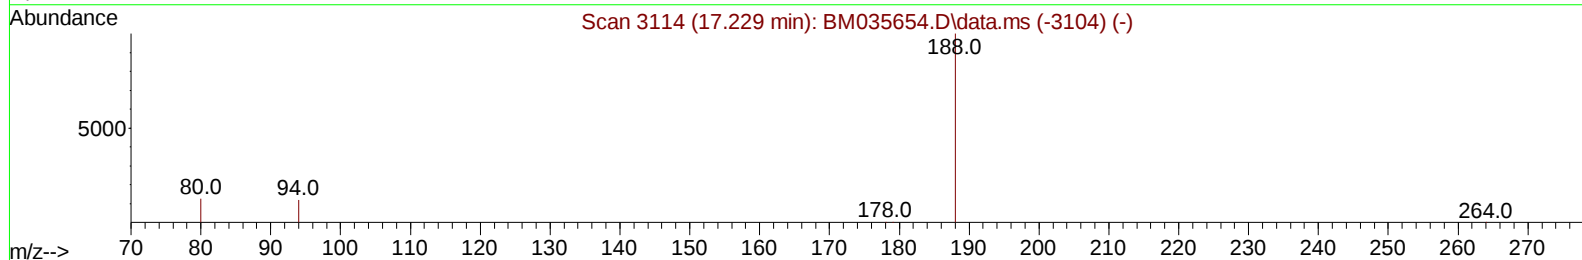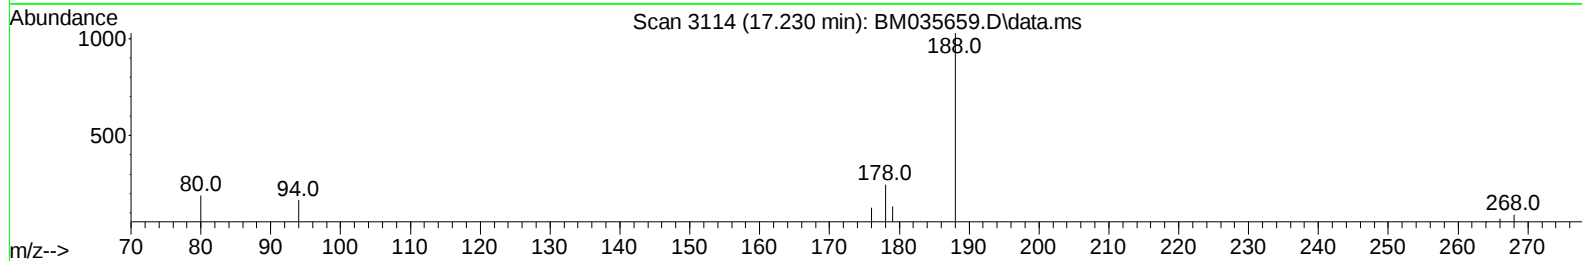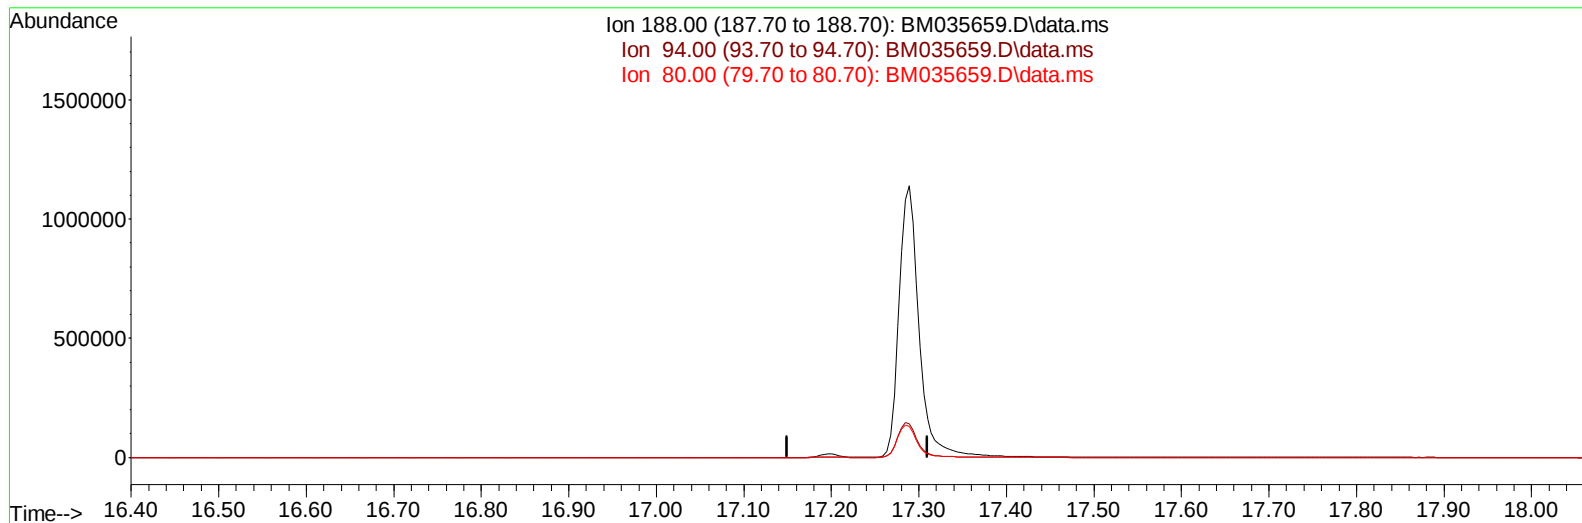

TIC: BM035659.D\data.ms

(13) Phenanthrene-d10 (I)




17.230min (-17.230) 0.00 ng/u1

response 0

Ion	Exp%	Act%
188.00	100.00	0.00
94.00	12.00	0.00#
80.00	13.50	0.00#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062322\
Data File : BM035659.D
Acq On : 24 Jun 2022 12:46
Operator : CG/JU
Sample : PB145603BL
Misc :
ALS Vial : 43 Sample Multiplier: 1

Quant Time: Jun 25 04:05:39 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM061822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 20 01:56:13 2022
Response via : Initial Calibration

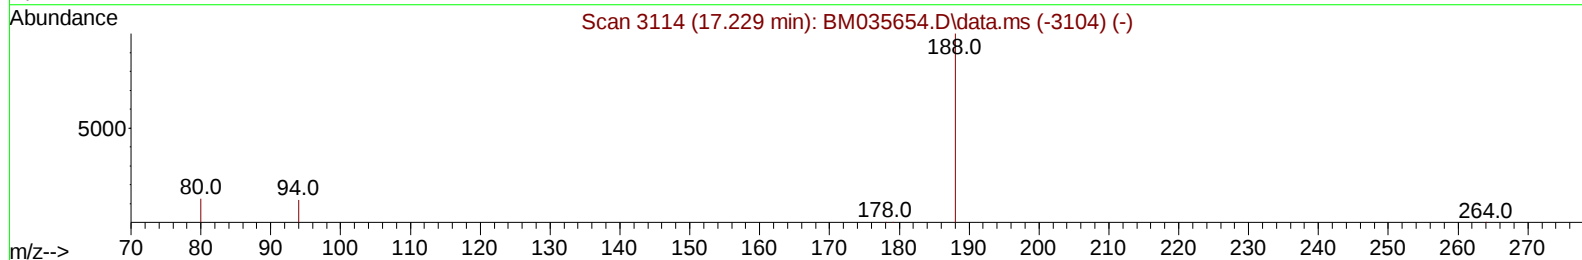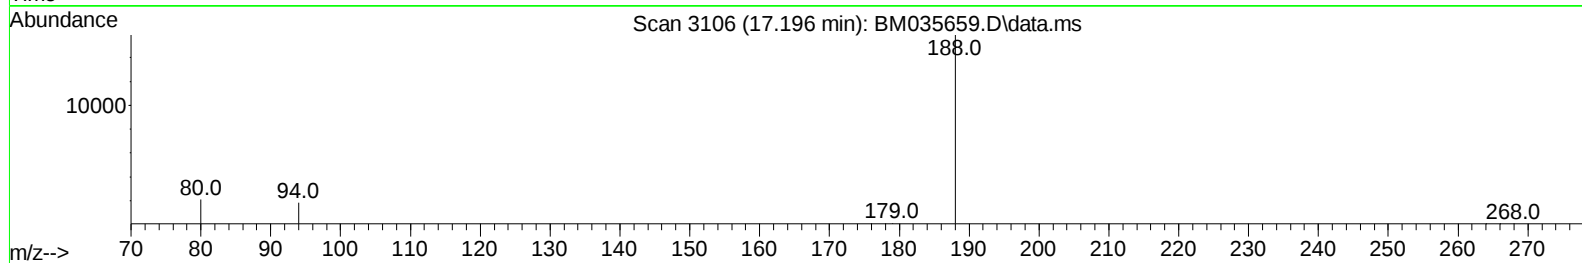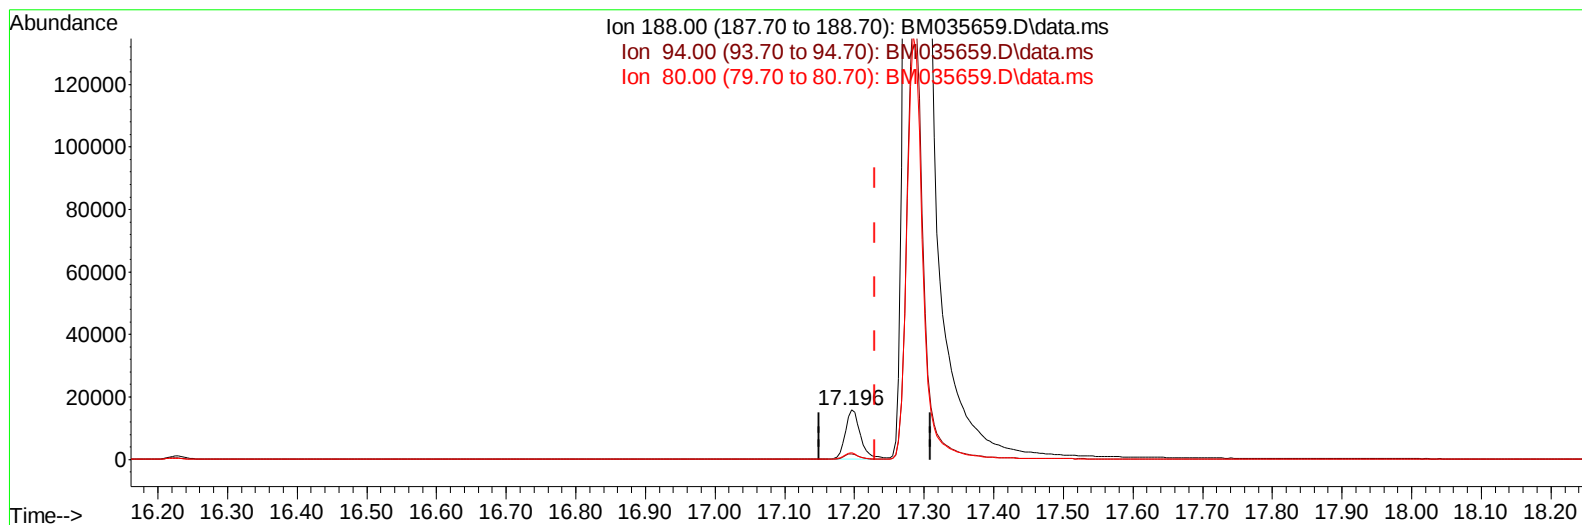

TIC: BM035659.D\data.ms

(13) Phenanthrene-d10 (I)




17.196min (-0.034) 0.40 ng/ul m

response 23958

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	12.00	11.41
80.00	13.50	13.10
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062322\
Data File : BM035659.D
Acq On : 24 Jun 2022 12:46
Operator : CG/JU
Sample : PB145603BL
Misc :
ALS Vial : 43 Sample Multiplier: 1

Quant Time: Jun 28 09:59:25 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM061822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 20 01:56:13 2022
Response via : Initial Calibration

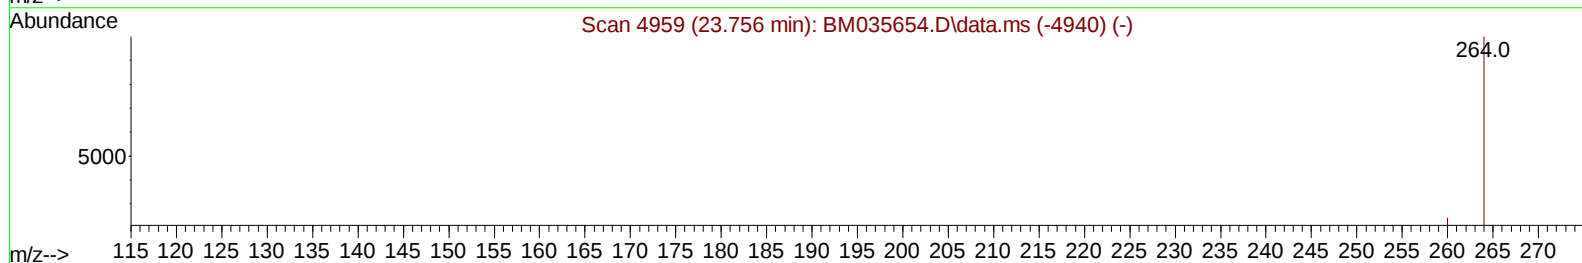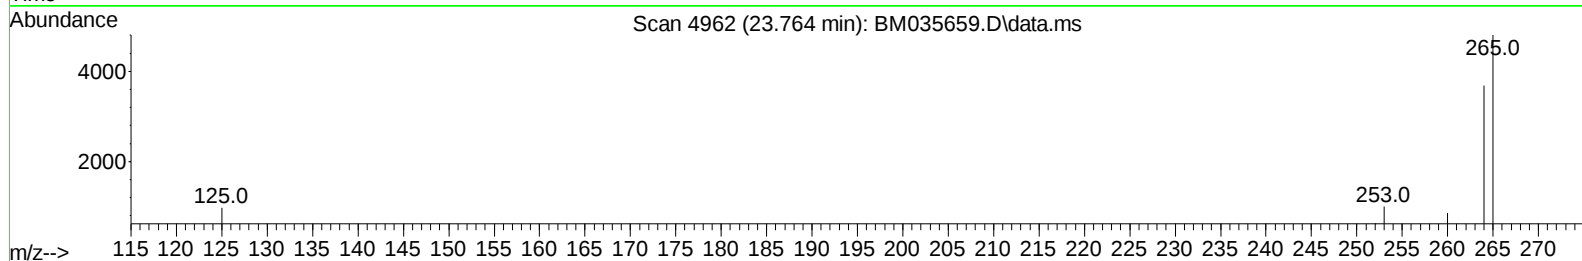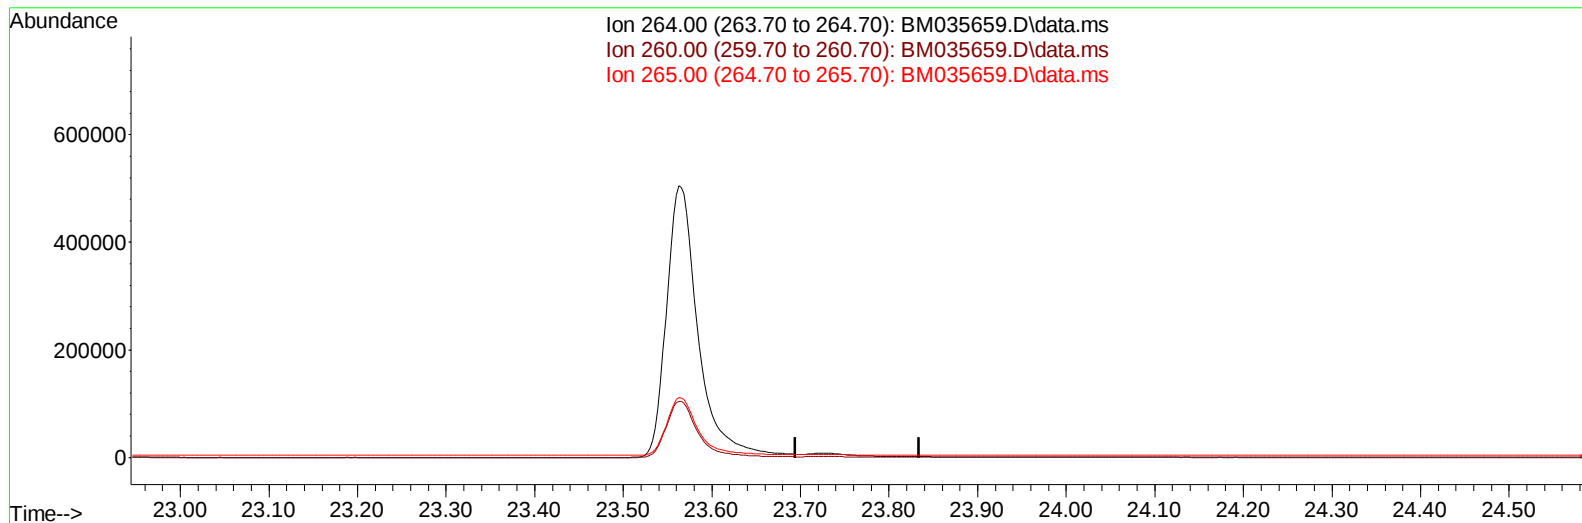

TIC: BM035659.D\data.ms

(23) Perylene-d12 (I)




23.764min (-23.764) 0.00 ng/ul

response 0

Ion	Exp%	Act%
264.00	100.00	0.00
260.00	26.30	0.00#
265.00	123.50	0.00#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062322\
Data File : BM035659.D
Acq On : 24 Jun 2022 12:46
Operator : CG/JU
Sample : PB145603BL
Misc :
ALS Vial : 43 Sample Multiplier: 1

Quant Time: Jun 25 04:05:39 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM061822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 20 01:56:13 2022
Response via : Initial Calibration

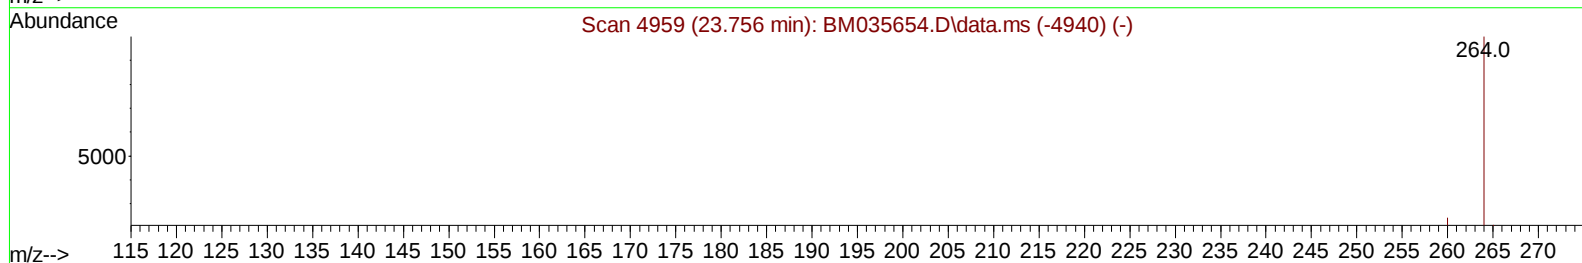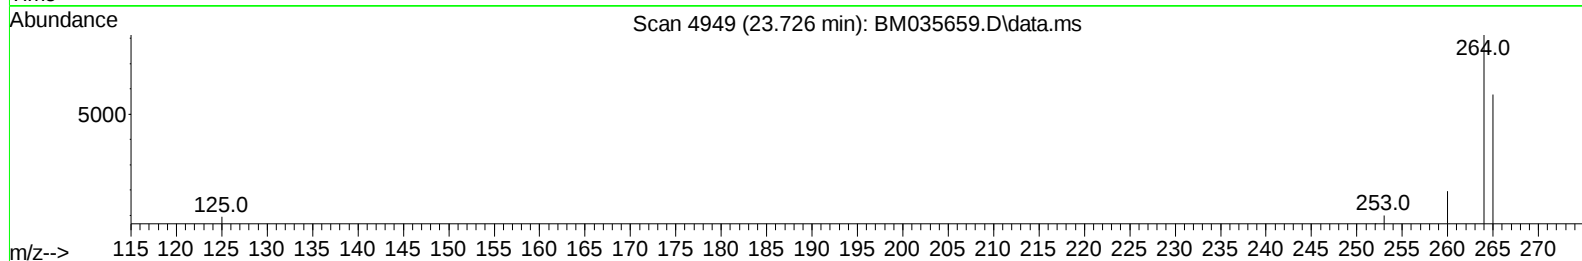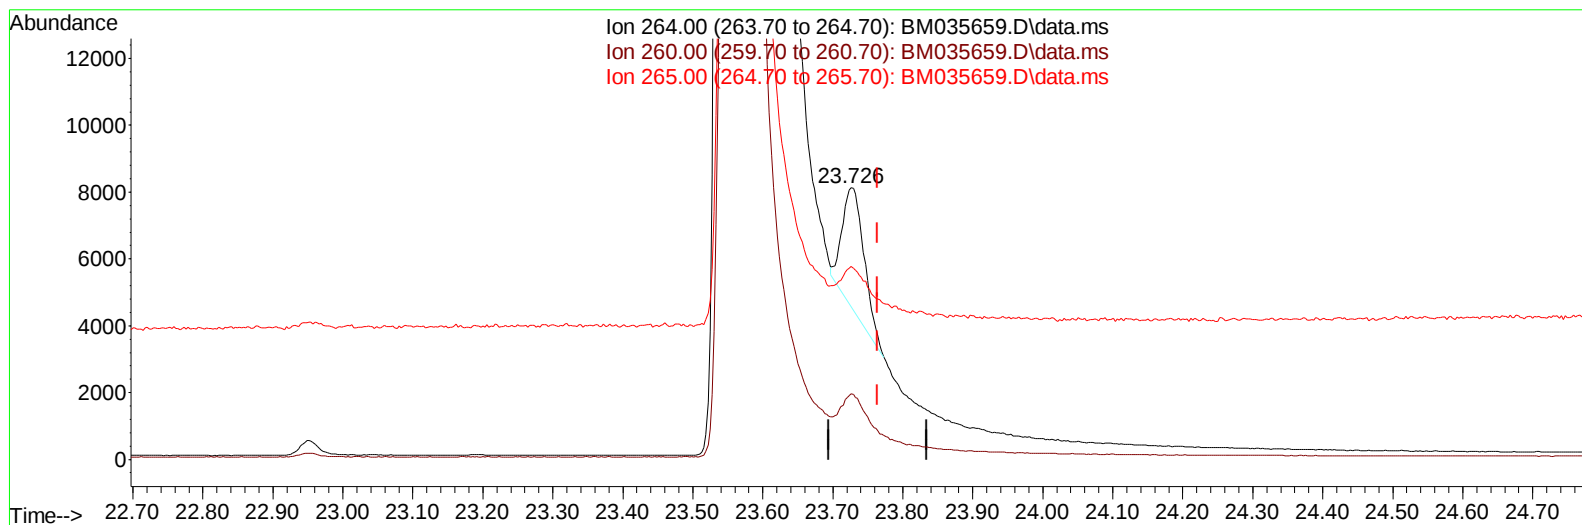

TIC: BM035659.D\data.ms

(23) Perylene-d12 (I)

23.726min (-0.038) 0.40 ng/ul m

response 7627

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.30	24.10
265.00	123.50	71.00#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062322\
 Data File : BM035659.D
 Acq On : 24 Jun 2022 12:46
 Operator : CG/JU
 Sample : PB145603BL
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Quant Time: Jun 25 04:05:39 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM061822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 20 01:56:13 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.820	152	6217	0.400	ng/ul	-0.04
4) Naphthalene-d8	10.600	136	20774	0.400	ng/ul	-0.04
9) Acenaphthene-d10	14.446	164	12930m	0.400	ng/ul	-0.02
13) Phenanthrene-d10	17.196	188	23958m	0.400	ng/ul	-0.03
17) Chrysene-d12	21.423	240	14070	0.400	ng/ul	0.01
23) Perylene-d12	23.726	264	7627m	0.400	ng/ul	-0.04
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.260	96	46547	5.321	ng/ul	-0.01
6) 2-Methylnaphthalene-d10	12.250	152	9833	0.318	ng/ul	0.00
18) Fluoranthene-d10	19.234	212	17896	0.379	ng/ul	-0.02

Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062322\
Data File : BM035659.D
Acq On : 24 Jun 2022 12:46
Operator : CG/JU
Sample : PB145603BL
Misc :
ALS Vial : 43 Sample Multiplier: 1

Quant Time: Jun 25 04:05:39 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM061822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 20 01:56:13 2022
Response via : Initial Calibration

