




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062322\
Data File : BM035674.D
Acq On : 24 Jun 2022 22:52
Operator : CG/JU
Sample : N3358-16RE
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4S9RE

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 06/27/2022
Supervised By :Yogesh Patel 06/28/2022

Quant Time: Jun 25 04:06:34 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM061822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 20 01:56:13 2022
Response via : Initial Calibration

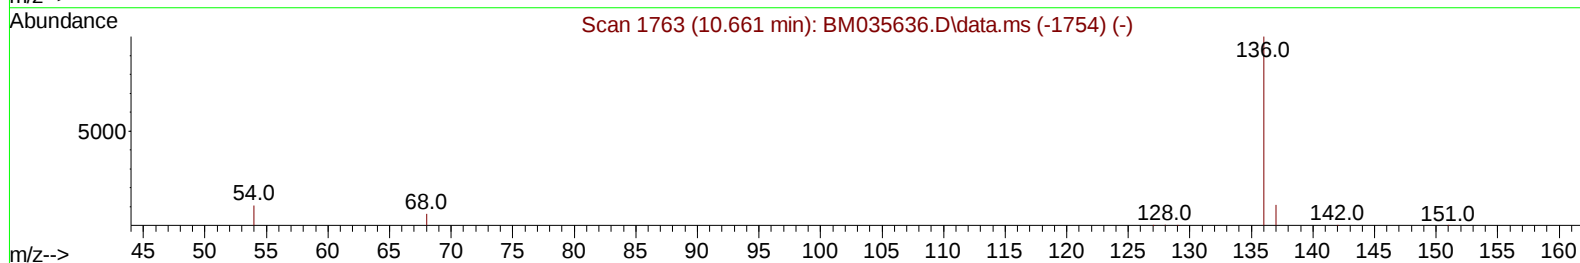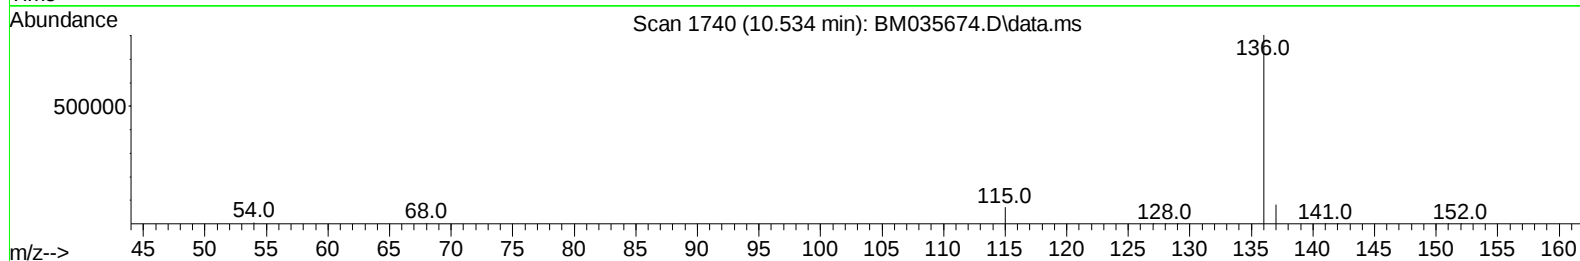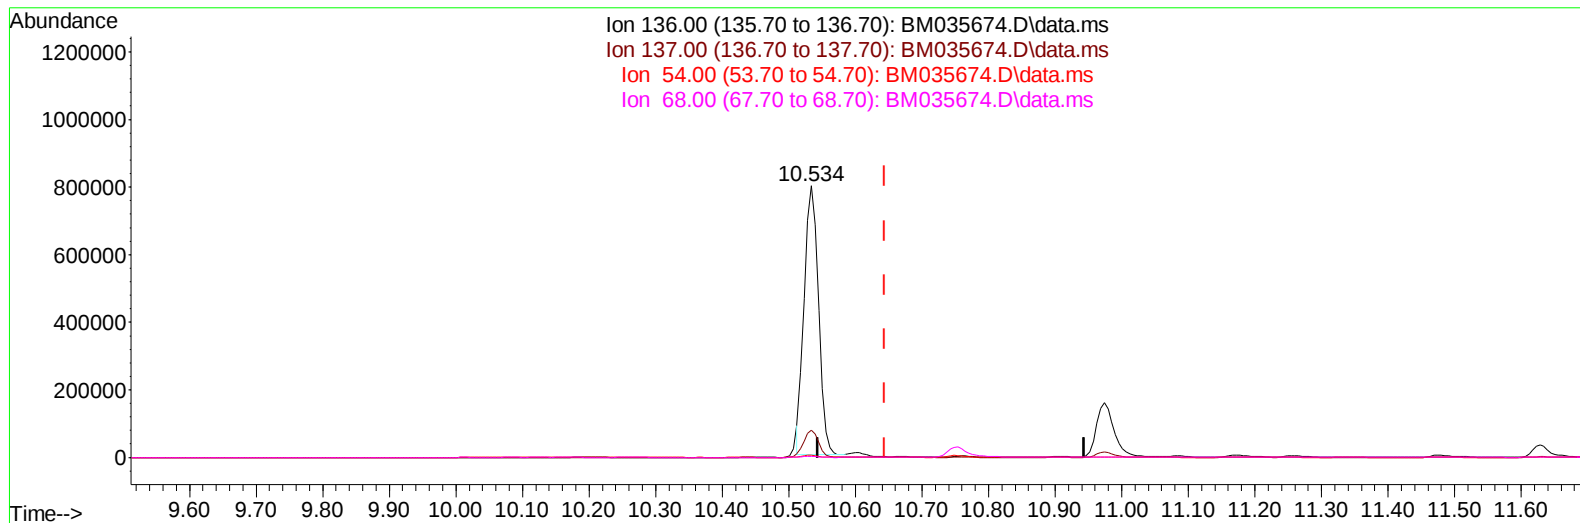

TIC: BM035674.D\data.ms

(4) Naphthalene-d8 (I)

10.534min (-0.110) 0.40 ng/u1

response 1186481

Ion	Exp%	Act%
136.00	100.00	100.00
137.00	11.70	10.04
54.00	12.80	0.87#
68.00	8.70	0.47#




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062322\
Data File : BM035674.D
Acq On : 24 Jun 2022 22:52
Operator : CG/JU
Sample : N3358-16RE
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4S9RE

Manual IntegrationsAPPROVED

Quant Time: Jun 25 04:06:34 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM061822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 20 01:56:13 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/27/2022
Supervised By :Yogesh Patel 06/28/2022

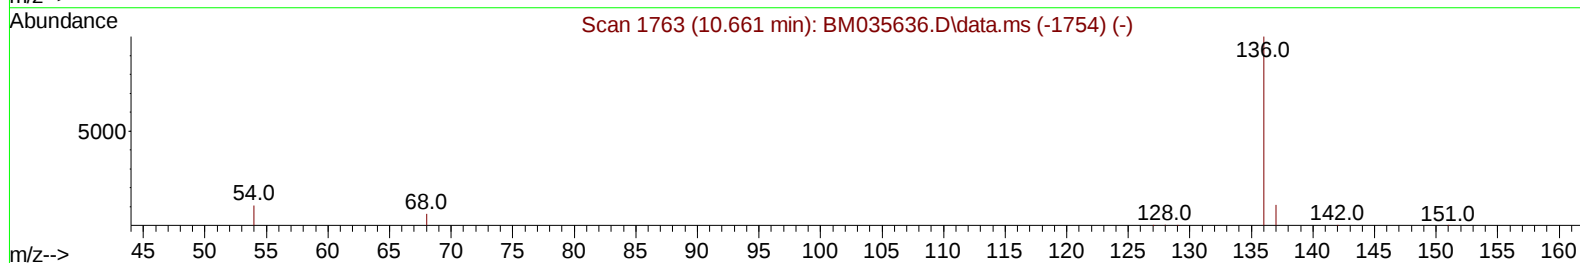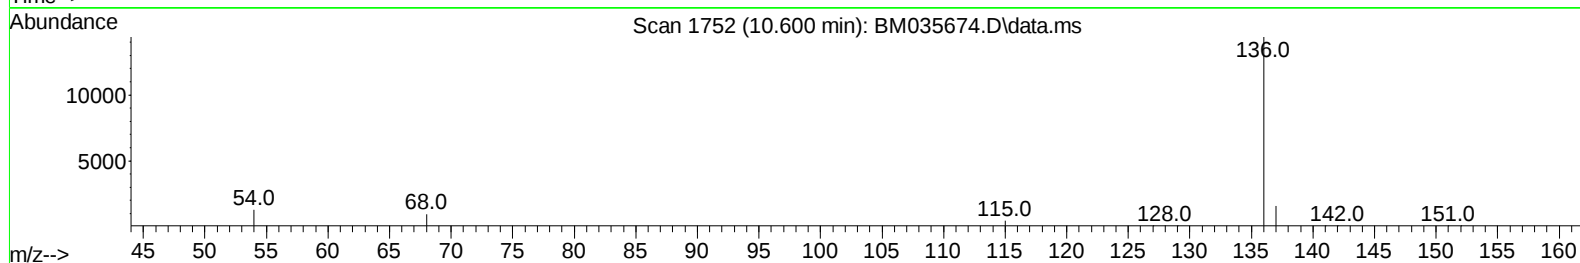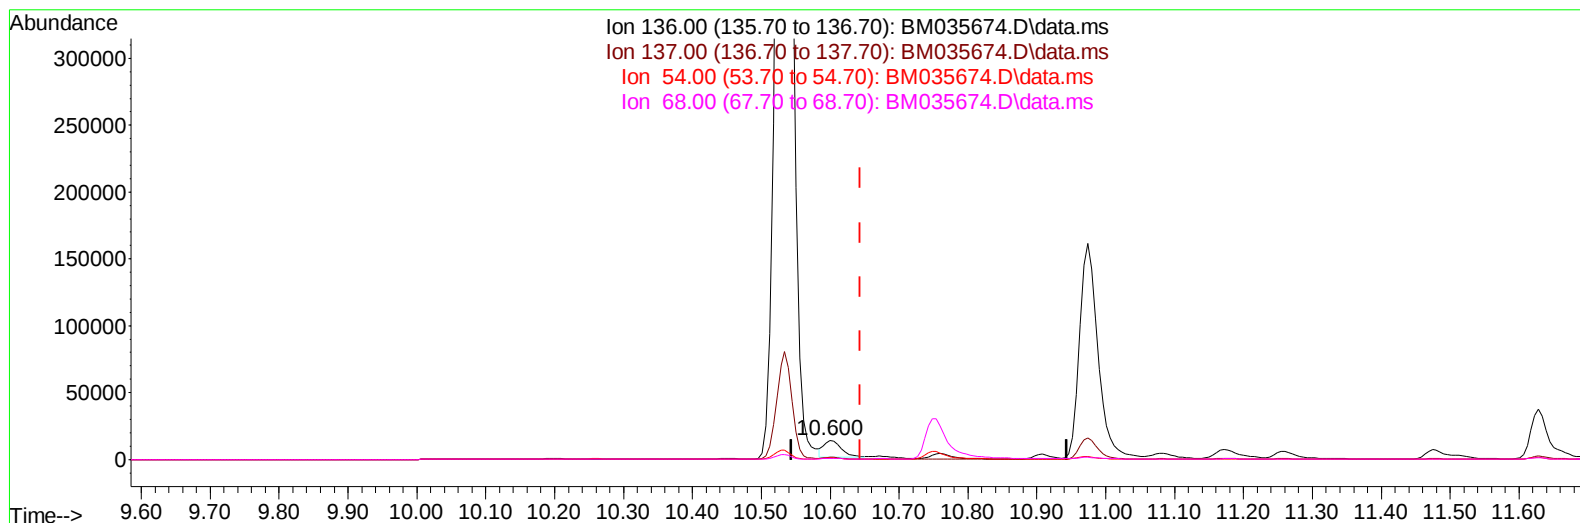

TIC: BM035674.D\data.ms

(4) Naphthalene-d8 (I)

10.600min (-0.044) 0.40 ng/ul m

response 22666

Ion	Exp%	Act%
136.00	100.00	100.00
137.00	11.70	11.08
54.00	12.80	8.95#
68.00	8.70	6.76#




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062322\
 Data File : BM035674.D
 Acq On : 24 Jun 2022 22:52
 Operator : CG/JU
 Sample : N3358-16RE
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4S9RE

Manual IntegrationsAPPROVED

Quant Time: Jun 25 04:06:34 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM061822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 20 01:56:13 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/27/2022
 Supervised By :Yogesh Patel 06/28/2022

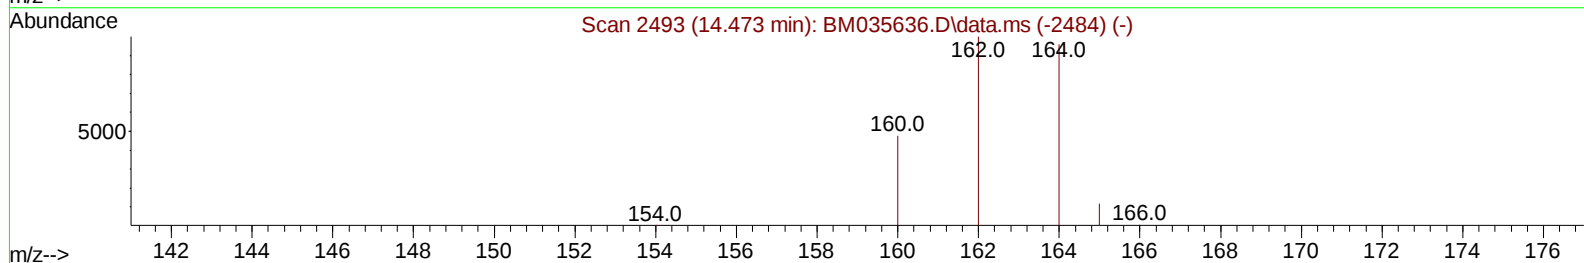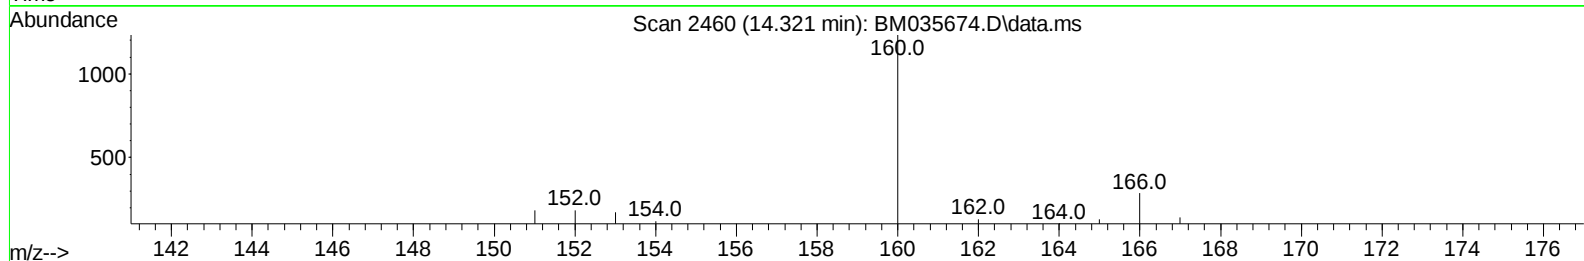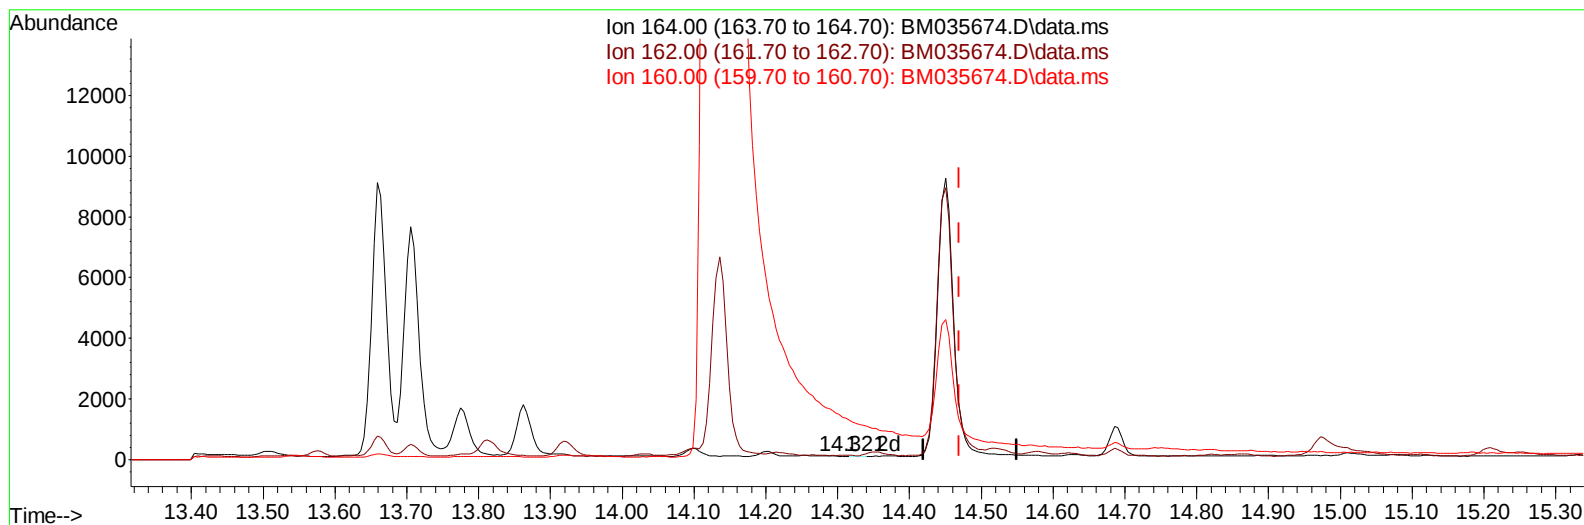

TIC: BM035674.D\data.ms

(9) Acenaphthene-d10 (I)

14.321min (-0.149) 0.40 ng/u1

response 6

Ion	Exp%	Act%
164.00	100.00	100.00
162.00	106.40	125.96
160.00	49.90	1184.62#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062322\
 Data File : BM035674.D
 Acq On : 24 Jun 2022 22:52
 Operator : CG/JU
 Sample : N3358-16RE
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4S9RE

Manual IntegrationsAPPROVED

Quant Time: Jun 25 04:06:34 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM061822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 20 01:56:13 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/27/2022
 Supervised By :Yogesh Patel 06/28/2022

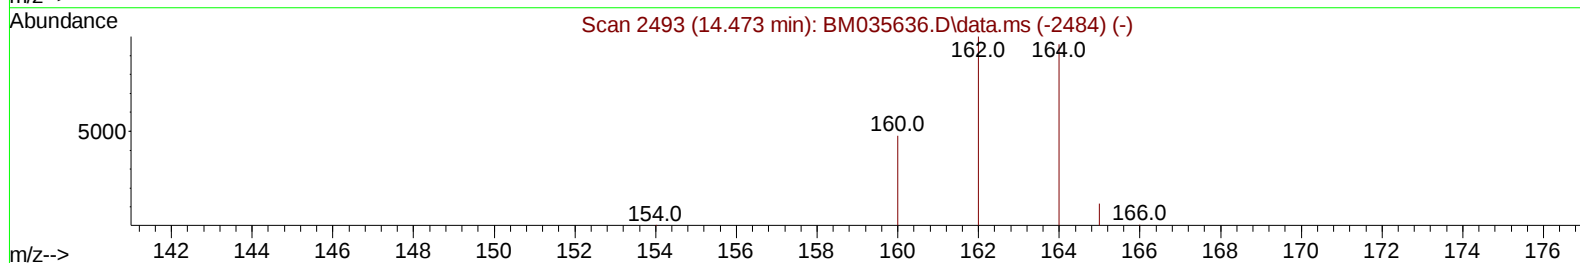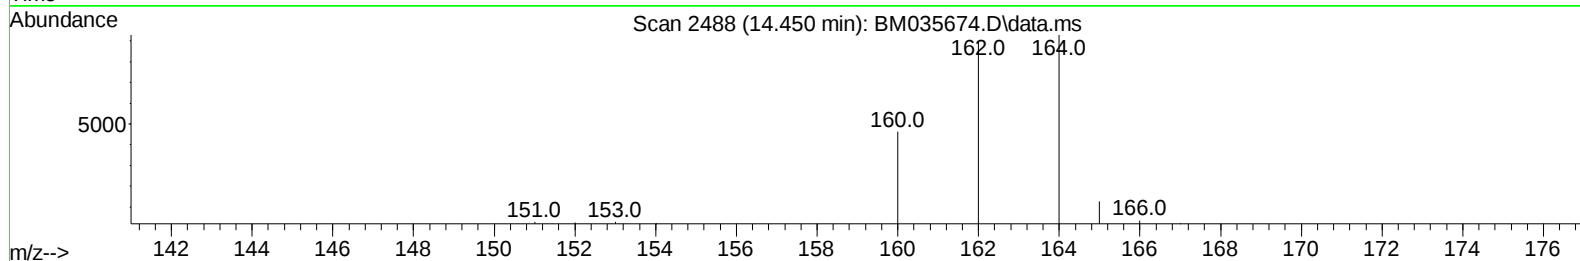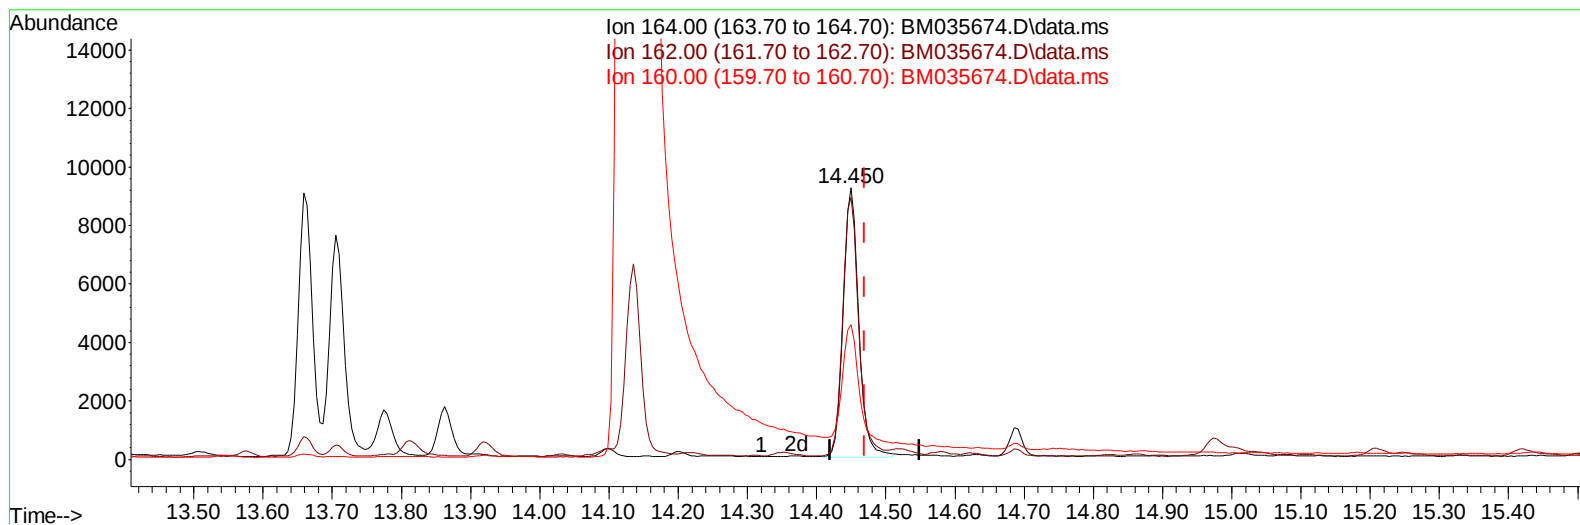

TIC: BM035674.D\data.ms

(9) Acenaphthene-d10 (I)

14.450min (-0.019) 0.40 ng/u1 m

response 14331

Ion	Exp%	Act%
164.00	100.00	100.00
162.00	106.40	96.47
160.00	49.90	49.73
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062322\
 Data File : BM035674.D
 Acq On : 24 Jun 2022 22:52
 Operator : CG/JU
 Sample : N3358-16RE
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4S9RE

Manual IntegrationsAPPROVED

Quant Time: Jun 25 04:06:34 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM061822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 20 01:56:13 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/27/2022
 Supervised By :Yogesh Patel 06/28/2022

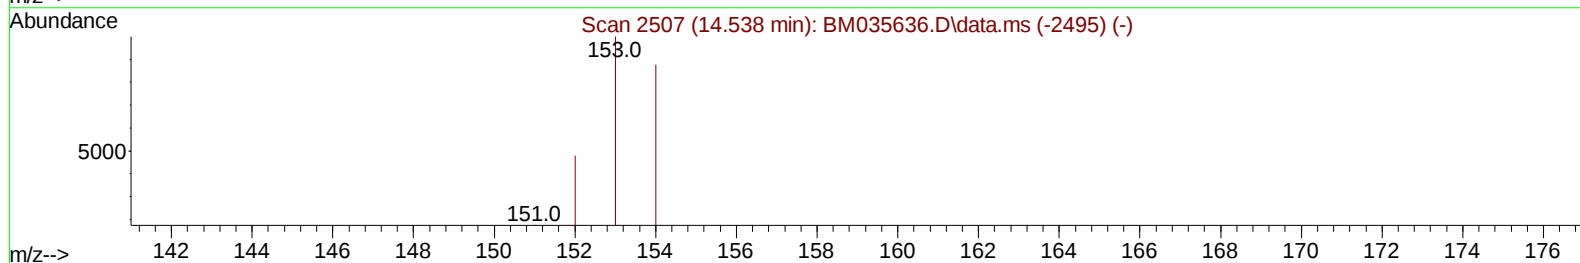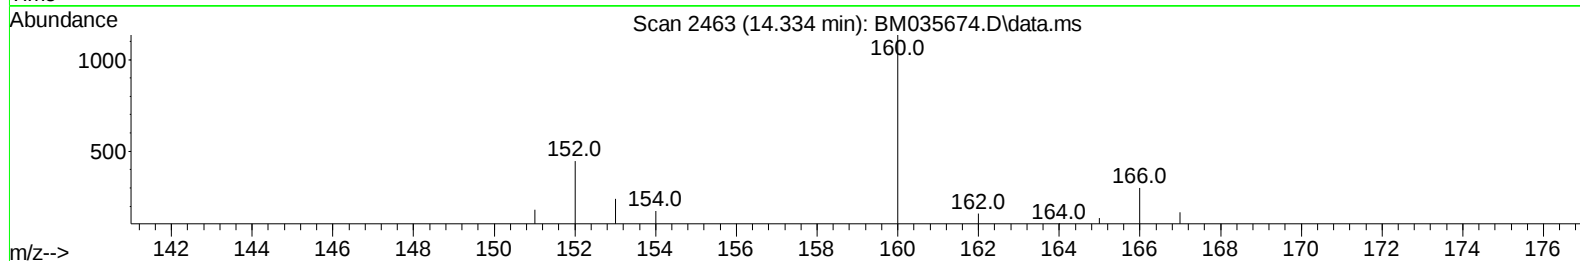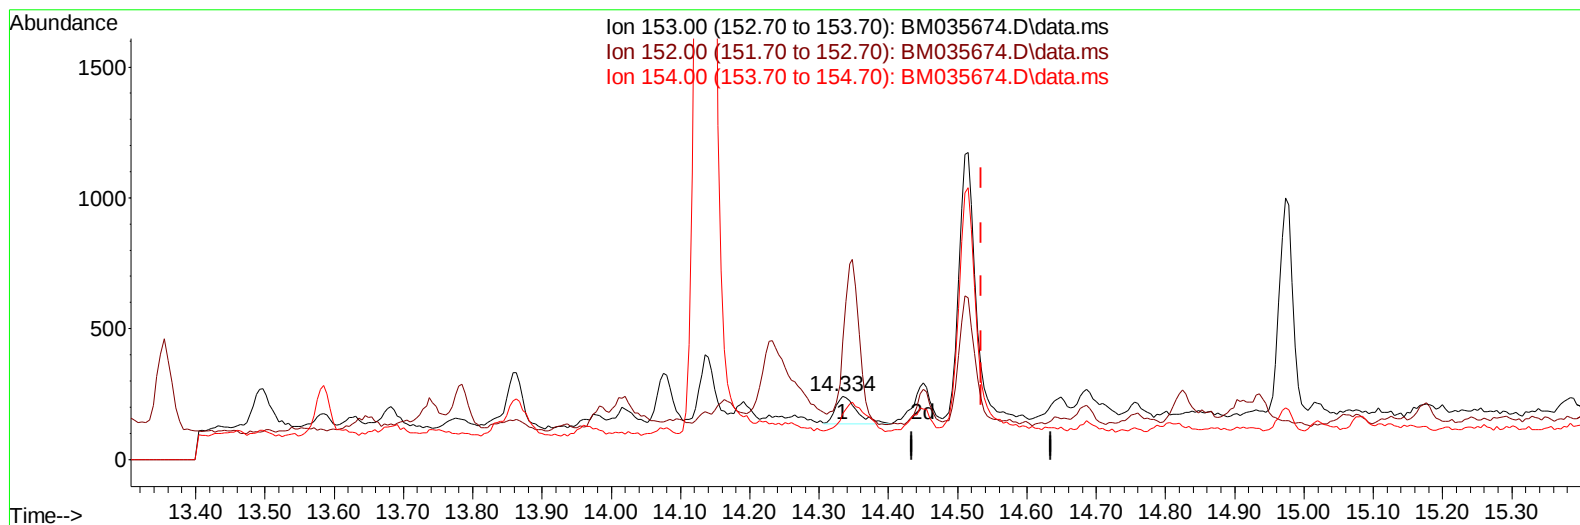

TIC: BM035674.D\data.ms

(11) Acenaphthene (C)

14.334min (-0.200) 0.00 ng/u1

response 217

Ion	Exp%	Act%
153.00	100.00	100.00
152.00	50.00	185.12#
154.00	86.40	72.31
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062322\
 Data File : BM035674.D
 Acq On : 24 Jun 2022 22:52
 Operator : CG/JU
 Sample : N3358-16RE
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4S9RE

Manual IntegrationsAPPROVED

Quant Time: Jun 25 04:06:34 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM061822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 20 01:56:13 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/27/2022
 Supervised By :Yogesh Patel 06/28/2022

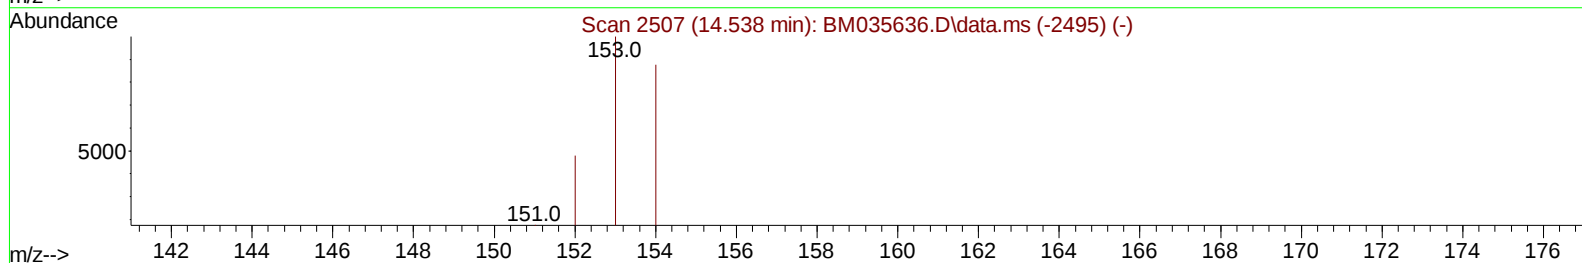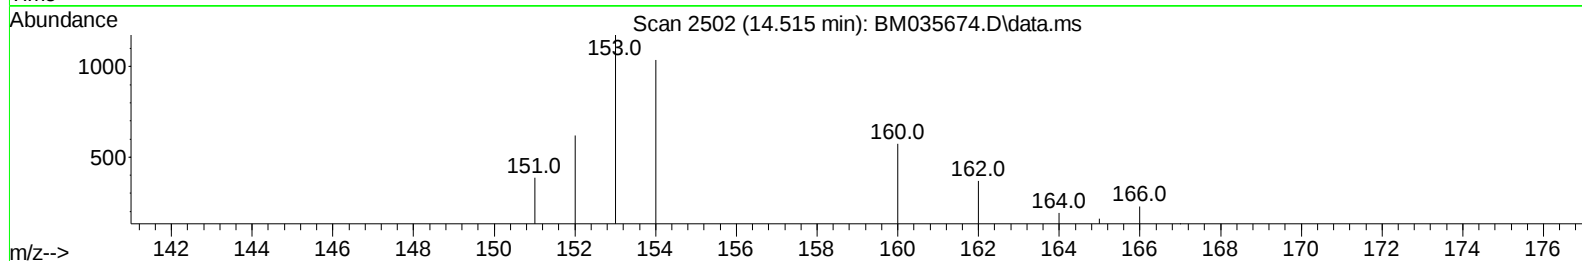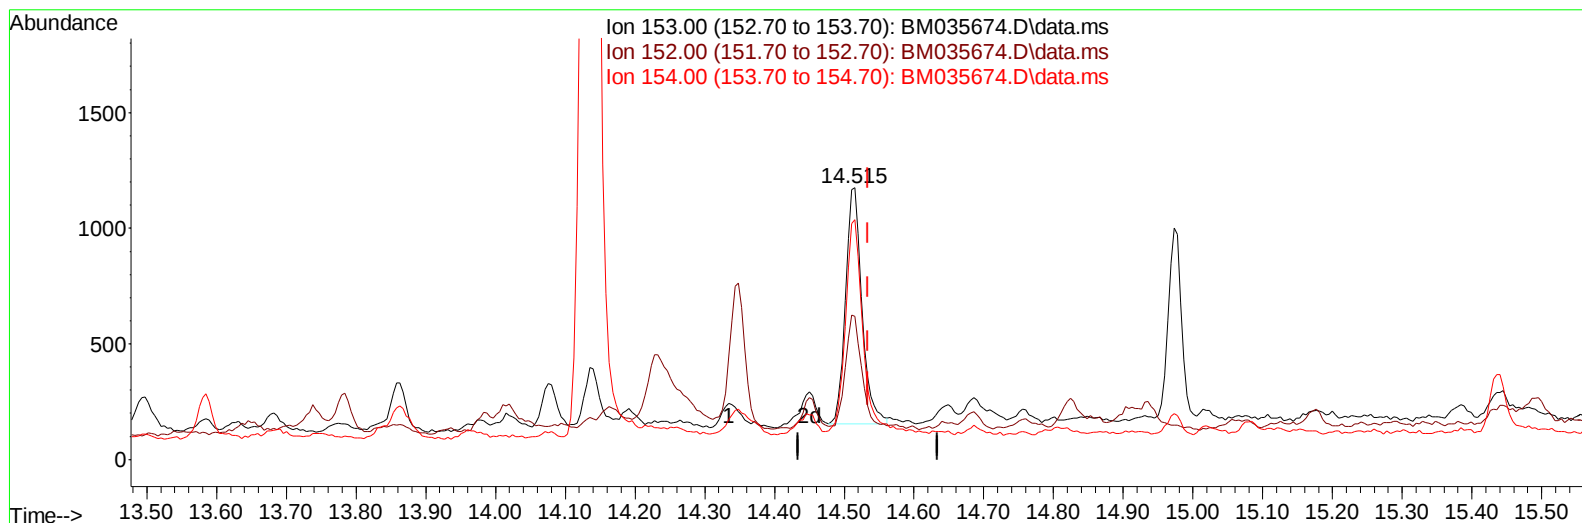

TIC: BM035674.D\data.ms

(11) Acenaphthene (C)

14.515min (-0.019) 0.03 ng/ul m

response 1681

Ion	Exp%	Act%
153.00	100.00	100.00
152.00	50.00	52.64
154.00	86.40	88.42
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062322\
 Data File : BM035674.D
 Acq On : 24 Jun 2022 22:52
 Operator : CG/JU
 Sample : N3358-16RE
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4S9RE

Manual IntegrationsAPPROVED

Quant Time: Jun 25 04:06:34 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM061822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 20 01:56:13 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/27/2022
 Supervised By :Yogesh Patel 06/28/2022

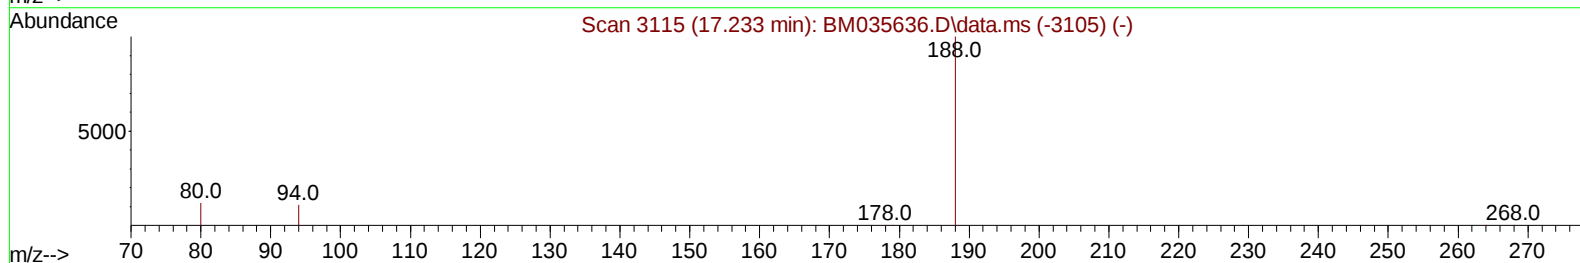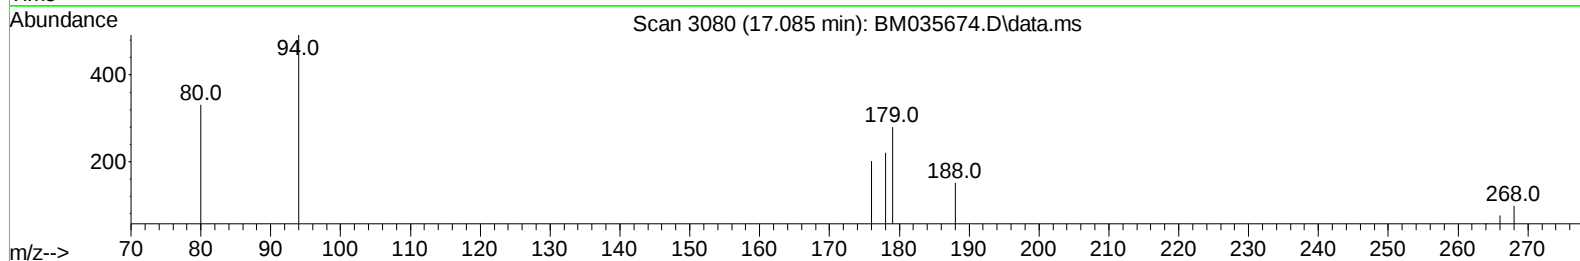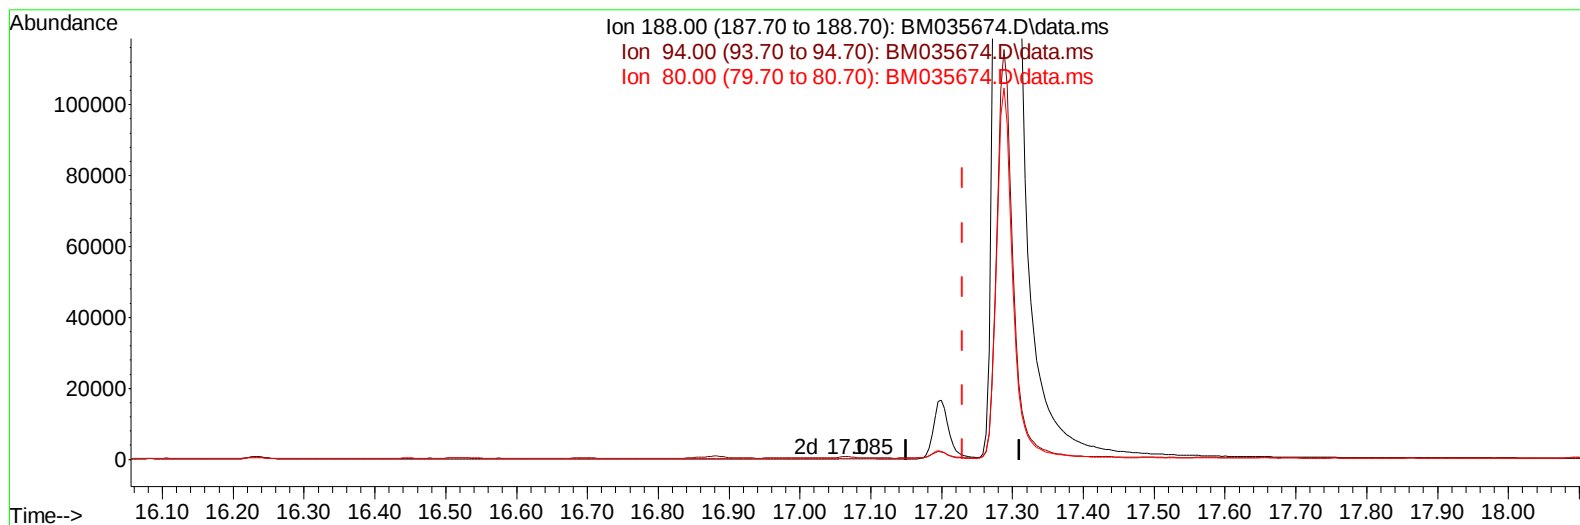

TIC: BM035674.D\data.ms

(13) Phenanthrene-d10 (I)

17.085min (-0.144) 0.40 ng/u1

response 64

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	12.00	325.83#
80.00	13.50	219.21#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062322\
Data File : BM035674.D
Acq On : 24 Jun 2022 22:52
Operator : CG/JU
Sample : N3358-16RE
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4S9RE

Manual IntegrationsAPPROVED

Quant Time: Jun 25 04:06:34 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM061822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 20 01:56:13 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/27/2022
Supervised By :Yogesh Patel 06/28/2022

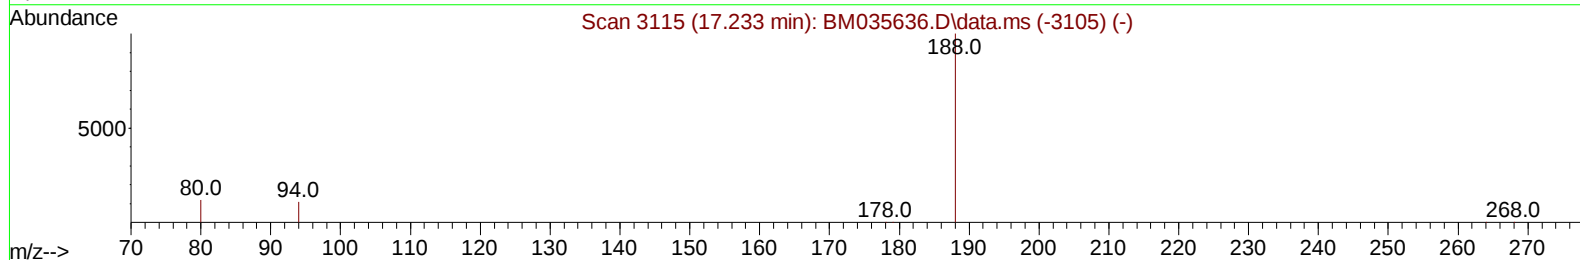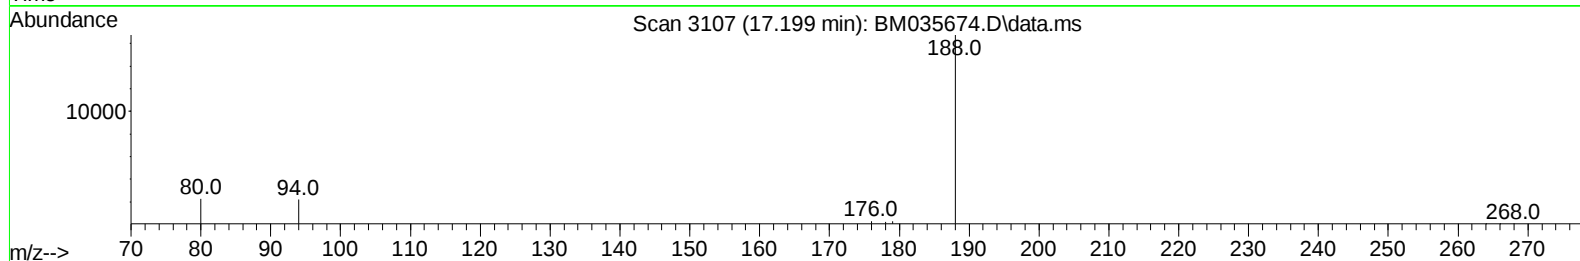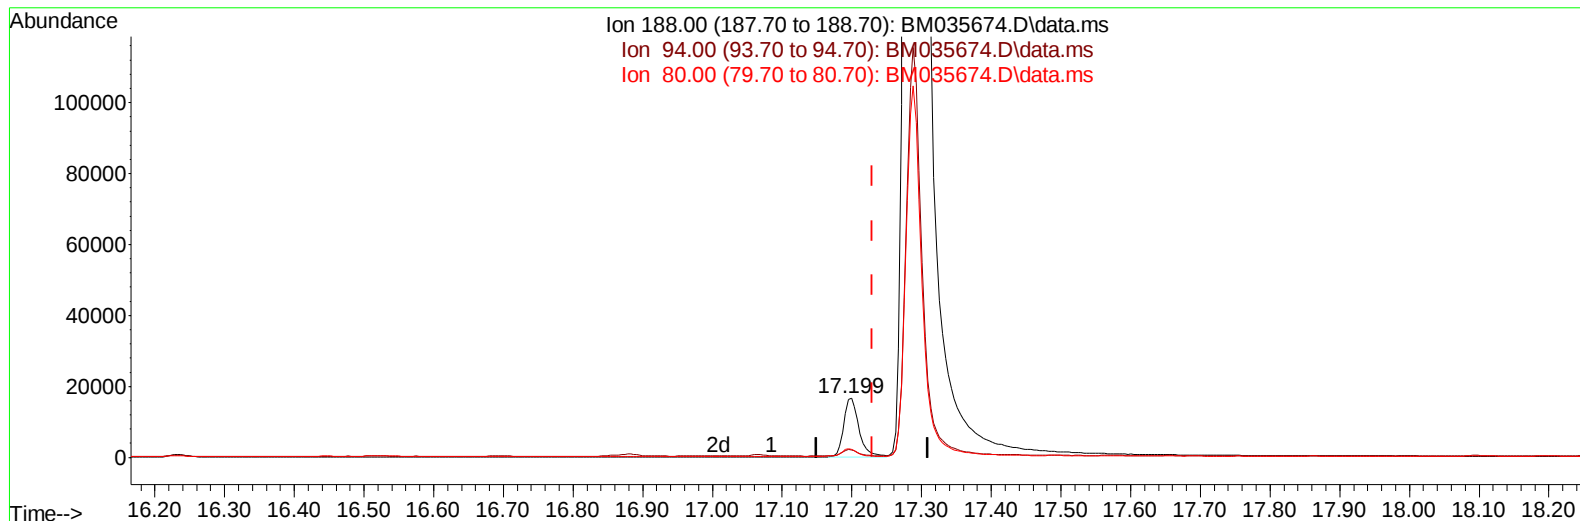

TIC: BM035674.D\data.ms

(13) Phenanthrene-d10 (I)

17.199min (-0.030) 0.40 ng/u1 m

response 25113

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	12.00	13.02
80.00	13.50	13.63
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062322\
 Data File : BM035674.D
 Acq On : 24 Jun 2022 22:52
 Operator : CG/JU
 Sample : N3358-16RE
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4S9RE

Manual IntegrationsAPPROVED

Quant Time: Jun 25 04:06:34 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM061822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 20 01:56:13 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/27/2022
 Supervised By :Yogesh Patel 06/28/2022

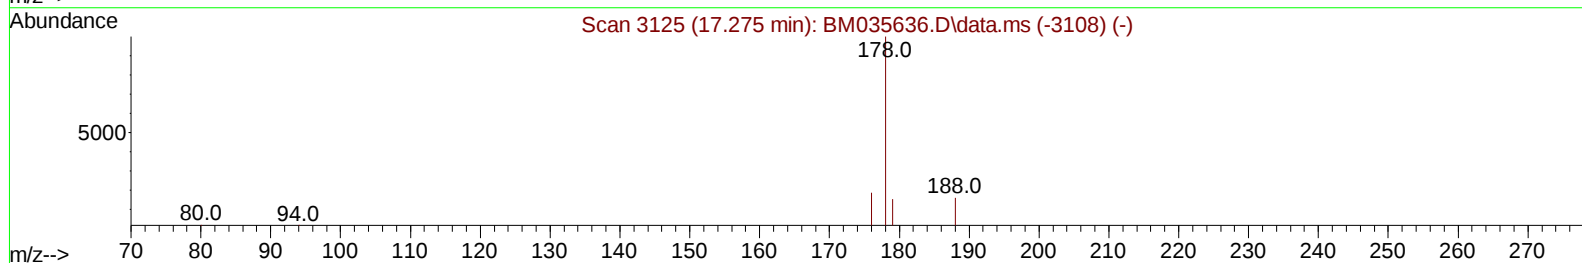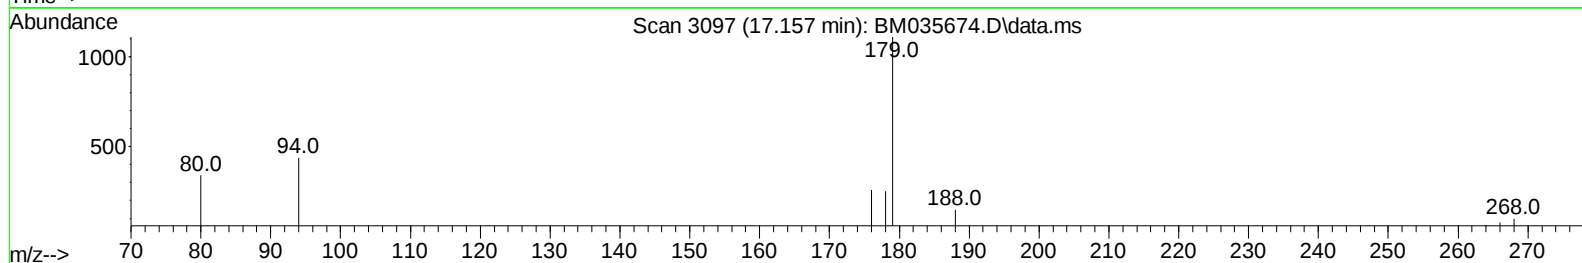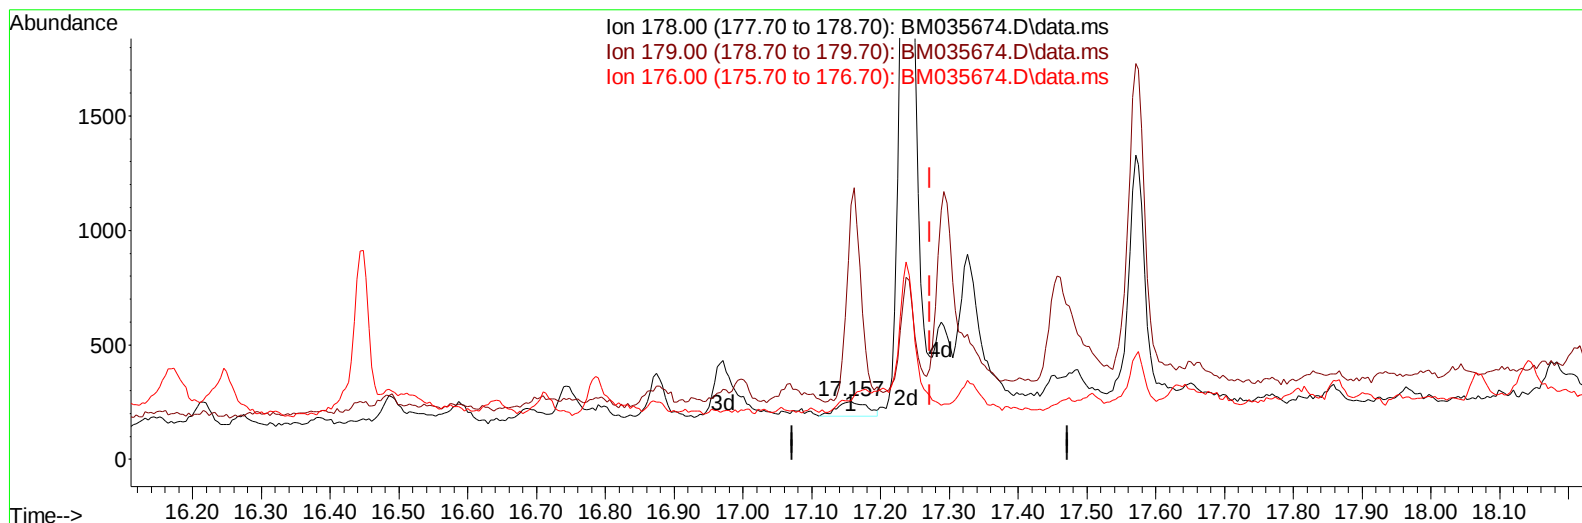

TIC: BM035674.D\data.ms

(15) Phenanthrene

17.157min (-0.115) 0.00 ng/u1

response 193

Ion	Exp%	Act%
178.00	100.00	100.00
179.00	16.50	438.74#
176.00	20.30	101.58#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062322\
 Data File : BM035674.D
 Acq On : 24 Jun 2022 22:52
 Operator : CG/JU
 Sample : N3358-16RE
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4S9RE

Manual IntegrationsAPPROVED

Quant Time: Jun 25 04:06:34 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM061822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 20 01:56:13 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/27/2022
 Supervised By :Yogesh Patel 06/28/2022

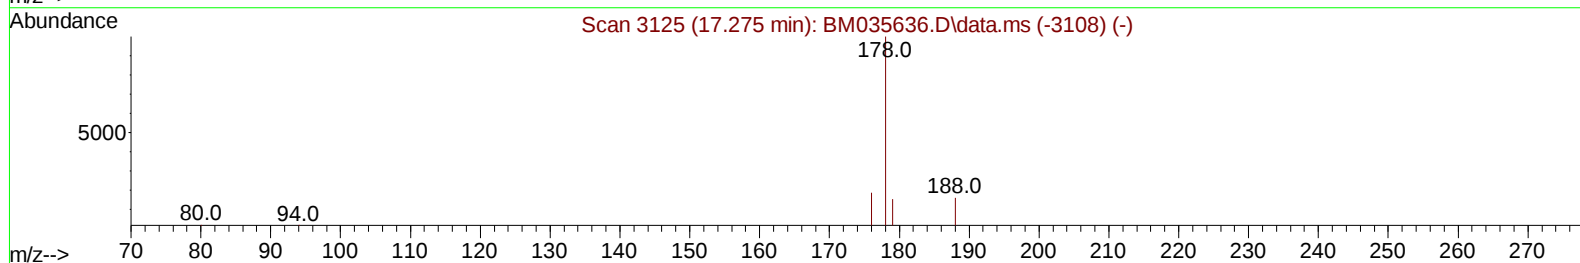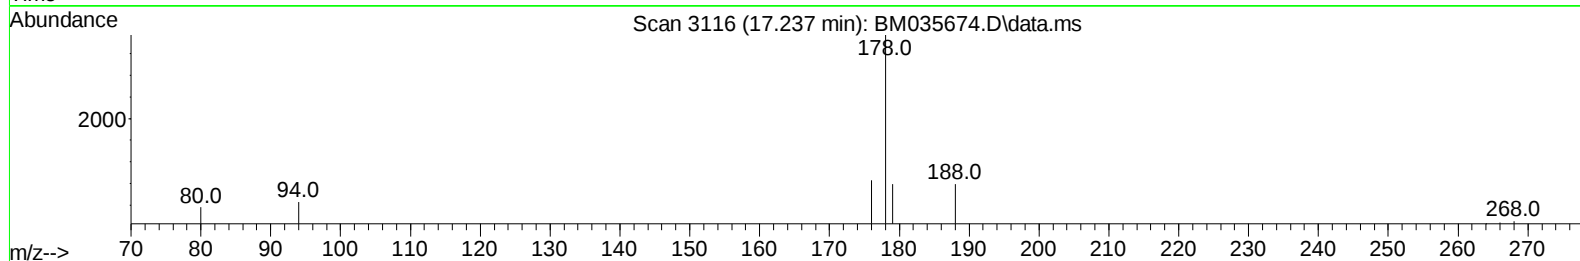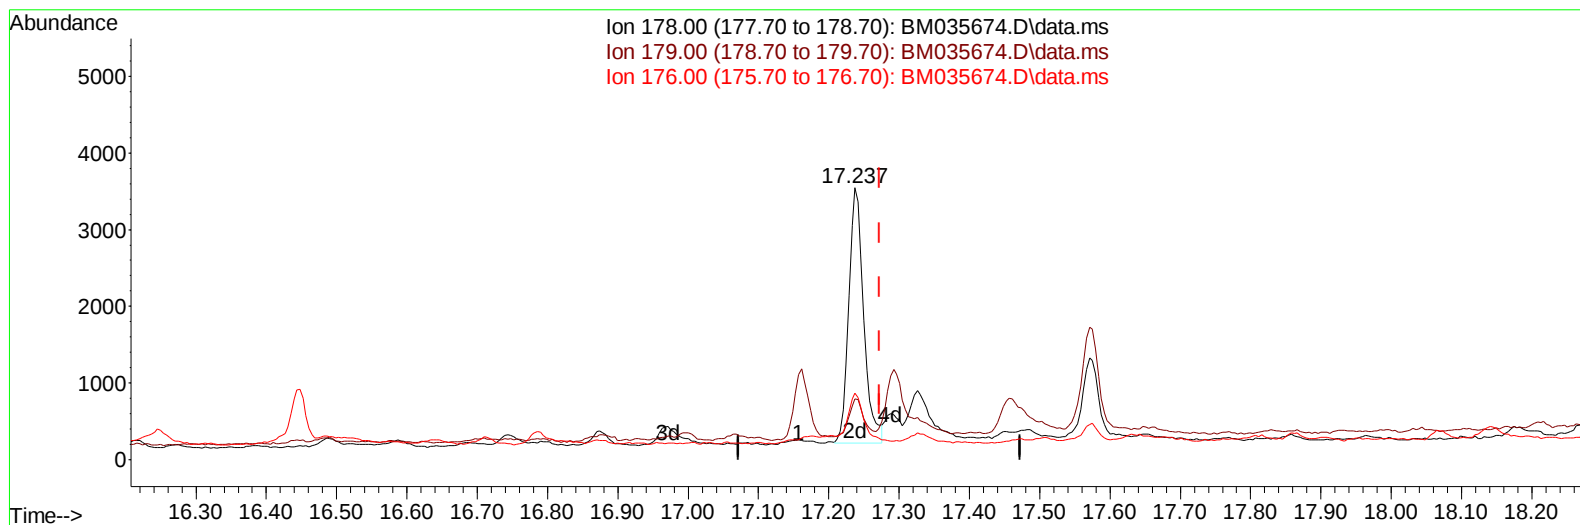

TIC: BM035674.D\data.ms

(15) Phenanthrene

17.237min (-0.035) 0.05 ng/u1 m

response 4964

Ion	Exp%	Act%
178.00	100.00	100.00
179.00	16.50	22.40#
176.00	20.30	24.34
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062322\
 Data File : BM035674.D
 Acq On : 24 Jun 2022 22:52
 Operator : CG/JU
 Sample : N3358-16RE
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4S9RE

Manual IntegrationsAPPROVED

Quant Time: Jun 25 04:06:34 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM061822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 20 01:56:13 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/27/2022
 Supervised By :Yogesh Patel 06/28/2022

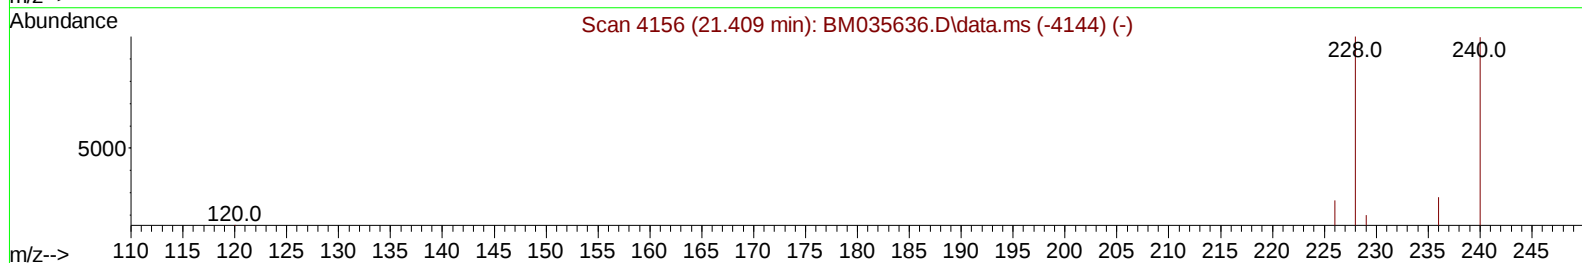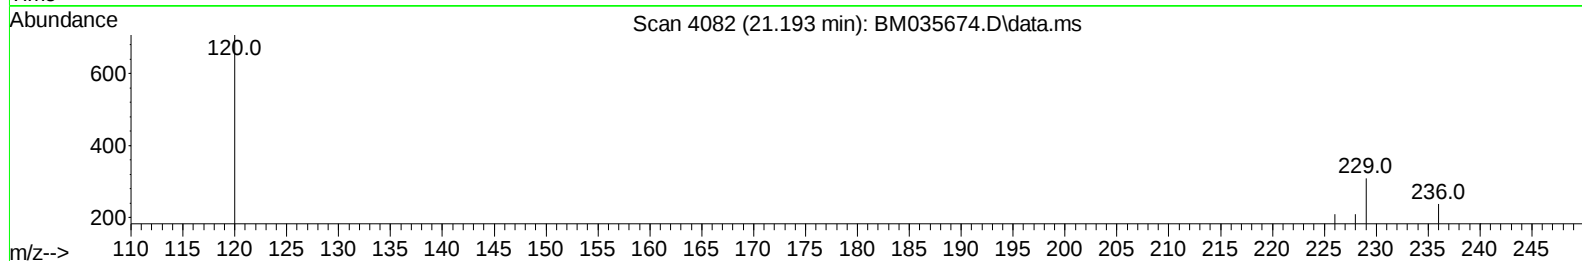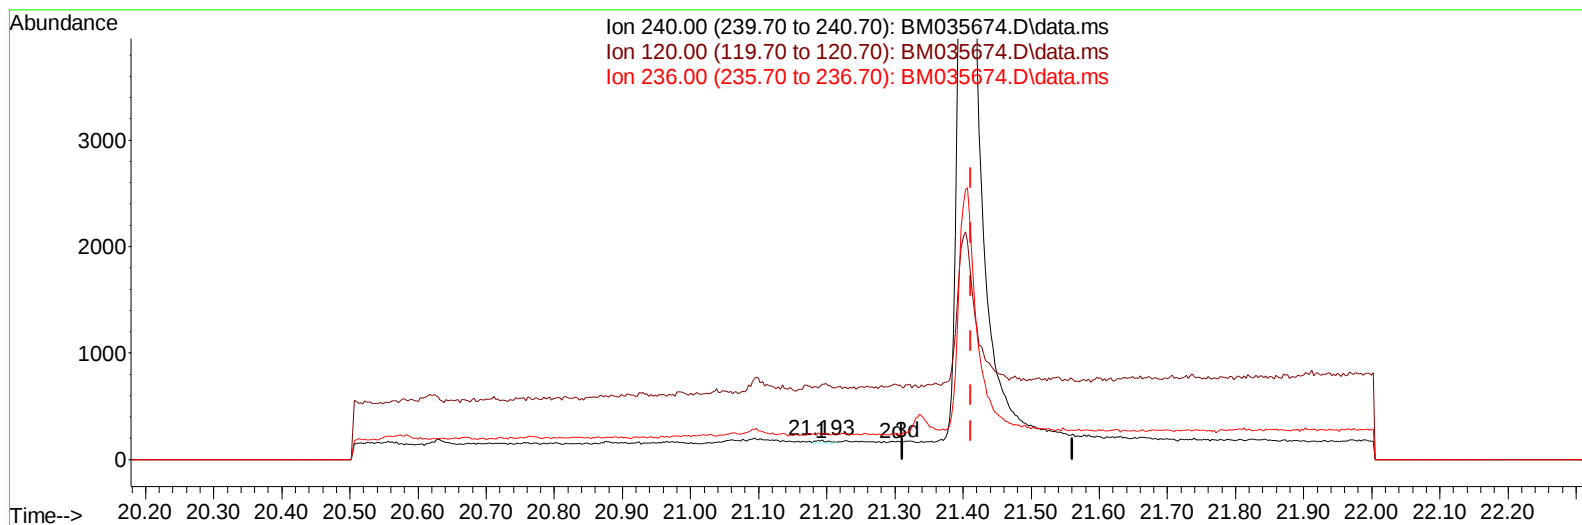

TIC: BM035674.D\data.ms

(17) Chrysene-d12

21.193min (-0.218) 0.40 ng/u1

response 31

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	22.80	386.34#
236.00	30.40	130.60#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062322\
Data File : BM035674.D
Acq On : 24 Jun 2022 22:52
Operator : CG/JU
Sample : N3358-16RE
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4S9RE

Manual IntegrationsAPPROVED

Quant Time: Jun 25 04:06:34 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM061822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 20 01:56:13 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/27/2022
Supervised By :Yogesh Patel 06/28/2022

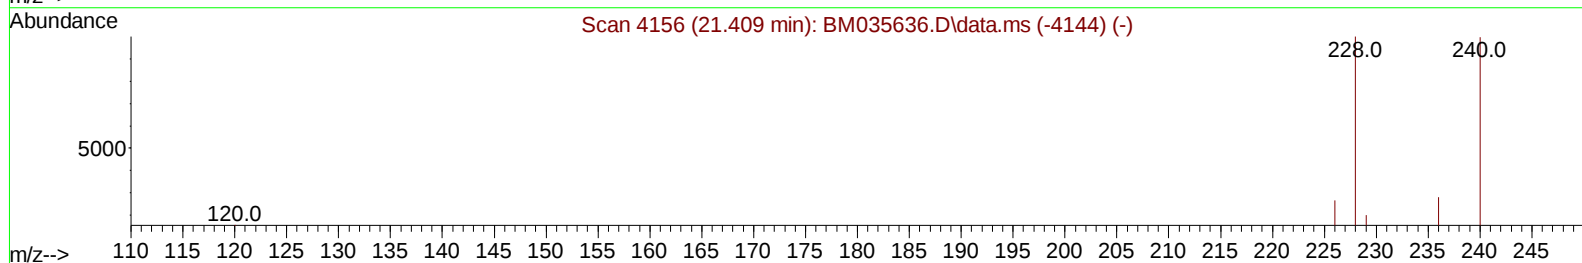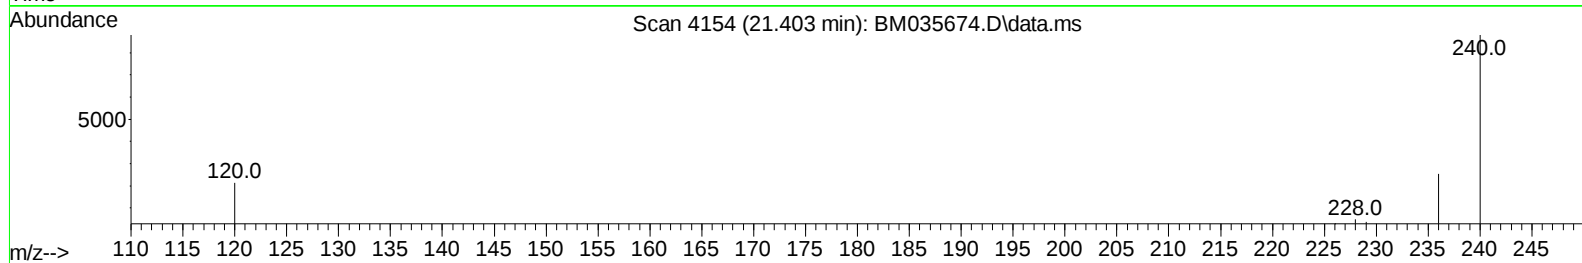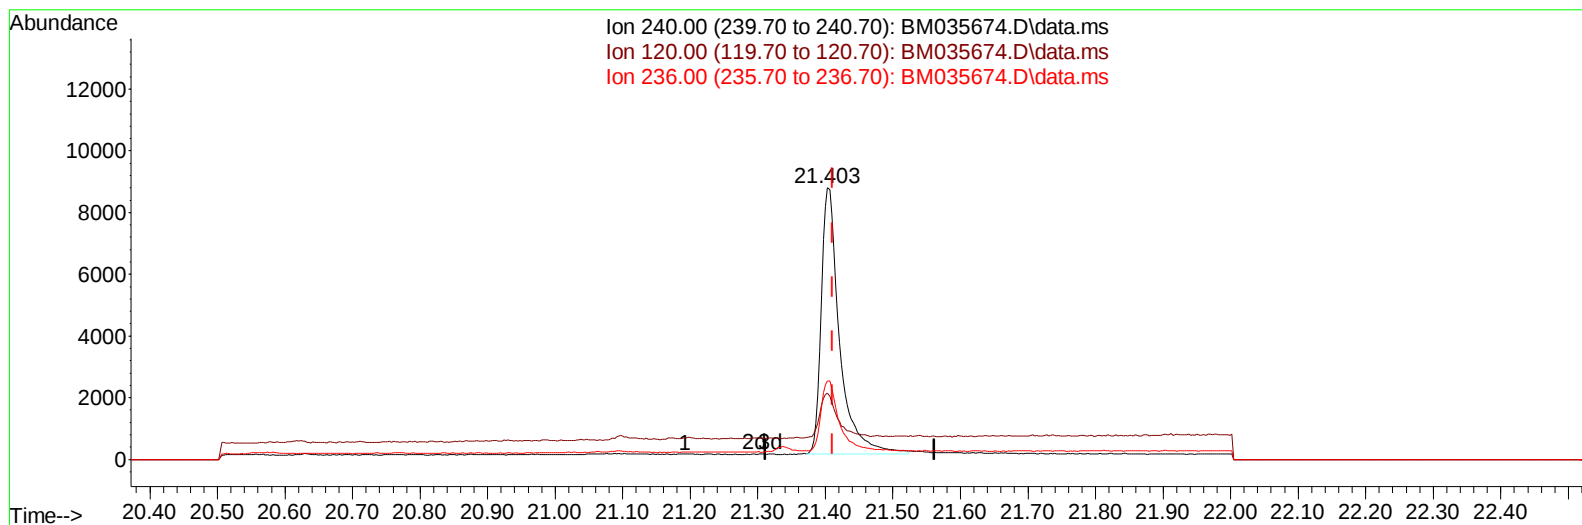

TIC: BM035674.D\data.ms

(17) Chrysene-d12

21.403min (-0.008) 0.40 ng/ul m

response 16194

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	22.80	24.32
236.00	30.40	28.79
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062322\
 Data File : BM035674.D
 Acq On : 24 Jun 2022 22:52
 Operator : CG/JU
 Sample : N3358-16RE
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4S9RE

Manual IntegrationsAPPROVED

Quant Time: Jun 25 04:06:34 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM061822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 20 01:56:13 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/27/2022
 Supervised By :Yogesh Patel 06/28/2022

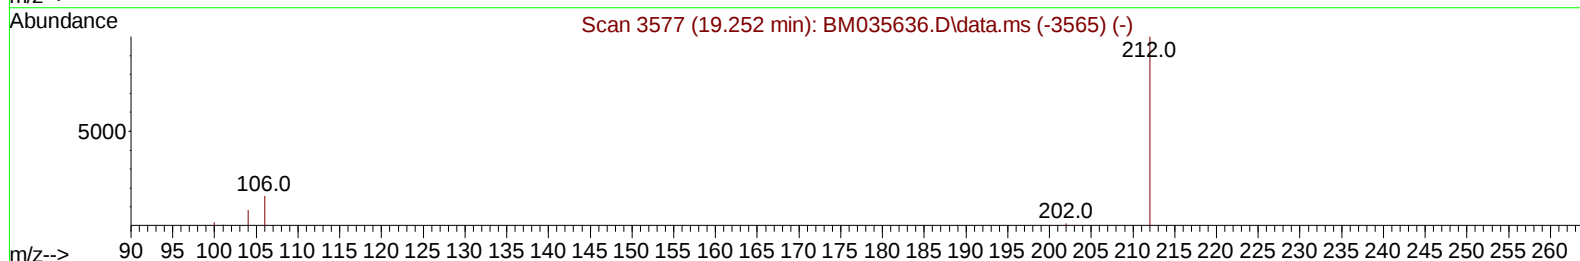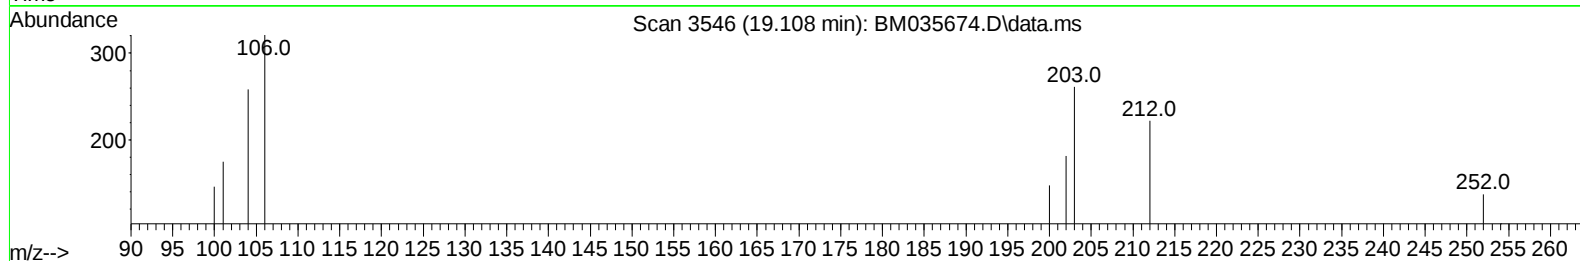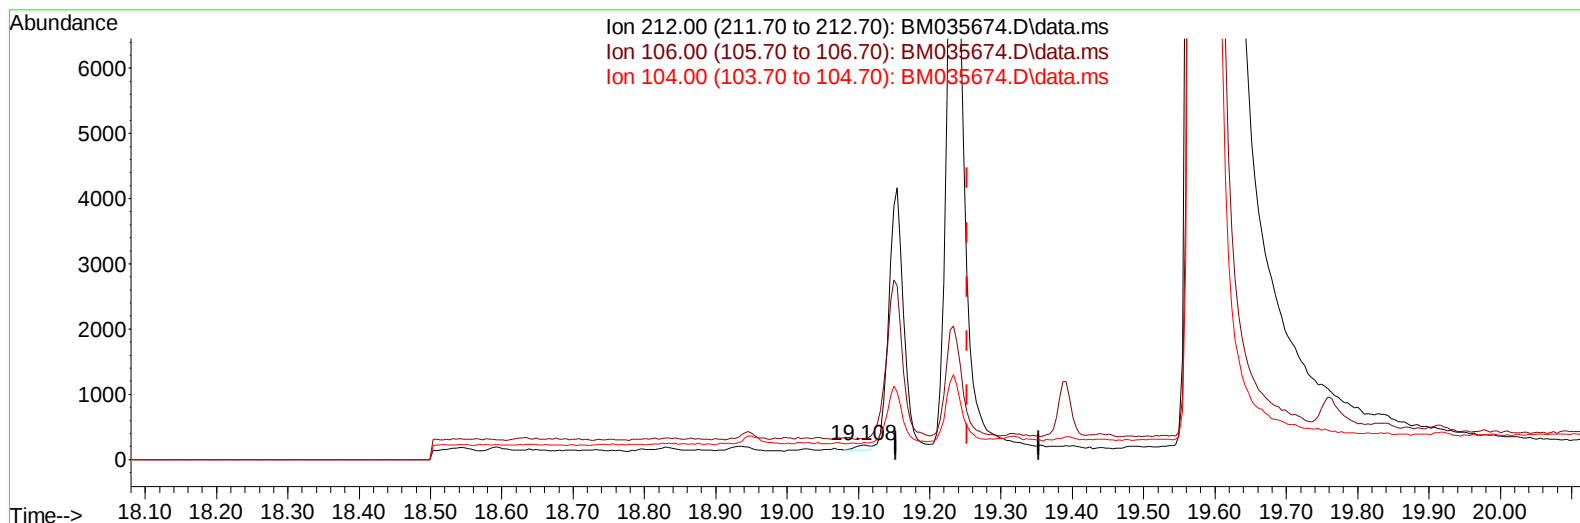

TIC: BM035674.D\data.ms

(18) Fluoranthene-d10 (SURR)

19.108min (-0.145) 0.00 ng/u1

response 123

Ion	Exp%	Act%
212.00	100.00	100.00
106.00	17.00	0.00#
104.00	9.90	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062322\
 Data File : BM035674.D
 Acq On : 24 Jun 2022 22:52
 Operator : CG/JU
 Sample : N3358-16RE
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4S9RE

Manual IntegrationsAPPROVED

Quant Time: Jun 25 04:06:34 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM061822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 20 01:56:13 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/27/2022
 Supervised By :Yogesh Patel 06/28/2022

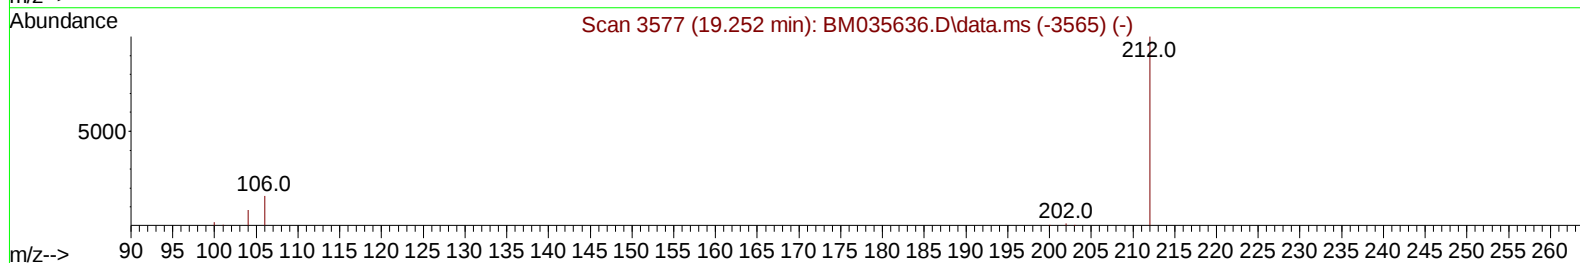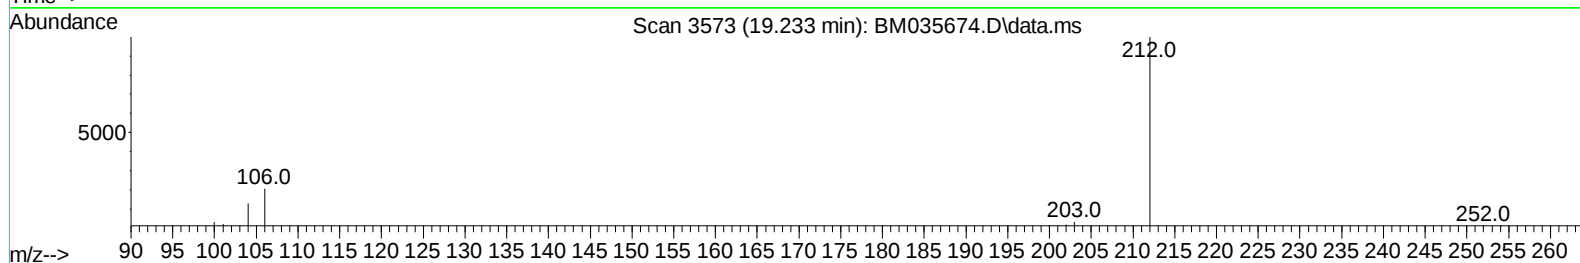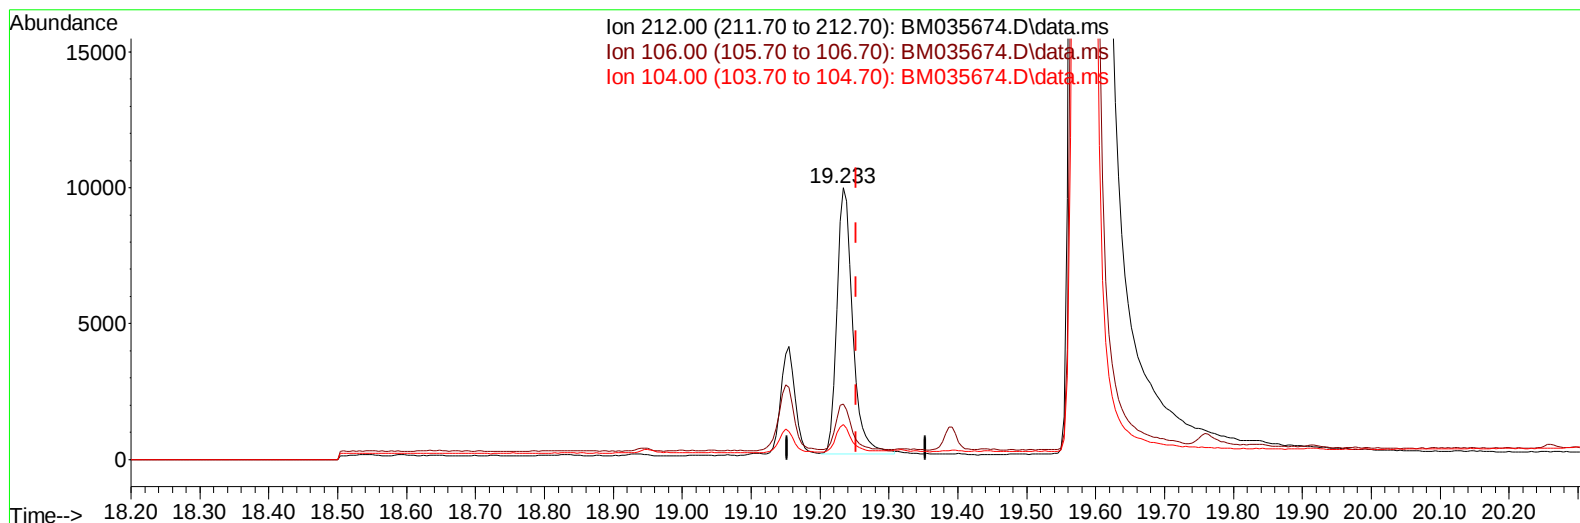

TIC: BM035674.D\data.ms

(18) Fluoranthene-d10 (SURR)

19.233min (-0.020) 0.29 ng/ul m

response 15627

Ion	Exp%	Act%
212.00	100.00	100.00
106.00	17.00	0.00#
104.00	9.90	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062322\
 Data File : BM035674.D
 Acq On : 24 Jun 2022 22:52
 Operator : CG/JU
 Sample : N3358-16RE
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4S9RE

Manual IntegrationsAPPROVED

Quant Time: Jun 25 04:06:34 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM061822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 20 01:56:13 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/27/2022
 Supervised By :Yogesh Patel 06/28/2022

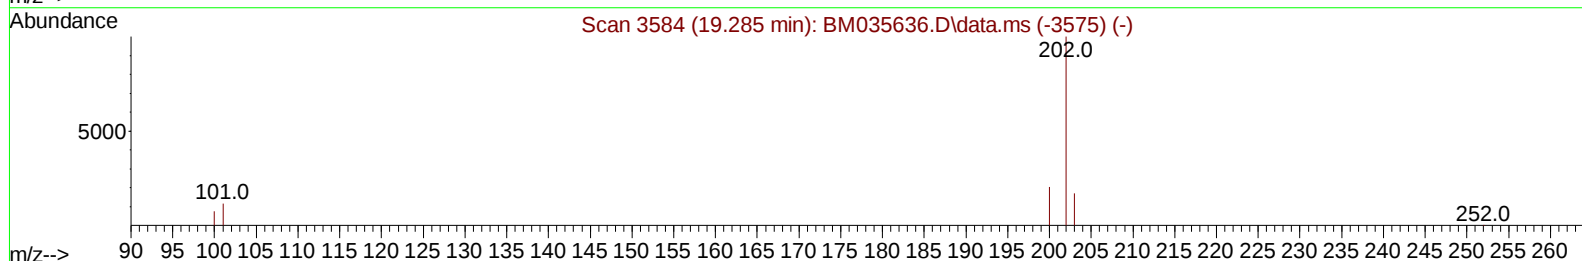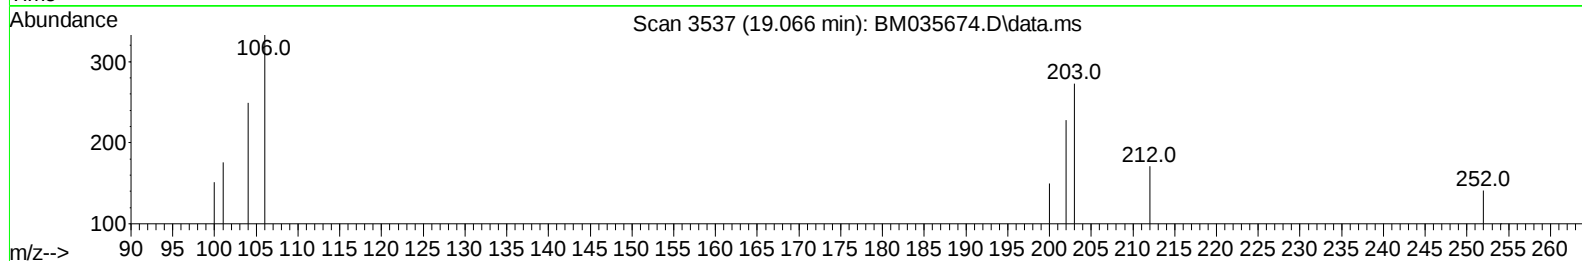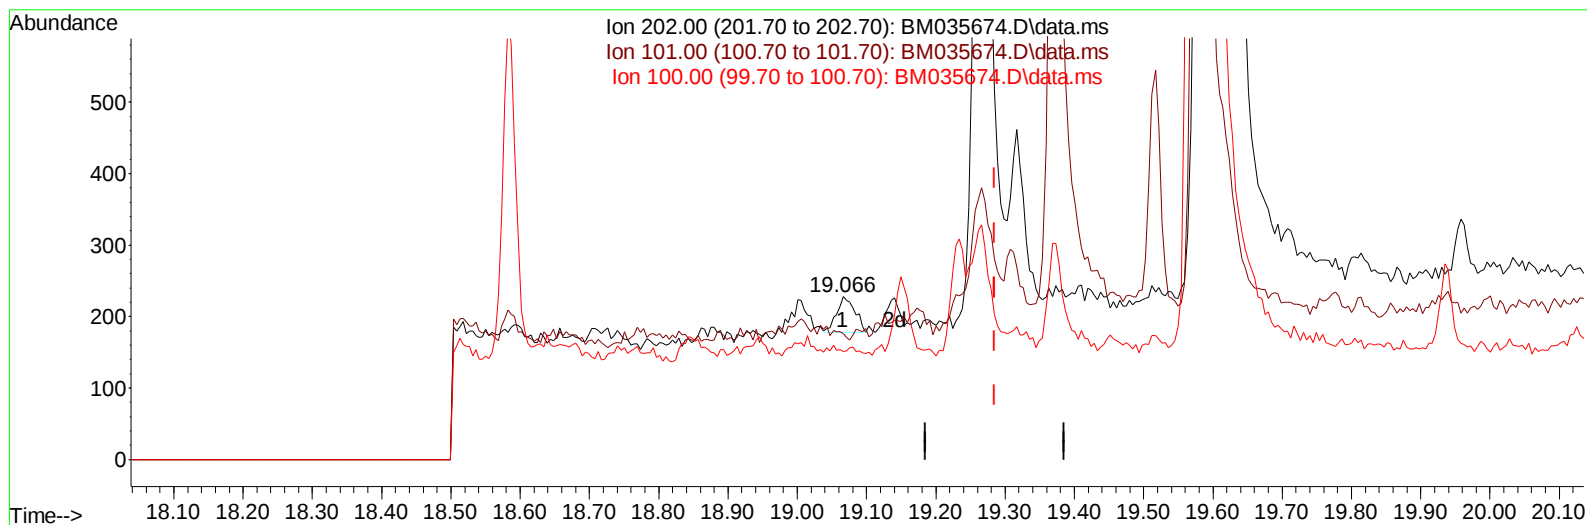

TIC: BM035674.D\data.ms

(19) Fluoranthene (C)

19.066min (-0.219) 0.00 ng/u1

response 90

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	12.50	77.19#
100.00	9.40	66.23#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062322\
 Data File : BM035674.D
 Acq On : 24 Jun 2022 22:52
 Operator : CG/JU
 Sample : N3358-16RE
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4S9RE

Manual IntegrationsAPPROVED

Quant Time: Jun 25 04:06:34 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM061822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 20 01:56:13 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/27/2022
 Supervised By :Yogesh Patel 06/28/2022

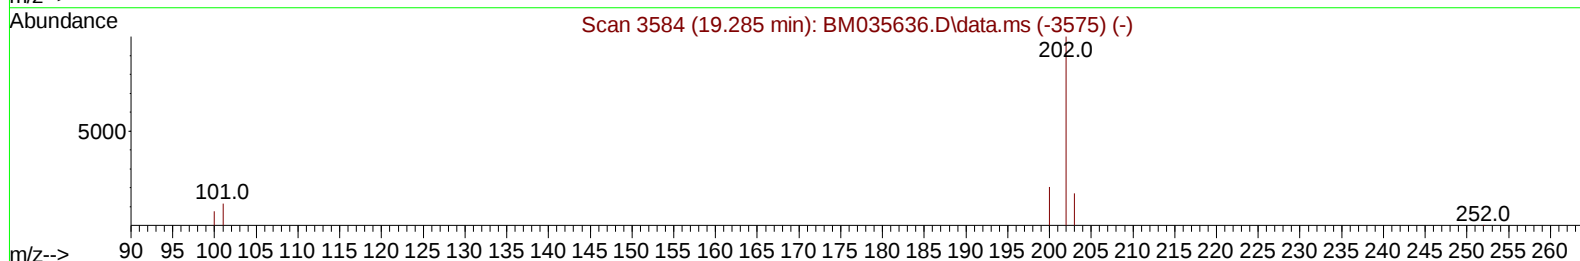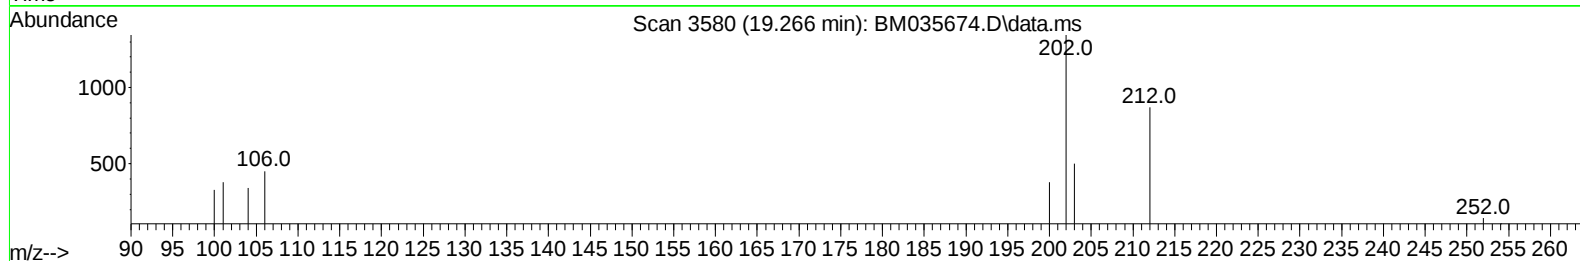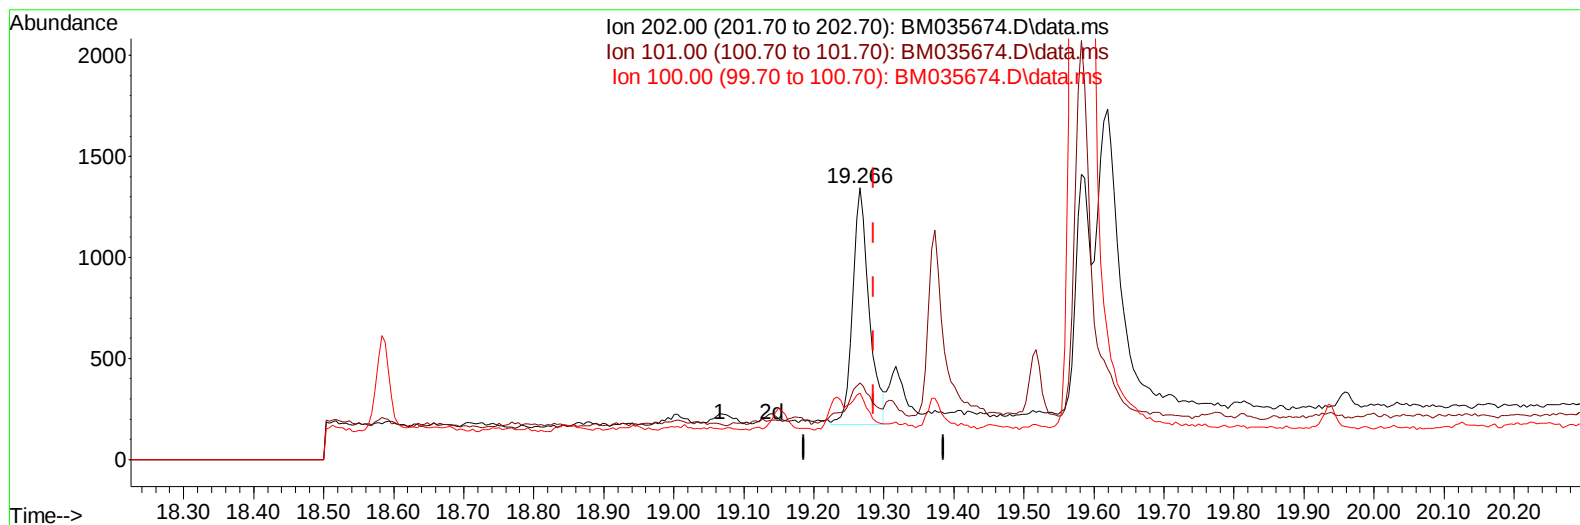

TIC: BM035674.D\data.ms

(19) Fluoranthene (C)

19.266min (-0.020) 0.02 ng/u1 m

response 1927

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	12.50	28.27#
100.00	9.40	24.40#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062322\
 Data File : BM035674.D
 Acq On : 24 Jun 2022 22:52
 Operator : CG/JU
 Sample : N3358-16RE
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4S9RE

Manual IntegrationsAPPROVED

Quant Time: Jun 25 04:06:34 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM061822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 20 01:56:13 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/27/2022
 Supervised By :Yogesh Patel 06/28/2022

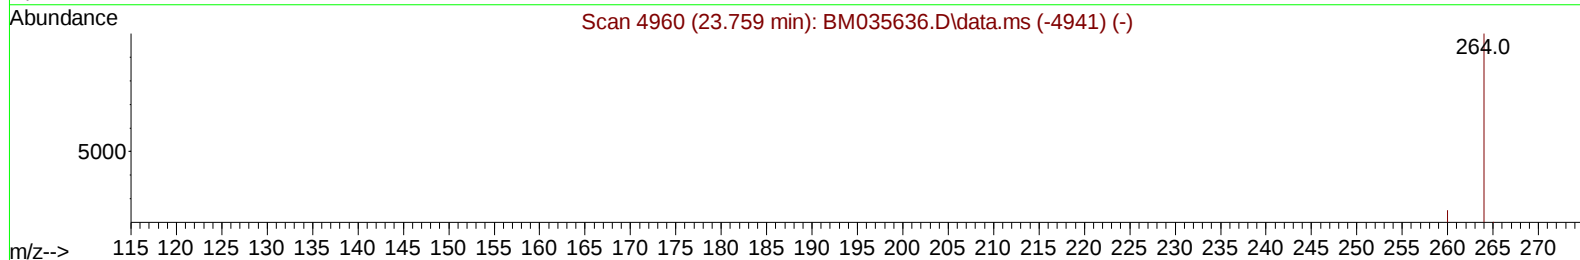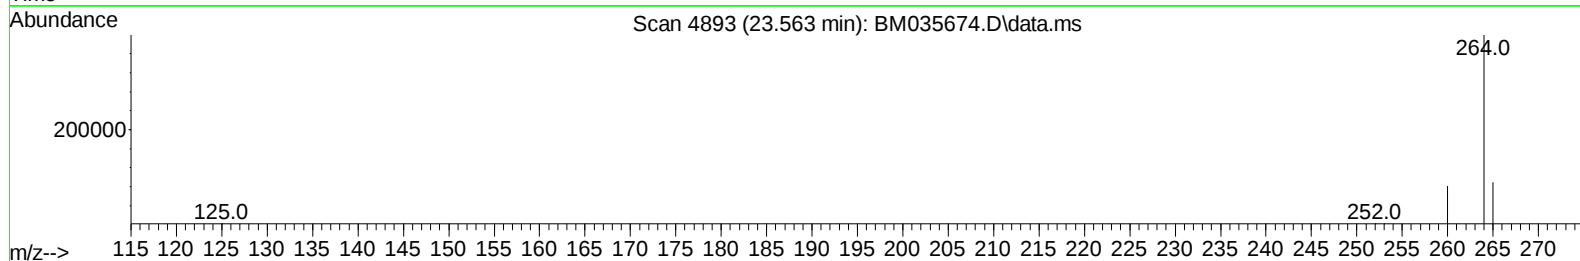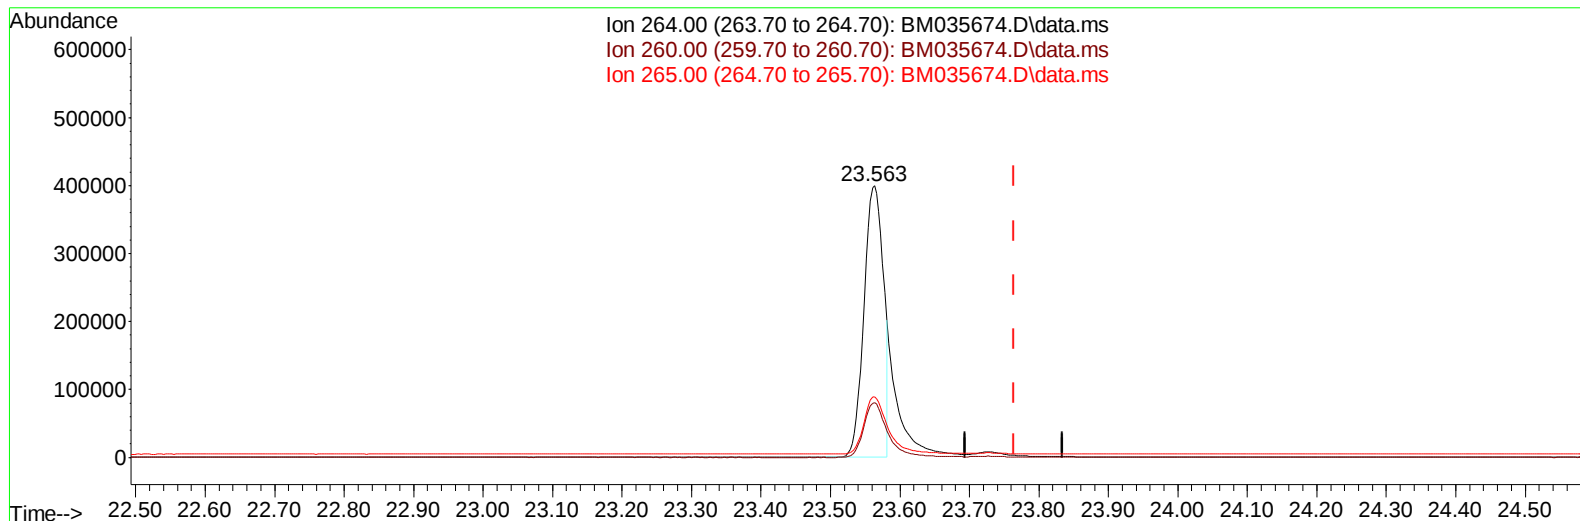

TIC: BM035674.D\data.ms

(23) Perylene-d12 (I)

23.563min (-0.201) 0.40 ng/u1

response 767937

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.30	20.24#
265.00	123.50	22.23#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062322\
 Data File : BM035674.D
 Acq On : 24 Jun 2022 22:52
 Operator : CG/JU
 Sample : N3358-16RE
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4S9RE

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 06/27/2022
 Supervised By :Yogesh Patel 06/28/2022

Quant Time: Jun 25 04:06:34 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM061822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 20 01:56:13 2022
 Response via : Initial Calibration

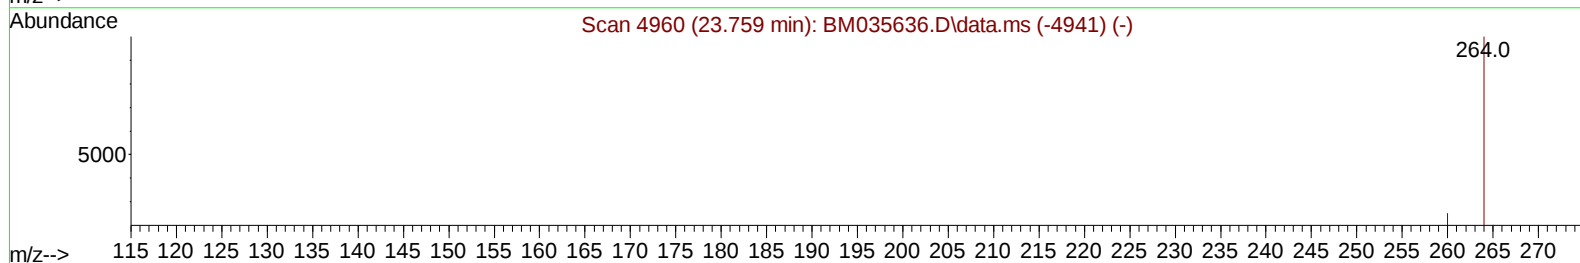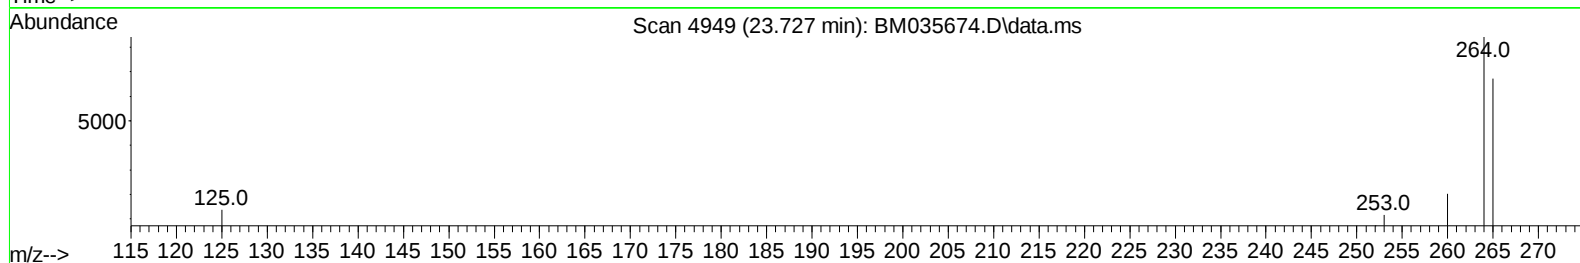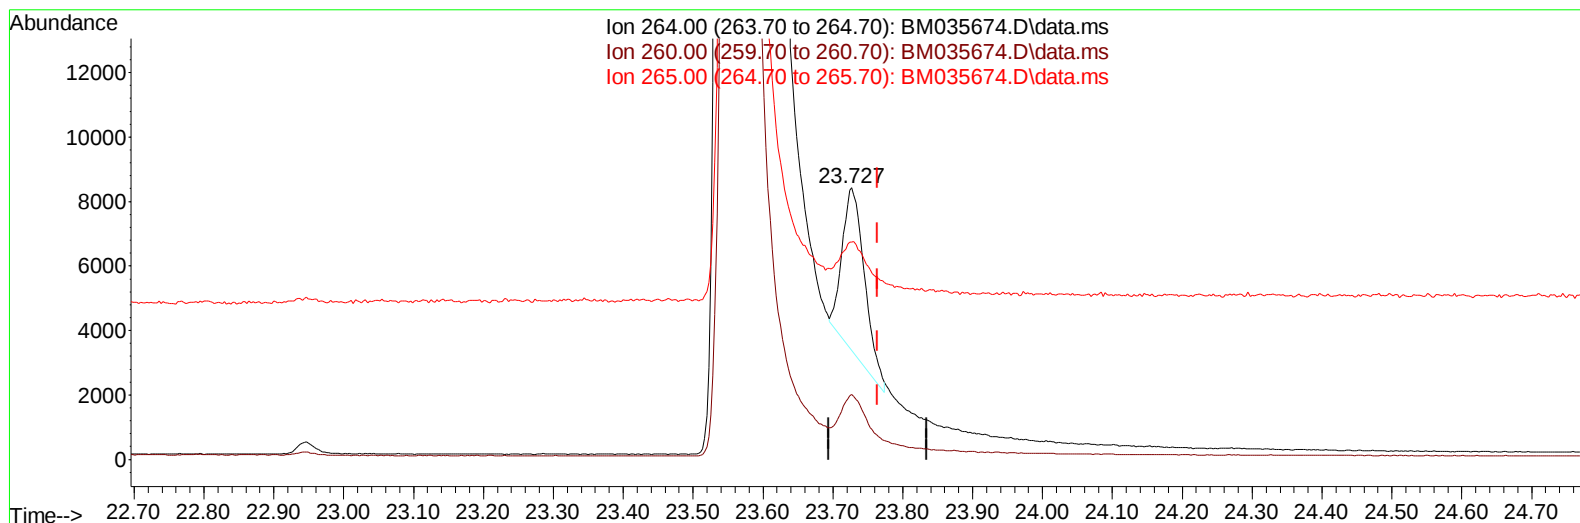

TIC: BM035674.D\data.ms

(23) Perylene-d12 (I)

23.727min (-0.037) 0.40 ng/ul m

response 11057

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.30	24.02
265.00	123.50	79.95#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062322\
 Data File : BM035674.D
 Acq On : 24 Jun 2022 22:52
 Operator : CG/JU
 Sample : N3358-16RE
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4S9RE

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 06/27/2022
 Supervised By :Yogesh Patel 06/28/2022

Quant Time: Jun 25 04:06:34 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM061822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 20 01:56:13 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.825	152		5727	0.400	ng/ul	-0.03
4) Naphthalene-d8	10.600	136		22666m	0.400	ng/ul	-0.04
9) Acenaphthene-d10	14.450	164		14331m	0.400	ng/ul	-0.02
13) Phenanthrene-d10	17.199	188		25113m	0.400	ng/ul	-0.03
17) Chrysene-d12	21.403	240		16194m	0.400	ng/ul	0.00
23) Perylene-d12	23.727	264		11057m	0.400	ng/ul	-0.04
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.264	96		29713	3.687	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.206	152		7295	0.217	ng/ul	-0.04
18) Fluoranthene-d10	19.233	212		15627m	0.287	ng/ul	-0.02
Target Compounds							Qvalue
5) Naphthalene	10.655	128		7190	0.094	ng/ul	98
11) Acenaphthene	14.515	153		1681m	0.028	ng/ul	
15) Phenanthrene	17.237	178		4964m	0.054	ng/ul	
19) Fluoranthene	19.266	202		1927m	0.023	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062322\
Data File : BM035674.D
Acq On : 24 Jun 2022 22:52
Operator : CG/JU
Sample : N3358-16RE
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4S9RE

Manual IntegrationsAPPROVED

Quant Time: Jun 25 04:06:34 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM061822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 20 01:56:13 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/27/2022
Supervised By :Yogesh Patel 06/28/2022

