




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062322\
 Data File : BM035677.D
 Acq On : 25 Jun 2022 00:42
 Operator : CG/JU
 Sample : N3359-11RE
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4S5RE

Manual IntegrationsAPPROVED

Quant Time: Jul 01 04:11:04 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM061822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 20 01:56:13 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/27/2022
 Supervised By :Yogesh Patel 06/28/2022

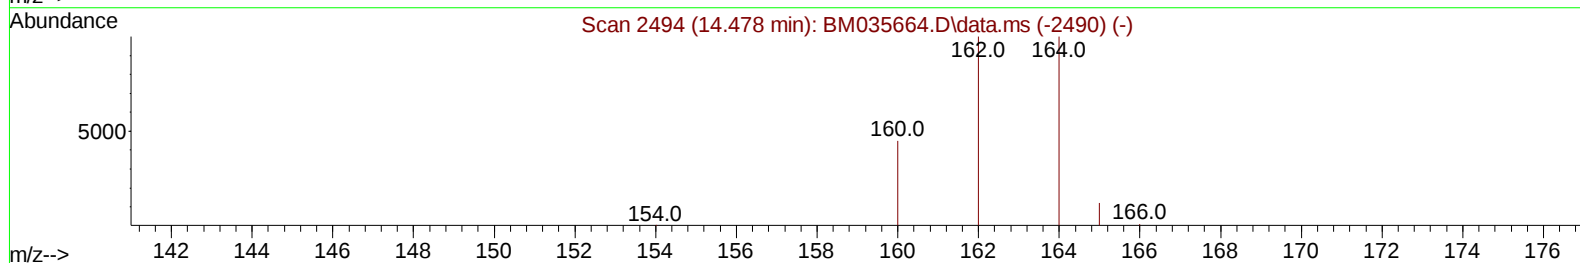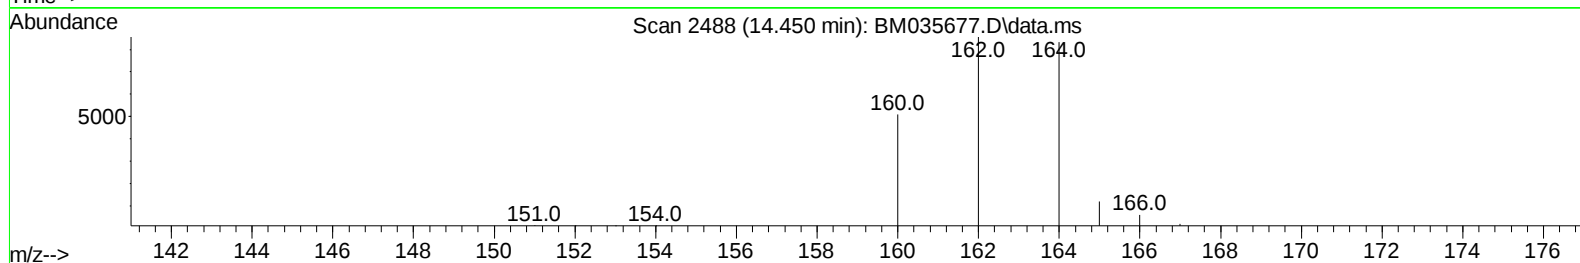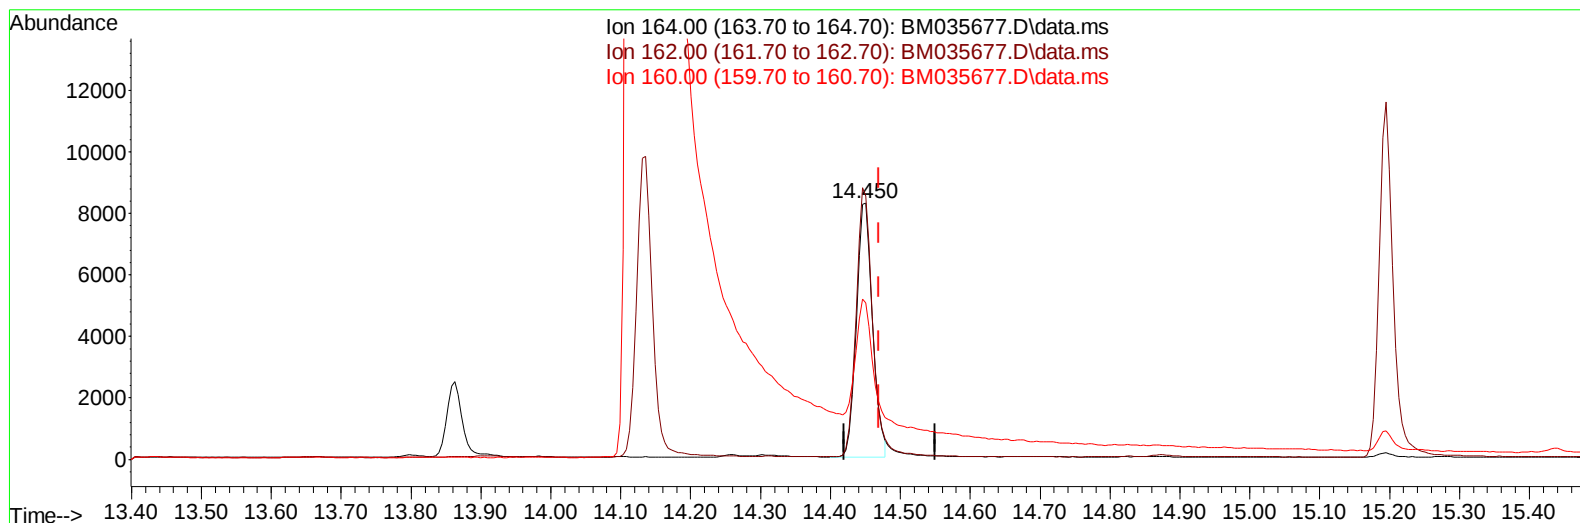

TIC: BM035677.D\data.ms

(9) Acenaphthene-d10 (I)

14.450min (-0.019) 0.40 ng/u1

response 13115

Ion	Exp%	Act%
164.00	100.00	100.00
162.00	106.40	102.64
160.00	49.90	61.04#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062322\
Data File : BM035677.D
Acq On : 25 Jun 2022 00:42
Operator : CG/JU
Sample : N3359-11RE
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4S5RE

Manual IntegrationsAPPROVED

Quant Time: Jun 25 04:06:44 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM061822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 20 01:56:13 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/27/2022
Supervised By :Yogesh Patel 06/28/2022

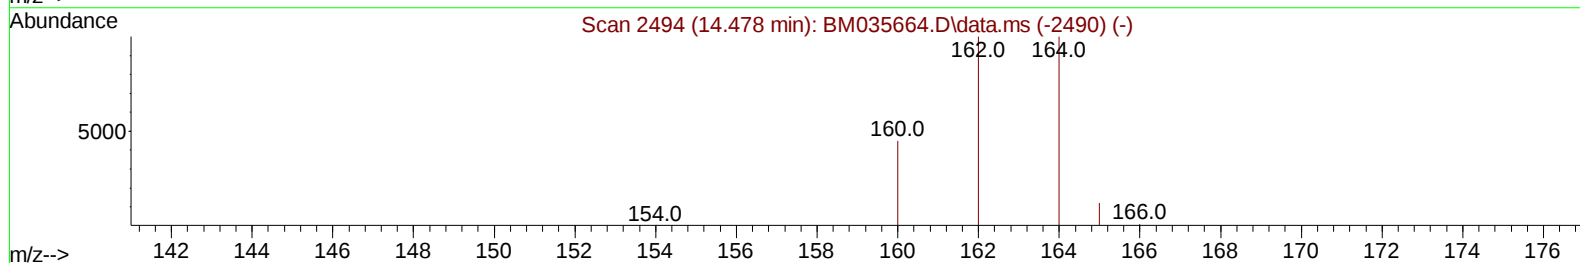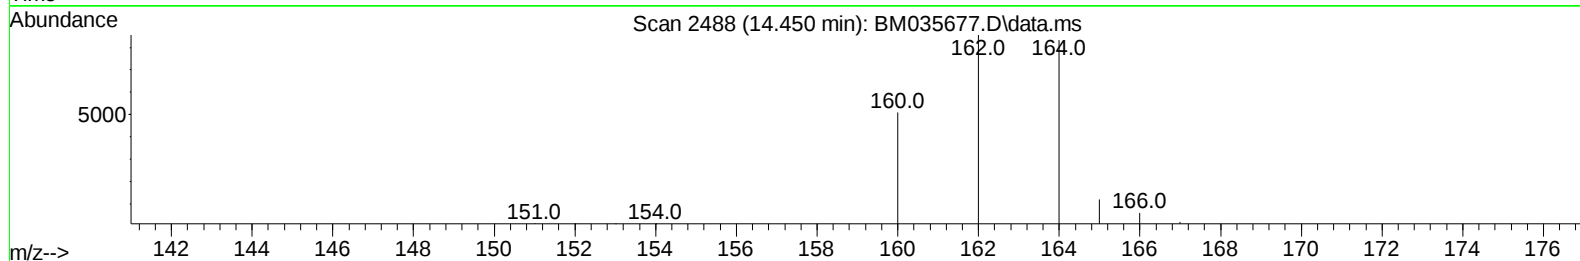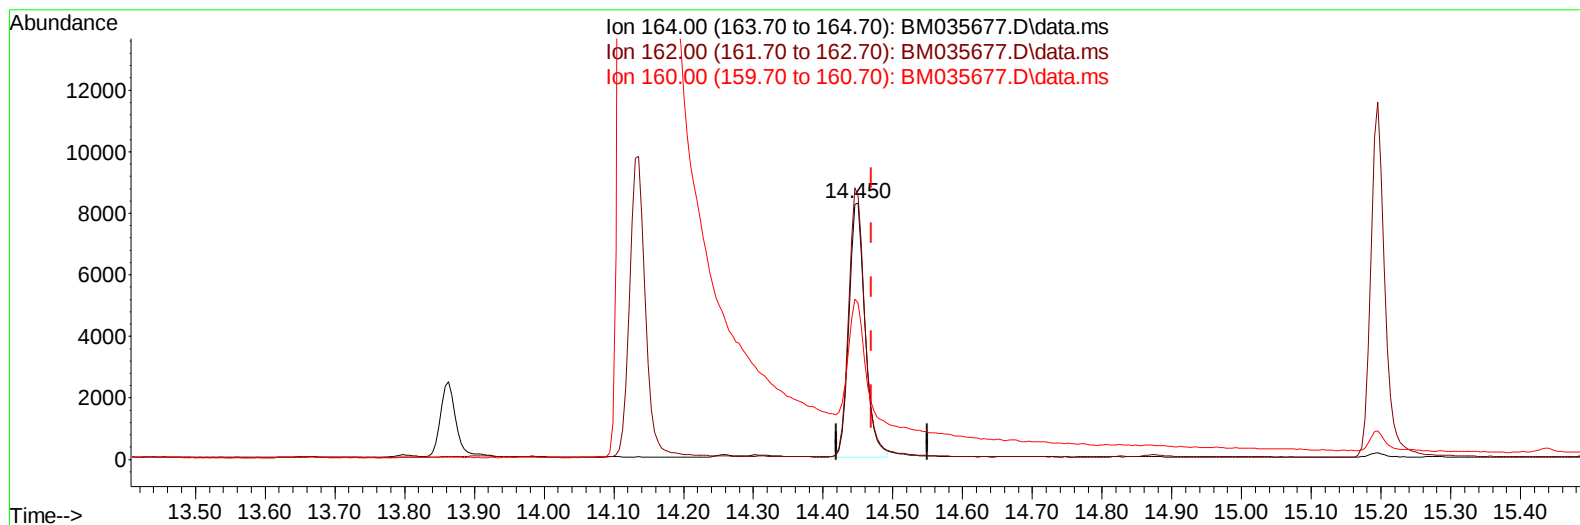

TIC: BM035677.D\data.ms

(9) Acenaphthene-d10 (I)

14.450min (-0.019) 0.40 ng/ul m

response 13394

Ion	Exp%	Act%
164.00	100.00	100.00
162.00	106.40	102.64
160.00	49.90	61.04#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062322\
 Data File : BM035677.D
 Acq On : 25 Jun 2022 00:42
 Operator : CG/JU
 Sample : N3359-11RE
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4S5RE

Manual IntegrationsAPPROVED

Quant Time: Jul 01 04:11:04 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM061822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 20 01:56:13 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/27/2022
 Supervised By :Yogesh Patel 06/28/2022

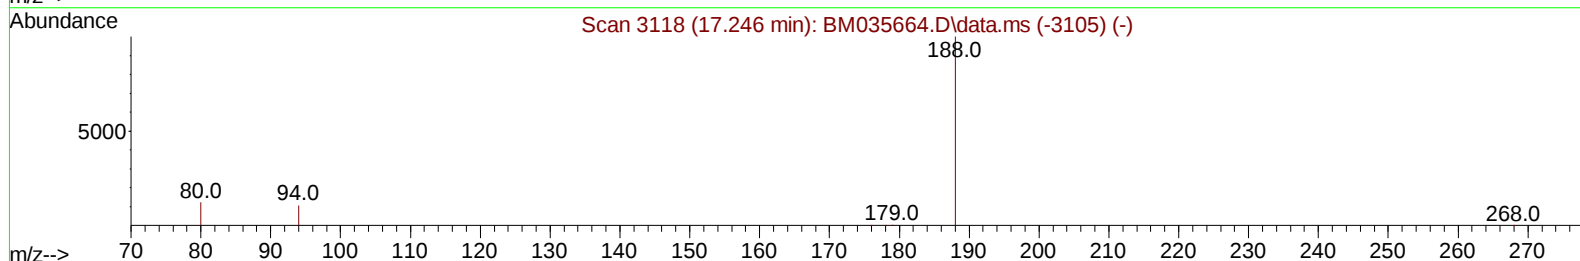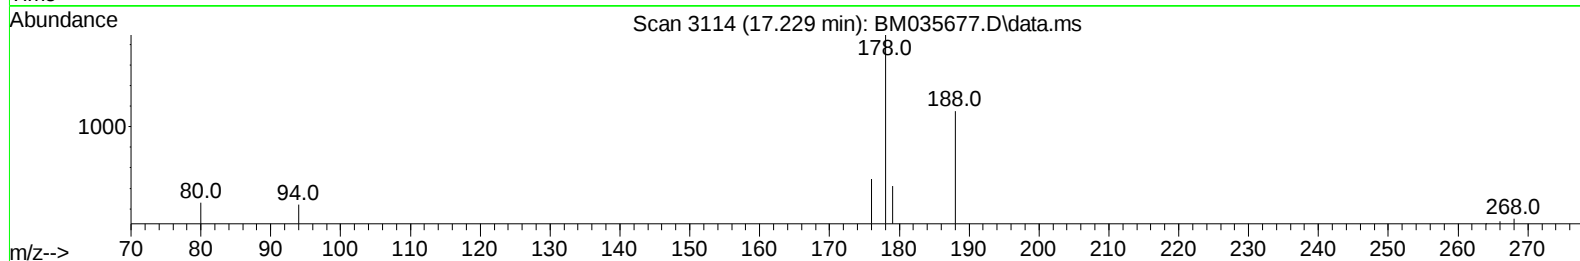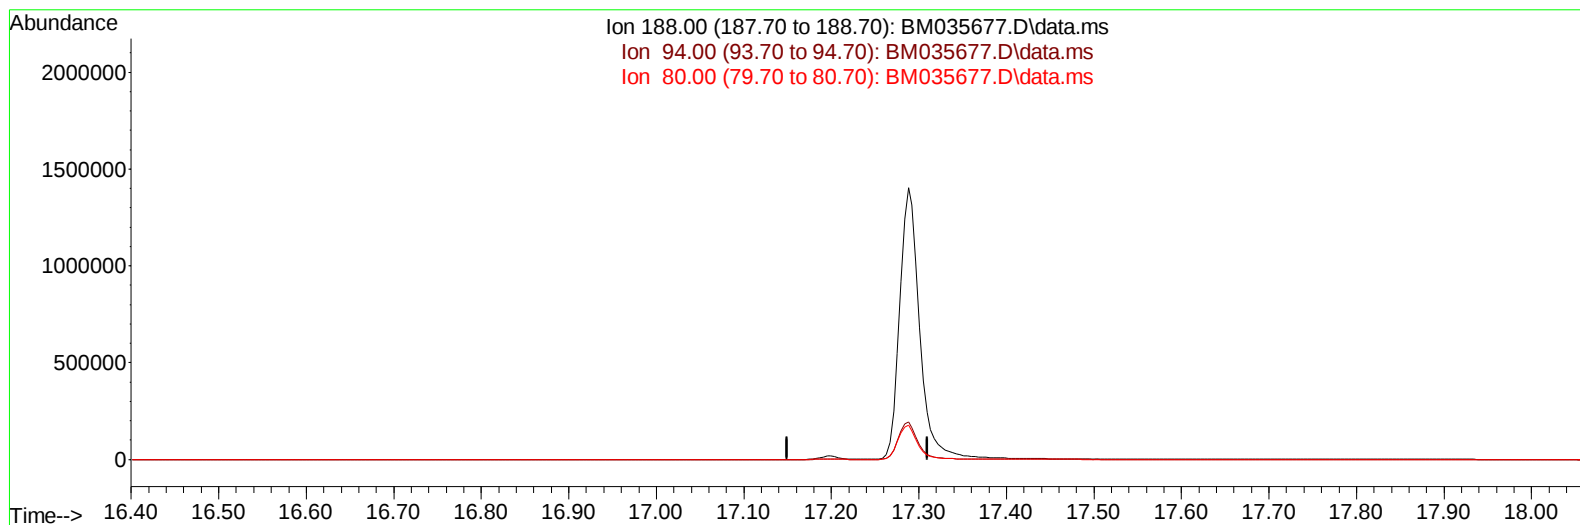

TIC: BM035677.D\data.ms

(13) Phenanthrene-d10 (I)

17.230min (-17.230) 0.00 ng/u1

response 0

Ion	Exp%	Act%
188.00	100.00	0.00
94.00	12.00	0.00#
80.00	13.50	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062322\
 Data File : BM035677.D
 Acq On : 25 Jun 2022 00:42
 Operator : CG/JU
 Sample : N3359-11RE
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4S5RE

Manual IntegrationsAPPROVED

Quant Time: Jun 25 04:06:44 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM061822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 20 01:56:13 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/27/2022
 Supervised By :Yogesh Patel 06/28/2022

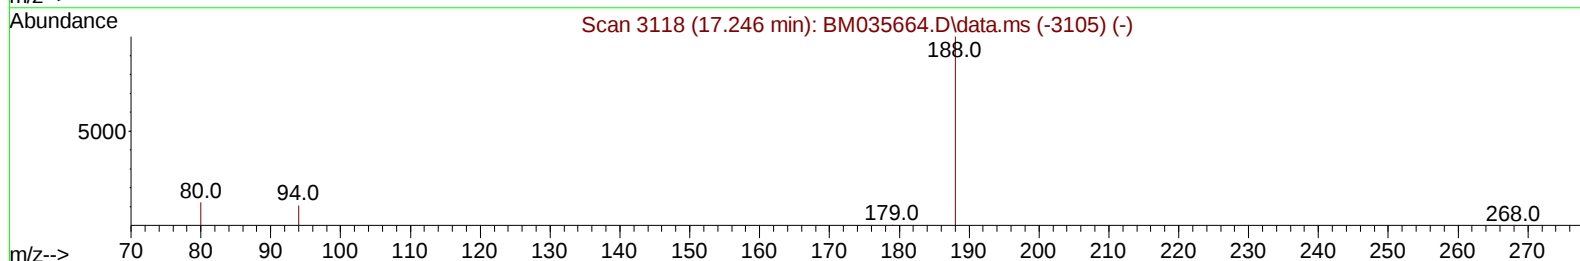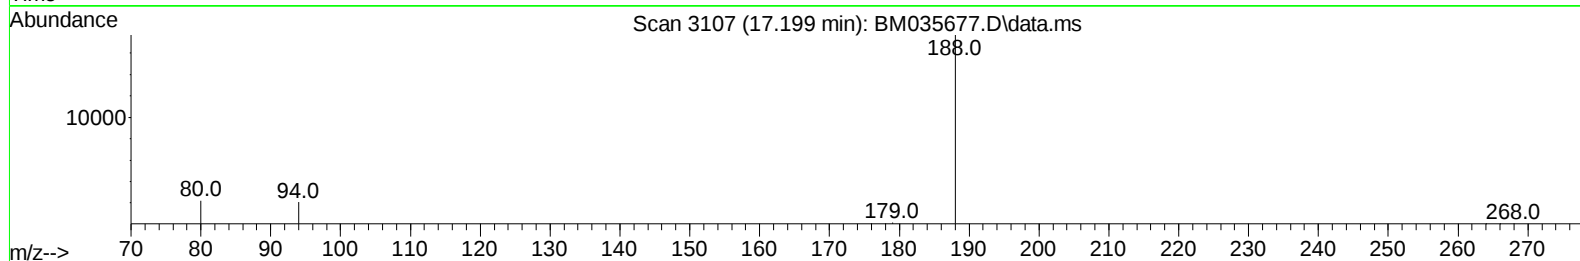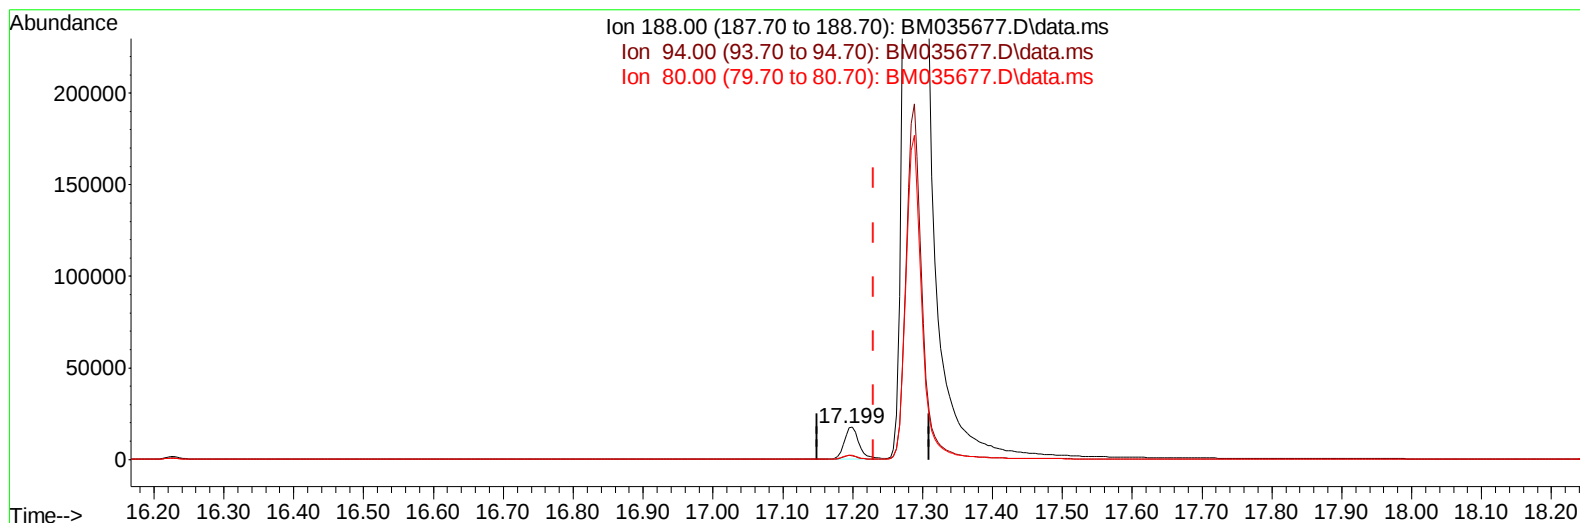

TIC: BM035677.D\data.ms

(13) Phenanthrene-d10 (I)

17.199min (-0.030) 0.40 ng/ul m

response 26244

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	12.00	11.71
80.00	13.50	12.59
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062322\
 Data File : BM035677.D
 Acq On : 25 Jun 2022 00:42
 Operator : CG/JU
 Sample : N3359-11RE
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4S5RE

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 06/27/2022
 Supervised By :Yogesh Patel 06/28/2022

Quant Time: Jun 25 04:06:44 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM061822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 20 01:56:13 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.825	152	5773	0.400	ng/ul	-0.03
4) Naphthalene-d8	10.606	136	21406	0.400	ng/ul	-0.04
9) Acenaphthene-d10	14.450	164	13394m	0.400	ng/ul	-0.02
13) Phenanthrene-d10	17.199	188	26244m	0.400	ng/ul	-0.03
17) Chrysene-d12	21.406	240	17046	0.400	ng/ul	0.00
23) Perylene-d12	23.724	264	21169	0.400	ng/ul	#-0.04
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.264	96	33815	4.163	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.239	152	10596	0.333	ng/ul	0.00
18) Fluoranthene-d10	19.233	212	26193	0.457	ng/ul	-0.02
Target Compounds						Qvalue
5) Naphthalene	10.655	128	4047	0.056	ng/ul#	89
7) 2-Methylnaphthalene	12.316	142	1021	0.025	ng/ul	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062322\
Data File : BM035677.D
Acq On : 25 Jun 2022 00:42
Operator : CG/JU
Sample : N3359-11RE
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4S5RE

Manual IntegrationsAPPROVED

Quant Time: Jun 25 04:06:44 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM061822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 20 01:56:13 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/27/2022
Supervised By :Yogesh Patel 06/28/2022

