

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062322\
 Data File : BM035644.D
 Acq On : 24 Jun 2022 03:08
 Operator : CG/JU
 Sample : N3359-06
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4S2

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 06/24/2022
 Supervised By :Yogesh Patel 06/28/2022

Quant Time: Jun 24 04:24:39 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM061822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 20 01:56:13 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.816	152	5932	0.400	ng/ul	-0.04
4) Naphthalene-d8	10.600	136	22184	0.400	ng/ul	-0.04
9) Acenaphthene-d10	14.446	164	13041m	0.400	ng/ul	-0.02
13) Phenanthrene-d10	17.195	188	23554m	0.400	ng/ul	-0.03
17) Chrysene-d12	21.395	240	15900	0.400	ng/ul	-0.02
23) Perylene-d12	23.721	264	17906	0.400	ng/ul	#-0.04
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.260	96	36321	4.352	ng/ul	-0.01
6) 2-Methylnaphthalene-d10	12.217	152	11640	0.353	ng/ul	-0.03
18) Fluoranthene-d10	19.229	212	23232	0.435	ng/ul	-0.02
Target Compounds						
5) Naphthalene	10.650	128	3131	0.042	ng/ul#	Qvalue 89

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062322\
Data File : BM035644.D
Acq On : 24 Jun 2022 03:08
Operator : CG/JU
Sample : N3359-06
Misc :
ALS Vial : 27 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
EW4S2

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 06/24/2022
Supervised By :Yogesh Patel 06/28/2022


Quant Time: Jun 24 04:24:39 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM061822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 20 01:56:13 2022
Response via : Initial Calibration

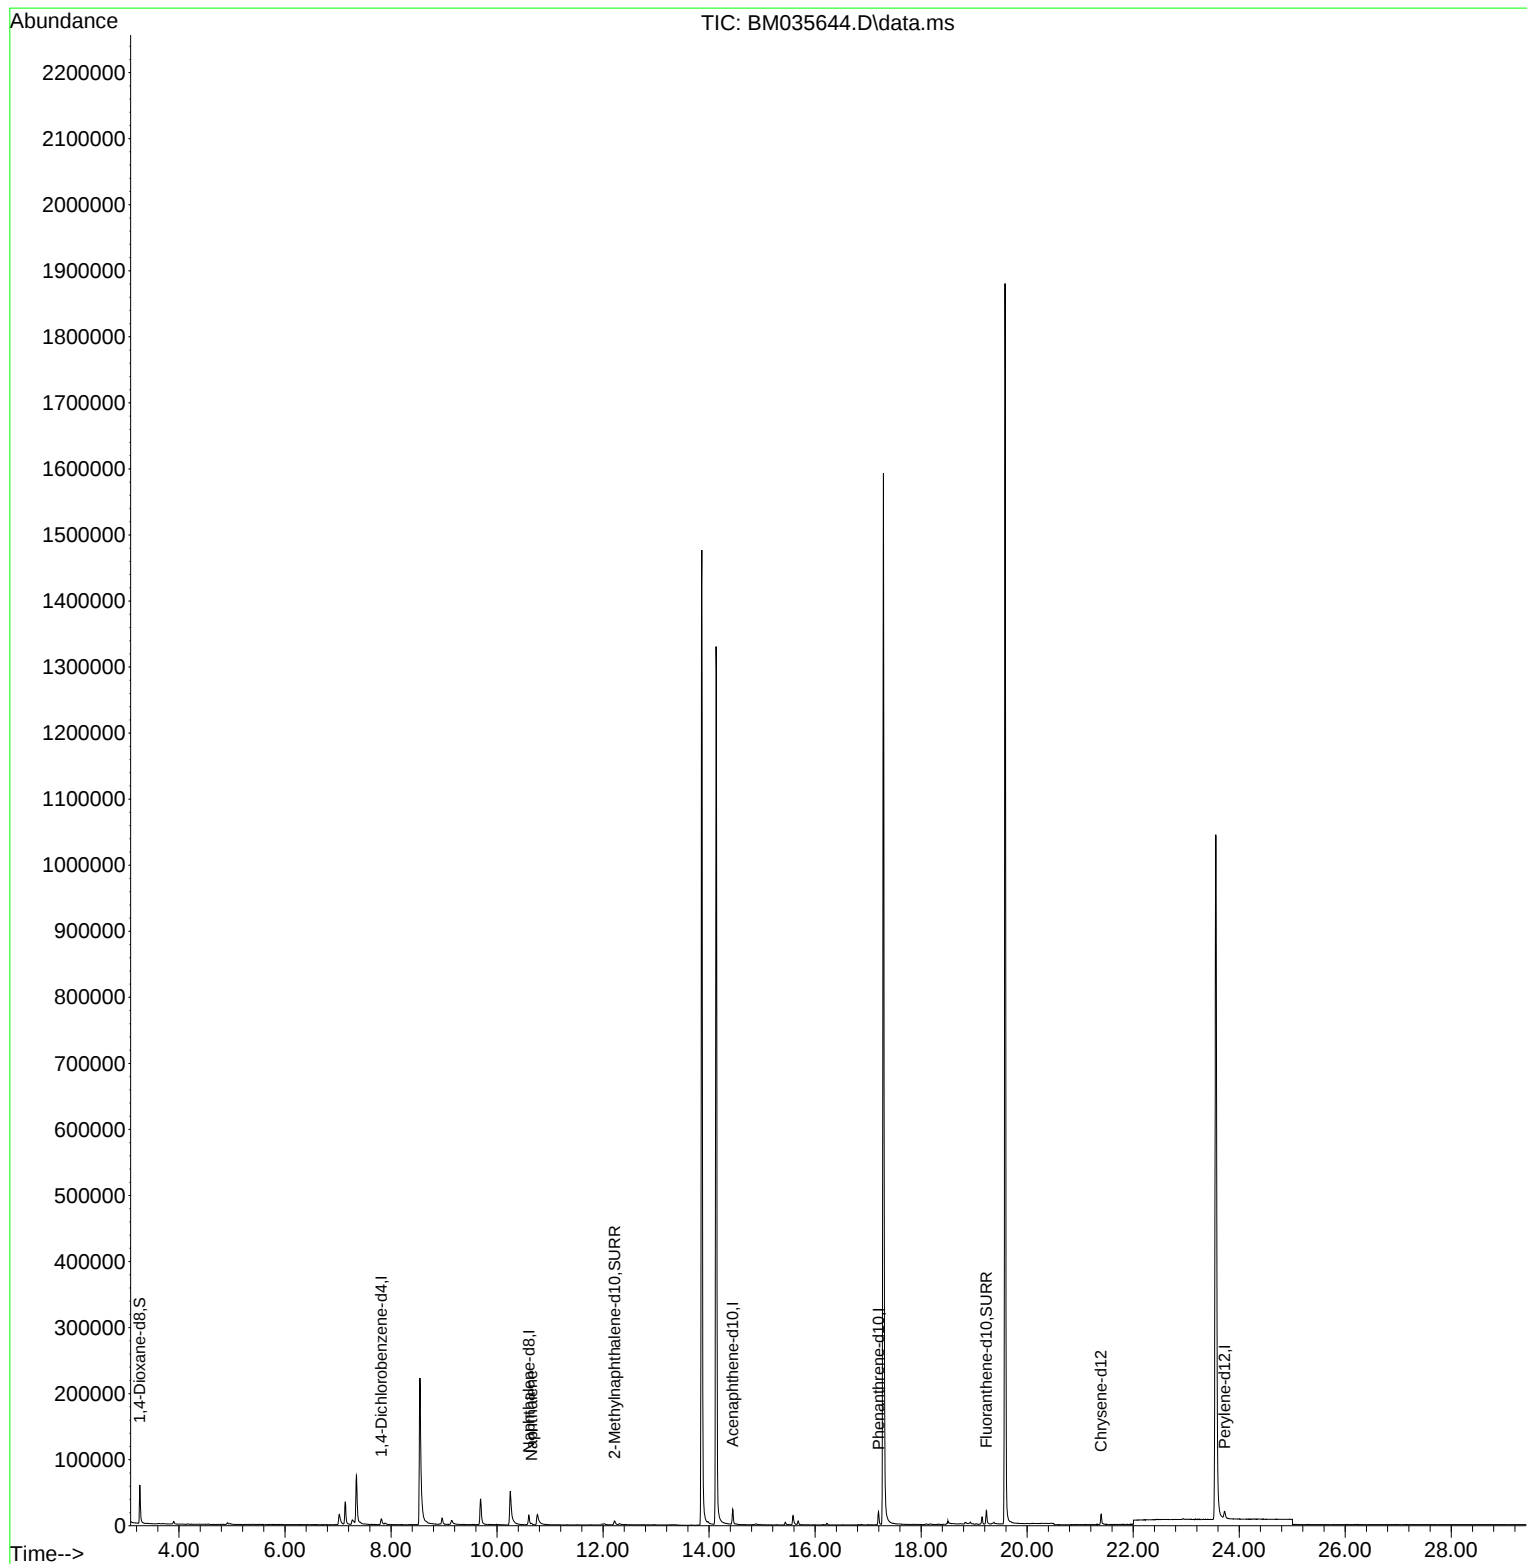

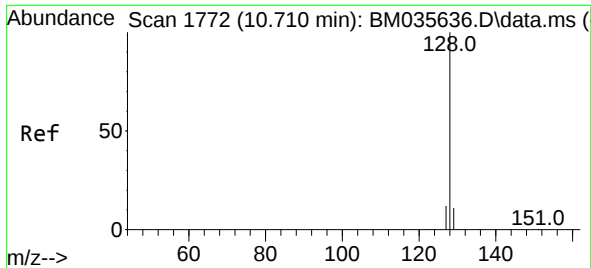

#5
Naphthalene
Concen: 0.042 ng/ul
RT: 10.650 min Scan# 1772
Delta R.T. -0.044 min
Lab File: BM035644.D
Acq: 24 Jun 2022 03:08

Instrument :
BNA_M
ClientSampleId :
EW4S2

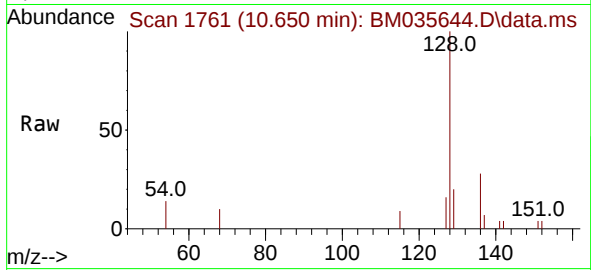

Tgt Ion:128 Resp: 313
Ion Ratio Lower Upper
128 100
129 20.5 10.1 15.1
127 15.7 11.4 17.2

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 06/24/2022
Supervised By :Yogesh Patel 06/28/2022

