

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM062322\  
 Data File : BM035647.D  
 Acq On : 24 Jun 2022 04:56  
 Operator : CG/JU  
 Sample : N3359-05  
 Misc :  
 ALS Vial : 30 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 EW4S1

Manual Integrations  
 APPROVED

Reviewed By :Jagrut Upadhyay 06/24/2022  
 Supervised By :Yogesh Patel 06/28/2022

Quant Time: Jun 24 06:00:18 2022  
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_M\METHODS\SFAM-EPA-SIM-BM061822.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Mon Jun 20 01:56:13 2022  
 Response via : Initial Calibration

| Compound                    | R.T.   | QIon | Response | Conc  | Units  | Dev(Min)     |
|-----------------------------|--------|------|----------|-------|--------|--------------|
| -----                       |        |      |          |       |        |              |
| Internal Standards          |        |      |          |       |        |              |
| 1) 1,4-Dichlorobenzene-d4   | 7.820  | 152  | 5358     | 0.400 | ng/ul  | -0.04        |
| 4) Naphthalene-d8           | 10.600 | 136  | 20009    | 0.400 | ng/ul  | -0.04        |
| 9) Acenaphthene-d10         | 14.446 | 164  | 13044m   | 0.400 | ng/ul  | -0.02        |
| 13) Phenanthrene-d10        | 17.196 | 188  | 27826m   | 0.400 | ng/ul  | -0.03        |
| 17) Chrysene-d12            | 21.405 | 240  | 20324    | 0.400 | ng/ul  | 0.00         |
| 23) Perylene-d12            | 23.723 | 264  | 23958    | 0.400 | ng/ul  | #-0.04       |
| System Monitoring Compounds |        |      |          |       |        |              |
| 3) 1,4-Dioxane-d8           | 3.260  | 96   | 28558    | 3.788 | ng/ul  | -0.01        |
| 6) 2-Methylnaphthalene-d10  | 12.233 | 152  | 10545    | 0.355 | ng/ul  | -0.01        |
| 18) Fluoranthene-d10        | 19.230 | 212  | 28346    | 0.415 | ng/ul  | -0.02        |
| Target Compounds            |        |      |          |       |        |              |
| 5) Naphthalene              | 10.649 | 128  | 2812     | 0.041 | ng/ul# | Qvalue<br>87 |
| -----                       |        |      |          |       |        |              |

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM062322\  
Data File : BM035647.D  
Acq On : 24 Jun 2022 04:56  
Operator : CG/JU  
Sample : N3359-05  
Misc :  
ALS Vial : 30 Sample Multiplier: 1


Instrument :  
BNA\_M  
ClientSampleId :  
EW4S1

Manual Integrations  
APPROVED

Reviewed By :Jagrut Upadhyay 06/24/2022  
Supervised By :Yogesh Patel 06/28/2022


Quant Time: Jun 24 06:00:18 2022  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_M\METHODS\SFAM-EPA-SIM-BM061822.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Jun 20 01:56:13 2022  
Response via : Initial Calibration

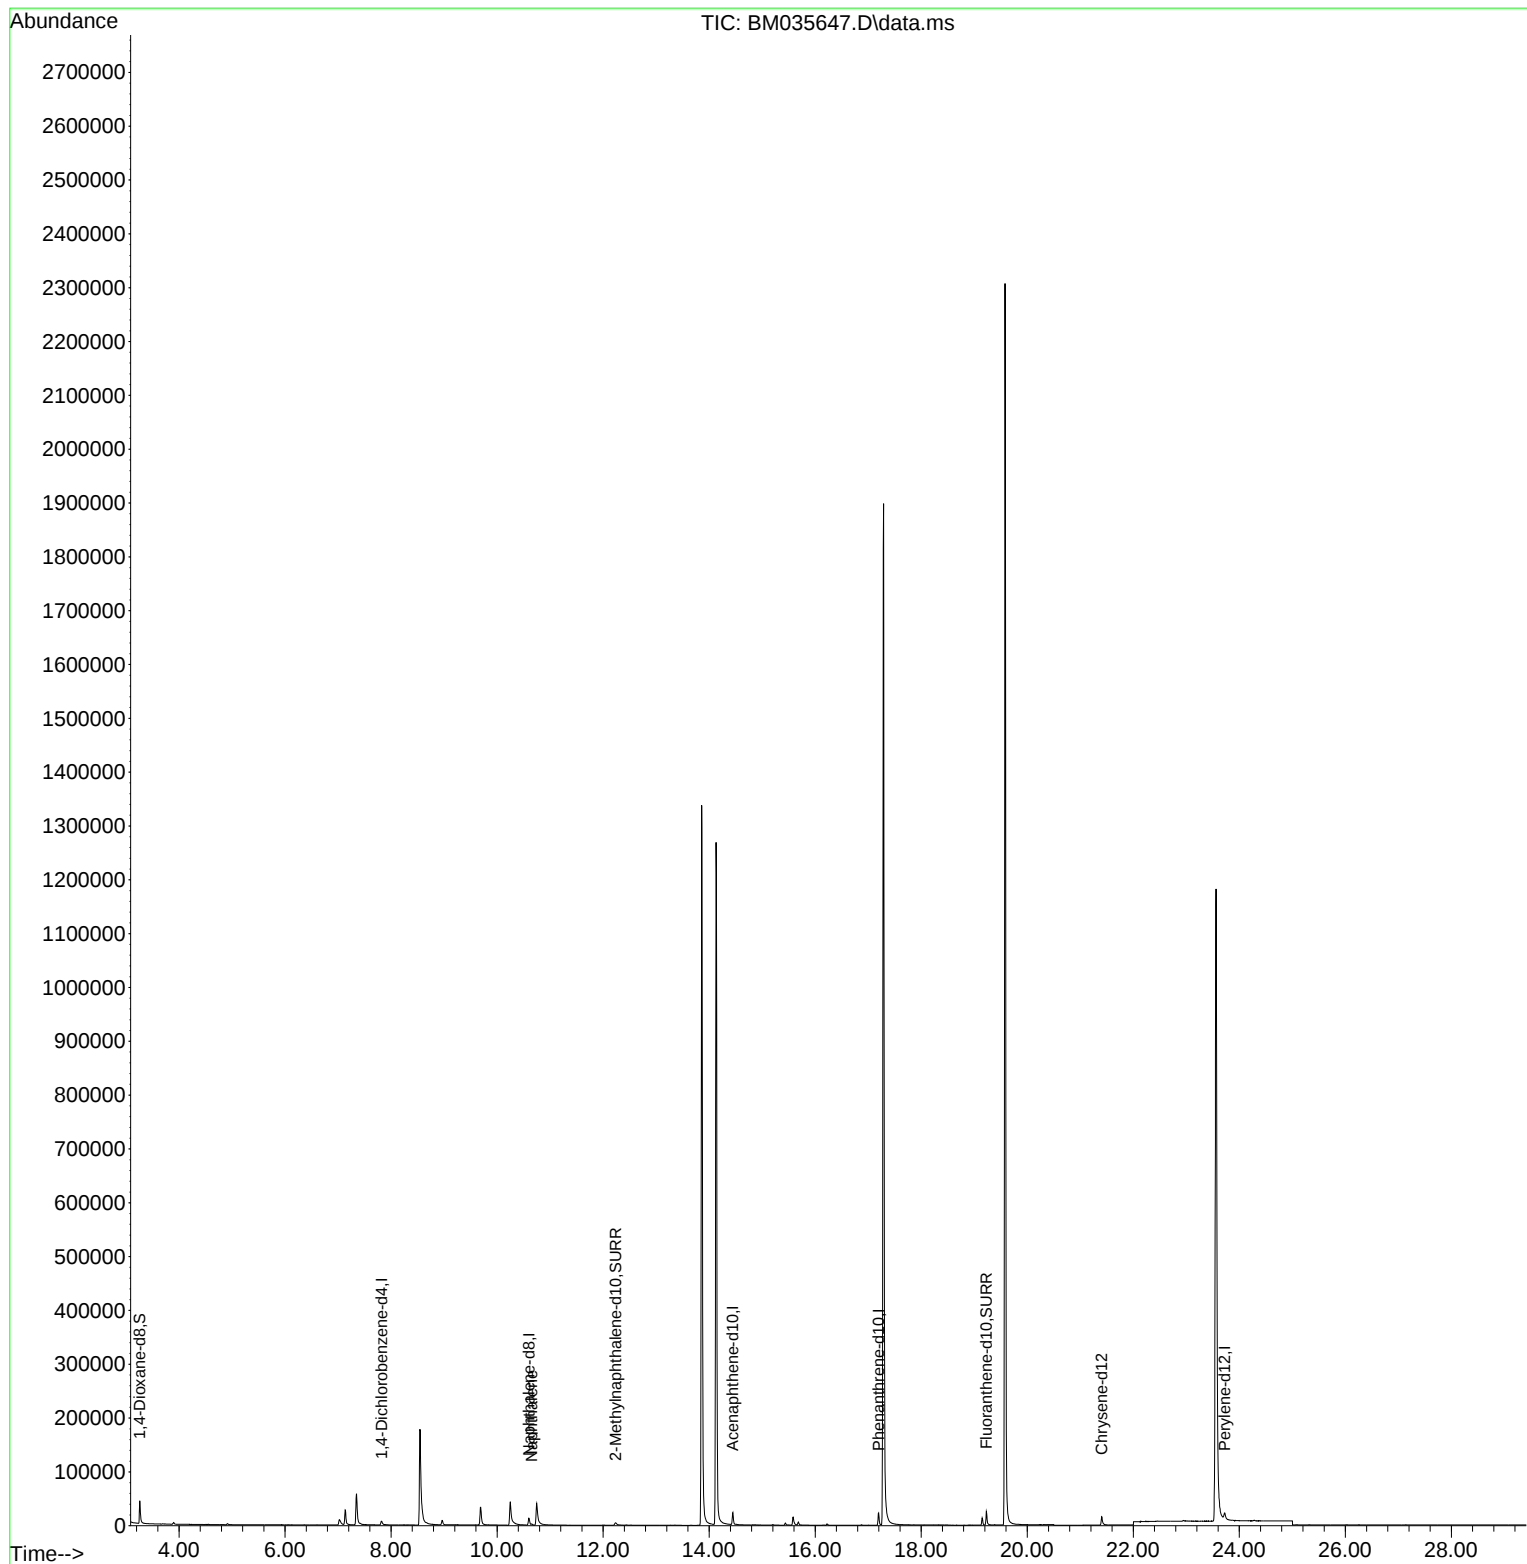

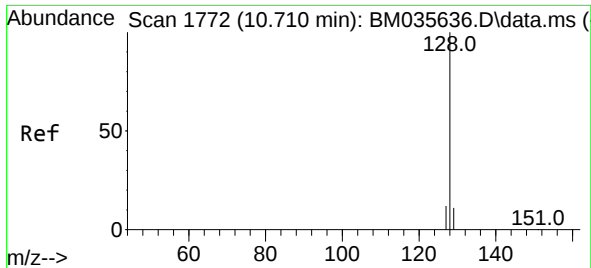

#5  
Naphthalene  
Concen: 0.041 ng/ul  
RT: 10.649 min Scan# 11  
Delta R.T. -0.044 min  
Lab File: BM035647.D  
Acq: 24 Jun 2022 04:56

Instrument :  
BNA\_M  
ClientSampleId :  
EW4S1

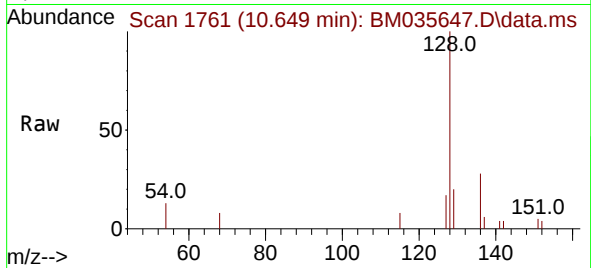

Tgt Ion:128 Resp: 2812  
Ion Ratio Lower Upper  
128 100  
129 20.3 10.1 15.1  
127 16.9 11.4 17.2

Manual Integrations  
APPROVED

Reviewed By :Jagrut Upadhyay 06/24/2022  
Supervised By :Yogesh Patel 06/28/2022

