

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM062322\  
 Data File : BM035671.D  
 Acq On : 24 Jun 2022 21:02  
 Operator : CG/JU  
 Sample : N3358-05  
 Misc :  
 ALS Vial : 55 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 EW4S1

Manual Integrations  
 APPROVED

Reviewed By :Jagrut Upadhyay 06/27/2022  
 Supervised By :Yogesh Patel 06/28/2022

Quant Time: Jun 25 04:06:25 2022  
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_M\METHODS\SFAM-EPA-SIM-BM061822.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Mon Jun 20 01:56:13 2022  
 Response via : Initial Calibration

| Compound                    | R.T.   | QIon | Response | Conc  | Units  | Dev(Min)     |
|-----------------------------|--------|------|----------|-------|--------|--------------|
| -----                       |        |      |          |       |        |              |
| Internal Standards          |        |      |          |       |        |              |
| 1) 1,4-Dichlorobenzene-d4   | 7.825  | 152  | 5235     | 0.400 | ng/ul  | -0.03        |
| 4) Naphthalene-d8           | 10.605 | 136  | 17290    | 0.400 | ng/ul  | -0.04        |
| 9) Acenaphthene-d10         | 14.450 | 164  | 10835m   | 0.400 | ng/ul  | -0.02        |
| 13) Phenanthrene-d10        | 17.199 | 188  | 22684m   | 0.400 | ng/ul  | -0.03        |
| 17) Chrysene-d12            | 21.412 | 240  | 14821    | 0.400 | ng/ul  | 0.00         |
| 23) Perylene-d12            | 23.724 | 264  | 8103m    | 0.400 | ng/ul  | -0.04        |
| System Monitoring Compounds |        |      |          |       |        |              |
| 3) 1,4-Dioxane-d8           | 3.264  | 96   | 29210    | 3.966 | ng/ul  | 0.00         |
| 6) 2-Methylnaphthalene-d10  | 12.244 | 152  | 9509     | 0.370 | ng/ul  | 0.00         |
| 18) Fluoranthene-d10        | 19.233 | 212  | 23590    | 0.474 | ng/ul  | -0.02        |
| Target Compounds            |        |      |          |       |        |              |
| 5) Naphthalene              | 10.655 | 128  | 2713     | 0.046 | ng/ul# | Qvalue<br>88 |
| -----                       |        |      |          |       |        |              |

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM062322\  
Data File : BM035671.D  
Acq On : 24 Jun 2022 21:02  
Operator : CG/JU  
Sample : N3358-05  
Misc :  
ALS Vial : 55 Sample Multiplier: 1


Instrument :  
BNA\_M  
ClientSampleId :  
EW4S1

Manual Integrations  
APPROVED

Reviewed By :Jagrut Upadhyay 06/27/2022  
Supervised By :Yogesh Patel 06/28/2022


Quant Time: Jun 25 04:06:25 2022  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_M\METHODS\SFAM-EPA-SIM-BM061822.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Jun 20 01:56:13 2022  
Response via : Initial Calibration

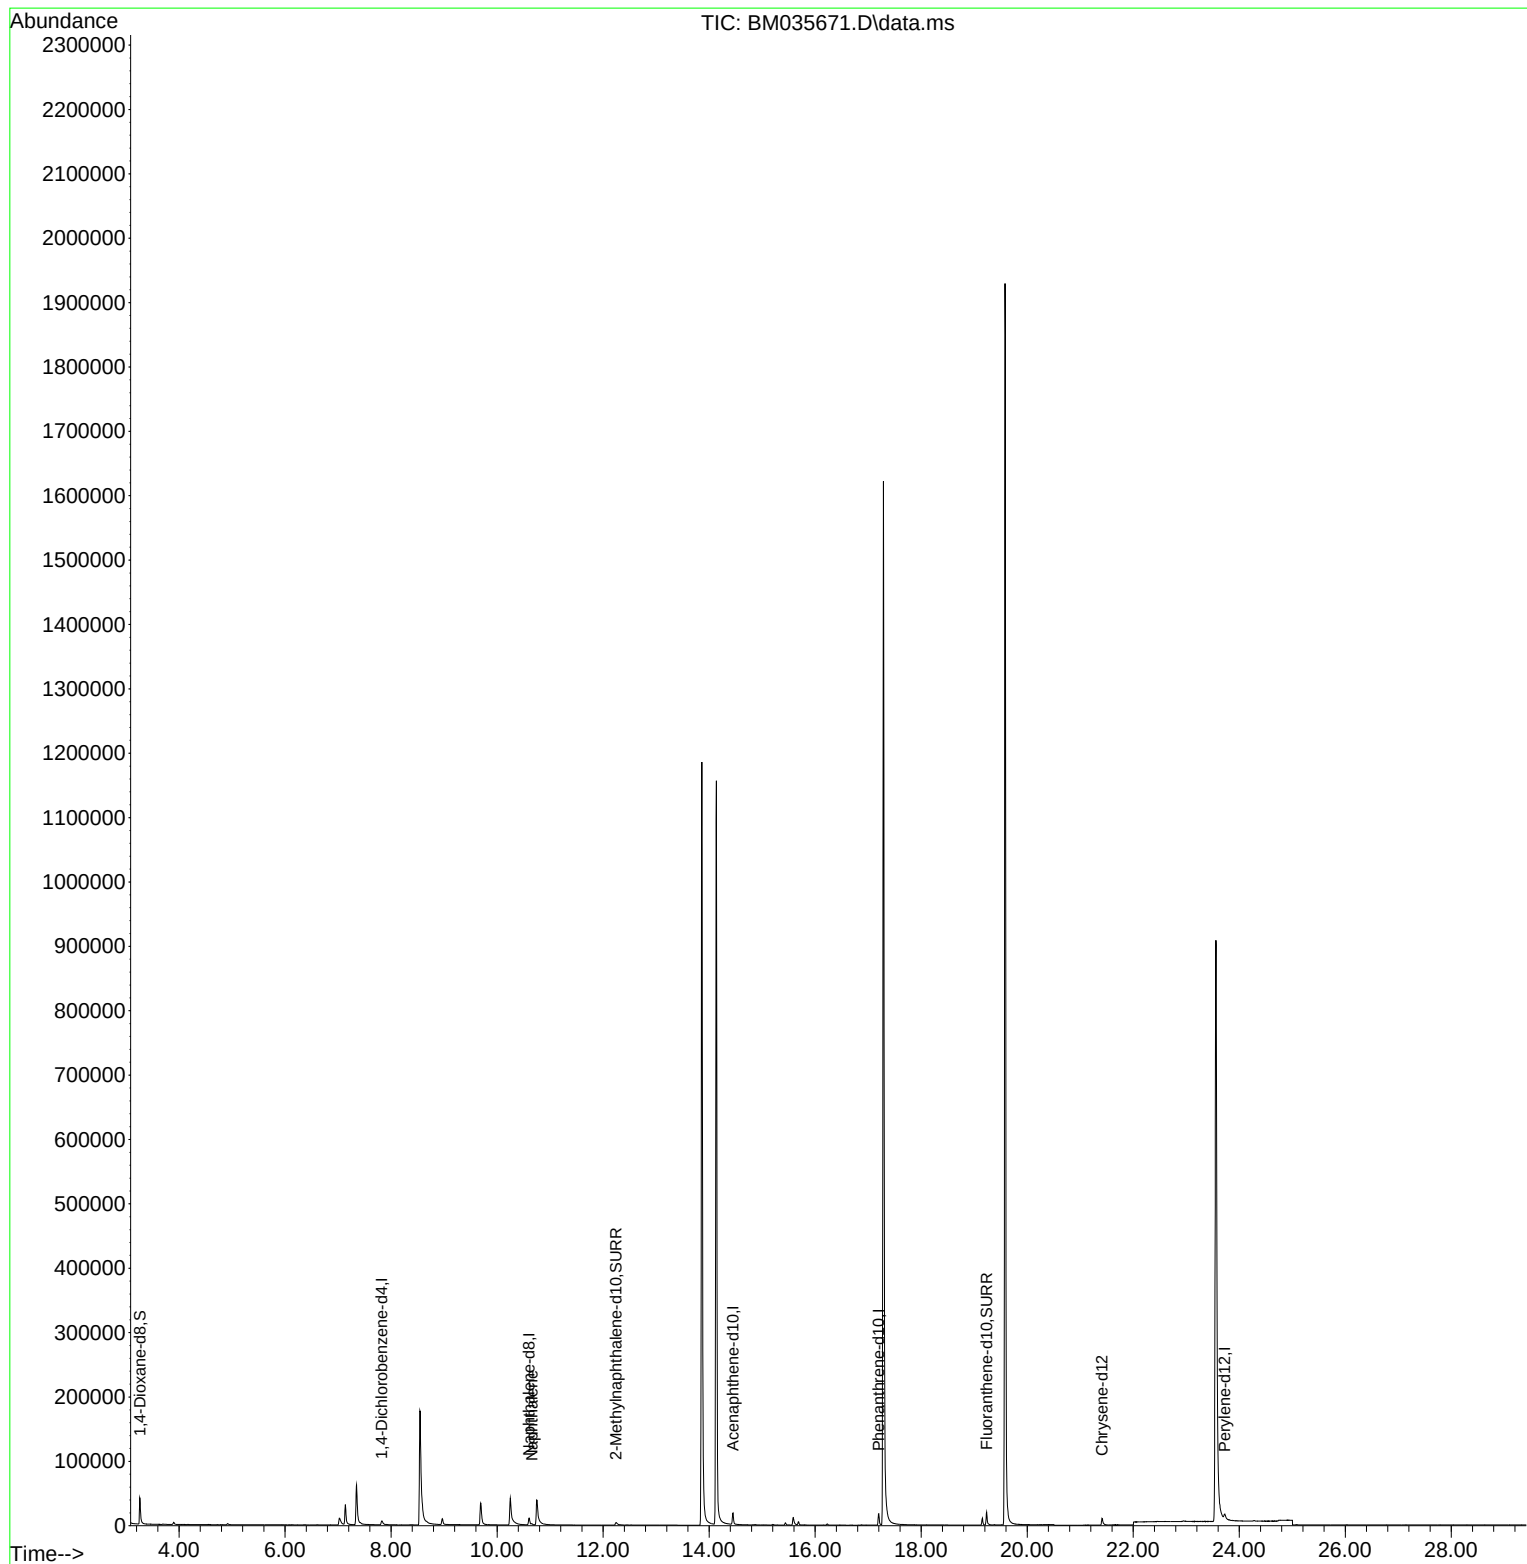

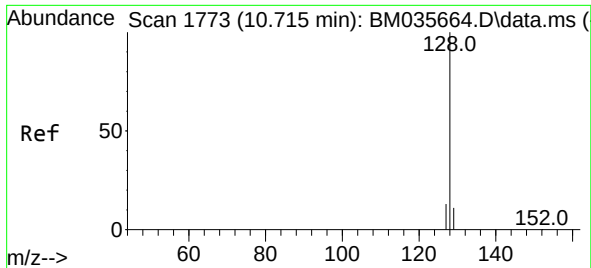

#5  
Naphthalene  
Concen: 0.046 ng/ul  
RT: 10.655 min Scan# 11  
Delta R.T. -0.039 min  
Lab File: BM035671.D  
Acq: 24 Jun 2022 21:02

Instrument :  
BNA\_M  
ClientSampleId :  
EW4S1

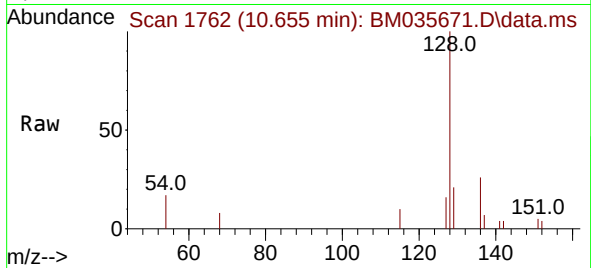

Tgt Ion:128 Resp: 271  
Ion Ratio Lower Upper  
128 100  
129 21.1 10.1 15.1  
127 15.8 11.4 17.2

Manual Integrations  
APPROVED

Reviewed By :Jagrut Upadhyay 06/27/2022  
Supervised By :Yogesh Patel 06/28/2022

