

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062323\
 Data File : BM040373.D
 Acq On : 23 Jun 2023 13:40
 Operator : MA/JU
 Sample : PB153416BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK416

Quant Time: Jun 24 01:36:48 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 23 00:44:24 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.949	152	6940	0.400	ng/ul	0.00
4) Naphthalene-d8	10.756	136	24976	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.591	164	11866	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.336	188	23926	0.400	ng/ul	0.00
17) Chrysene-d12	21.515	240	16150	0.400	ng/ul	0.00
23) Perylene-d12	23.929	264	17178	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.329	96	56774	5.208	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.345	152	11450	0.327	ng/ul	0.00
18) Fluoranthene-d10	19.361	212	17604	0.340	ng/ul	0.00
Target Compounds						Qvalue
12) Fluorene	15.581	166	3727	0.078	ng/ul#	15
20) Pyrene	19.723	202	2924	0.040	ng/ul#	1
26) Benzo(a)pyrene	23.774	252	5379	0.090	ng/ul#	58


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062323\
Data File : BM040373.D
Acq On : 23 Jun 2023 13:40
Operator : MA/JU
Sample : PB153416BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK416

Quant Time: Jun 24 01:36:48 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 23 00:44:24 2023
Response via : Initial Calibration




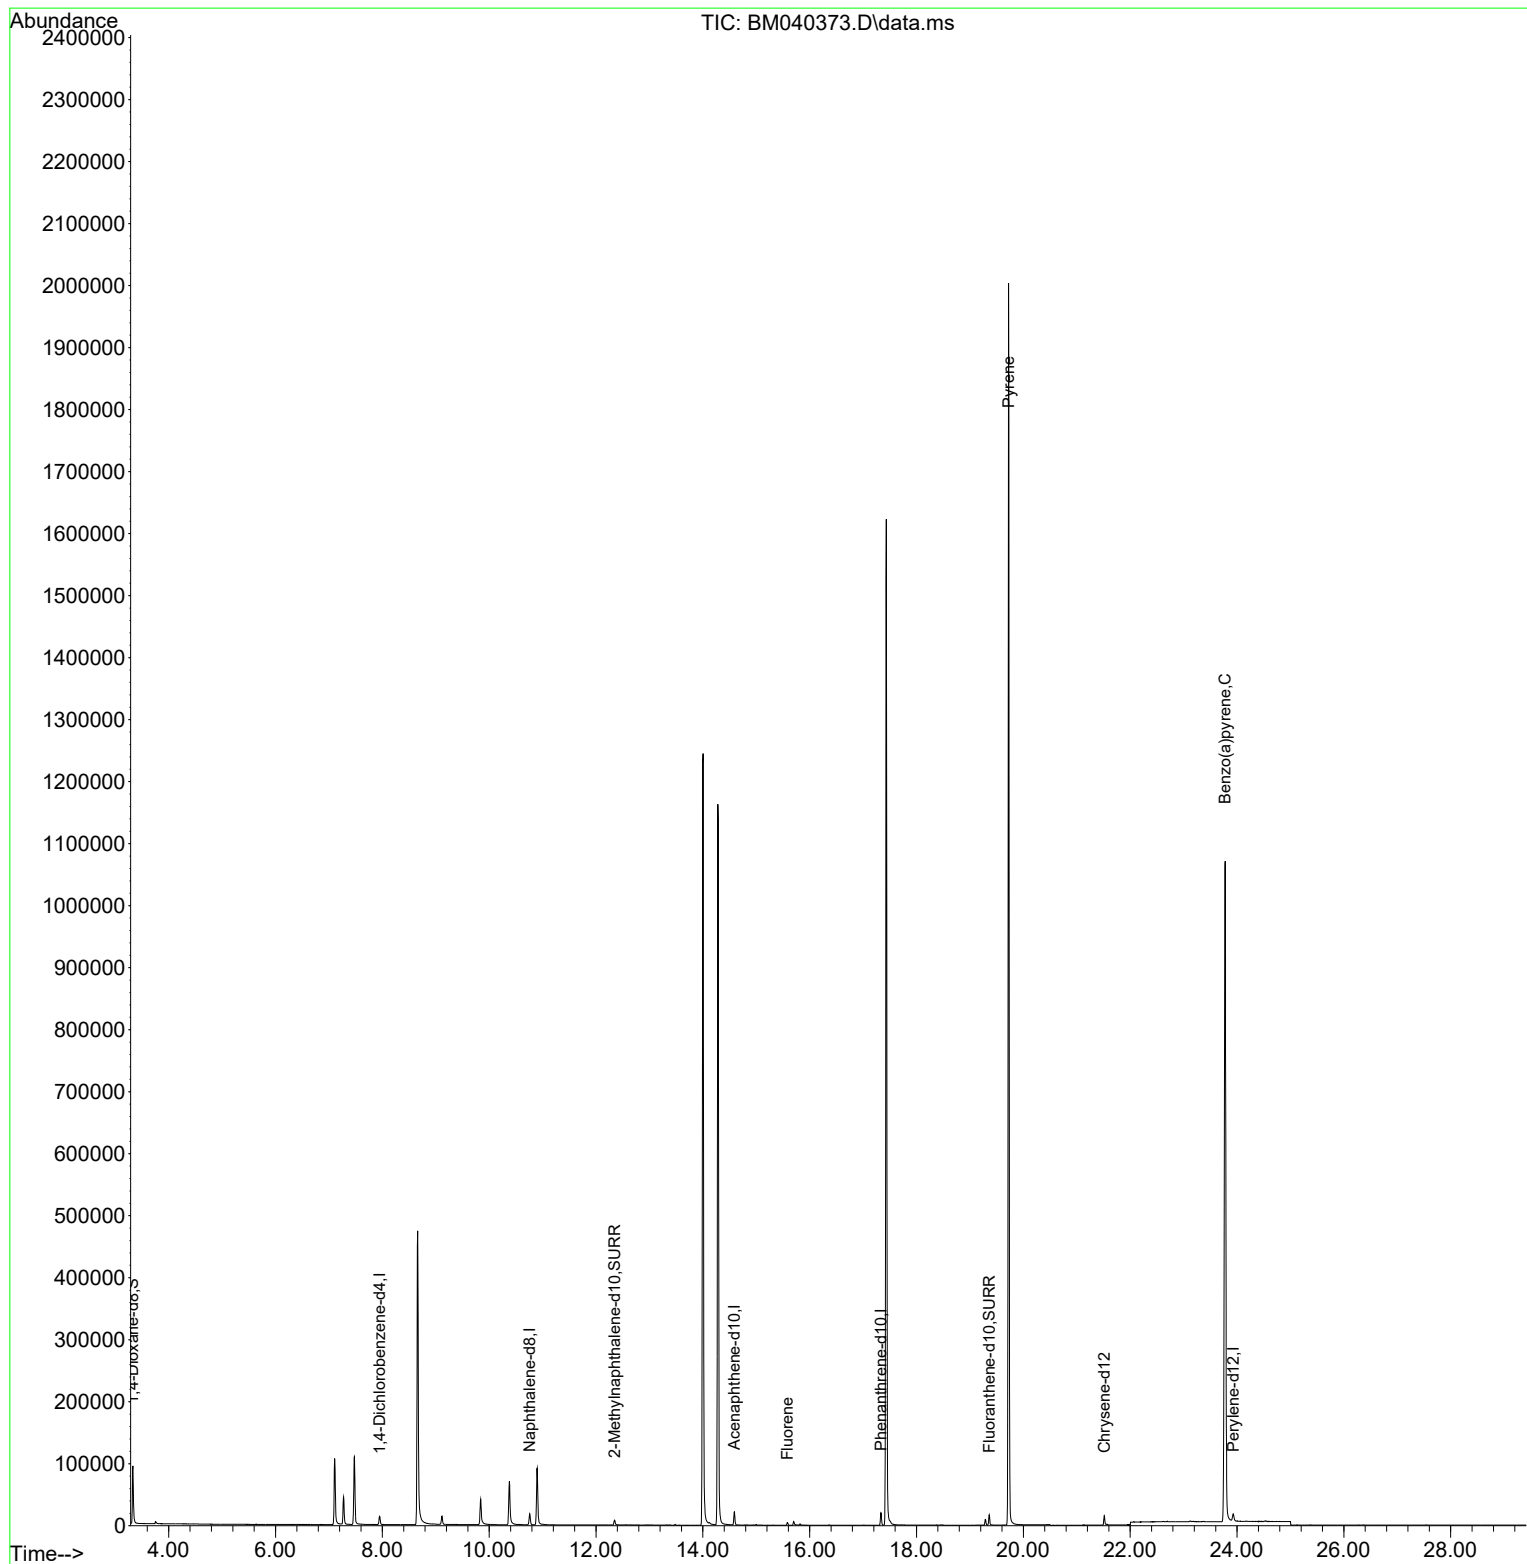


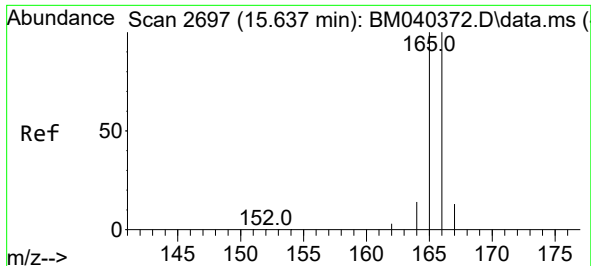

#12
Fluorene
Concen: 0.078 ng/ul
RT: 15.581 min Scan# 20
Delta R.T. -0.060 min
Lab File: BM040373.D
Acq: 23 Jun 2023 13:40




Instrument :
BNA_M
ClientSampleId :
SBLK416


Tgt Ion:166 Resp: 3727
Ion Ratio Lower Upper
166 100
165 8.3 79.6 119.4#
167 31.4 11.4 17.0#

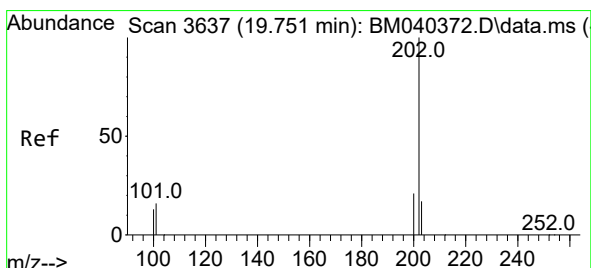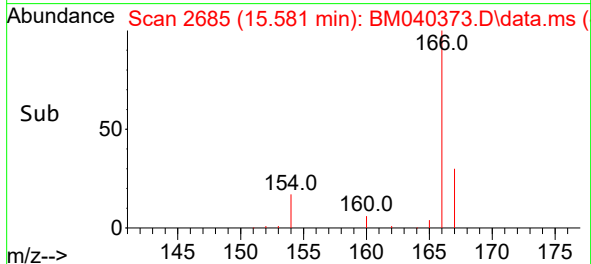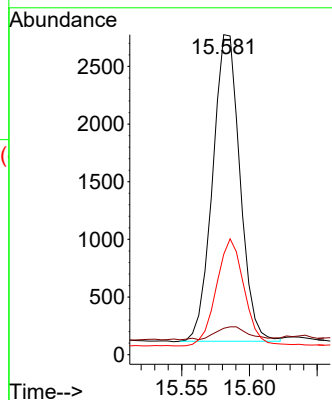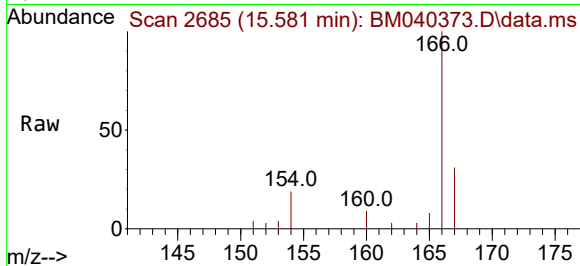

#20
Pyrene
Concen: 0.040 ng/ul
RT: 19.723 min Scan# 3631
Delta R.T. -0.033 min
Lab File: BM040373.D
Acq: 23 Jun 2023 13:40


Tgt Ion:202 Resp: 2924
Ion Ratio Lower Upper
202 100
101 169.2 12.6 18.8#
100 1278.2 9.8 14.6#

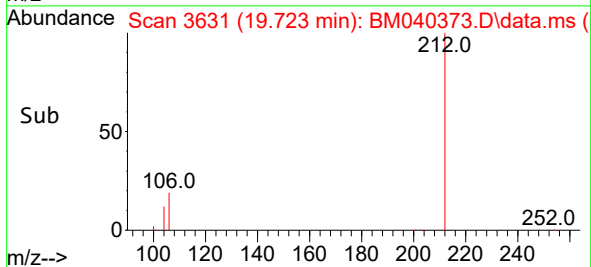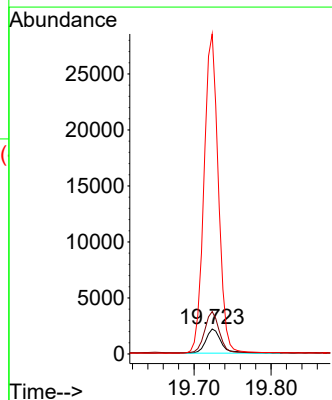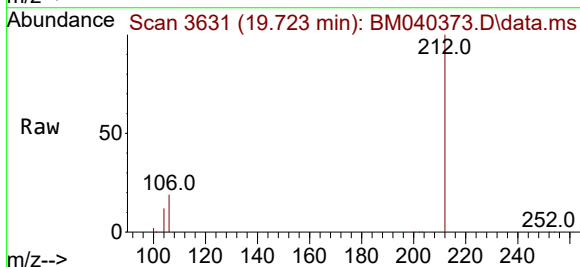

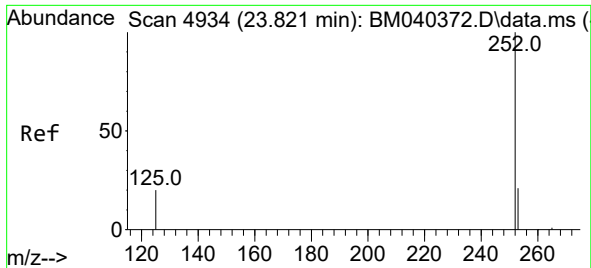

#26
Benzo(a)pyrene
Concen: 0.090 ng/ul
RT: 23.774 min Scan# 4918
Delta R.T. -0.050 min
Lab File: BM040373.D
Acq: 23 Jun 2023 13:40

Instrument :
BNA_M
ClientSampleId :
SBLK416

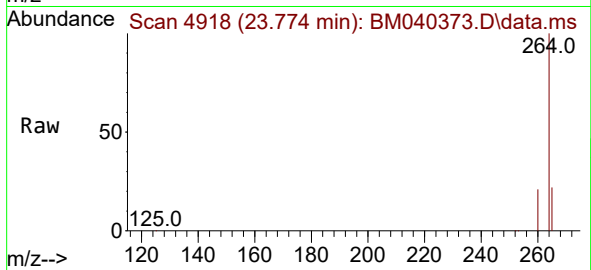

Tgt Ion:252 Resp: 5379
Ion Ratio Lower Upper
252 100
253 48.8 22.9 34.3#
125 49.5 21.0 31.4#

