

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062323\
 Data File : BM040379.D
 Acq On : 23 Jun 2023 17:20
 Operator : MA/JU
 Sample : PB153416BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK416

Quant Time: Jun 24 01:37:45 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 23 00:44:24 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.949	152	7751	0.400	ng/ul	0.00
4) Naphthalene-d8	10.756	136	28540	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.586	164	13803	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.332	188	27540	0.400	ng/ul	0.00
17) Chrysene-d12	21.515	240	18342	0.400	ng/ul	0.00
23) Perylene-d12	23.929	264	17937	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.329	96	64121	5.267	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.345	152	13195	0.330	ng/ul	0.00
18) Fluoranthene-d10	19.361	212	20249	0.344	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.581	166	4274	0.077	ng/ul#	15
20) Pyrene	19.723	202	3469	0.042	ng/ul#	1
26) Benzo(a)pyrene	23.777	252	5793	0.093	ng/ul#	57


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062323\
Data File : BM040379.D
Acq On : 23 Jun 2023 17:20
Operator : MA/JU
Sample : PB153416BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK416

Quant Time: Jun 24 01:37:45 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 23 00:44:24 2023
Response via : Initial Calibration




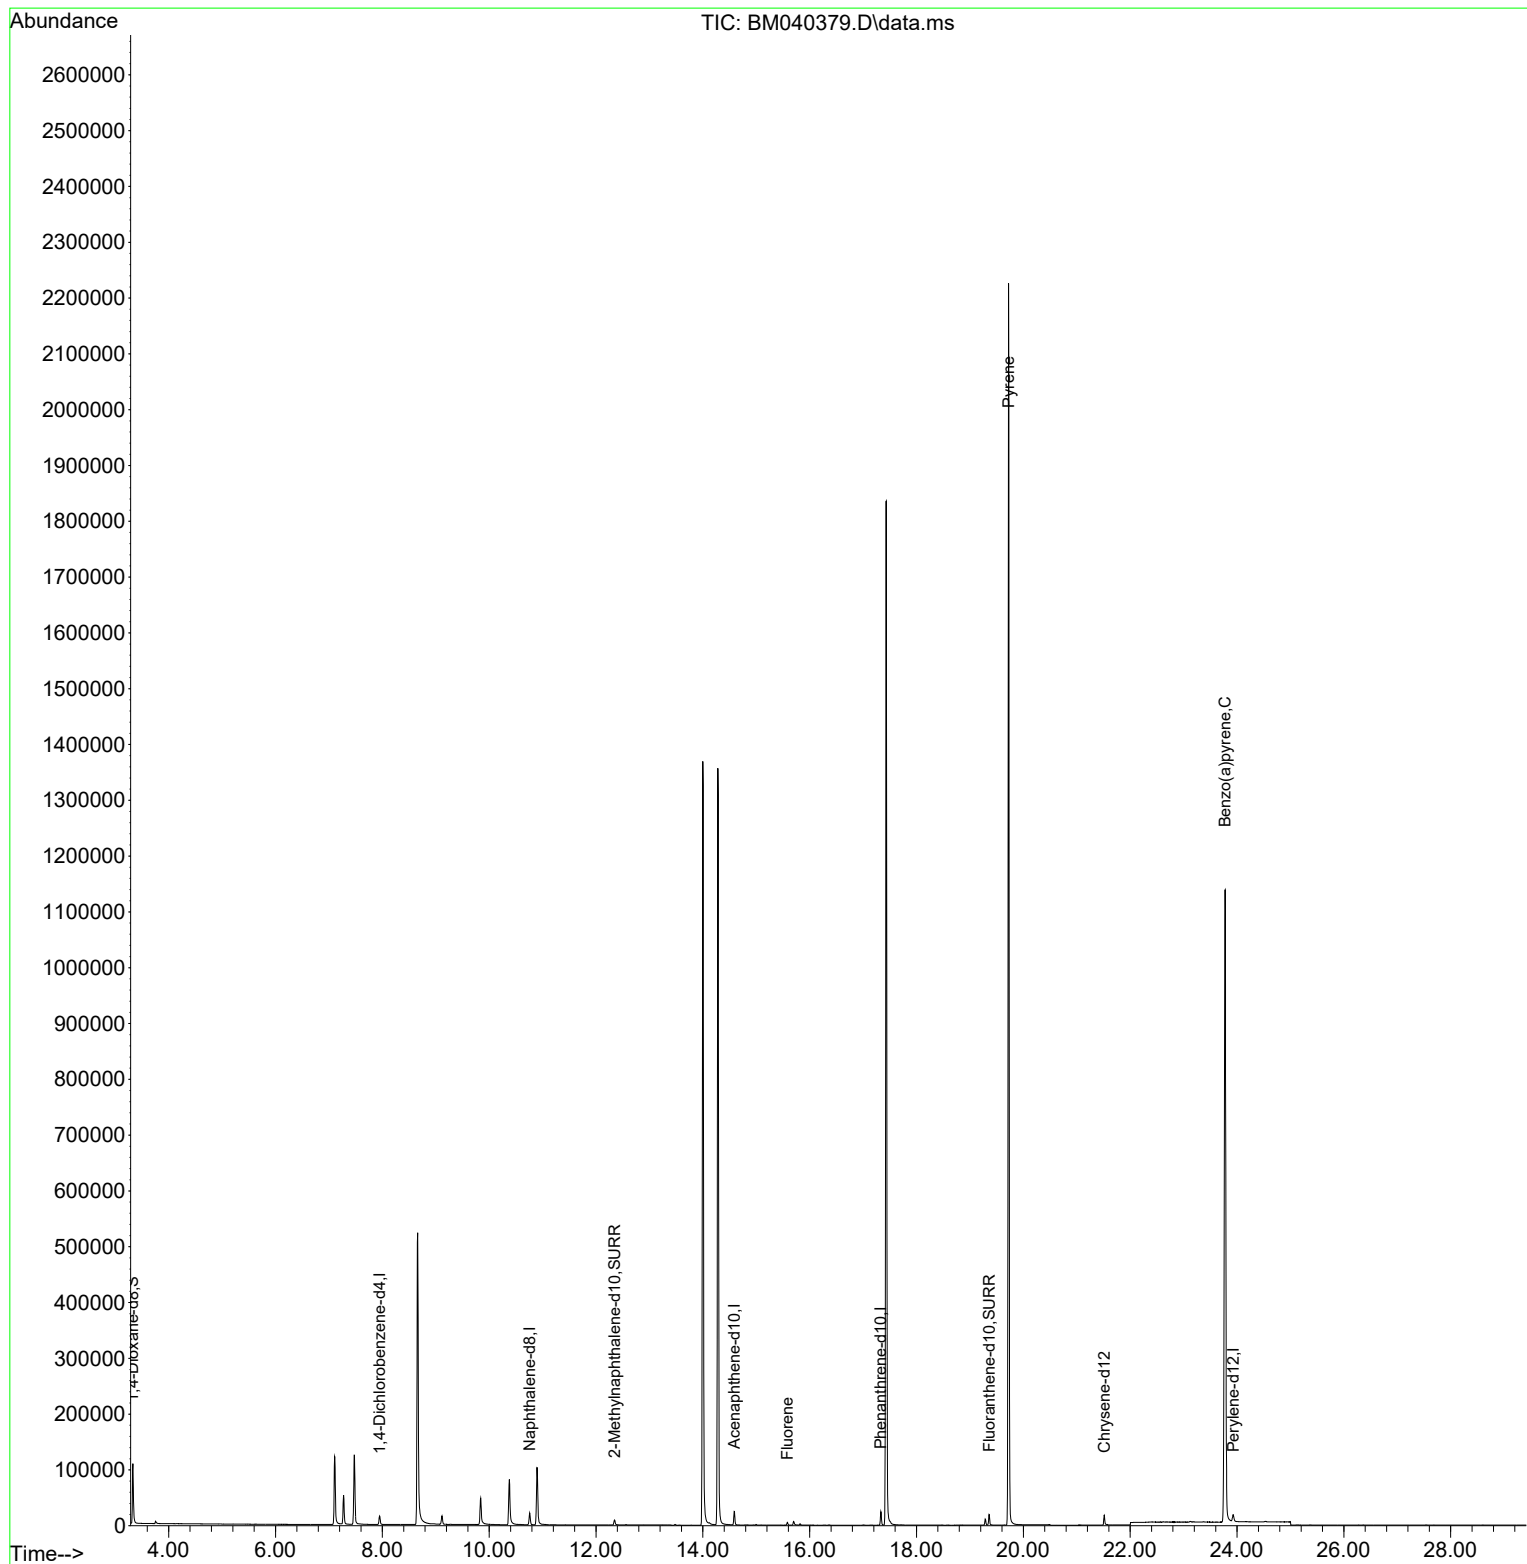


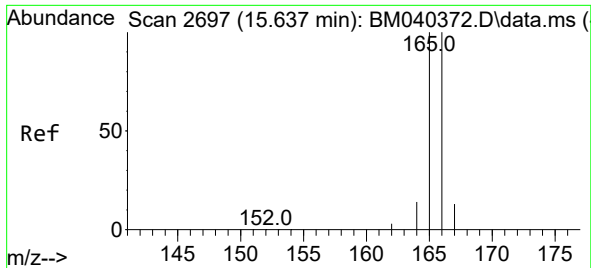

#12
Fluorene
Concen: 0.077 ng/ul
RT: 15.581 min Scan# 20
Delta R.T. -0.060 min
Lab File: BM040379.D
Acq: 23 Jun 2023 17:20




Instrument :
BNA_M
ClientSampleId :
SBLK416


Tgt Ion:166 Resp: 4274
Ion Ratio Lower Upper
166 100
165 8.5 79.6 119.4#
167 32.5 11.4 17.0#

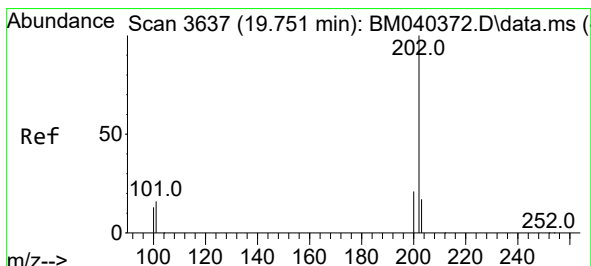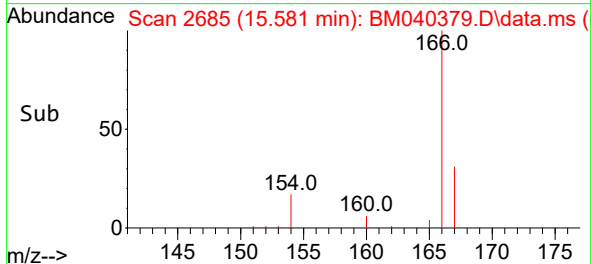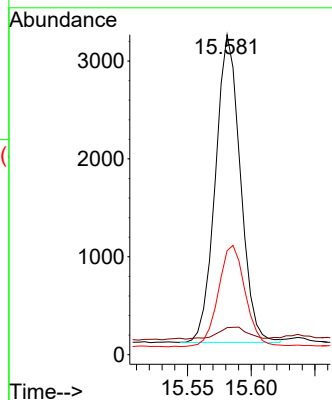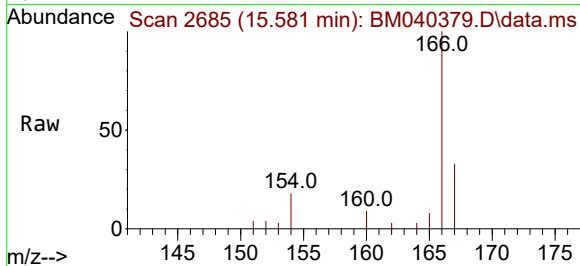

#20
Pyrene
Concen: 0.042 ng/ul
RT: 19.723 min Scan# 3631
Delta R.T. -0.033 min
Lab File: BM040379.D
Acq: 23 Jun 2023 17:20


Tgt Ion:202 Resp: 3469
Ion Ratio Lower Upper
202 100
101 167.0 12.6 18.8#
100 1284.8 9.8 14.6#

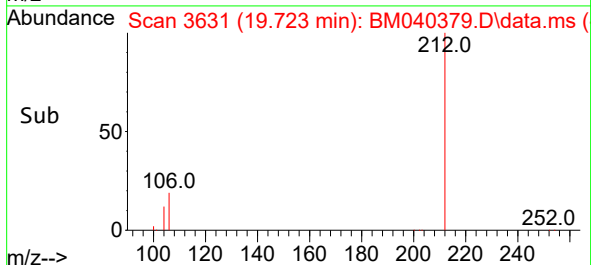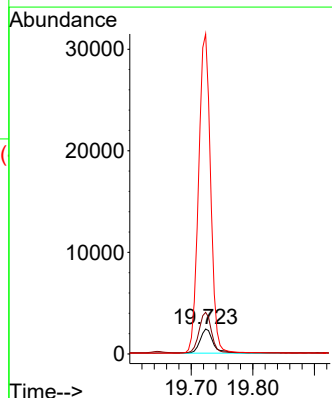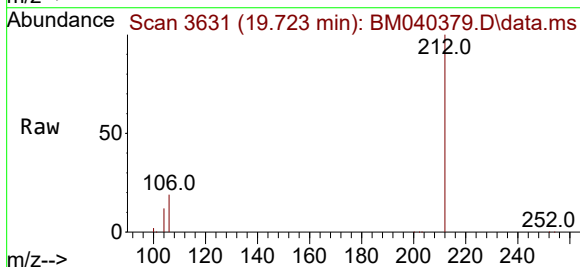

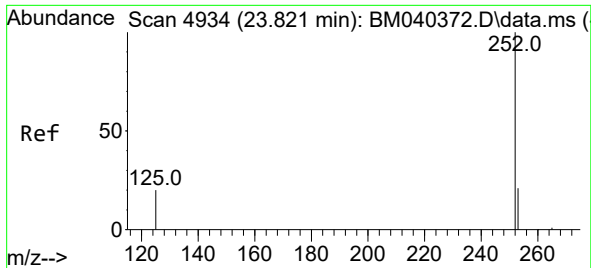

#26
Benzo(a)pyrene
Concen: 0.093 ng/ul
RT: 23.777 min Scan# 4919
Delta R.T. -0.047 min
Lab File: BM040379.D
Acq: 23 Jun 2023 17:20

Instrument :
BNA_M
ClientSampleId :
SBLK416

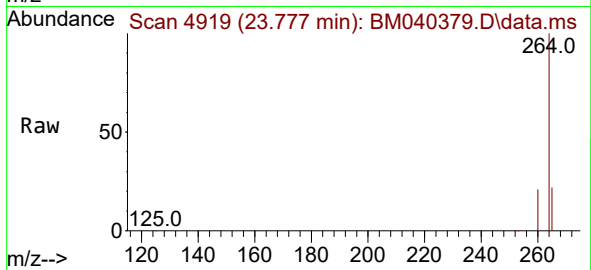

Tgt Ion:252 Resp: 5793
Ion Ratio Lower Upper
252 100
253 49.6 22.9 34.3#
125 50.5 21.0 31.4#

