


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM062419\
 Data File : BM021141.D
 Acq On : 24 Jun 2019 09:24
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM062019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jun 20 15:39:58 2019

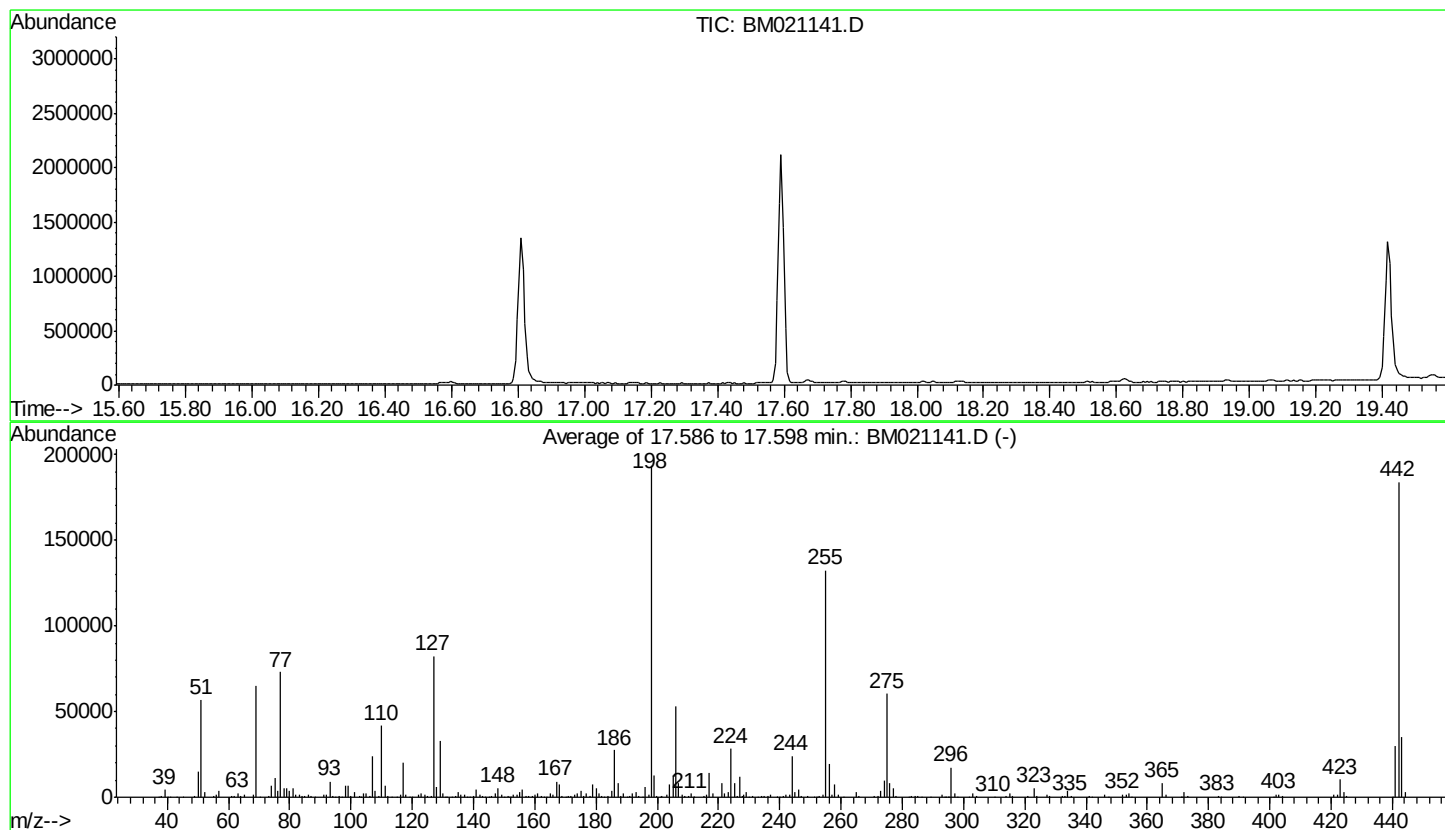

AutoFind: Scans 2482, 2483, 2484; Background Corrected with Scan 2475

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.4	56832	PASS
68	69	0.00	2	1.8	1195	PASS
69	198	0.00	100	33.5	64842	PASS
70	69	0.00	2	0.5	336	PASS
127	198	10	80	42.7	82565	PASS
197	198	0.00	2	0.7	1435	PASS
198	198	100	100	100.0	193514	PASS
199	198	5	9	6.7	13060	PASS
275	198	10	60	31.2	60362	PASS
365	198	1	100	4.4	8498	PASS
441	198	0.01	100	15.3	29629	PASS
442	198	50	100	95.0	183829	PASS
443	442	15	24	19.1	35122	PASS