


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM062421\
Data File : BM030579.D
Acq On : 24 Jun 2021 17:26
Operator : CG/JU
Sample : PB137202BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK202

Manual Integrations
APPROVED

mohammad
6/25/2021 1:08:30 PM

Quant Time: Jun 24 18:06:06 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SFAM-EPA-SIM-BM062321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 24 12:48:41 2021
Response via : Initial Calibration

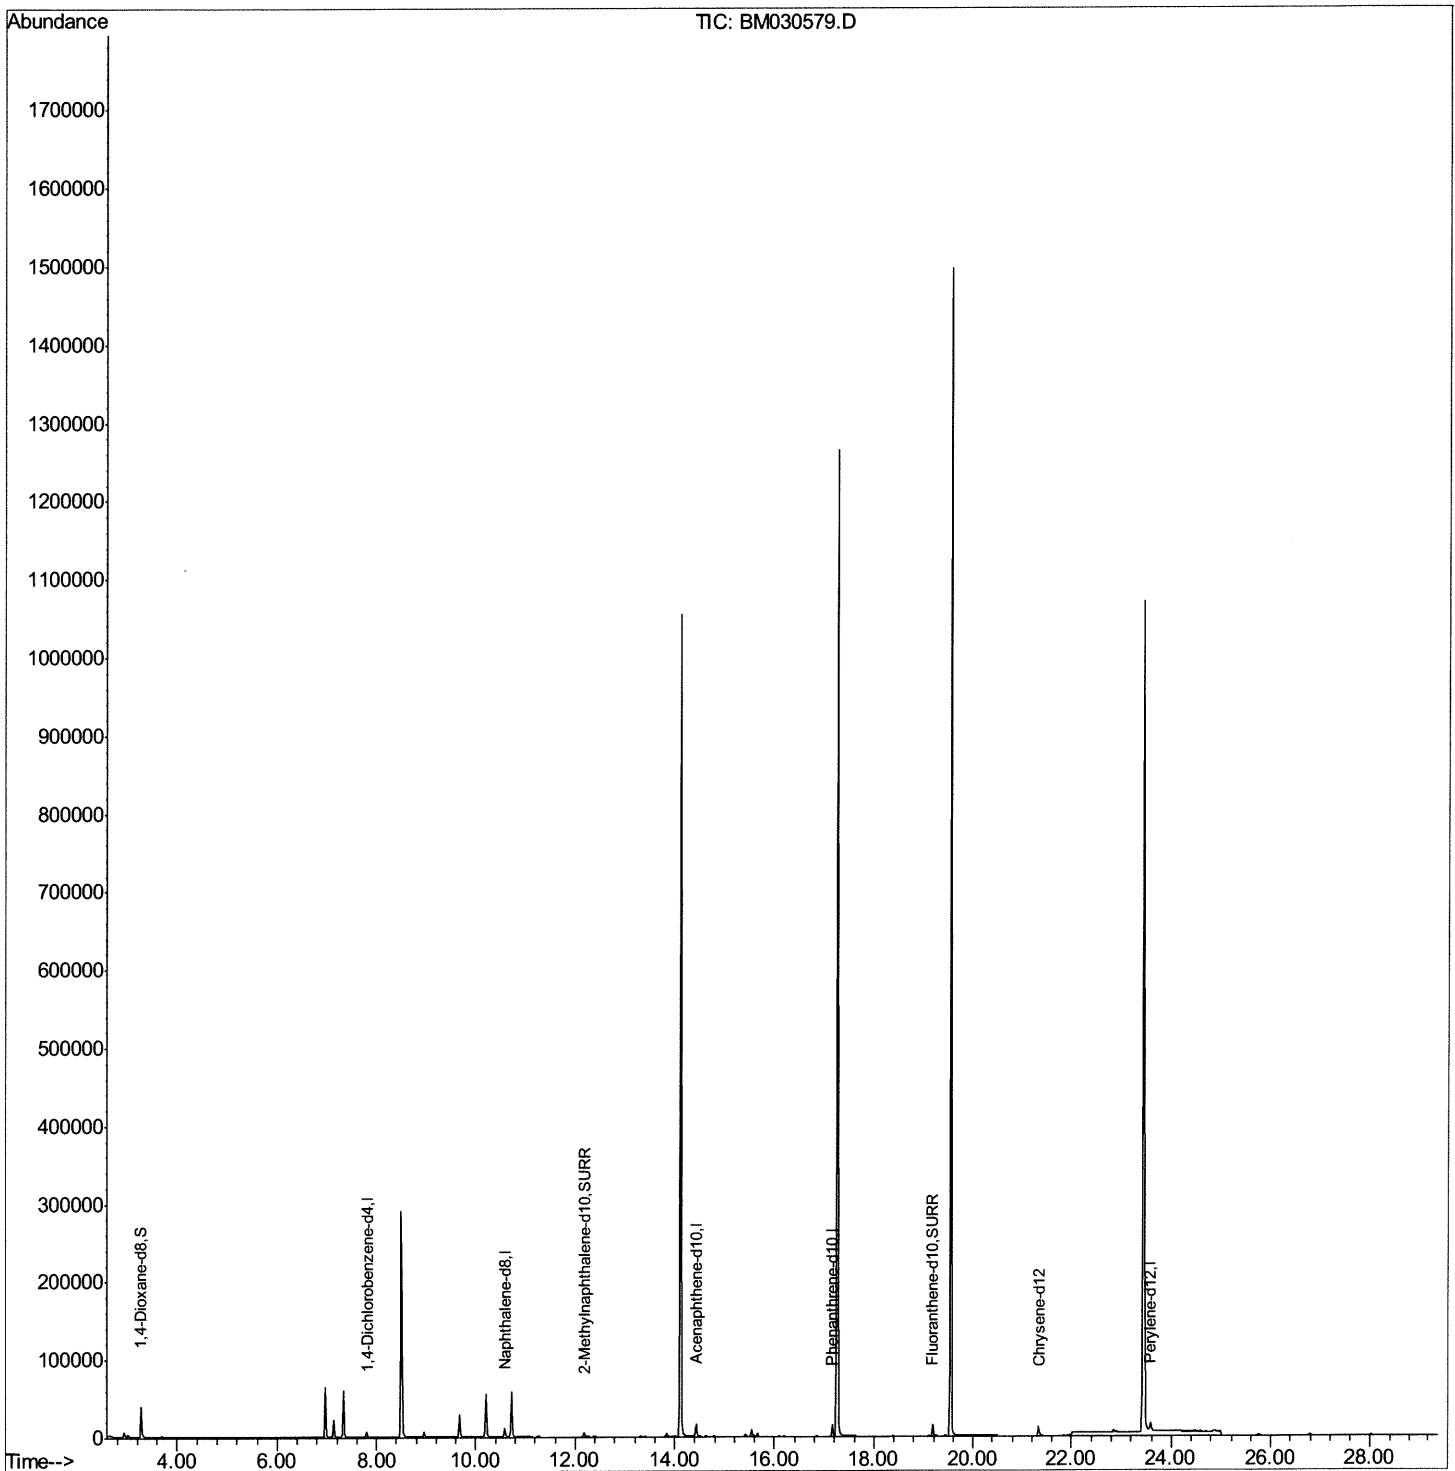

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM062421\
Data File : BM030579.D
Acq On : 24 Jun 2021 17:26
Operator : CG/JU
Sample : PB137202BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK202

Manual Integrations
APPROVED

mohammad
6/25/2021 1:08:30 PM

Quant Time: Jun 24 18:05:02 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SFAM-EPA-SIM-BM062321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 24 12:48:41 2021
Response via : Initial Calibration

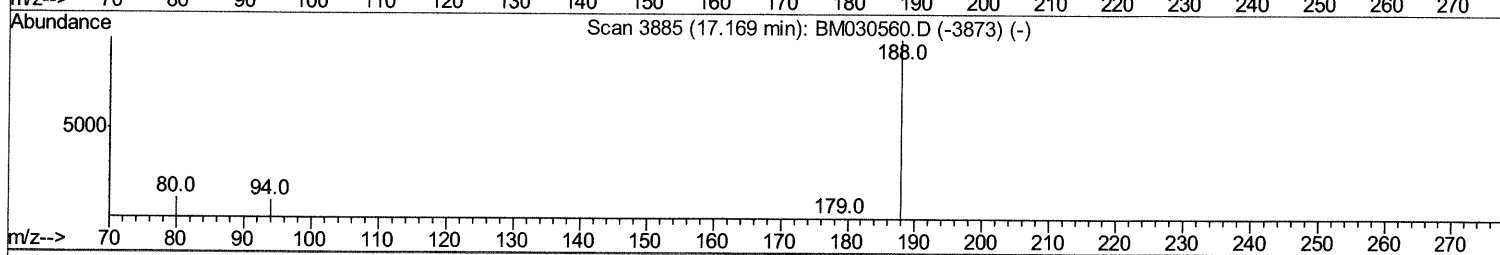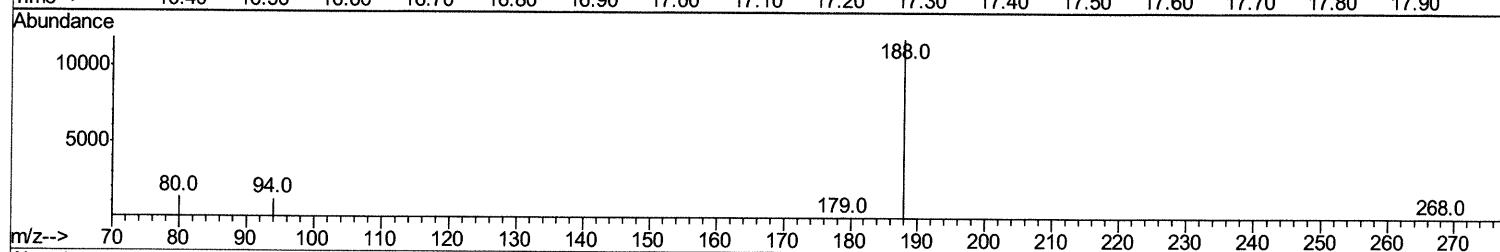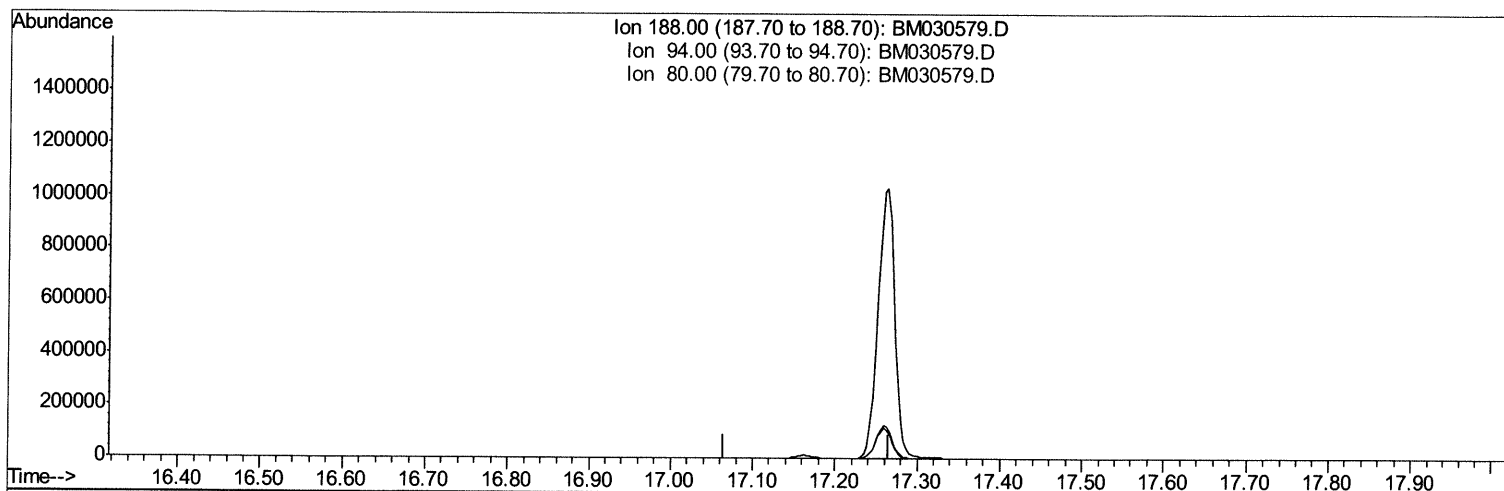

TIC: BM030579.D

(13) Phenanthrene-d10 (I)

17.166min (-17.166) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	10.30	0.00#
80.00	11.60	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM062421\
 Data File : BM030579.D
 Acq On : 24 Jun 2021 17:26
 Operator : CG/JU
 Sample : PB137202BL
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK202

Manual Integrations
 APPROVED

mohammad
 6/25/2021 1:08:30 PM

Quant Time: Jun 24 18:05:02 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SFAM-EPA-SIM-BM062321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jun 24 12:48:41 2021
 Response via : Initial Calibration

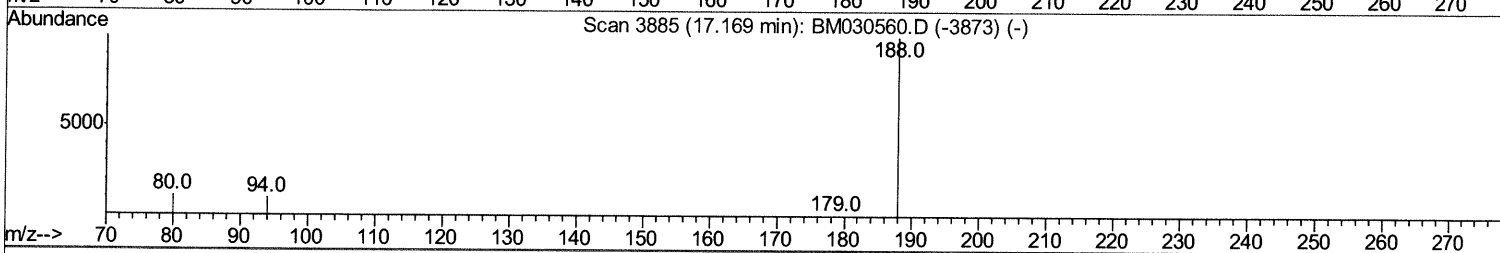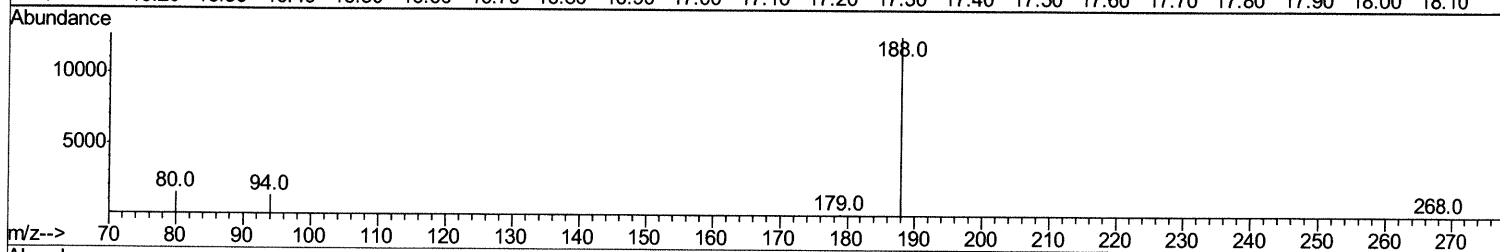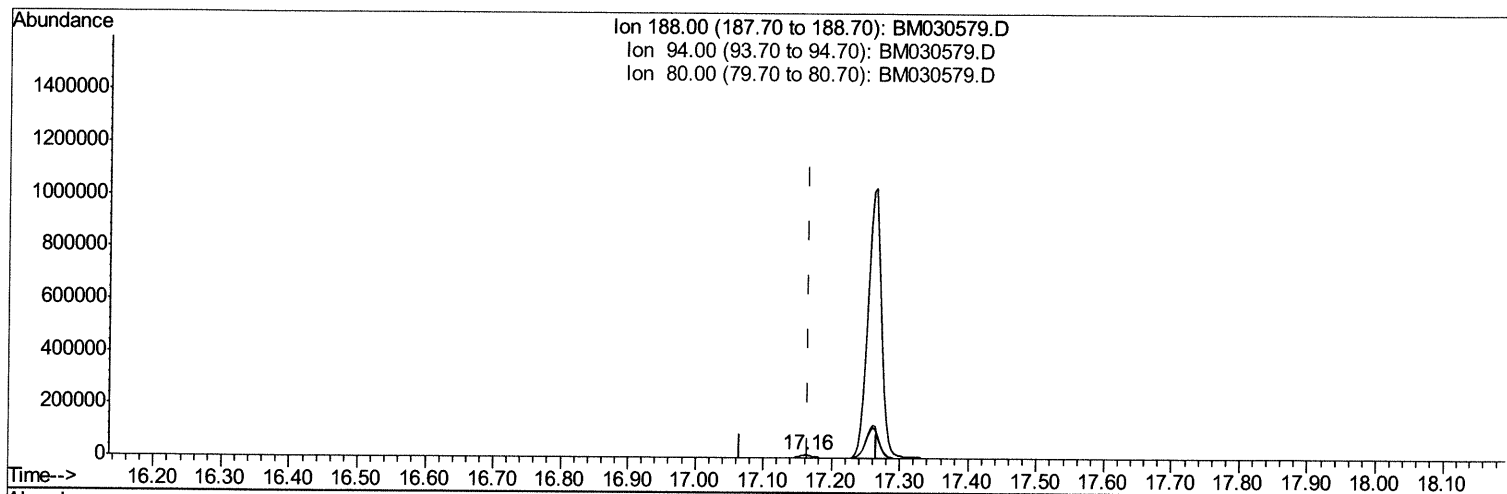

TIC: BM030579.D

(13) Phenanthrene-d10 (I)

17.162min (-0.004) 0.40ng/ul m 06/28/21 JU

response 17447

Ion	Exp%	Act%
188.00	100	100
94.00	10.30	10.56
80.00	11.60	11.69
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM062421\
Data File : BM030579.D
Acq On : 24 Jun 2021 17:26
Operator : CG/JU
Sample : PB137202BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK202

Manual Integrations
APPROVED

mohammad
6/25/2021 1:08:30 PM

Quant Time: Jun 24 18:06:06 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SFAM-EPA-SIM-BM062321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 24 12:48:41 2021
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.80	152	3860	0.40	ng/ul	0.00
4) Naphthalene-d8	10.59	136	15280	0.40	ng/ul	0.00
9) Acenaphthene-d10	14.43	164	9436	0.40	ng/ul	0.00
13) Phenanthrene-d10	17.16	188	17447m >	0.40	ng/ul >	0.00
17) Chrysene-d12	21.34	240	13494	0.40	ng/ul	0.00
23) Perylene-d12	23.59	264	16114	0.40	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.28	96	25405	6.15	ng/ul	-0.01
6) 2-Methylnaphthalene-d10	12.18	152	8506	0.35	ng/ul	0.00
18) Fluoranthene-d10	19.18	212	16474	0.40	ng/ul	0.00

Target Compounds	Ovalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed