

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062421\
 Data File : BM030583.D
 Acq On : 24 Jun 2021 19:52
 Operator : CG/JU
 Sample : M2662-18
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGDE7

Quant Time: Jun 25 02:26:53 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM062321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jun 24 12:48:41 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.798	152	3561	0.400	ng/ul	0.00
4) Naphthalene-d8	10.585	136	14415	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.424	164	8871	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.162	188	18023	0.400	ng/ul	0.00
17) Chrysene-d12	21.330	240	15578	0.400	ng/ul	0.00
23) Perylene-d12	23.588	264	15251	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.279	96	9799	2.572	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.178	152	4100	0.178	ng/ul	0.00
18) Fluoranthene-d10	19.184	212	11025	0.231	ng/ul	0.00
Target Compounds						
					Qvalue	
5) Naphthalene	10.635	128	2432	0.057	ng/ul#	92
19) Fluoranthene	19.214	202	2281	0.032	ng/ul#	74
20) Pyrene	19.573	202	1679	0.023	ng/ul#	65


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062421\
Data File : BM030583.D
Acq On : 24 Jun 2021 19:52
Operator : CG/JU
Sample : M2662-18
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGDE7

Quant Time: Jun 25 02:26:53 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM062321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 24 12:48:41 2021
Response via : Initial Calibration




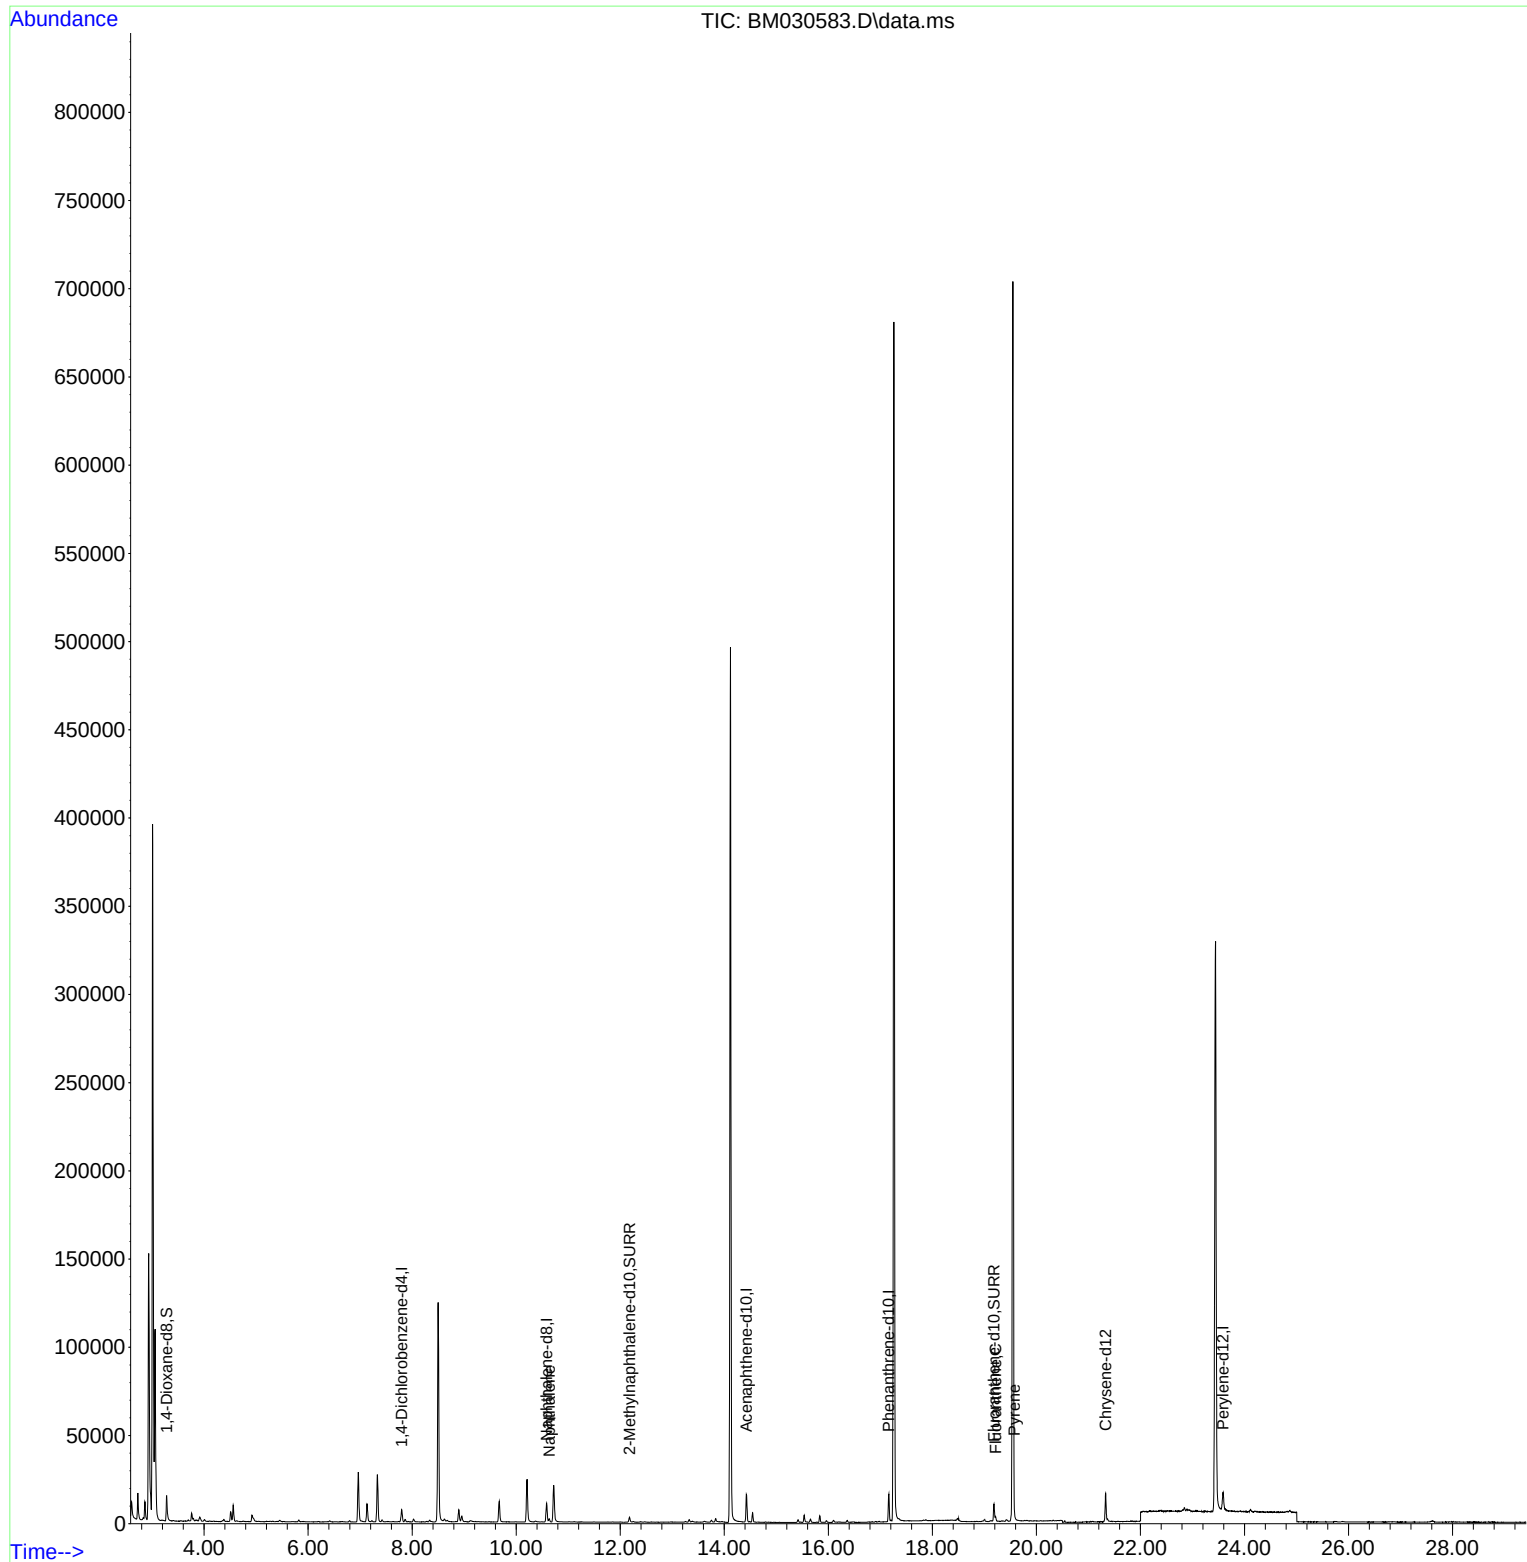


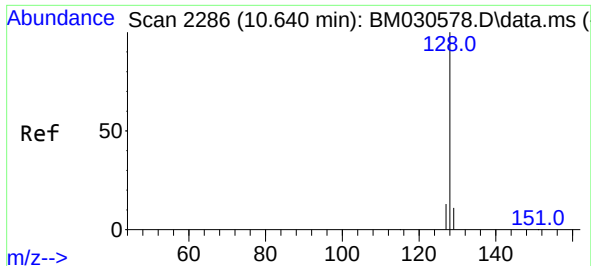

#5
Naphthalene
Concen: 0.057 ng/ul
RT: 10.635 min Scan# 2285
Delta R.T. -0.005 min
Lab File: BM030583.D
Acq: 24 Jun 2021 19:52




Instrument :
BNA_M
ClientSampled :
BGDE7


Tgt Ion:128 Resp: 2432
Ion Ratio Lower Upper
128 100
129 15.1 9.0 13.6#
127 16.3 10.9 16.3

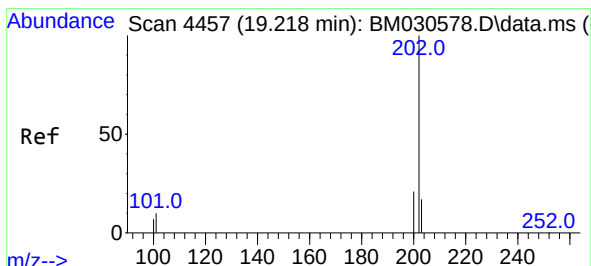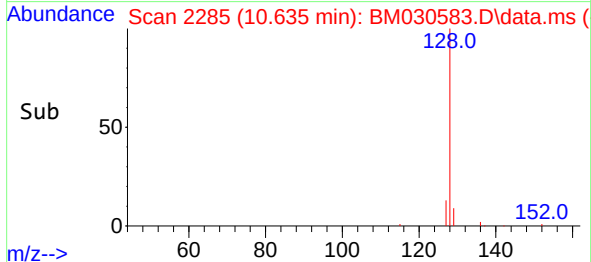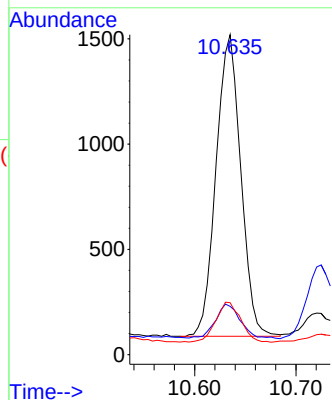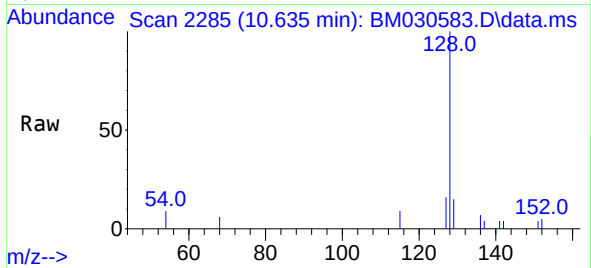

#19
Fluoranthene
Concen: 0.032 ng/ul
RT: 19.214 min Scan# 4456
Delta R.T. -0.004 min
Lab File: BM030583.D
Acq: 24 Jun 2021 19:52

Tgt Ion:202 Resp: 2281
Ion Ratio Lower Upper
202 100
101 20.7 8.8 13.2#
100 18.3 6.9 10.3#

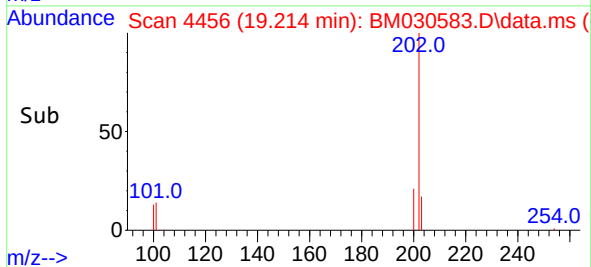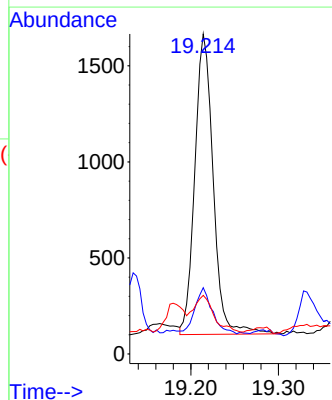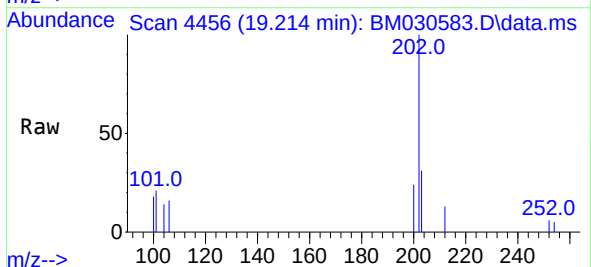

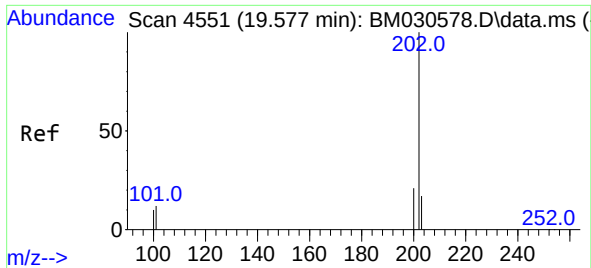

#20
Pyrene
Concen: 0.023 ng/ul
RT: 19.573 min Scan# 4550
Delta R.T. -0.008 min
Lab File: BM030583.D
Acq: 24 Jun 2021 19:52

Instrument :
BNA_M
ClientSampleId :
BGDE7

Tgt Ion:202 Resp: 1679
Ion Ratio Lower Upper
202 100
101 22.0 10.1 15.1#
100 28.6 8.2 12.2#

