
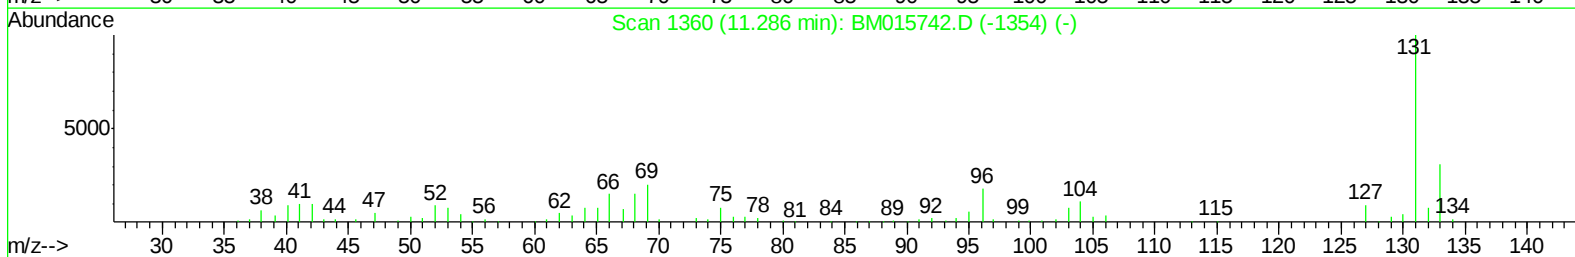
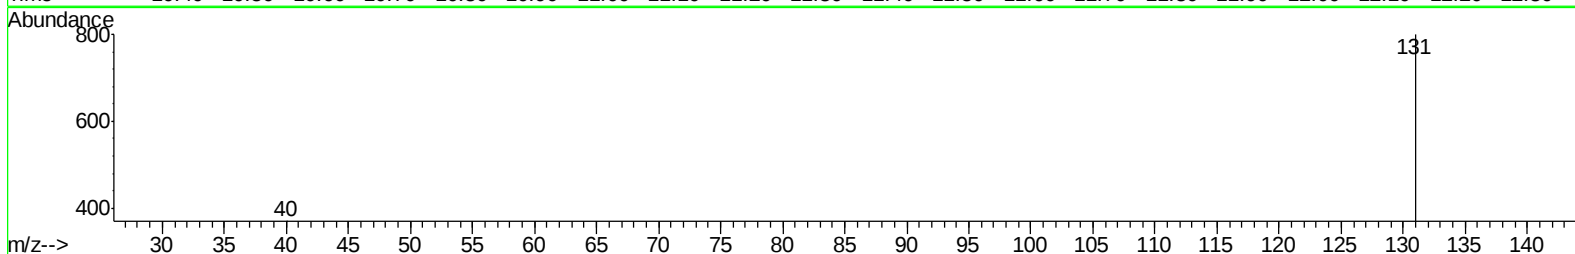


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM062518\
Data File : BM015745.D
Acq On : 25 Jun 2018 12:11
Operator : SJ/JU
Sample : J3569-25 5X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Quant Time: Jun 26 01:36:08 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM060818MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jun 26 01:35:35 2018
Response via : Initial Calibration

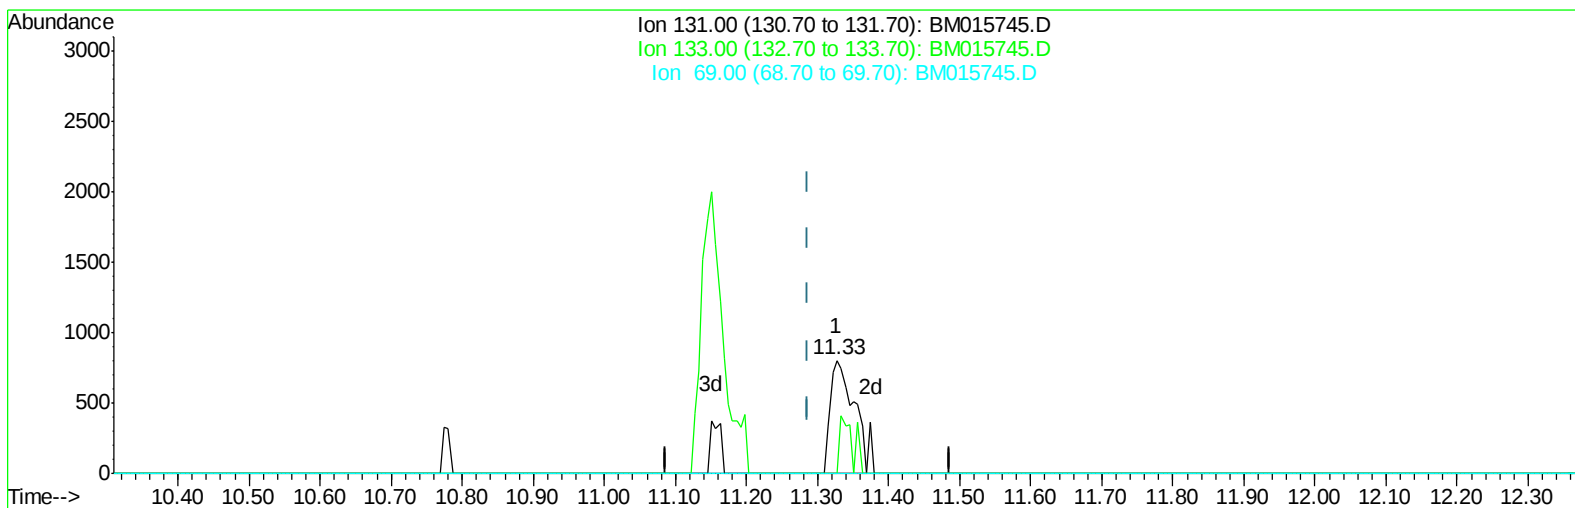

TIC: BM015745.D

(29) 4-Chloroaniline-d4 (S)

11.327min (+0.041) 0.26ng/ul m

response 1775

Ion	Exp%	Act%
131.00	100	100
133.00	32.10	0.00#
69.00	16.20	0.00#
0.00	0.00	0.00