

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM062518\
 Data File : BM015743.D
 Acq On : 25 Jun 2018 10:52
 Operator : SJ/JU
 Sample : PB110519BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Jun 26 01:35:57 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM060818MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jun 26 01:35:35 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.32	152	82090	20.00	ng/ul	0.00
18) Naphthalene-d8	11.15	136	363751	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.93	164	204115	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.66	188	459171	20.00	ng/ul	0.00
77) Chrysene-d12	21.77	240	454423	20.00	ng/ul	0.00
85) Perylene-d12	24.17	264	423552	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.53	96	11295	6.69	ng/uL	0.00
5) Phenol-d5	7.46	99	215676	28.94	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.63	67	143952	31.97	ng/ul	0.00
9) 2-Chlorophenol-d4	7.84	132	190156	33.37	ng/ul	0.00
13) 4-Methylphenol-d8	9.03	113	181105	28.21	ng/ul	0.00
19) Nitrobenzene-d5	9.50	128	86688	35.44	ng/ul	0.00
22) 2-Nitrophenol-d4	10.23	143	95035	36.13	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.77	165	180176	33.08	ng/ul	0.00
29) 4-Chloroaniline-d4	11.29	131	261993	43.16	ng/ul	0.00
43) Dimethylphthalate-d6	14.33	166	621406	36.77	ng/ul	0.00
46) Acenaphthylene-d8	14.63	160	707223	38.80	ng/ul	0.00
51) 4-Nitrophenol-d4	15.13	143	72545	22.24	ng/ul	0.00
57) Fluorene-d10	15.92	176	516414	36.11	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	16.05	200	69478	25.12	ng/ul	0.00
70) Anthracene-d10	17.76	188	803341	38.38	ng/ul	0.00
78) Pyrene-d10	20.02	212	891238	45.59	ng/ul	0.00
89) Benzo(a)pyrene-d12	24.02	264	821114	38.67	ng/ul	0.00


Target Compounds				Ovalue
45) 2,6-Dinitrotoluene	14.34	165	3361	1.050 ng/ul# 38


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM062518\
Data File : BM015743.D
Acq On : 25 Jun 2018 10:52
Operator : SJ/JU
Sample : PB110519BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Jun 26 01:35:57 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM060818MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jun 26 01:35:35 2018
Response via : Initial Calibration

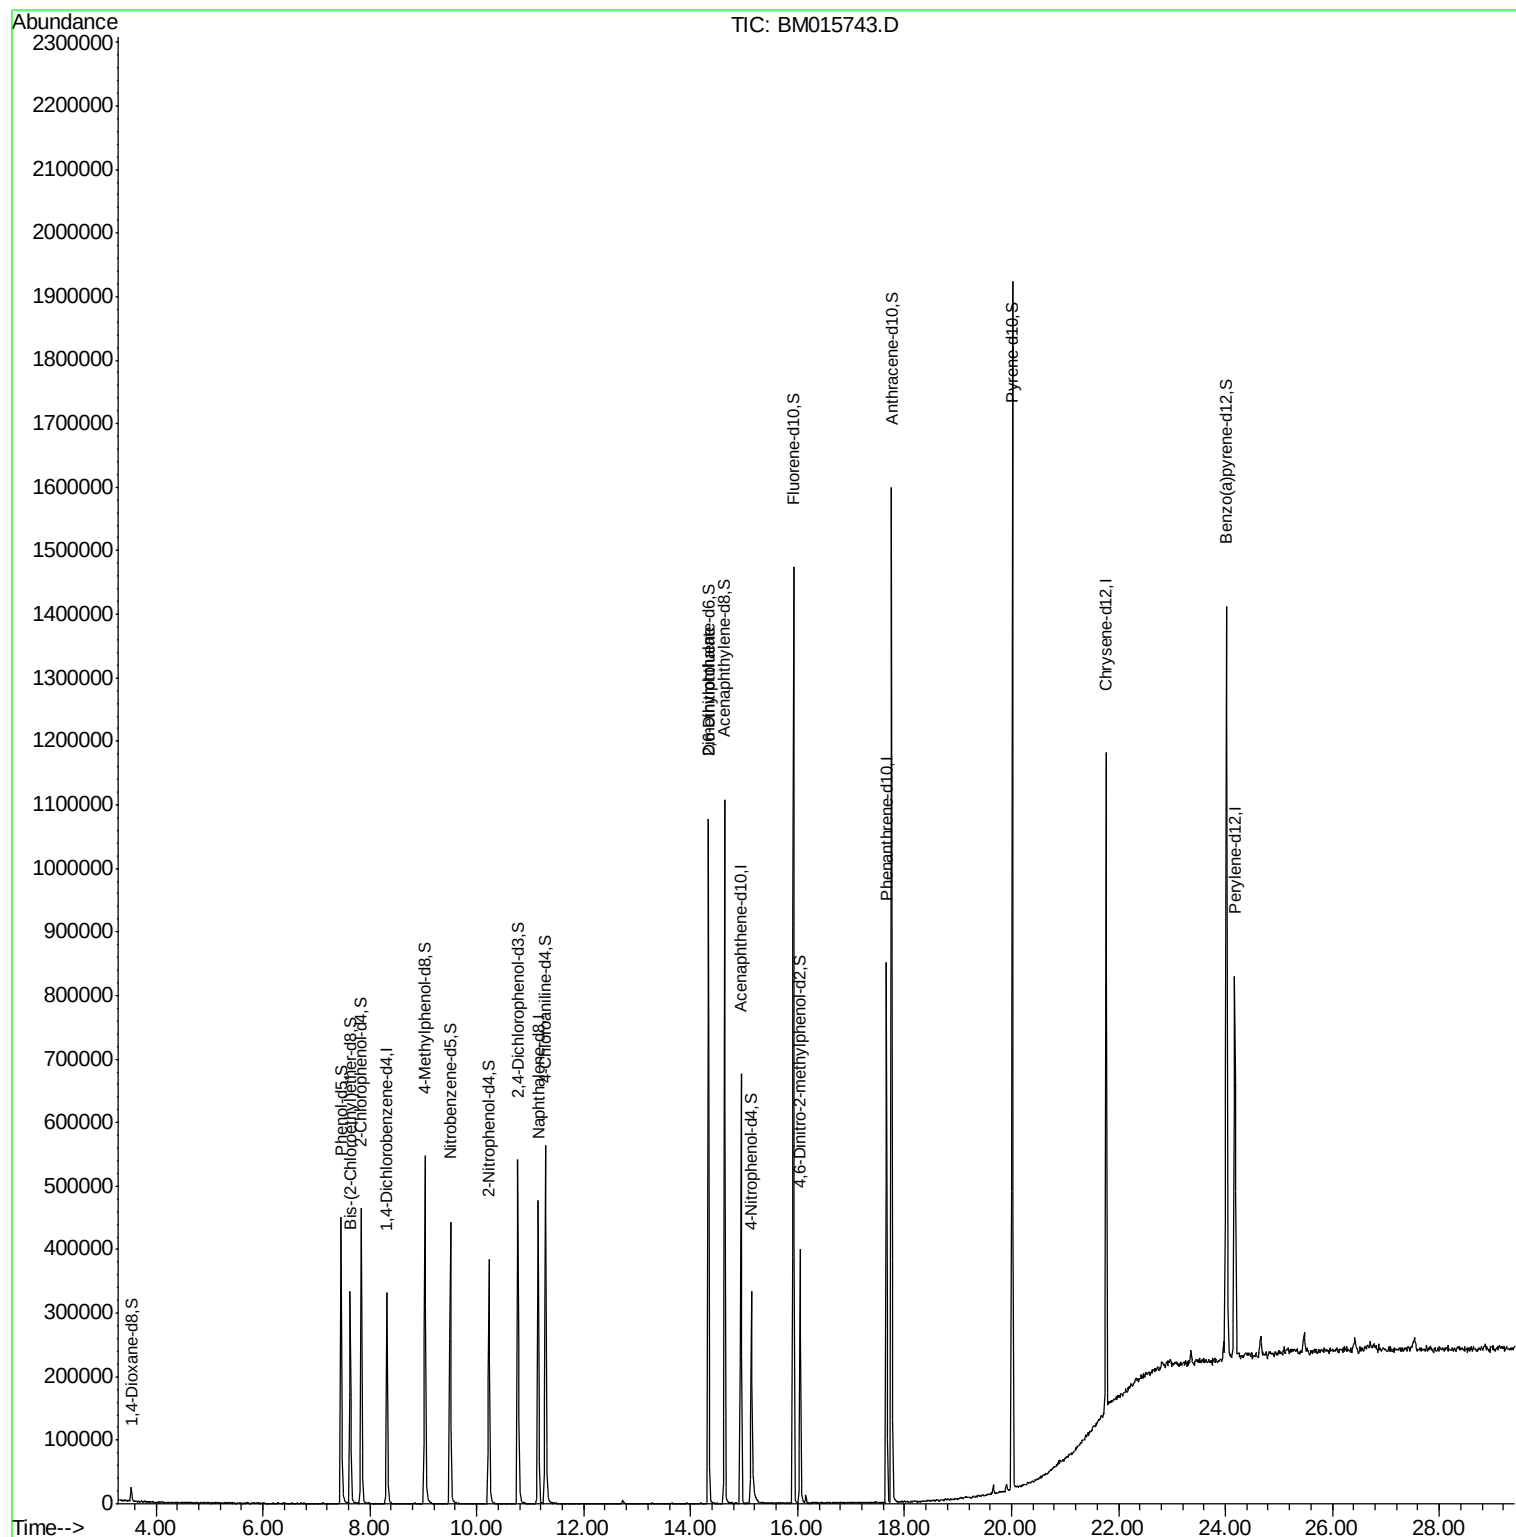

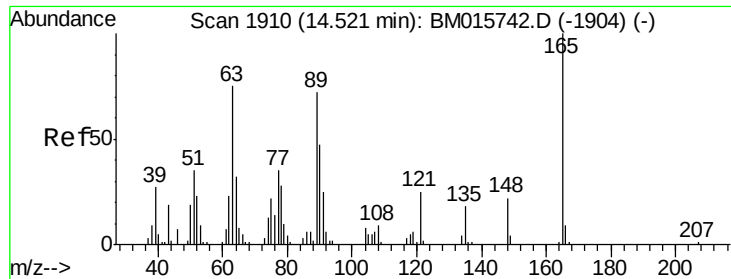

#45
 2,6-Dinitrotoluene
 Concen: 1.050 ng/ul
 RT: 14.34 min Scan# 1879
 Delta R.T. -0.18 min
 Lab File: BM015743.D
 Acq: 25 Jun 2018 10:52

Instrument :
 BNA_M
 ClientSampleId :

Tot Ion	Ratio	Lower	Upper
165	100		
89	0.0	42.4	63.6#
121	34.6	16.6	24.8#

