

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM062518\
 Data File : BM015744.D
 Acq On : 25 Jun 2018 11:34
 Operator : SJ/JU
 Sample : PB110517BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Jun 26 01:36:01 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM060818MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jun 26 01:35:35 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.32	152	81099	20.00	ng/ul	0.00
18) Naphthalene-d8	11.15	136	356717	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.93	164	202437	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.66	188	451797	20.00	ng/ul	0.00
77) Chrysene-d12	21.77	240	444095	20.00	ng/ul	0.00
85) Perylene-d12	24.17	264	417239	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.53	96	12581	7.54	ng/uL	0.00
5) Phenol-d5	7.46	99	212177	28.82	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.63	67	144413	32.47	ng/ul	0.00
9) 2-Chlorophenol-d4	7.84	132	186261	33.09	ng/ul	0.00
13) 4-Methylphenol-d8	9.03	113	179349	28.28	ng/ul	0.00
19) Nitrobenzene-d5	9.50	128	86368	36.01	ng/ul	0.00
22) 2-Nitrophenol-d4	10.23	143	94804	36.75	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.76	165	175277	32.81	ng/ul	0.00
29) 4-Chloroaniline-d4	11.29	131	255789	42.97	ng/ul	0.00
43) Dimethylphthalate-d6	14.33	166	618136	36.88	ng/ul	0.00
46) Acenaphthylene-d8	14.63	160	697805	38.60	ng/ul	0.00
51) 4-Nitrophenol-d4	15.13	143	71351	22.05	ng/ul	0.00
57) Fluorene-d10	15.92	176	511609	36.07	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	16.05	200	68844	25.30	ng/ul	0.00
70) Anthracene-d10	17.76	188	803465	39.01	ng/ul	0.00
78) Pyrene-d10	20.01	212	881061	46.12	ng/ul	0.00
89) Benzo(a)pyrene-d12	24.03	264	821213	39.26	ng/ul	0.00

Target Compounds


				Ovalue	
15) N-Nitroso-di-n-propylamine	9.03	70	5680	1.082 ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM062518\
Data File : BM015744.D
Acq On : 25 Jun 2018 11:34
Operator : SJ/JU
Sample : PB110517BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Jun 26 01:36:01 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM060818MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jun 26 01:35:35 2018
Response via : Initial Calibration

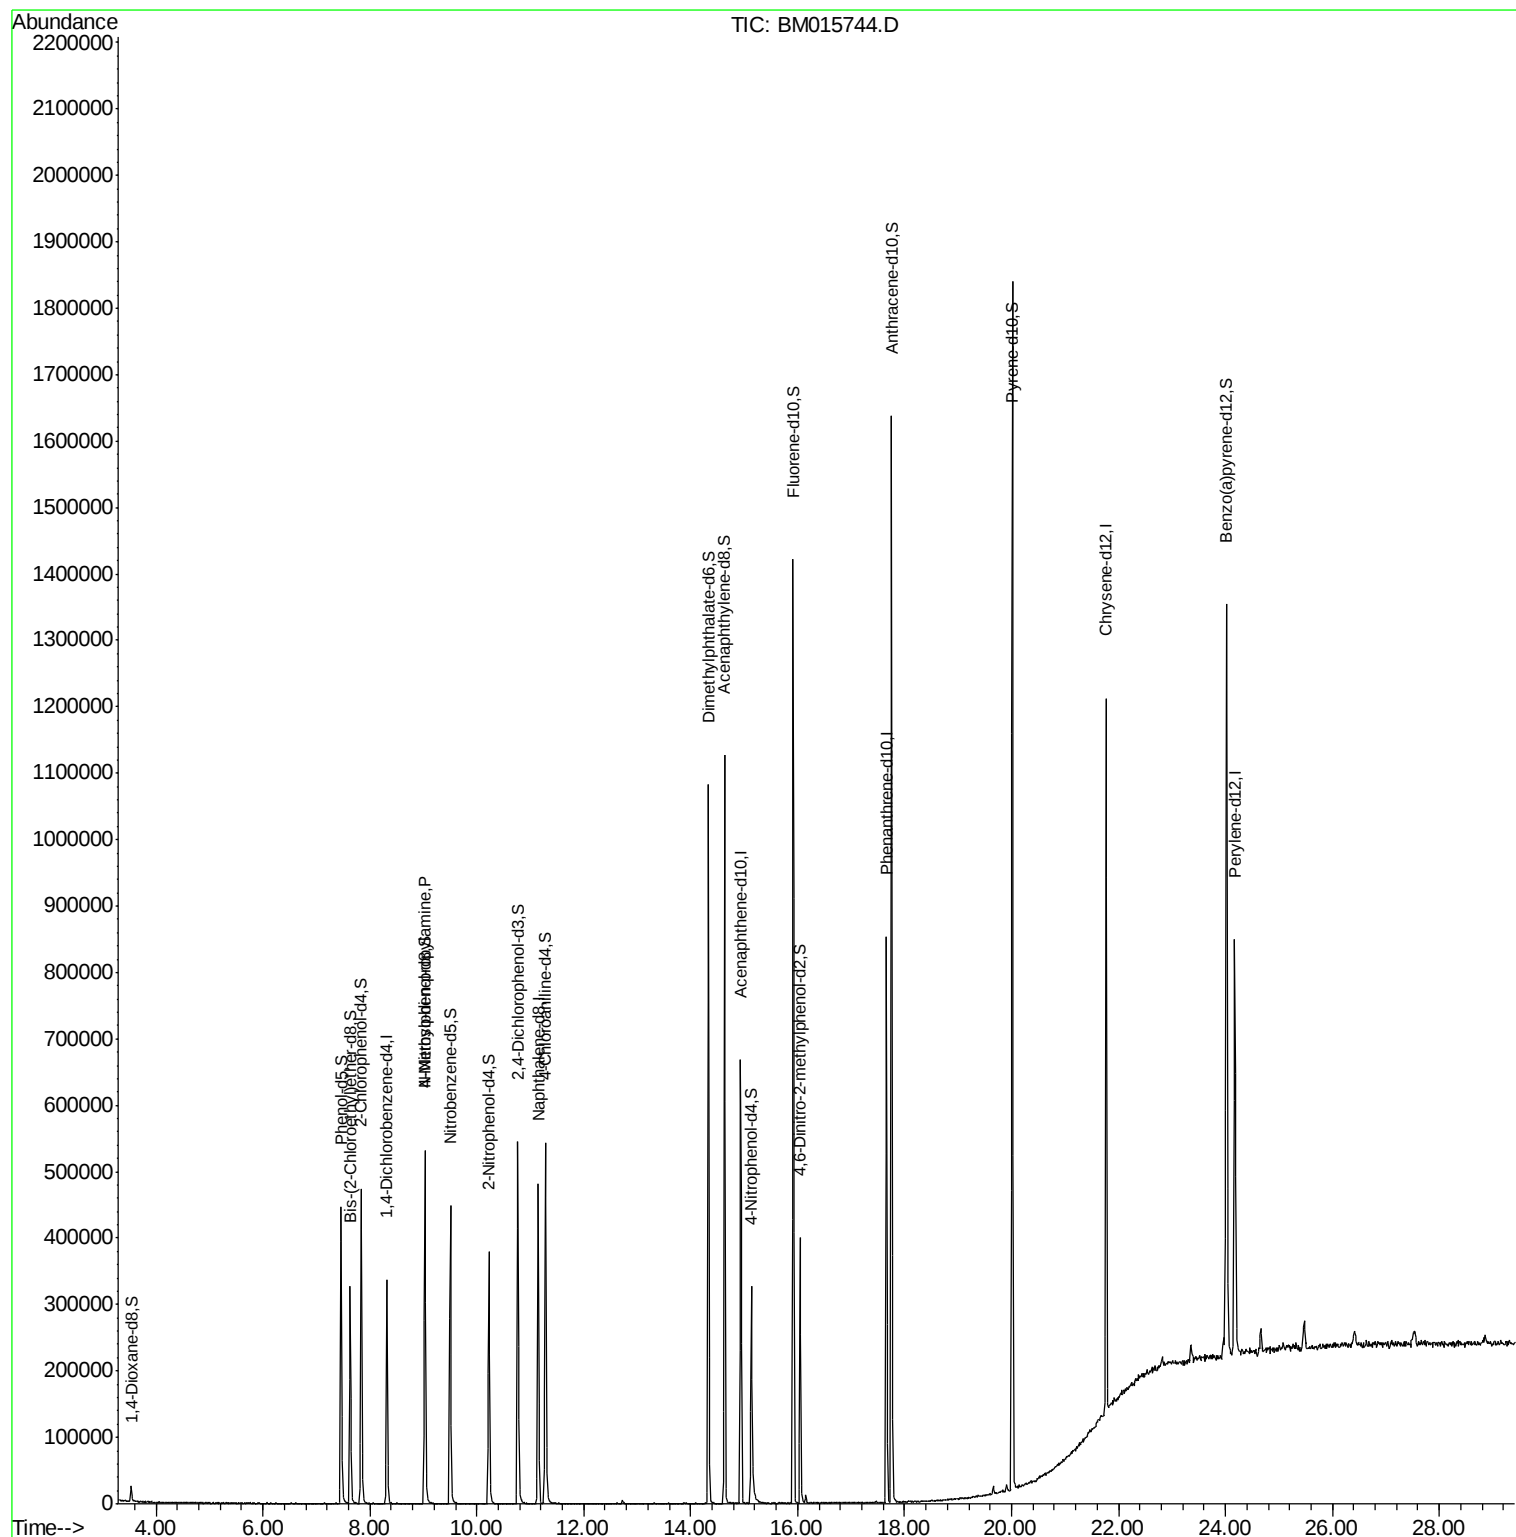

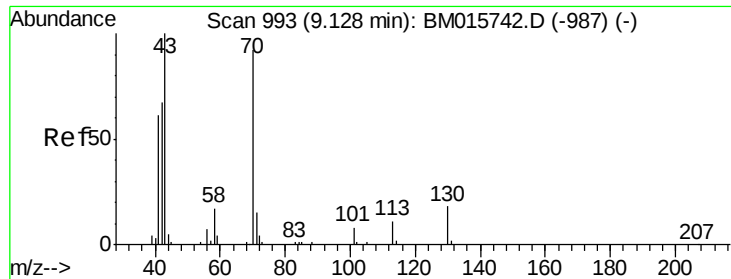

#15
 N-Nitroso-di-n-propylamine
 Concen: 1.082 ng/ul
 RT: 9.03 min Scan# 976
 Delta R.T. -0.10 min
 Lab File: BM015744.D
 Acq: 25 Jun 2018 11:34

Instrument :
 BNA_M
 ClientSampleId :

Tot Ion	Ratio	Lower	Upper
70	100		
42	518.8	35.4	53.0#
101	0.0	8.4	12.6#
130	0.0	18.2	27.4#

