

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM062518\
 Data File : BM015752.D
 Acq On : 25 Jun 2018 16:29
 Operator : SJ/JU
 Sample : J3569-13
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Jun 26 01:36:56 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM060818MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jun 26 01:35:35 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.32	152	106037	20.00	ng/ul	0.00
18) Naphthalene-d8	11.15	136	469999	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.93	164	258763	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.66	188	589285	20.00	ng/ul	0.00
77) Chrysene-d12	21.77	240	648374	20.00	ng/ul	0.00
85) Perylene-d12	24.17	264	610731	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.53	96	10547	4.83	ng/uL	0.00
5) Phenol-d5	7.46	99	220710	22.93	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.63	67	142853	24.56	ng/ul	0.00
9) 2-Chlorophenol-d4	7.84	132	191165	25.97	ng/ul	0.00
13) 4-Methylphenol-d8	9.03	113	185729	22.40	ng/ul	0.00
19) Nitrobenzene-d5	9.50	128	88605	28.04	ng/ul	0.00
22) 2-Nitrophenol-d4	10.23	143	98671	29.03	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.77	165	181313	25.76	ng/ul	0.00
29) 4-Chloroaniline-d4	11.29	131	253715	32.35	ng/ul	0.00
43) Dimethylphthalate-d6	14.33	166	570024	26.61	ng/ul	0.00
46) Acenaphthylene-d8	14.63	160	686171	29.70	ng/ul	0.00
51) 4-Nitrophenol-d4	15.14	143	60172	14.55	ng/ul	0.00
57) Fluorene-d10	15.92	176	490082	27.03	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	16.05	200	47152	13.28	ng/ul	0.00
70) Anthracene-d10	17.76	188	755877	28.14	ng/ul	0.00
78) Pyrene-d10	20.02	212	853503	30.60	ng/ul	0.00
89) Benzo(a)pyrene-d12	24.02	264	877799	28.67	ng/ul	0.00

Target Compounds


					Ovalue	
6) Phenol	7.49	94	17571	1.757	ng/ul#	68
44) Dimethylphthalate	14.38	163	216272	9.886	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM062518\
Data File : BM015752.D
Acq On : 25 Jun 2018 16:29
Operator : SJ/JU
Sample : J3569-13
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Jun 26 01:36:56 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM060818MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jun 26 01:35:35 2018
Response via : Initial Calibration

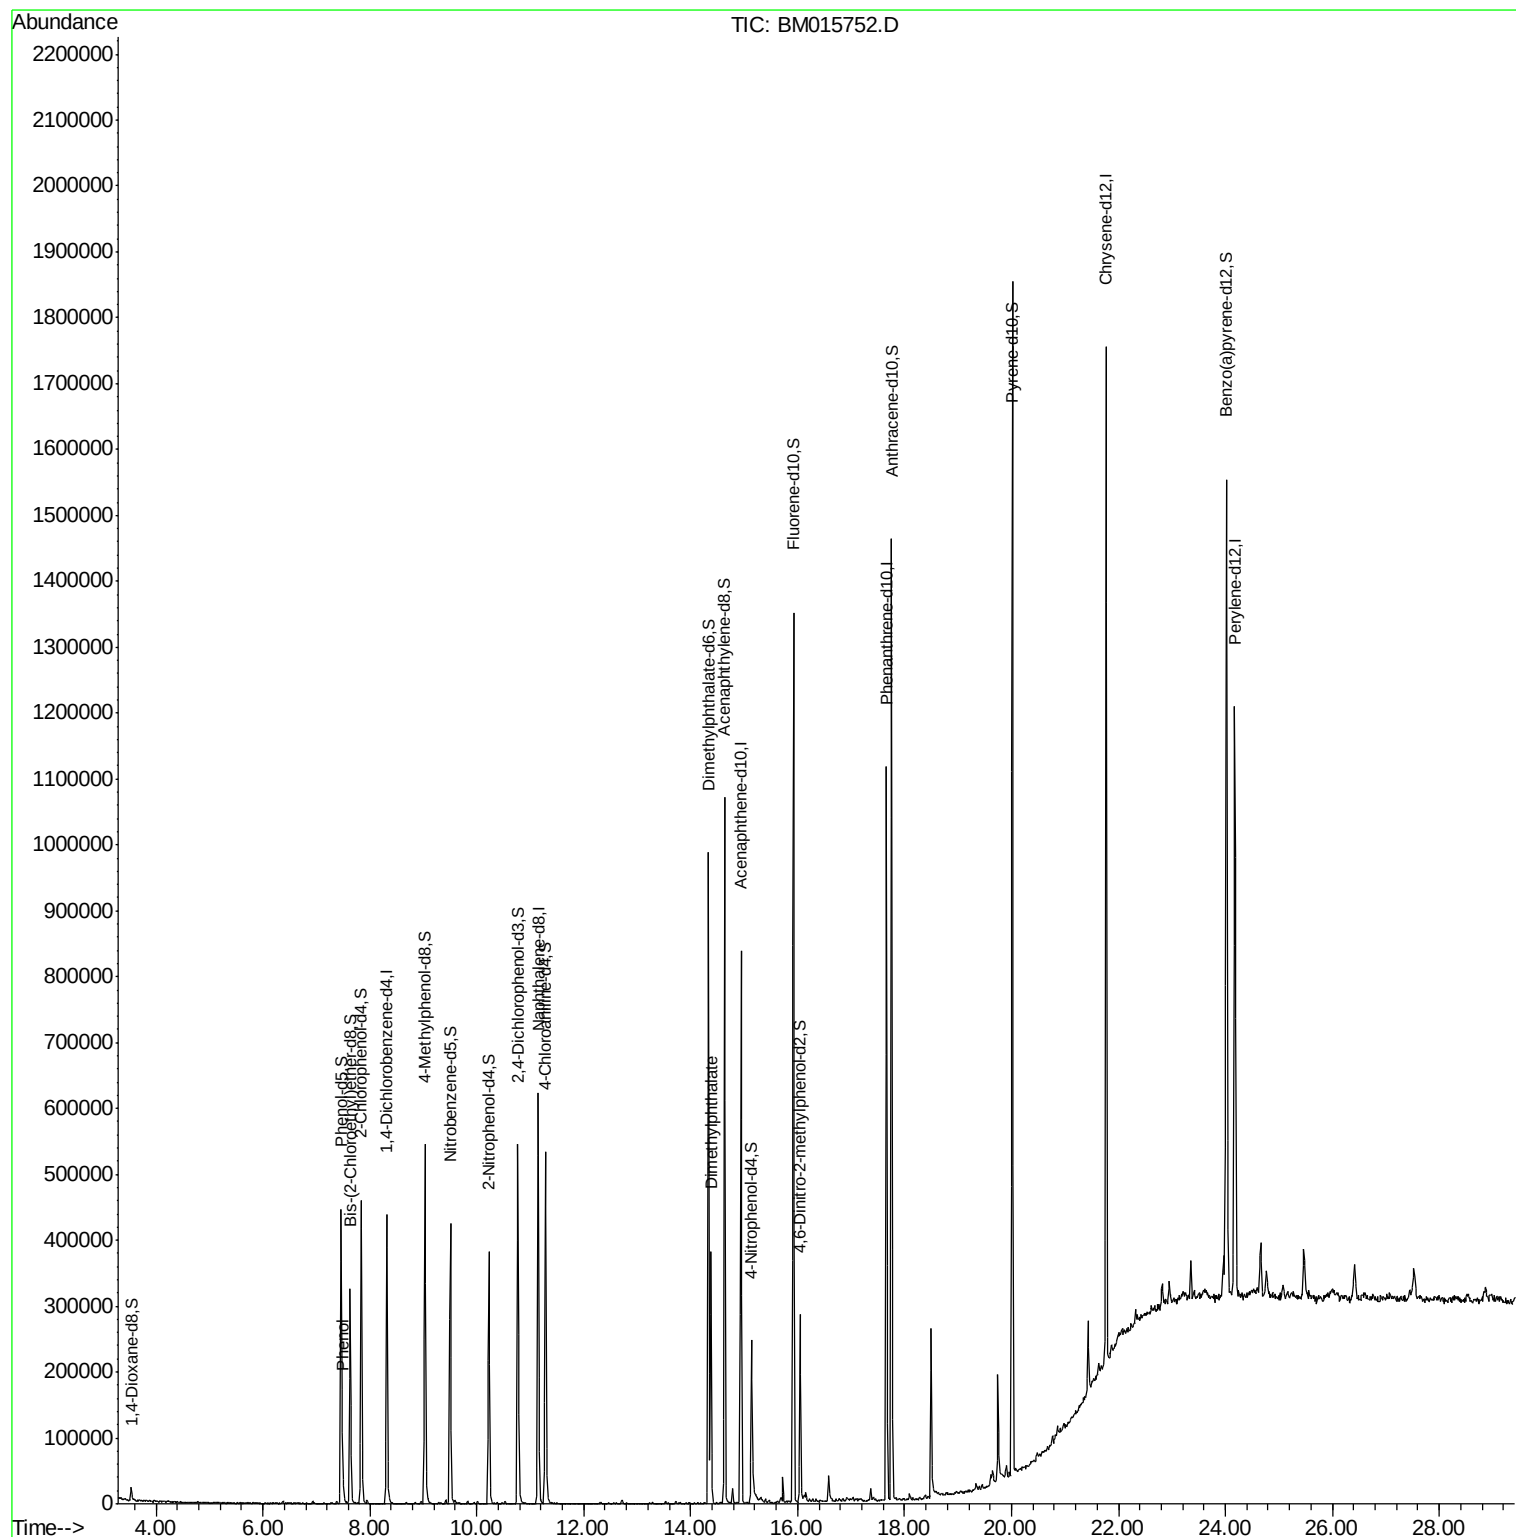

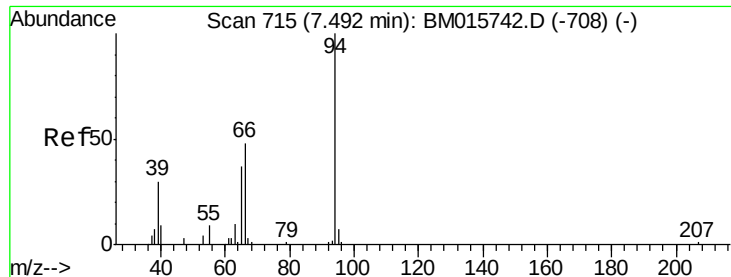

#6

Phenol

Concen: 1.757 ng/ul

RT: 7.49 min Scan# 715

Delta R.T. 0.00 min

Lab File: BM015752.D

Acq: 25 Jun 2018 16:29

Instrument :

BNA_M

ClientSampleId :


Tot Ion: 94 Resp: 17571

Ion Ratio Lower Upper

94 100

65 40.2 21.0 31.6#

66 57.9 29.3 43.9#



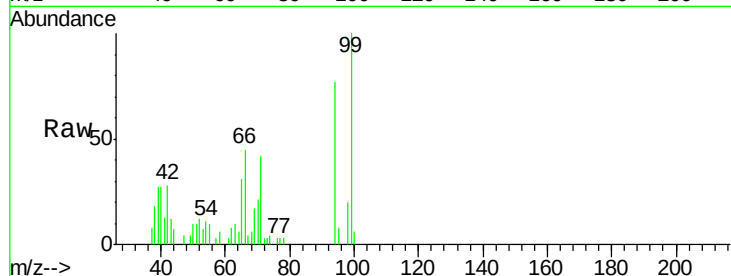


Abundance Ion 94.00 (93.70 to 94.70): BM015742.D (-708) (-)

Ion 65.00 (64.70 to 65.70): BM015742.D (-708) (-)

Ion 66.00 (65.70 to 66.70): BM015742.D (-708) (-)

Time-->

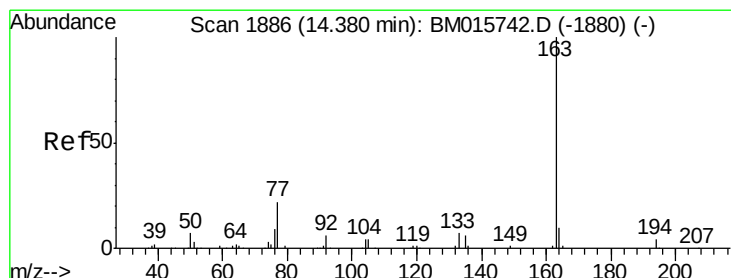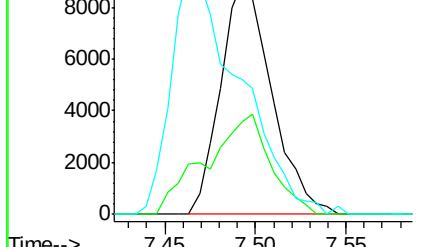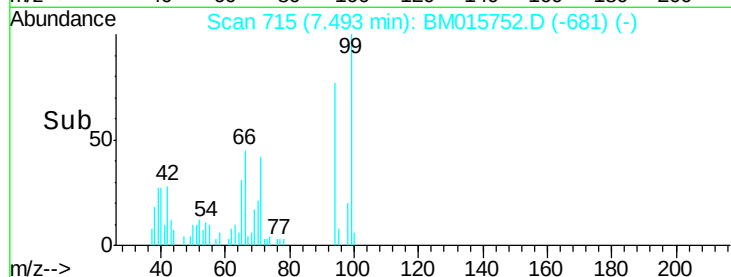

#44

Dimethylphthalate

Concen: 9.886 ng/ul

RT: 14.38 min Scan# 1886

Delta R.T. 0.00 min

Lab File: BM015752.D

Acq: 25 Jun 2018 16:29


Tgt Ion:163 Resp: 216272

Ion Ratio Lower Upper

163 100

194 4.3 3.2 4.8

164 10.1 7.8 11.8

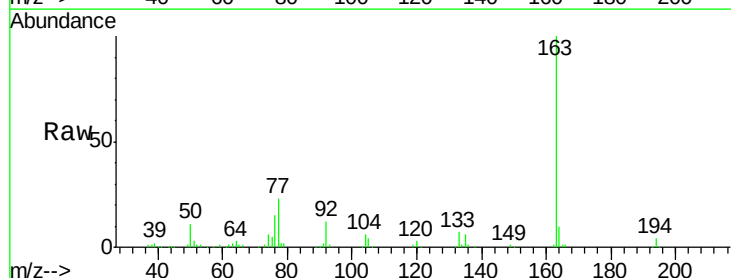

Abundance Ion 163.00 (162.70 to 163.70): BM015742.D (-1880) (-)

Ion 194.00 (193.70 to 194.70): BM015742.D (-1880) (-)

Ion 164.00 (163.70 to 164.70): BM015742.D (-1880) (-)

Time-->

