

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM062518\
 Data File : BM015753.D
 Acq On : 25 Jun 2018 17:06
 Operator : SJ/JU
 Sample : J3569-07
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DAXQ8

Quant Time: Jun 26 02:57:55 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM060818MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jun 26 01:35:35 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.32	152	118260	20.00	ng/ul	0.00
18) Naphthalene-d8	11.15	136	519340	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.93	164	285447	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.66	188	643166	20.00	ng/ul	0.00
77) Chrysene-d12	21.77	240	690771	20.00	ng/ul	0.00
85) Perylene-d12	24.17	264	625120	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.53	96	6955	2.86	ng/uL	0.00
5) Phenol-d5	7.46	99	137330	12.79	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.63	67	91124	14.05	ng/ul	0.00
9) 2-Chlorophenol-d4	7.84	132	121346	14.78	ng/ul	0.00
13) 4-Methylphenol-d8	9.03	113	110454	11.94	ng/ul	0.00
19) Nitrobenzene-d5	9.50	128	53839	15.42	ng/ul	0.00
22) 2-Nitrophenol-d4	10.23	143	58999	15.71	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.77	165	114518	14.72	ng/ul	0.00
29) 4-Chloroaniline-d4	11.29	131	127140	14.67	ng/ul	0.00
43) Dimethylphthalate-d6	14.33	166	362293	15.33	ng/ul	0.00
46) Acenaphthylene-d8	14.63	160	423737	16.62	ng/ul	0.00
51) 4-Nitrophenol-d4	15.14	143	42261	9.26	ng/ul	0.00
57) Fluorene-d10	15.92	176	312326	15.62	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	16.05	200	37405	9.65	ng/ul	0.00
70) Anthracene-d10	17.76	188	472407	16.11	ng/ul	0.00
78) Pyrene-d10	20.02	212	543179	18.28	ng/ul	0.00
89) Benzo(a)pyrene-d12	24.02	264	528758	16.87	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	14.38	163	162316	6.726	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM062518\
Data File : BM015753.D
Acq On : 25 Jun 2018 17:06
Operator : SJ/JU
Sample : J3569-07
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DAXQ8

Quant Time: Jun 26 02:57:55 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM060818MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jun 26 01:35:35 2018
Response via : Initial Calibration

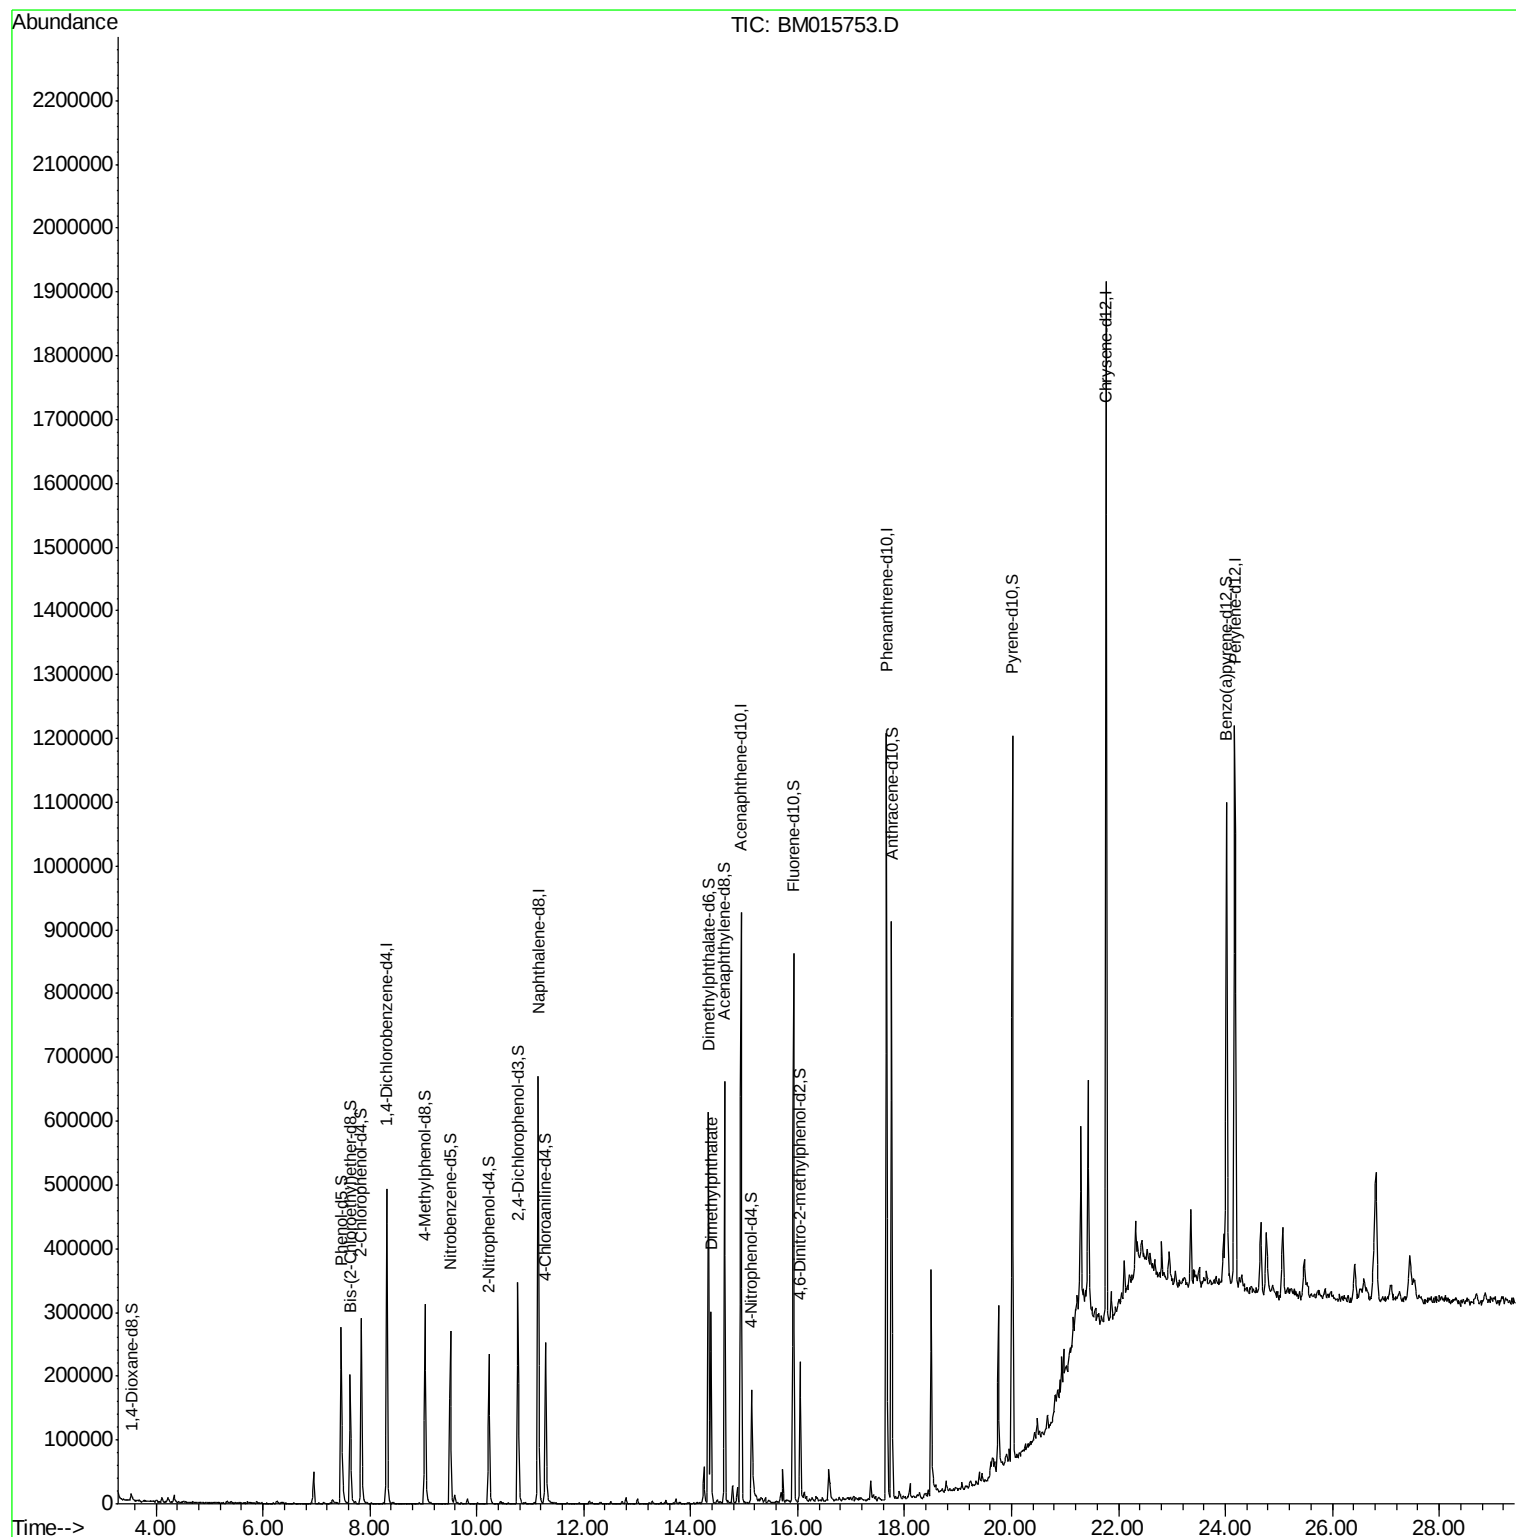

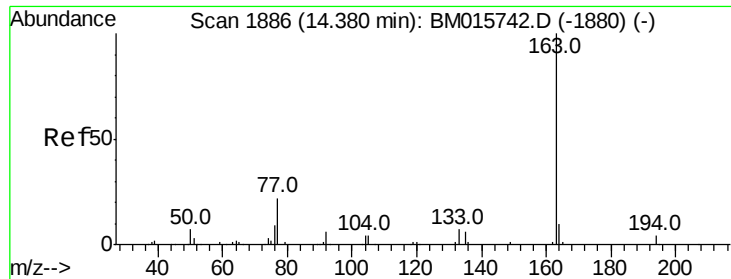

#44

Dimethylphthalate

Concen: 6.726 ng/ul

RT: 14.38 min Scan# 1886

Delta R.T. 0.00 min

Lab File: BM015753.D

Acq: 25 Jun 2018 17:06

Instrument :

BNA_M

ClientSampleId :

DAXQ8



Tot Ion:163 Resp: 162316

Ion Ratio Lower Upper

163 100

194 3.4 3.2 4.8

164 9.8 7.8 11.8

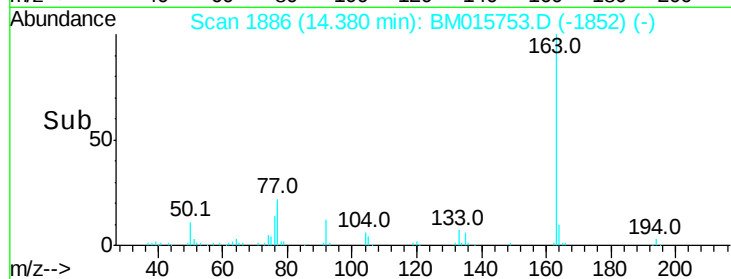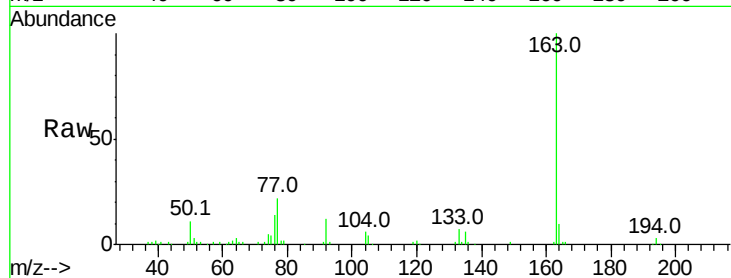

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

