

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM062519\
 Data File : BM021166.D
 Acq On : 25 Jun 2019 18:03
 Operator : HP/JU
 Sample : PB120587BL
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK87

Quant Time: Jun 26 01:38:31 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jun 26 01:32:57 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.77	152	178447	20.00	ng/ul	0.00
18) Naphthalene-d8	10.56	136	747144	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.41	164	531743	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.16	188	1391969	20.00	ng/ul	0.00
77) Chrysene-d12	21.34	240	1404256	20.00	ng/ul	0.00
85) Perylene-d12	23.61	264	1392976	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.28	96	5718	1.52	ng/uL	0.00
5) Phenol-d5	6.93	99	379652	24.44	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.10	67	267988	28.96	ng/ul	0.00
9) 2-Chlorophenol-d4	7.30	132	387744	30.72	ng/ul	0.00
13) 4-Methylphenol-d8	8.47	113	389891	30.07	ng/ul	0.00
19) Nitrobenzene-d5	8.93	128	195108	32.16	ng/ul	0.00
22) 2-Nitrophenol-d4	9.65	143	229692	34.11	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.17	165	490671	35.83	ng/ul	0.00
29) 4-Chloroaniline-d4	10.70	131	610381	42.73	ng/ul	0.00
43) Dimethylphthalate-d6	13.82	166	1857981	38.67	ng/ul	0.00
46) Acenaphthylene-d8	14.10	160	2100708	35.72	ng/ul	0.00
51) 4-Nitrophenol-d4	14.62	143	256379	32.80	ng/ul	0.00
57) Fluorene-d10	15.40	176	1609259	38.51	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.53	200	225983	26.41	ng/ul	0.00
70) Anthracene-d10	17.26	188	2819257	38.97	ng/ul	0.00
78) Pyrene-d10	19.55	212	3252343	38.60	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.47	264	3276251	39.86	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) 2,6-Dinitrotoluene	13.82	165	13154	1.576	ng/ul#	39




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM062519\
Data File : BM021166.D
Acq On : 25 Jun 2019 18:03
Operator : HP/JU
Sample : PB120587BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK87

Quant Time: Jun 26 01:38:31 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jun 26 01:32:57 2019
Response via : Initial Calibration

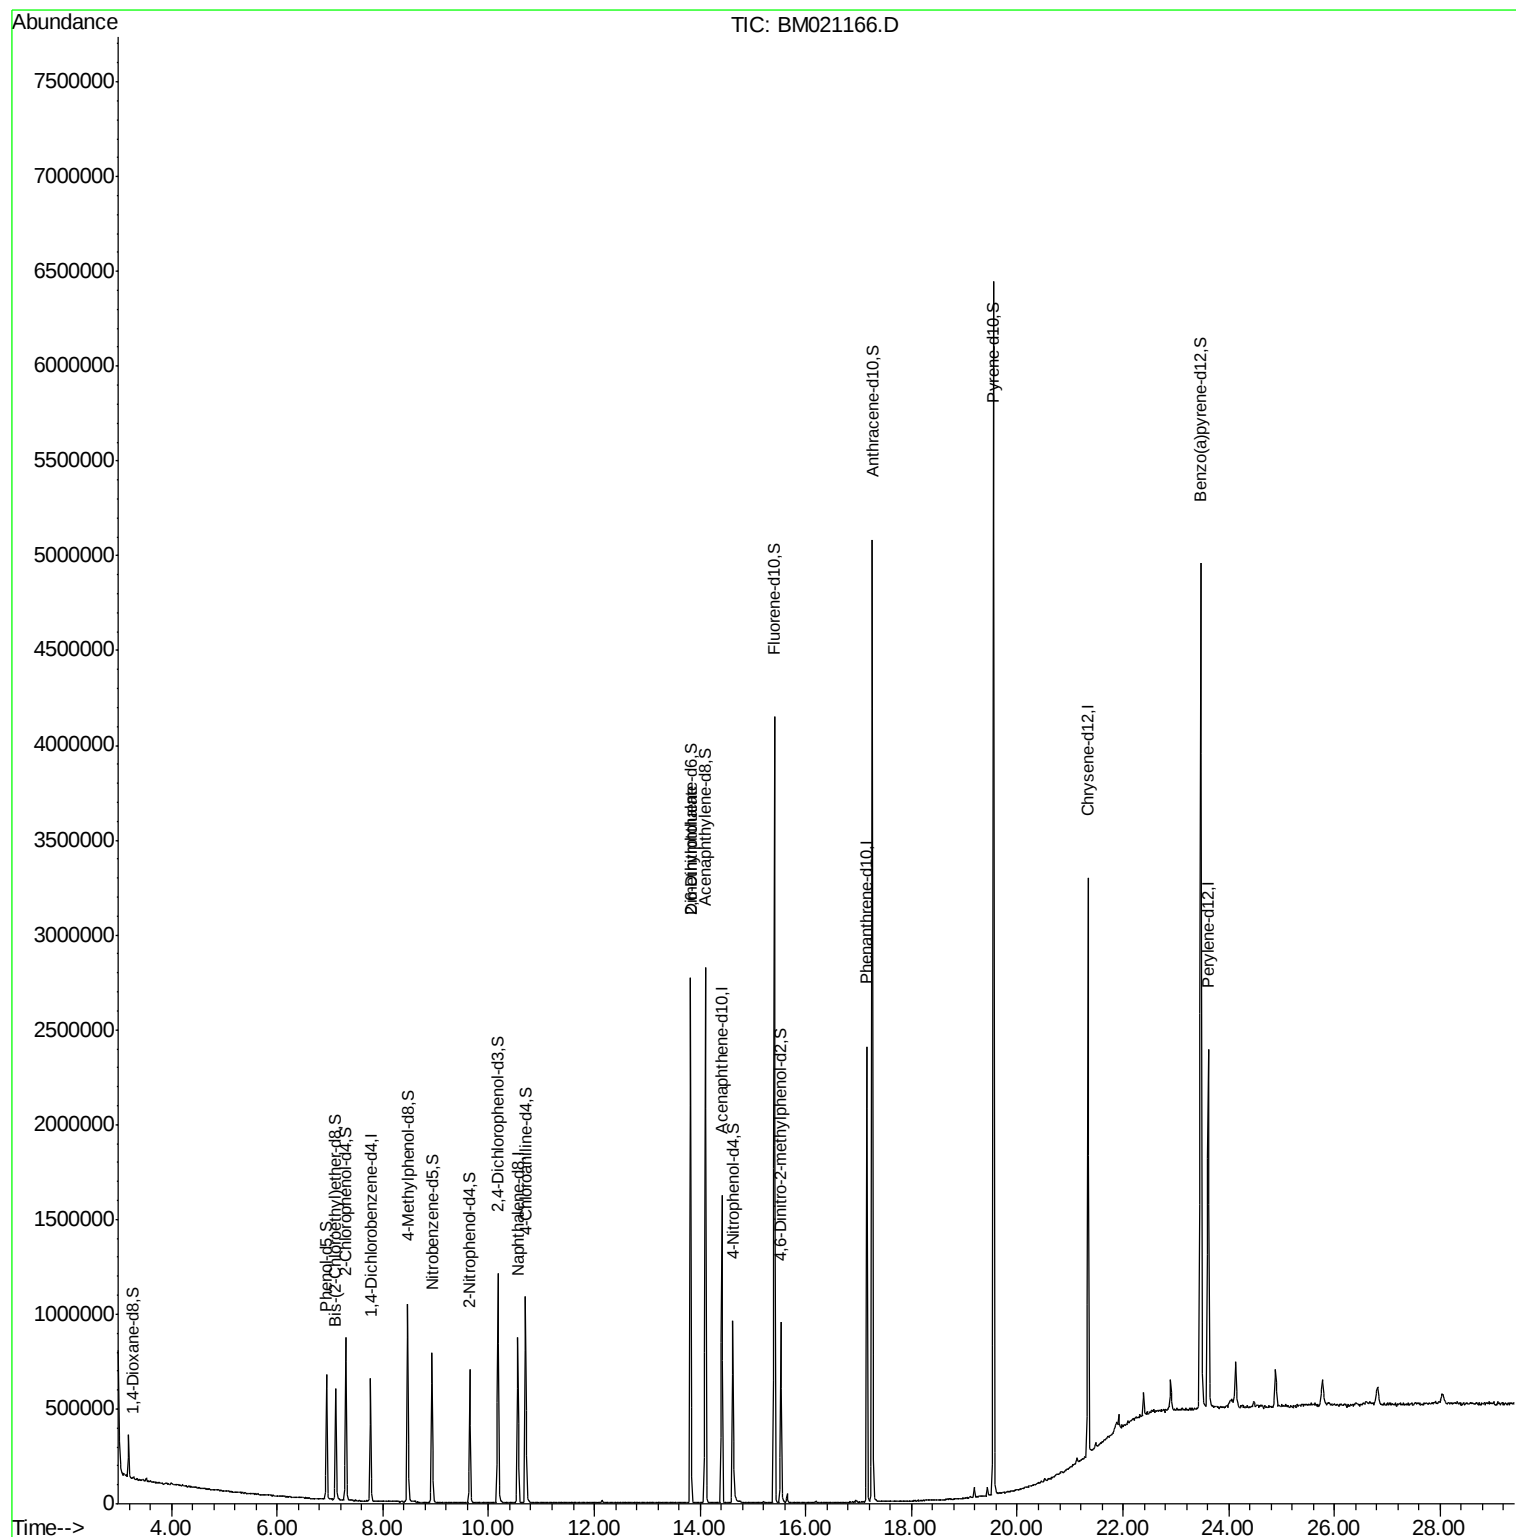

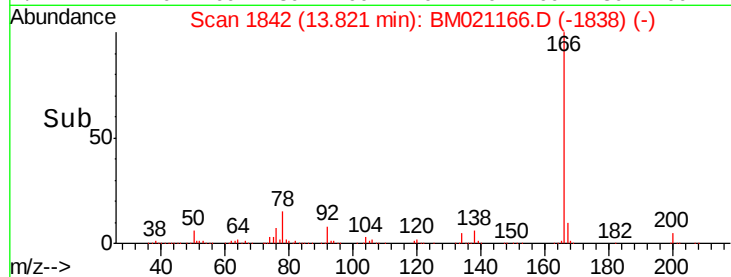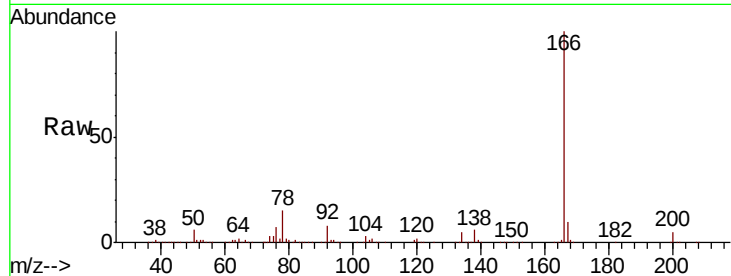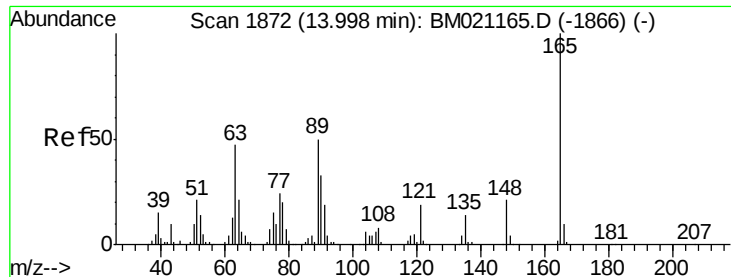

#45
 2,6-Dinitrotoluene
 Concen: 1.576 ng/ul
 RT: 13.82 min Scan# 1842
 Delta R.T. -0.18 min
 Lab File: BM021166.D
 Acq: 25 Jun 2019 18:03

Instrument :
 BNA_M
 ClientSampleId :
 SBLK87

Tgt Ion	Ratio	Lower	Upper
165	100		
89	0.0	43.6	65.4#
121	31.0	16.5	24.7#

