

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM062519\
 Data File : BM021169.D
 Acq On : 25 Jun 2019 19:51
 Operator : HP/JU
 Sample : K3289-17
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BFCM2

Quant Time: Jun 26 01:38:46 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jun 26 01:32:57 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.77	152	307265	20.00	ng/ul	0.00
18) Naphthalene-d8	10.56	136	1377268	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.41	164	946816	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.16	188	2312905	20.00	ng/ul	0.00
77) Chrysene-d12	21.34	240	1976640	20.00	ng/ul	0.00
85) Perylene-d12	23.61	264	1865942	20.00	ng/ul	-0.01

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.28	96	31271	4.83	ng/uL	0.00
5) Phenol-d5	6.94	99	143909	5.38	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.11	67	381780	23.96	ng/ul	0.00
9) 2-Chlorophenol-d4	7.30	132	435466	20.04	ng/ul	0.00
13) 4-Methylphenol-d8	8.47	113	289624	12.97	ng/ul	0.00
19) Nitrobenzene-d5	8.93	128	283049	25.31	ng/ul	0.00
22) 2-Nitrophenol-d4	9.65	143	325685	26.23	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.17	165	625383	24.77	ng/ul	0.00
29) 4-Chloroaniline-d4	10.70	131	122957	4.67	ng/ul	0.00
43) Dimethylphthalate-d6	13.82	166	2507503	29.31	ng/ul	0.00
46) Acenaphthylene-d8	14.10	160	2746279	26.22	ng/ul	0.00
51) 4-Nitrophenol-d4	14.62	143	66735	4.80	ng/ul	0.00
57) Fluorene-d10	15.40	176	2181098	29.31	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.53	200	383436	26.97	ng/ul	0.00
70) Anthracene-d10	17.26	188	3618141	30.10	ng/ul	0.00
78) Pyrene-d10	19.55	212	4074966	34.36	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.47	264	3464197	31.47	ng/ul	0.00


Target Compounds					Qvalue
2) 1,4-Dioxane	3.32	88	12637	1.930	ng/uL 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM062519\
Data File : BM021169.D
Acq On : 25 Jun 2019 19:51
Operator : HP/JU
Sample : K3289-17
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BFCM2

Quant Time: Jun 26 01:38:46 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jun 26 01:32:57 2019
Response via : Initial Calibration

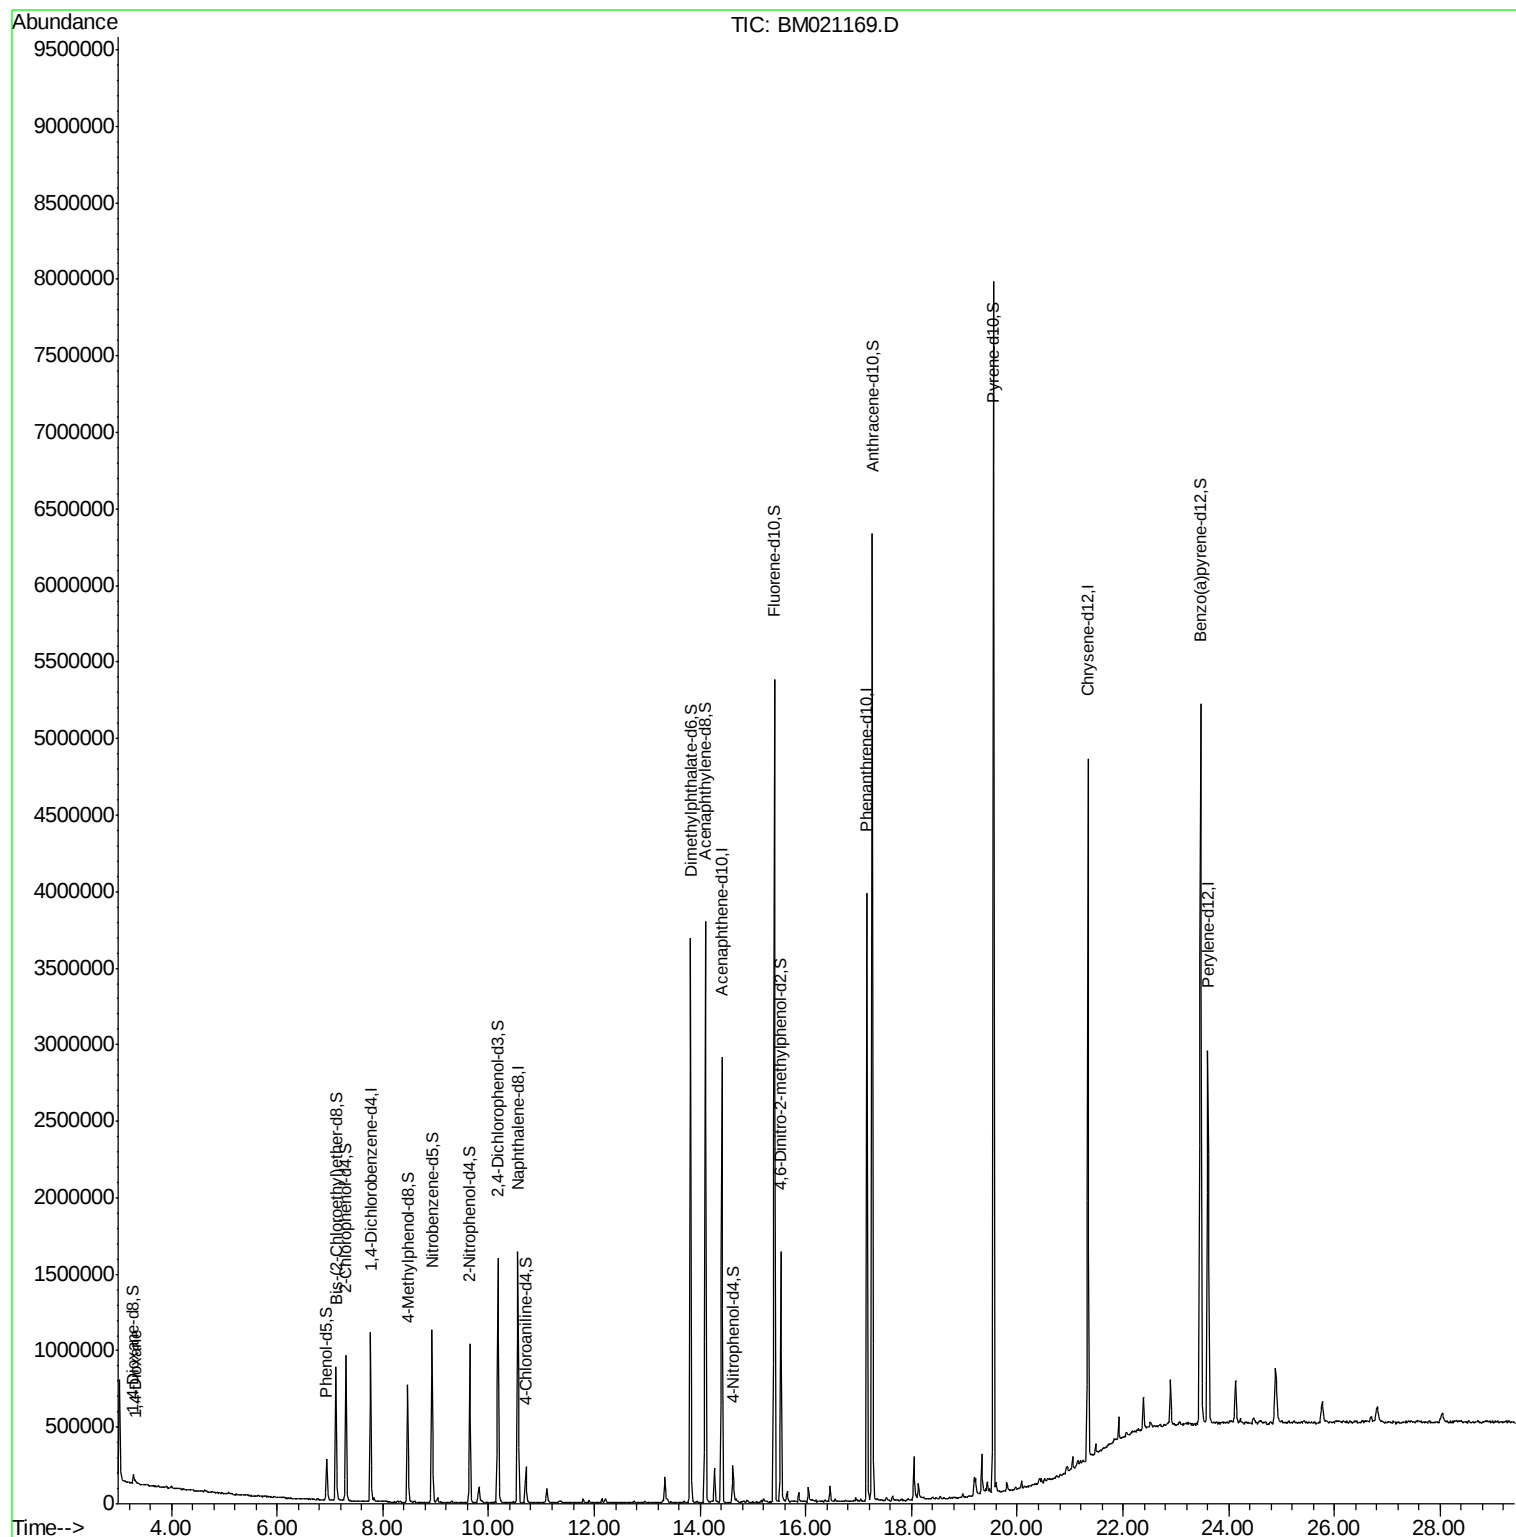

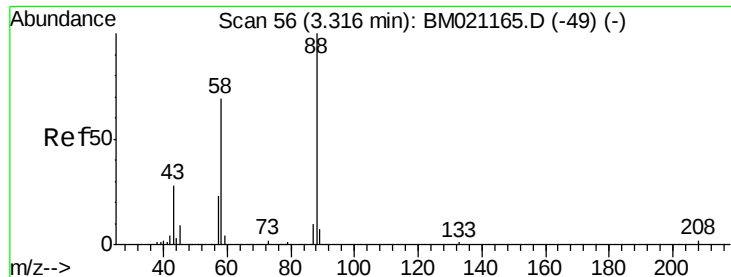

#2
 1,4-Dioxane
 Concen: 1.930 ng/uL
 RT: 3.32 min Scan# 56
 Delta R.T. -0.00 min
 Lab File: BM021169.D
 Acq: 25 Jun 2019 19:51

Instrument :
 BNA_M
 ClientSampleId :
 BFCM2

Tgt Ion: 88 Resp: 12637
 Ion Ratio Lower Upper
 88 100
 43 32.7 26.7 40.1
 58 62.2 52.6 78.8

