

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM062519\
 Data File : BM021153.D
 Acq On : 25 Jun 2019 10:12
 Operator : HP/JU
 Sample : K3289-02
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BFCL6

Quant Time: Jun 25 16:47:26 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jun 24 07:41:31 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.77	152	211273	20.00	ng/ul	0.00
18) Naphthalene-d8	10.56	136	930755	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.41	164	618465	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.16	188	1552411	20.00	ng/ul	0.00
77) Chrysene-d12	21.34	240	1565473	20.00	ng/ul	0.00
85) Perylene-d12	23.62	264	1593154	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.28	96	26129	5.87	ng/uL	0.00
5) Phenol-d5	6.94	99	110718	6.02	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.11	67	313557	28.62	ng/ul	0.00
9) 2-Chlorophenol-d4	7.30	132	346067	23.16	ng/ul	0.00
13) 4-Methylphenol-d8	8.47	113	224817	14.65	ng/ul	0.00
19) Nitrobenzene-d5	8.93	128	233496	30.90	ng/ul	0.00
22) 2-Nitrophenol-d4	9.65	143	266090	31.72	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.18	165	481132	28.20	ng/ul	0.00
29) 4-Chloroaniline-d4	10.70	131	93547	5.26	ng/ul	0.00
43) Dimethylphthalate-d6	13.82	166	1832582	32.79	ng/ul	0.00
46) Acenaphthylene-d8	14.10	160	2202891	32.20	ng/ul	0.00
51) 4-Nitrophenol-d4	14.63	143	37559	4.13	ng/ul	0.00
57) Fluorene-d10	15.40	176	1629512	33.52	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.53	200	251626	26.37	ng/ul	0.00
70) Anthracene-d10	17.26	188	2684341	33.27	ng/ul	0.00
78) Pyrene-d10	19.55	212	3109371	33.10	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.47	264	3133022	33.33	ng/ul	0.00


Target Compounds					Ovalue	
44) Dimethylphthalate	13.87	163	95257	1.873	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM062519\
Data File : BM021153.D
Acq On : 25 Jun 2019 10:12
Operator : HP/JU
Sample : K3289-02
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BFCL6

Quant Time: Jun 25 16:47:26 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jun 24 07:41:31 2019
Response via : Initial Calibration

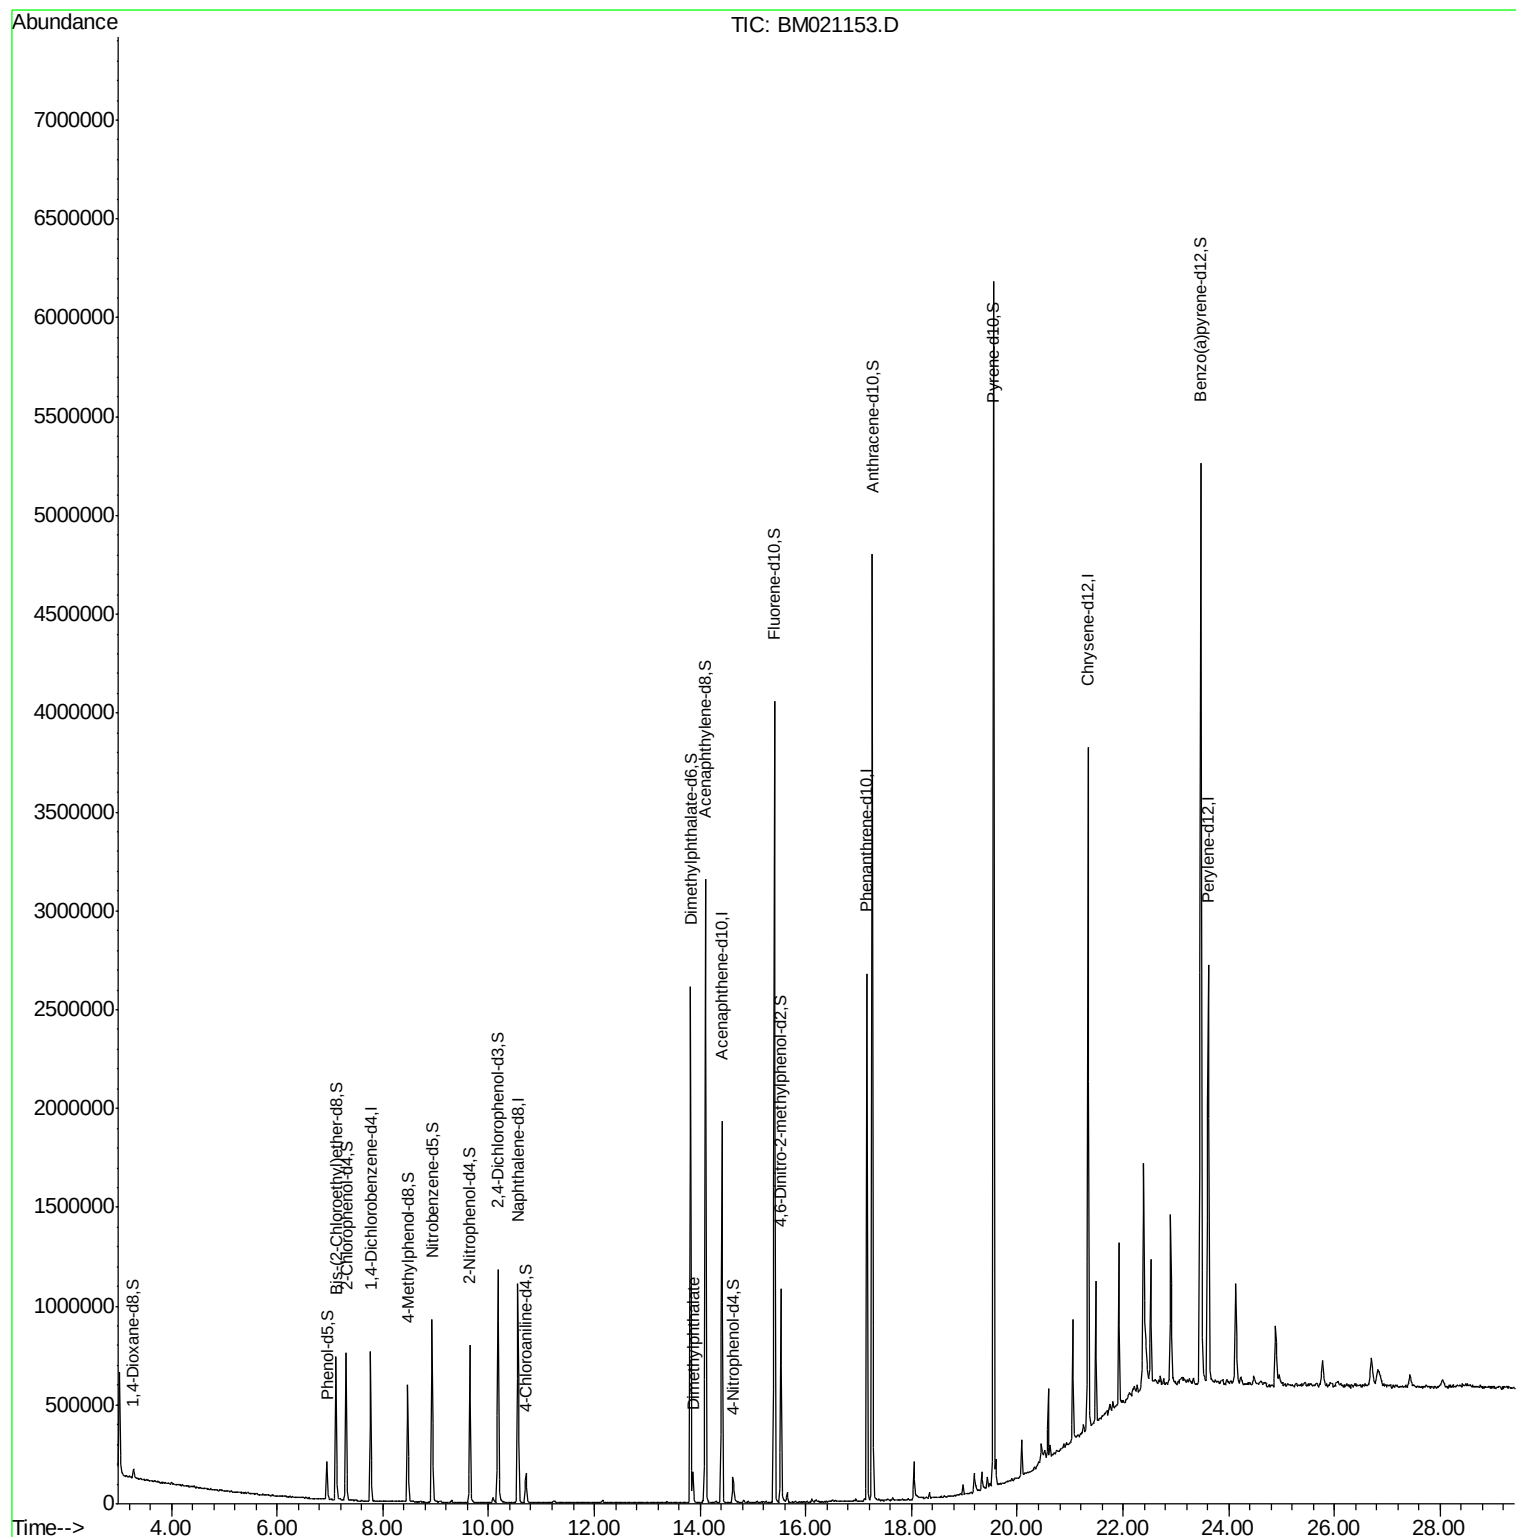

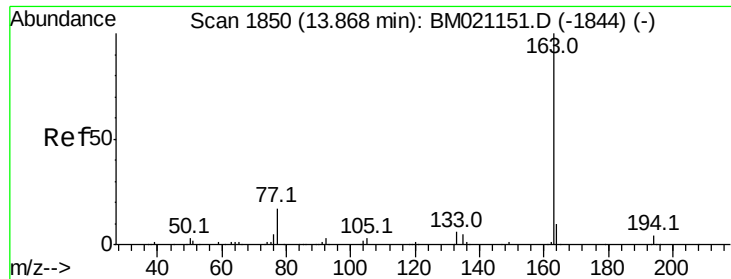

#44

Dimethylphthalate

Concen: 1.873 ng/ul

RT: 13.87 min Scan# 1850

Delta R.T. -0.01 min

Lab File: BM021153.D

Acq: 25 Jun 2019 10:12

Instrument :

BNA_M

ClientSampleId :

BFCL6


Tot Ion:163 Resp: 95257

Ion Ratio Lower Upper

163 100

194 5.0 3.4 5.2

164 10.3 7.7 11.5

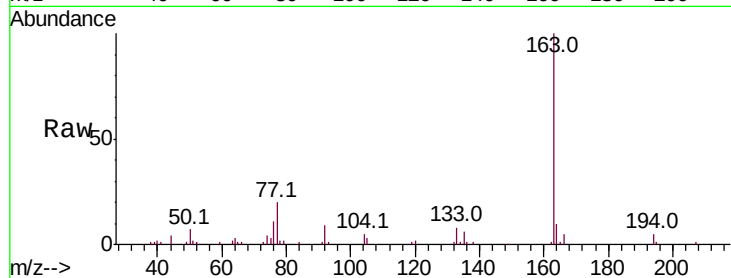

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

