

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM062519\
 Data File : BM021158.D
 Acq On : 25 Jun 2019 13:13
 Operator : HP/JU
 Sample : K3289-09
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BFCL5

Quant Time: Jun 25 17:15:12 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jun 24 07:41:31 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.77	152	291872	20.00	ng/ul	0.00
18) Naphthalene-d8	10.56	136	1306051	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.41	164	875866	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.16	188	2047464	20.00	ng/ul	0.00
77) Chrysene-d12	21.34	240	1482922	20.00	ng/ul	0.00
85) Perylene-d12	23.62	264	1503190	20.00	ng/ul	0.01

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.28	96	37268	6.06	ng/uL	0.00
5) Phenol-d5	6.94	99	158792	6.25	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.11	67	400681	26.47	ng/ul	0.00
9) 2-Chlorophenol-d4	7.30	132	461099	22.34	ng/ul	0.00
13) 4-Methylphenol-d8	8.47	113	313087	14.76	ng/ul	0.00
19) Nitrobenzene-d5	8.93	128	298571	28.15	ng/ul	0.00
22) 2-Nitrophenol-d4	9.65	143	346205	29.41	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.18	165	651230	27.21	ng/ul	0.00
29) 4-Chloroaniline-d4	10.70	131	73908	2.96	ng/ul	0.00
43) Dimethylphthalate-d6	13.82	166	2459413	31.08	ng/ul	0.00
46) Acenaphthylene-d8	14.10	160	2873595	29.66	ng/ul	0.00
51) 4-Nitrophenol-d4	14.63	143	50700	3.94	ng/ul	0.00
57) Fluorene-d10	15.40	176	2142800	31.13	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.53	200	344384	27.36	ng/ul	0.00
70) Anthracene-d10	17.26	188	3354705	31.53	ng/ul	0.00
78) Pyrene-d10	19.55	212	3382241	38.01	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.47	264	2848797	32.12	ng/ul	0.00


Target Compounds				Ovalue
2) 1,4-Dioxane	3.32	88	931952	149.835 ng/uL# 95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM062519\
Data File : BM021158.D
Acq On : 25 Jun 2019 13:13
Operator : HP/JU
Sample : K3289-09
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleID :
BFCL5

Quant Time: Jun 25 17:15:12 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jun 24 07:41:31 2019
Response via : Initial Calibration

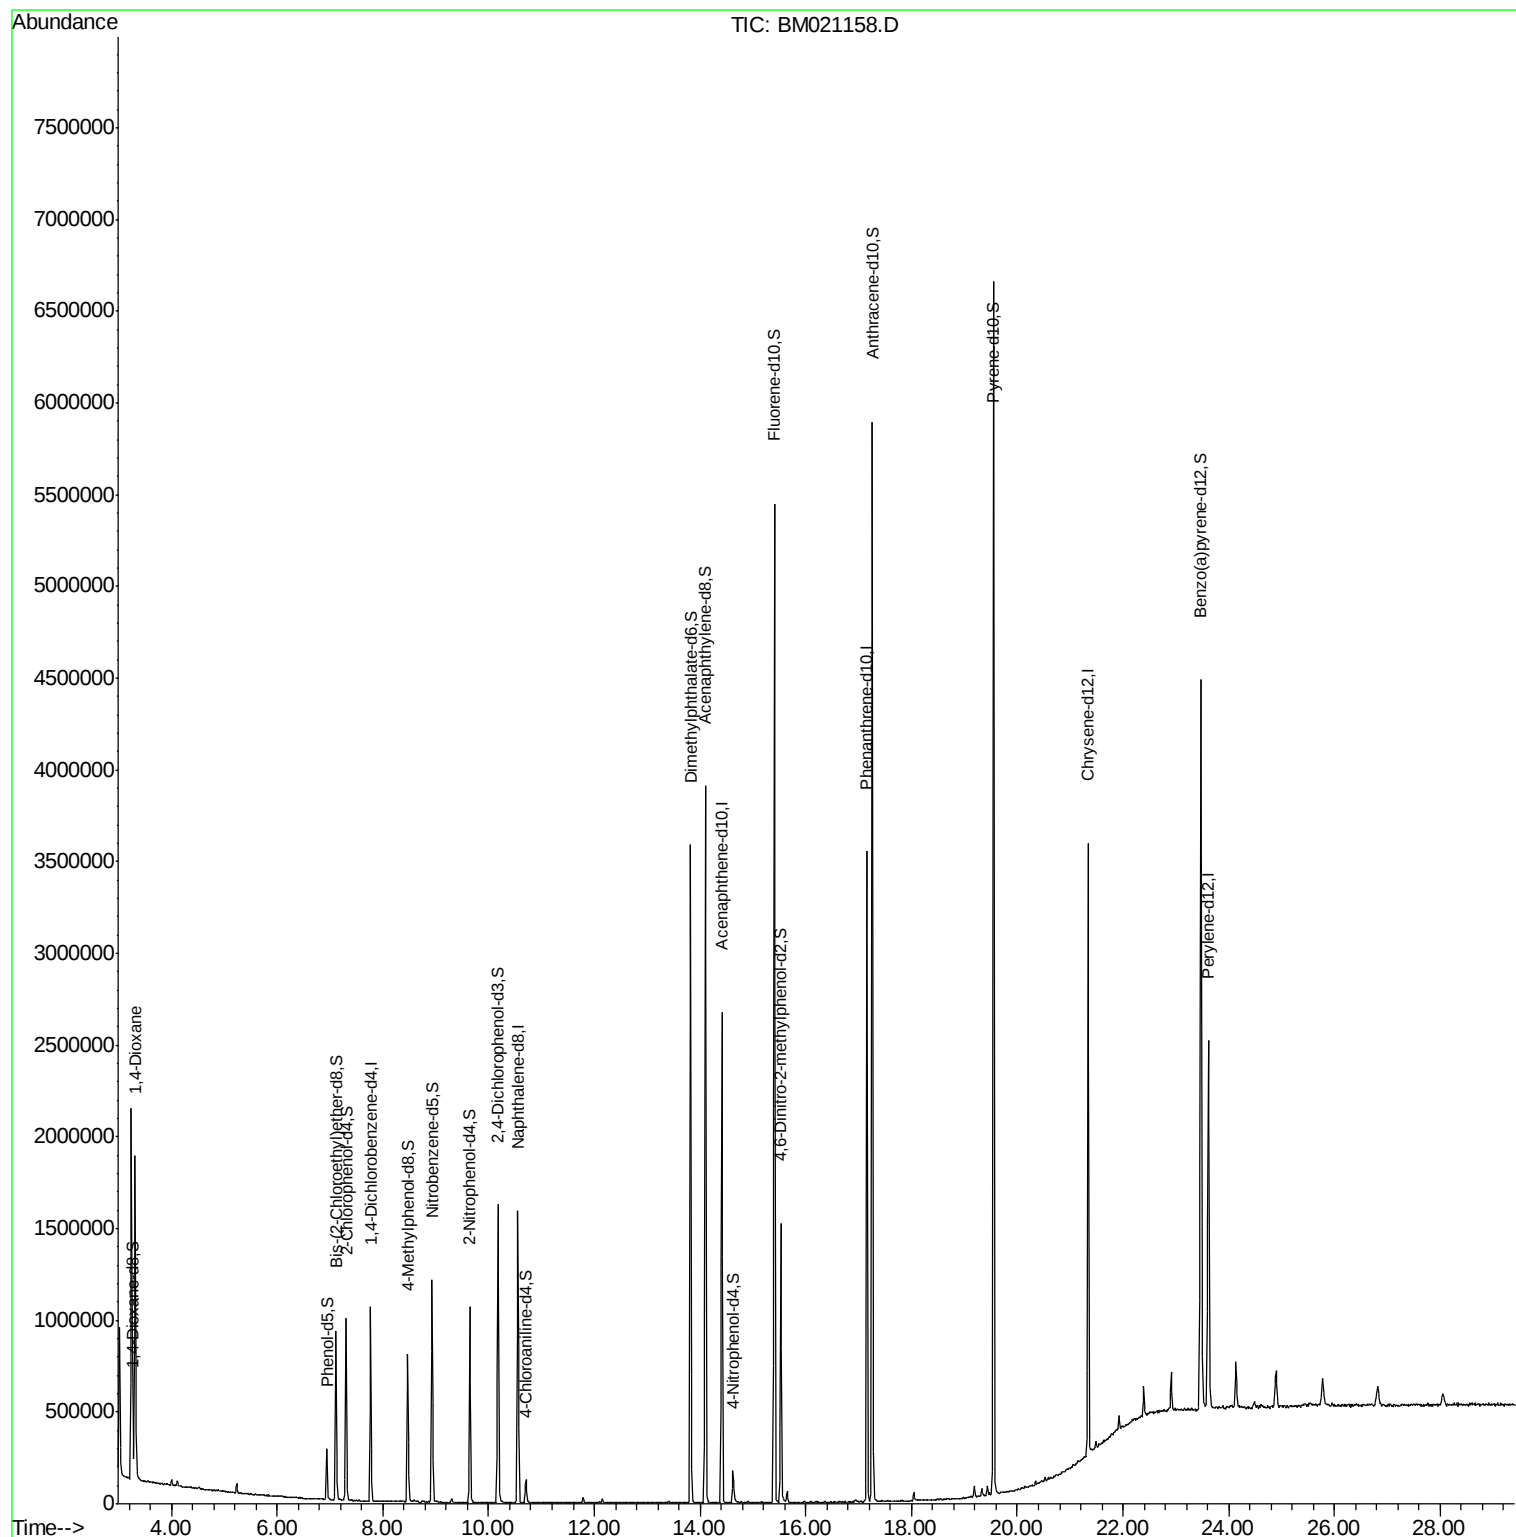

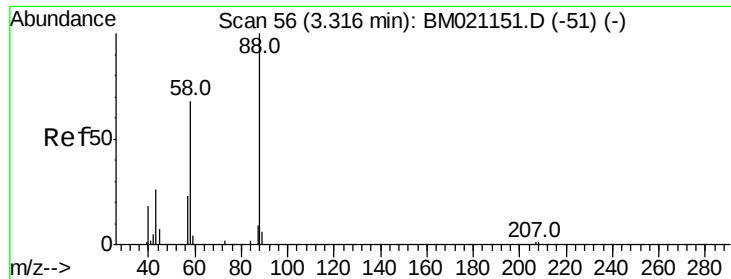

#2

1,4-Dioxane

Concen: 149.835 ng/uL

RT: 3.32 min Scan# 56

Delta R.T. -0.01 min

Lab File: BM021158.D

Acq: 25 Jun 2019 13:13

Instrument :
BNA_M
ClientSampleId :
BFCL5

Tot Ion: 88 Resp: 931952

Ion	Ratio	Lower	Upper
88	100		
43	25.8	26.7	40.1#
58	66.0	52.6	78.8

