

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM062519\
 Data File : BM021162.D
 Acq On : 25 Jun 2019 15:38
 Operator : HP/JU
 Sample : K3289-14
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BFCL1

Quant Time: Jun 25 17:22:33 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jun 24 07:41:31 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.77	152	321816	20.00	ng/ul	0.00
18) Naphthalene-d8	10.56	136	1443827	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.41	164	998342	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.16	188	2472340	20.00	ng/ul	0.00
77) Chrysene-d12	21.34	240	2134583	20.00	ng/ul	0.00
85) Perylene-d12	23.62	264	2007562	20.00	ng/ul	0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.29	96	30857	4.55	ng/uL	0.00
5) Phenol-d5	6.94	99	153894	5.49	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.11	67	396345	23.75	ng/ul	0.00
9) 2-Chlorophenol-d4	7.30	132	446769	19.63	ng/ul	0.00
13) 4-Methylphenol-d8	8.47	113	305122	13.05	ng/ul	0.00
19) Nitrobenzene-d5	8.93	128	296583	25.30	ng/ul	0.00
22) 2-Nitrophenol-d4	9.65	143	340066	26.13	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.17	165	628775	23.76	ng/ul	0.00
29) 4-Chloroaniline-d4	10.70	131	73870	2.68	ng/ul	0.00
43) Dimethylphthalate-d6	13.82	166	2407076	26.68	ng/ul	0.00
46) Acenaphthylene-d8	14.10	160	2870691	26.00	ng/ul	0.00
51) 4-Nitrophenol-d4	14.62	143	54929	3.74	ng/ul	0.00
57) Fluorene-d10	15.40	176	2161523	27.55	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.53	200	320077	21.06	ng/ul	0.00
70) Anthracene-d10	17.26	188	3539151	27.55	ng/ul	0.00
78) Pyrene-d10	19.55	212	3888391	30.36	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.48	264	3338441	28.19	ng/ul	0.01


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	13.87	163	101553	1.237	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM062519\
Data File : BM021162.D
Acq On : 25 Jun 2019 15:38
Operator : HP/JU
Sample : K3289-14
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BFCL1

Quant Time: Jun 25 17:22:33 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jun 24 07:41:31 2019
Response via : Initial Calibration

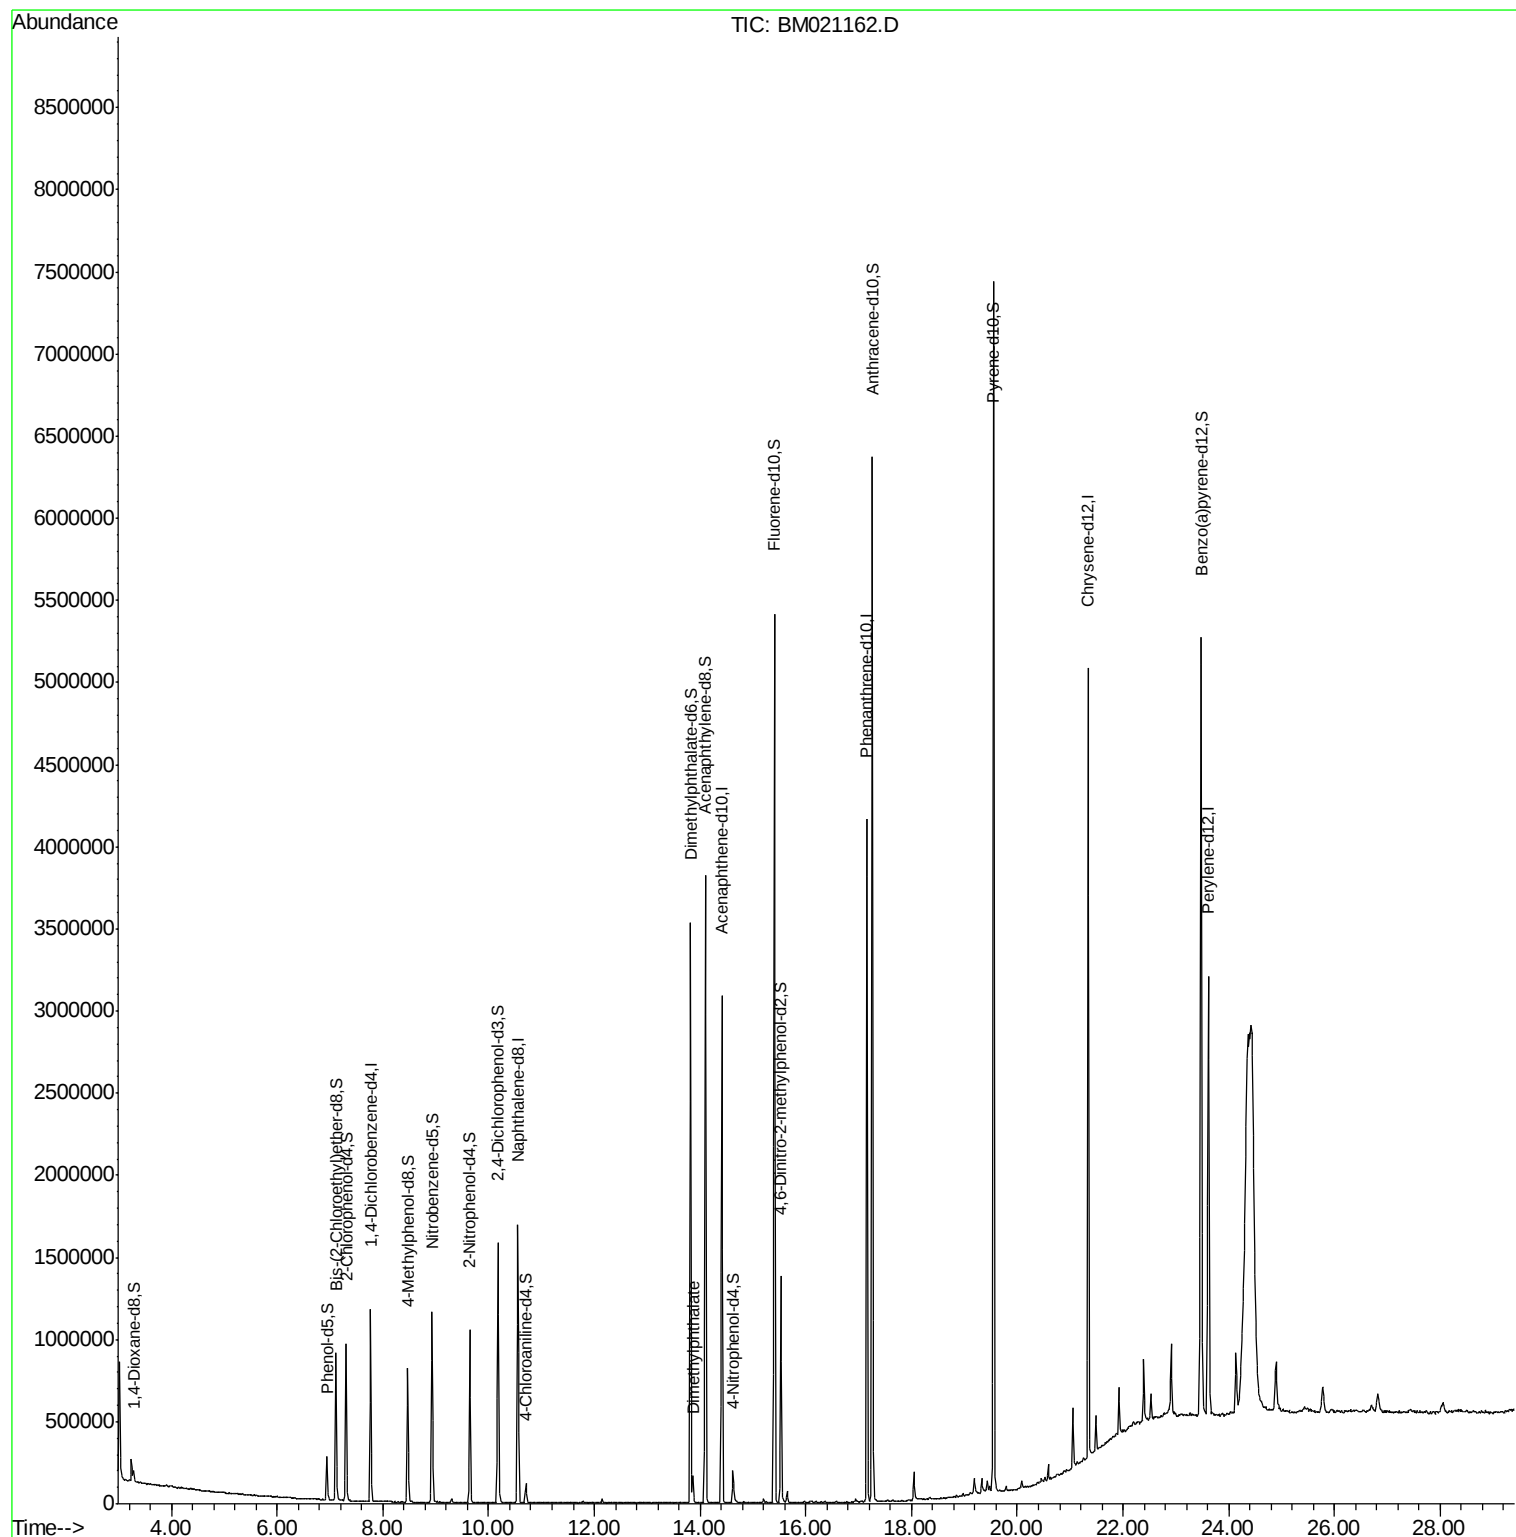

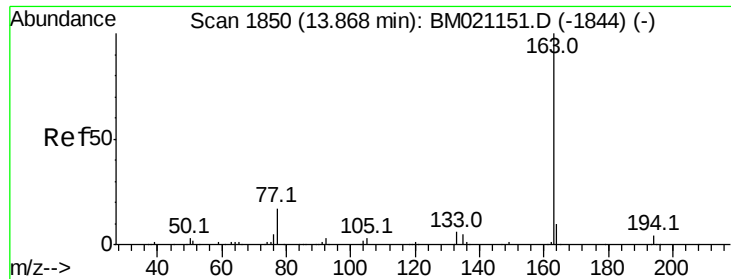

#44

Dimethylphthalate

Concen: 1.237 ng/ul

RT: 13.87 min Scan# 1850

Delta R.T. -0.01 min

Lab File: BM021162.D

Acq: 25 Jun 2019 15:38

Instrument :

BNA_M

ClientSampleId :

BFCL1


Tot Ion:163 Resp: 101553

Ion Ratio Lower Upper

163 100

194 4.9 3.4 5.2

164 10.1 7.7 11.5

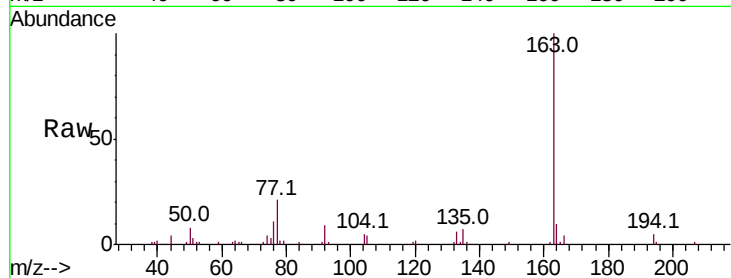

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

