

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM062519\
 Data File : BM021197.D
 Acq On : 26 Jun 2019 18:17
 Operator : HP/JU
 Sample : K3501-01
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C5AB9

Manual Integrations
 APPROVED

mohammad
 6/27/2019 8:17:55 AM

Quant Time: Jun 27 00:51:40 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jun 27 00:42:34 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.76	152	231635	20.00	ng/ul	0.00
18) Naphthalene-d8	10.55	136	1057139	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.40	164	695266	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.16	188	1569999	20.00	ng/ul	0.00
77) Chrysene-d12	21.34	240	1075091	20.00	ng/ul	0.00
85) Perylene-d12	23.62	264	1168440	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.29	96	15971	3.27	ng/uL	0.00
5) Phenol-d5	6.93	99	516632	25.62	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.10	67	295914	24.63	ng/ul	0.00
9) 2-Chlorophenol-d4	7.30	132	410018	25.03	ng/ul	0.00
13) 4-Methylphenol-d8	8.47	113	489051	29.06	ng/ul	0.00
19) Nitrobenzene-d5	8.93	128	245805	28.64	ng/ul	0.00
22) 2-Nitrophenol-d4	9.65	143	293716	30.82	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.17	165	588879	30.39	ng/ul	0.00
29) 4-Chloroaniline-d4	10.70	131	661804	32.75	ng/ul	0.00
43) Dimethylphthalate-d6	13.82	166	2240442	35.66	ng/ul	0.00
46) Acenaphthylene-d8	14.10	160	2478020	32.22	ng/ul	0.00
51) 4-Nitrophenol-d4	14.62	143	266500	26.08	ng/ul	0.00
57) Fluorene-d10	15.40	176	1904331	34.85	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.53	200	286097	29.64	ng/ul	0.00
70) Anthracene-d10	17.25	188	2845432	34.88	ng/ul	0.00
78) Pyrene-d10	19.55	212	2707501	41.97	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.48	264	2394708	34.74	ng/ul	0.00

Target Compounds

					Ovalue	
44) Dimethylphthalate	13.86	163	865715	15.138	ng/ul	98
69) Phenanthrene	17.20	178	273899	3.154	ng/ul	99
76) Fluoranthene	19.22	202	425985	4.540	ng/ul	99
79) Pyrene	19.58	202	347586	4.573	ng/ul	99
82) Benzo(a)anthracene	21.33	228	160510	2.190	ng/ul	99
83) Bis(2-ethylhexyl)phthalate	21.26	149	41845	1.045	ng/ul	97
84) Chrysene	21.38	228	173232	2.524	ng/ul	98
87) Benzo(b)fluoranthene	22.94	252	223955	3.026	ng/ul#	98
88) Benzo(k)fluoranthene	22.98	252	84197m	1.182	ng/ul	
90) Benzo(a)pyrene	23.52	252	144789	2.078	ng/ul	97
91) Indeno(1,2,3-cd)pyrene	25.91	276	101984	1.243	ng/ul	98
93) Benzo(g,h,i)perylene	26.61	276	86054	1.274	ng/ul	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM062519\
Data File : BM021197.D
Acq On : 26 Jun 2019 18:17
Operator : HP/JU
Sample : K3501-01
Misc :
ALS Vial : 46 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
C5AB9

Manual Integrations
APPROVED

mohammad
6/27/2019 8:17:55 AM

Quant Time: Jun 27 00:51:40 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jun 27 00:42:34 2019
Response via : Initial Calibration

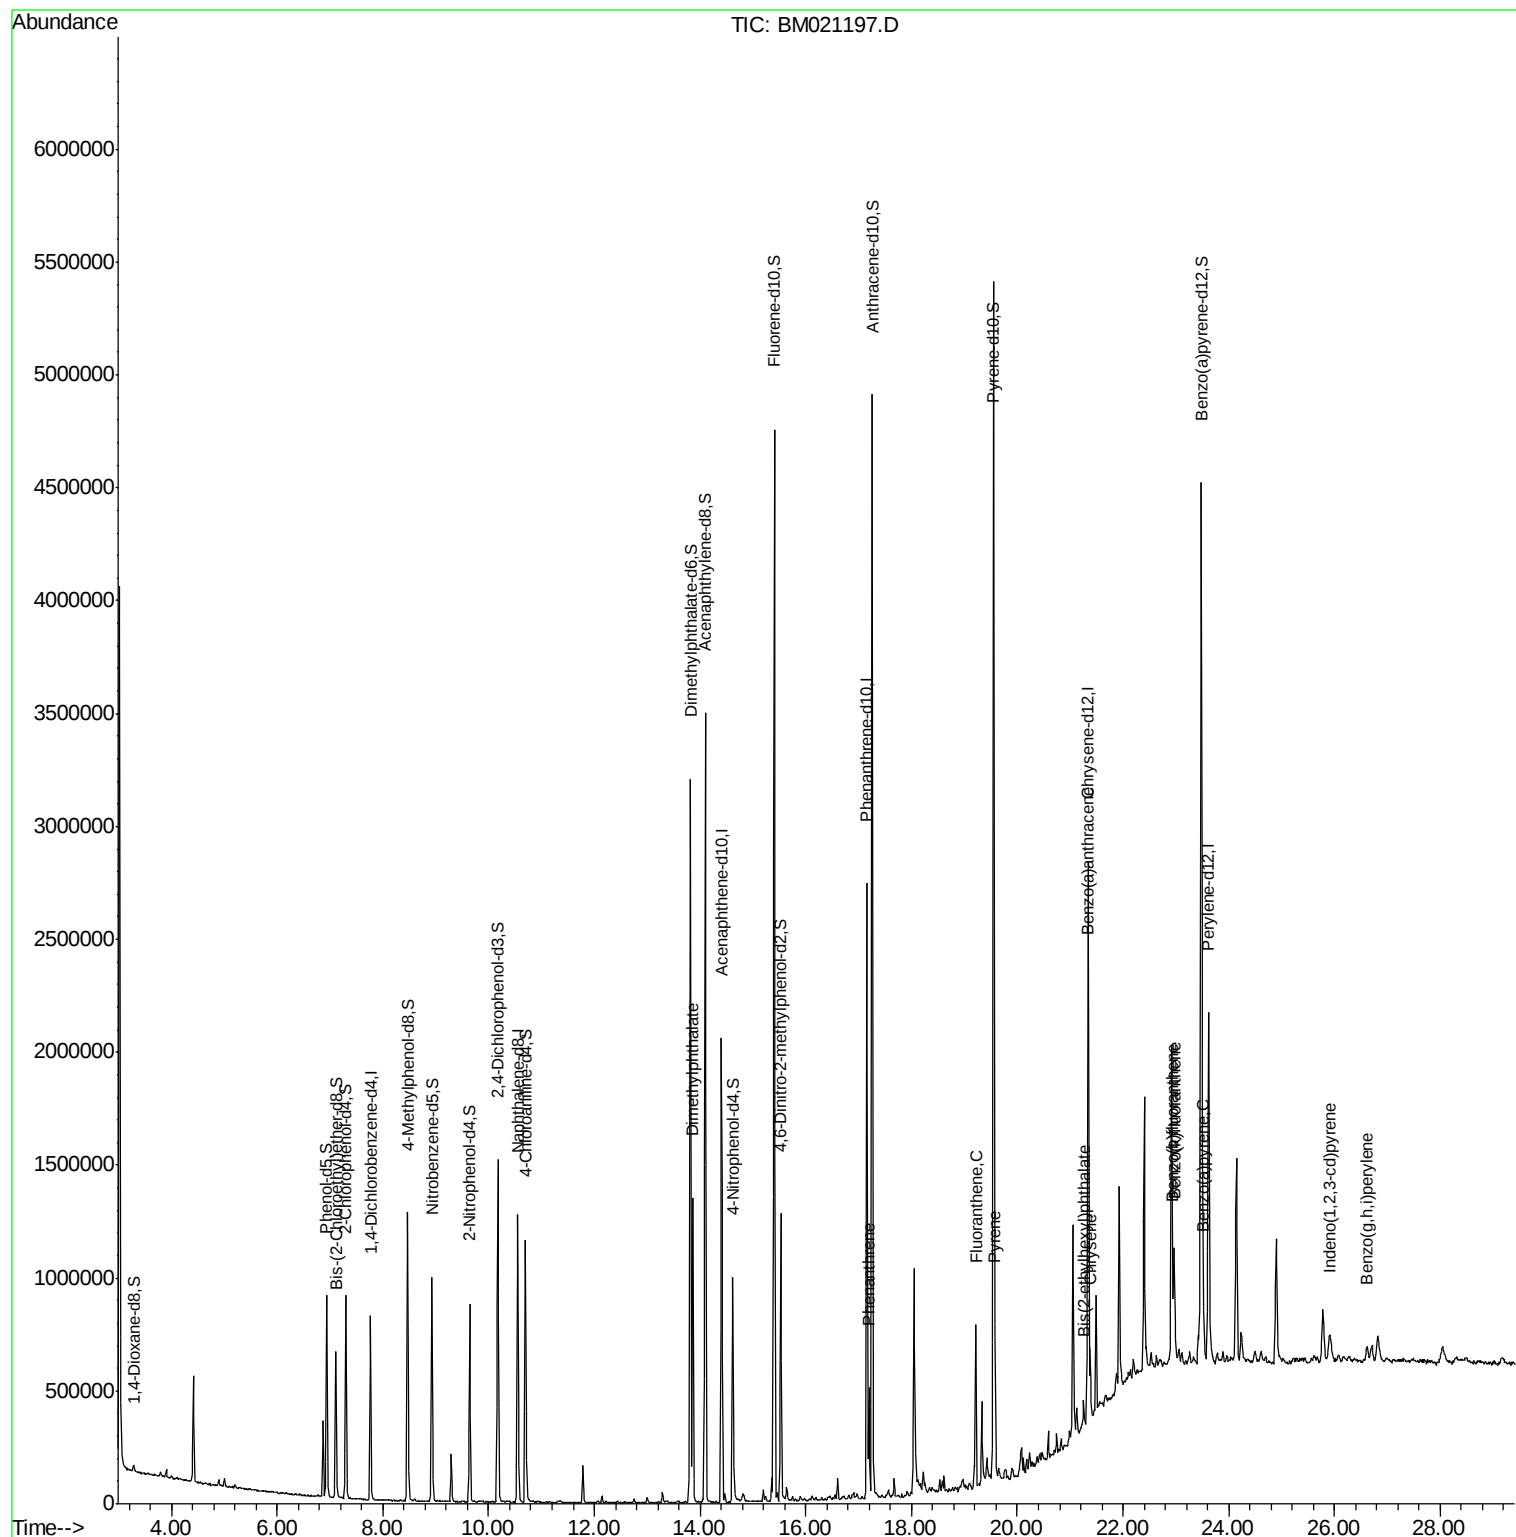

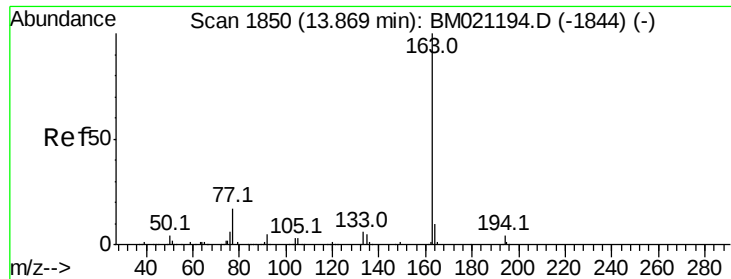





#44
Dimethylphthalate
Concen: 15.138 ng/ul
RT: 13.86 min Scan# 1849
Delta R.T. -0.01 min
Lab File: BM021197.D
Acq: 26 Jun 2019 18:17

Instrument :
BNA_M
ClientSampleId :
C5AB9

Tot Ion	Ratio	Lower	Upper
163	100		
194	4.3	3.4	5.2
164	10.5	7.7	11.5




Manual Integrations
APPROVED


mohammad
6/27/2019 8:17:55 AM

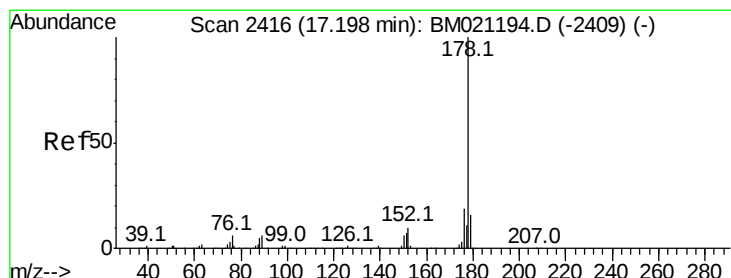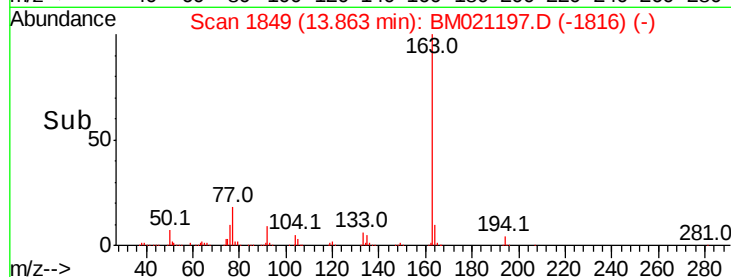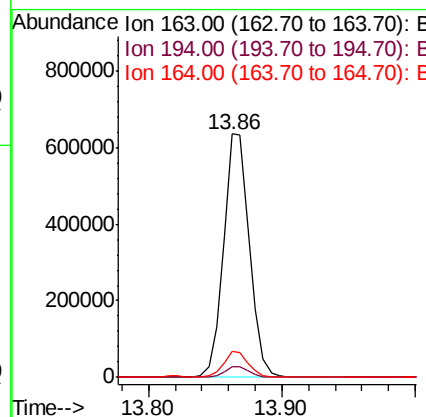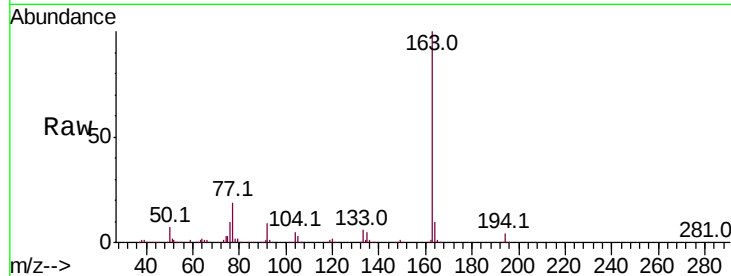

#69
Phenanthrene
Concen: 3.154 ng/ul
RT: 17.20 min Scan# 2416
Delta R.T. -0.00 min
Lab File: BM021197.D
Acq: 26 Jun 2019 18:17

Tgt Ion	Ratio	Lower	Upper
178	100		
179	15.5	11.8	17.8
176	19.2	15.0	22.6

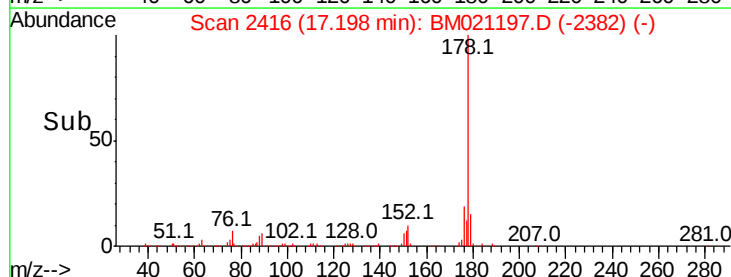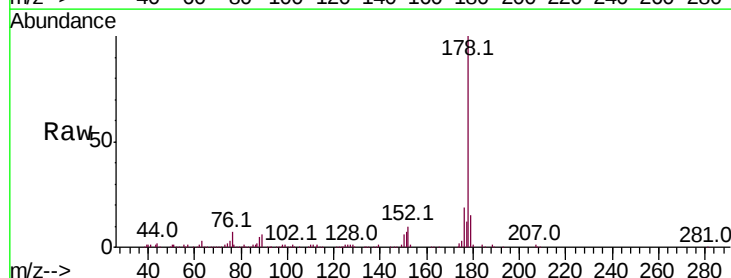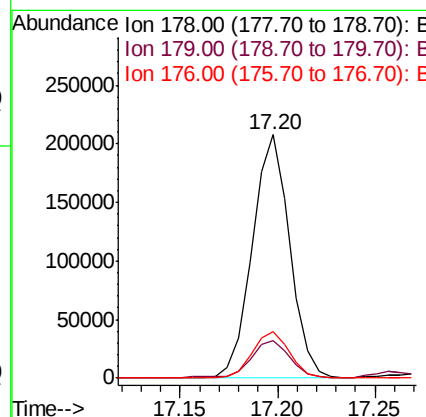

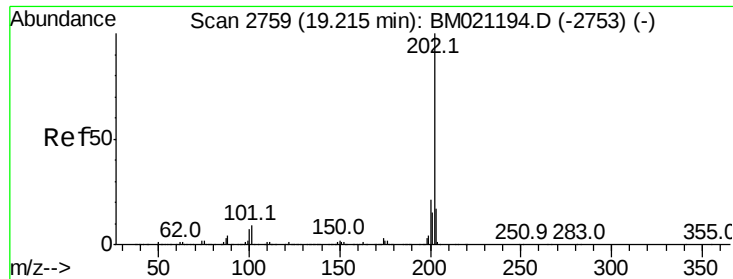





#76
Fluoranthene
Concen: 4.540 ng/ul
RT: 19.22 min Scan# 2759
Delta R.T. -0.00 min
Lab File: BM021197.D
Acq: 26 Jun 2019 18:17

Instrument :
BNA_M
ClientSampleId :
C5AB9

Tot Ion	Ratio	Resp	Lower	Upper
202	100	425985		
101	8.3		6.7	10.1
100	6.3		5.5	8.3




Manual Integrations
APPROVED


mohammad
6/27/2019 8:17:55 AM

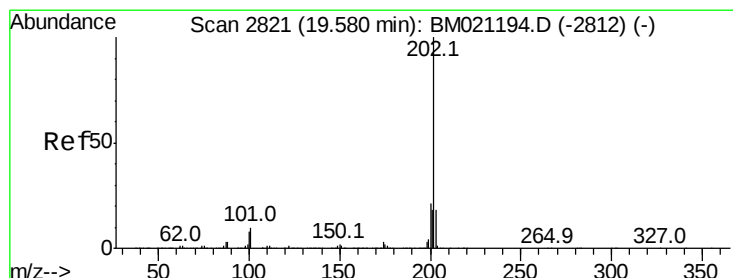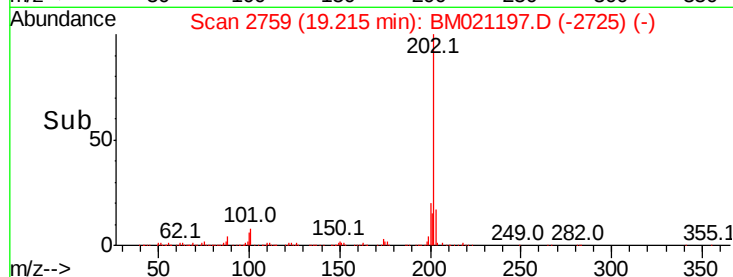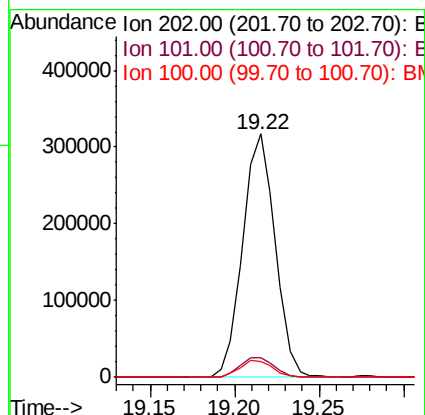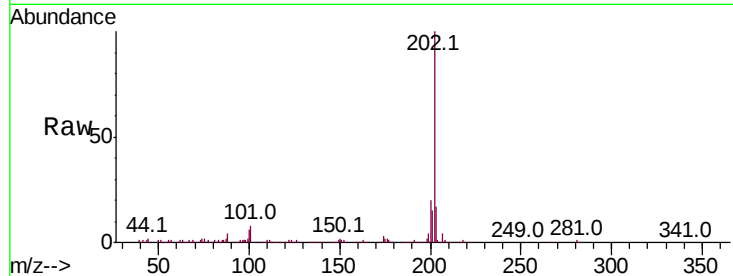

#79
Pyrene
Concen: 4.573 ng/ul
RT: 19.58 min Scan# 2821
Delta R.T. -0.00 min
Lab File: BM021197.D
Acq: 26 Jun 2019 18:17

Tgt Ion	Ratio	Resp	Lower	Upper
202	100	347586		
101	10.0		8.1	12.1
100	9.3		6.6	10.0

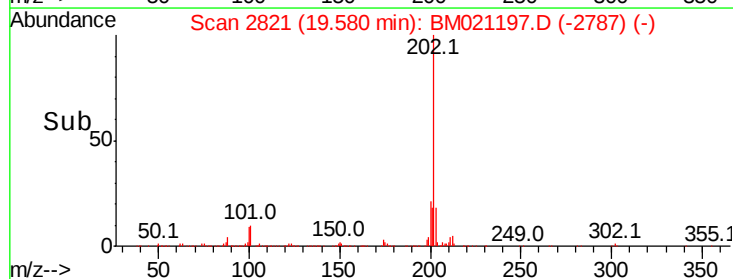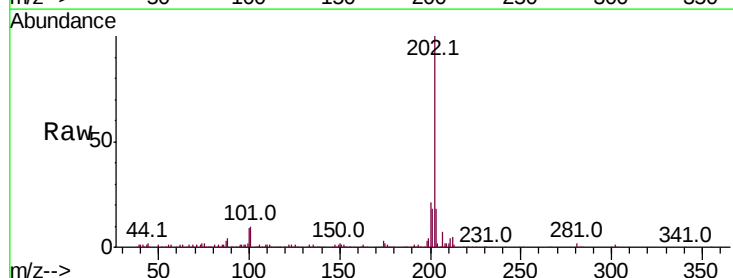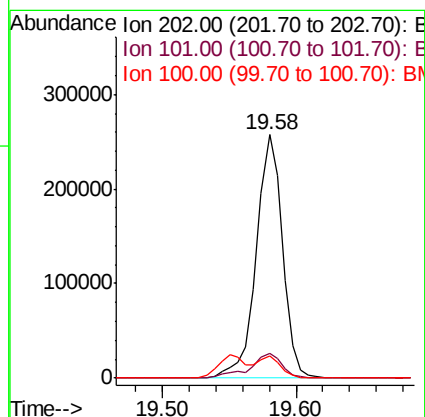

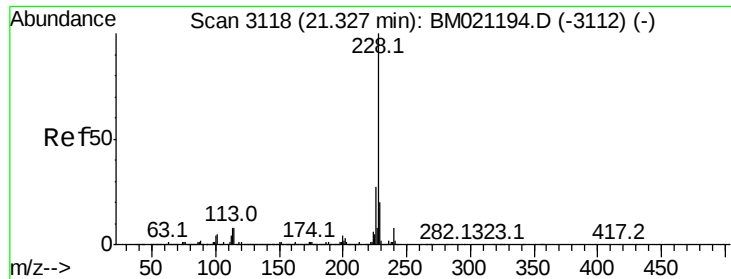





#82
 Benzo(a)anthracene
 Concen: 2.190 ng/ul
 RT: 21.33 min Scan# 3119
 Delta R.T. 0.01 min
 Lab File: BM021197.D
 Acq: 26 Jun 2019 18:17

Instrument :
 BNA_M
 ClientSampleId :
 C5AB9

Tot Ion	Ratio	Lower	Upper
228	100		
229	20.5	15.8	23.8
226	26.2	21.4	32.2




Manual Integrations
 APPROVED


mohammad
 6/27/2019 8:17:55 AM

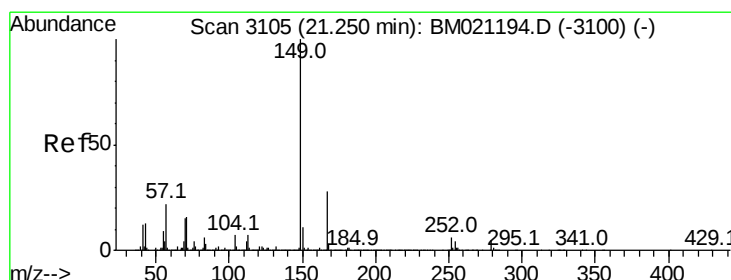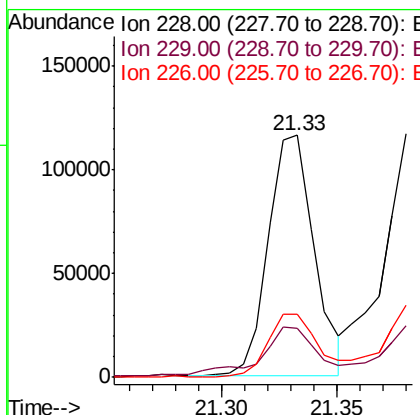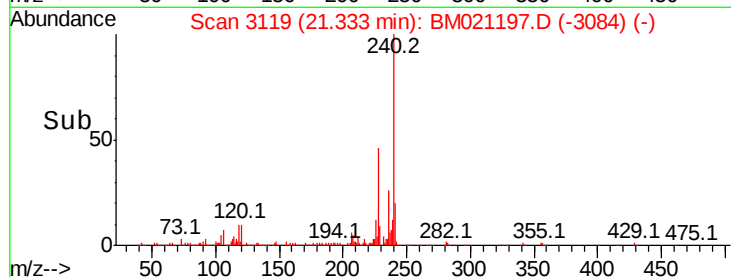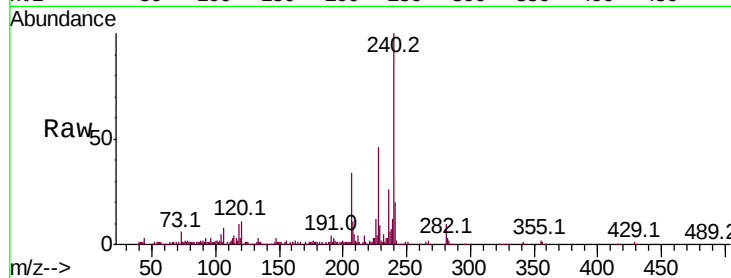

#83
 Bis(2-ethylhexyl)phthalate
 Concen: 1.045 ng/ul
 RT: 21.26 min Scan# 3106
 Delta R.T. 0.01 min
 Lab File: BM021197.D
 Acq: 26 Jun 2019 18:17

Tgt Ion	Ratio	Lower	Upper
149	100		
167	29.3	22.3	33.5
279	5.5	3.8	5.6

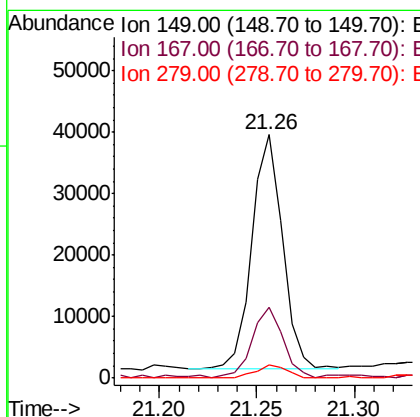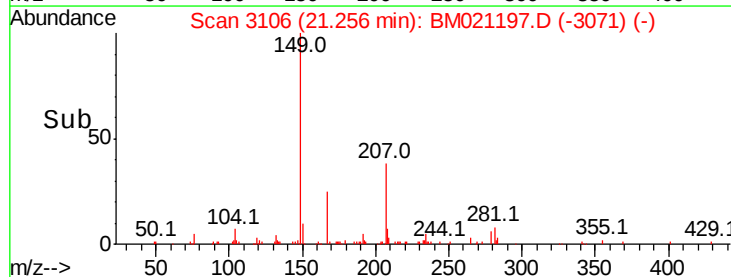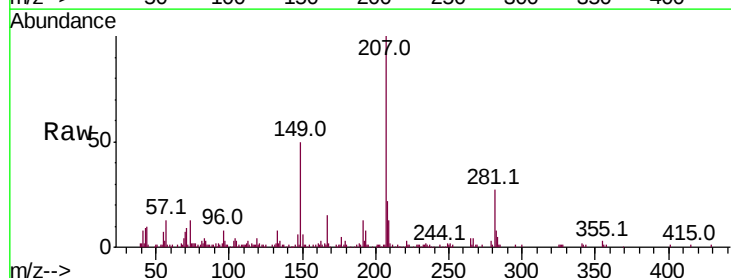

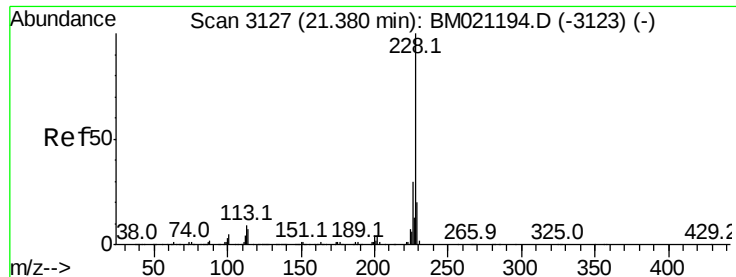

#84

Chrysene

Concen: 2.524 ng/ul

RT: 21.38 min Scan# 3127

Delta R.T. -0.00 min

Lab File: BM021197.D

Acq: 26 Jun 2019 18:17

Instrument :

BNA_M





ClientSampleId :

C5AB9

Tot Ion:	228	Resp:	173232
Ion Ratio	Lower	Upper	
228	100		
226	29.4	23.9	35.9
229	21.0	15.4	23.2

Manual Integrations
APPROVED

mohammad
6/27/2019 8:17:55 AM

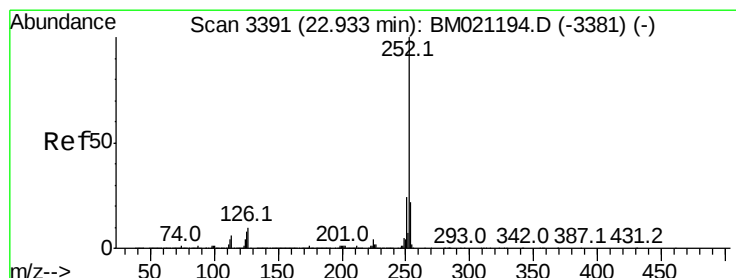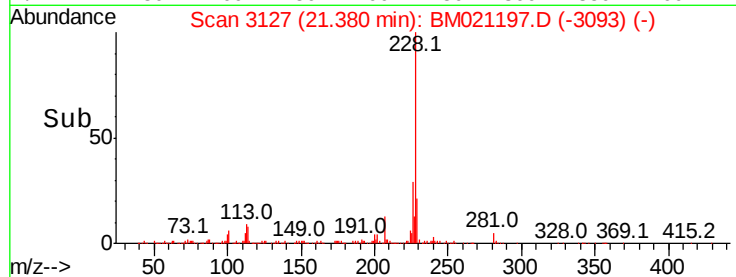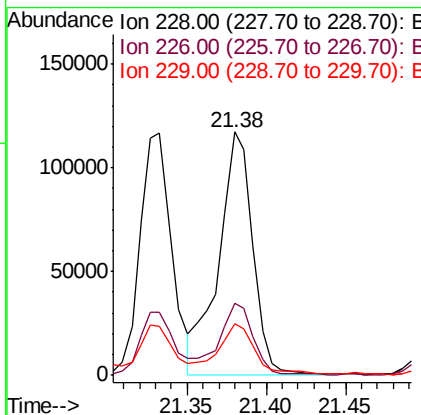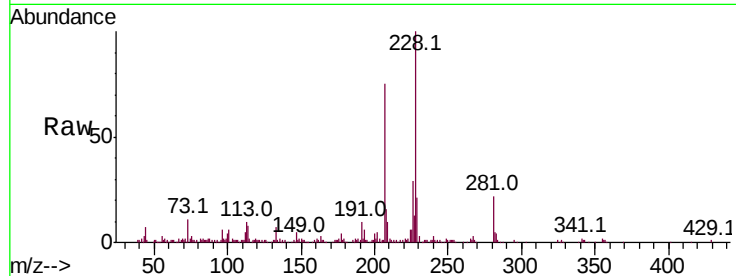

#87

Benzo(b)fluoranthene

Concen: 3.026 ng/ul




RT: 22.94 min Scan# 3392


Delta R.T. 0.01 min

Lab File: BM021197.D

Acq: 26 Jun 2019 18:17

Tgt Ion:	252	Resp:	223955
Ion Ratio	Lower	Upper	
252	100		
253	22.0	17.5	26.3
125	10.0	6.3	9.5#

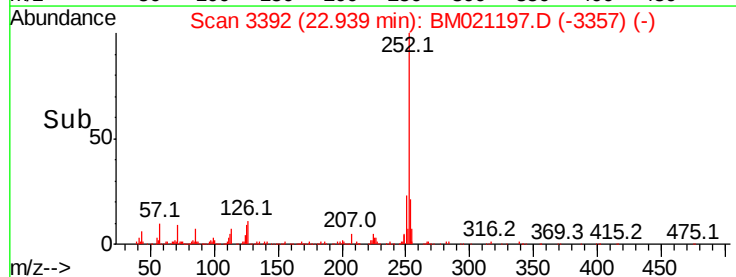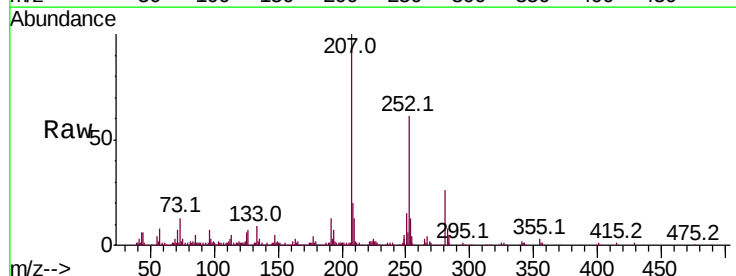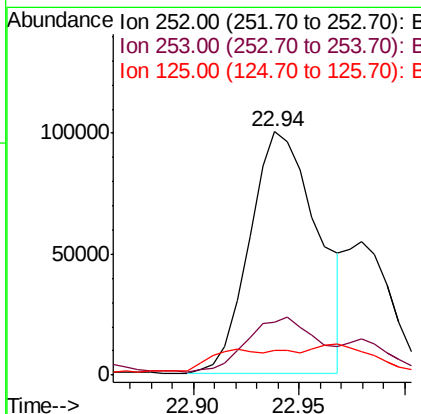

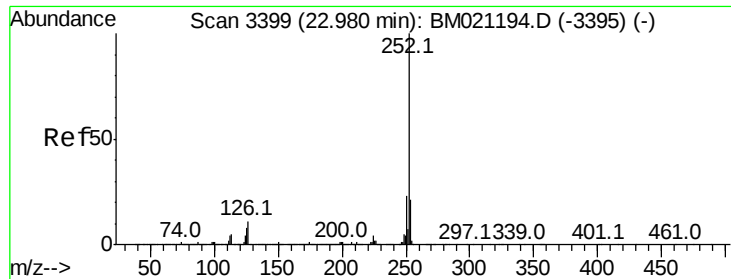

#88

Benzo(k)fluoranthene

Concen: 1.182 ng/ul m

RT: 22.98 min Scan# 3399

Delta R.T. -0.00 min

Lab File: BM021197.D

Acq: 26 Jun 2019 18:17

Instrument :

BNA_M


ClientSampleId :

C5AB9




Tot Ion:	252	Resp:	84197
Ion Ratio	Lower	Upper	
252	100		
253	26.7	17.5	26.3#
125	17.4	6.6	9.8#

Manual Integrations
APPROVED

mohammad
6/27/2019 8:17:55 AM

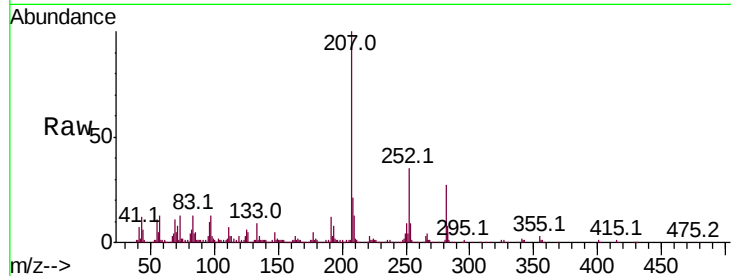

Abundance Ion 252.00 (251.70 to 252.70): E
Ion 253.00 (252.70 to 253.70): E
Ion 125.00 (124.70 to 125.70): E

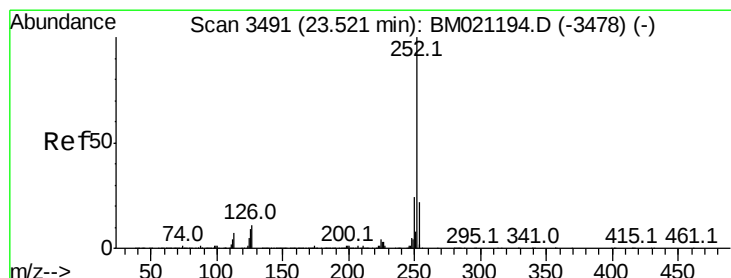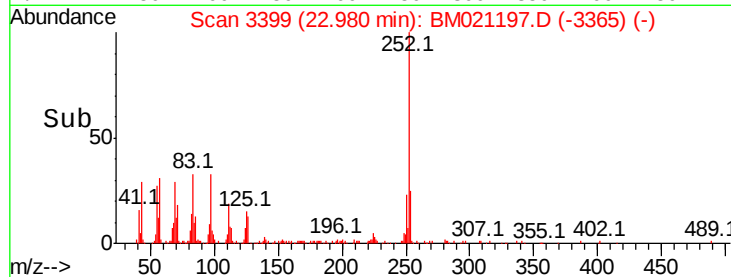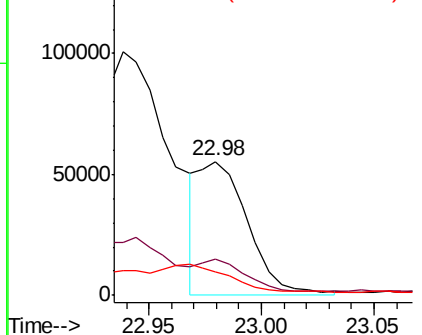

#90

Benzo(a)pyrene

Concen: 2.078 ng/ul

RT: 23.52 min Scan# 3491




Delta R.T. -0.00 min


Lab File: BM021197.D

Acq: 26 Jun 2019 18:17

Tgt Ion:	252	Resp:	144789
Ion Ratio	Lower	Upper	
252	100		
253	23.6	17.8	26.8
125	10.4	7.2	10.8

Abundance Ion 252.00 (251.70 to 252.70): E
Ion 253.00 (252.70 to 253.70): E
Ion 125.00 (124.70 to 125.70): E

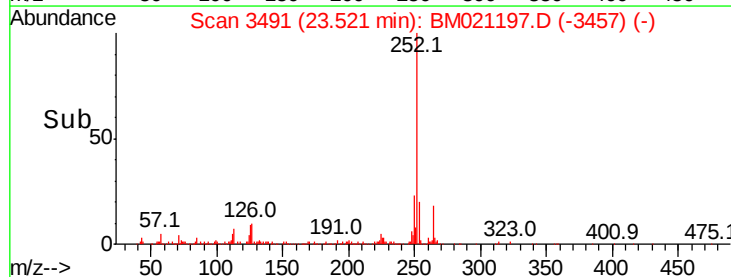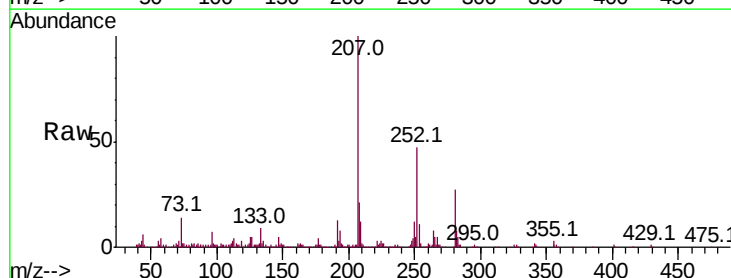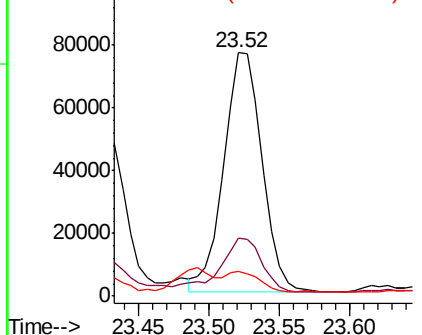

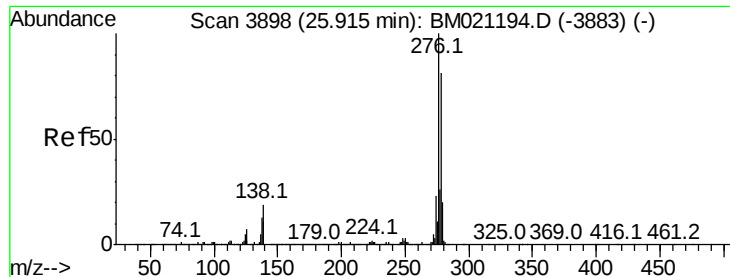

#91

Indeno(1,2,3-cd)pyrene

Concen: 1.243 ng/ul

RT: 25.91 min Scan# 3898

Delta R.T. -0.00 min

Lab File: BM021197.D

Acq: 26 Jun 2019 18:17

Instrument :

BNA_M





ClientSampleId :

C5AB9

Tot Ion:	276	Resp:	101984
Ion Ratio	Lower	Upper	
276	100		
138	18.6	15.9	23.9
277	24.8	20.4	30.6

Manual Integrations
APPROVED

mohammad
6/27/2019 8:17:55 AM

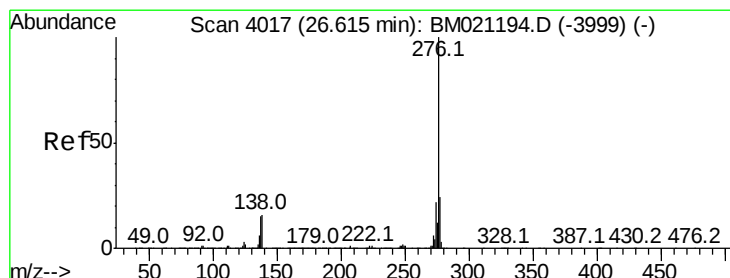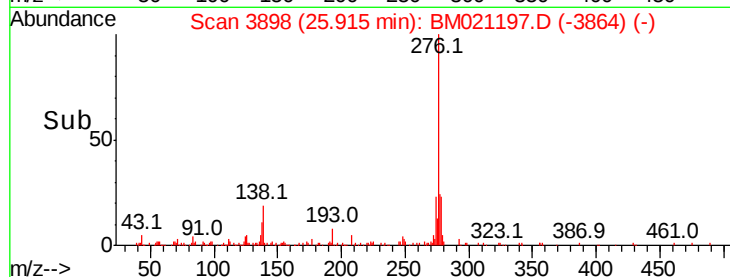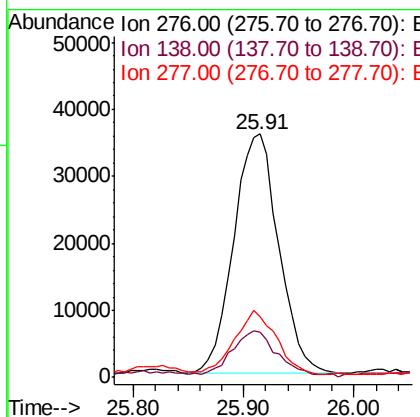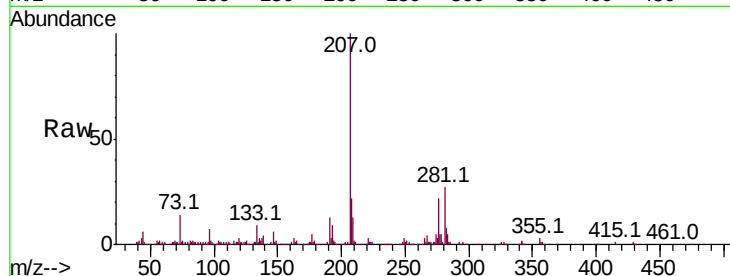

#93

Benzo(g,h,i)perylene

Concen: 1.274 ng/ul

RT: 26.61 min Scan# 4016

Delta R.T. -0.01 min

Lab File: BM021197.D

Acq: 26 Jun 2019 18:17

Tgt Ion:	276	Resp:	86054
Ion Ratio	Lower	Upper	
276	100		
138	18.2	14.6	21.8
277	24.3	18.9	28.3

