

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM062519\
 Data File : BM021181.D
 Acq On : 26 Jun 2019 03:05
 Operator : HP/JU
 Sample : PB120883BL
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK83

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.022	3	6	14	rVB	68688	96643	1.02%	0.119%
2	3.281	47	50	59	rVB2	56259	84869	0.90%	0.104%
3	6.934	665	671	680	rBV	1099045	1731359	18.26%	2.128%
4	7.110	695	701	712	rVB	858098	1333509	14.07%	1.639%
5	7.298	726	733	744	rVB	1162623	1831230	19.32%	2.251%
6	7.769	806	813	822	rVB	769541	1258217	13.27%	1.547%
7	8.469	925	932	943	rBV	1476265	2345039	24.73%	2.883%
8	8.928	1003	1010	1020	rBV	1134604	1879595	19.83%	2.310%
9	9.645	1125	1132	1141	rBV	999304	1637188	17.27%	2.012%
10	10.175	1215	1222	1234	rBV	1589451	2703389	28.51%	3.323%
11	10.551	1279	1286	1299	rVB	1179671	1991043	21.00%	2.447%
12	10.698	1303	1311	1332	rBV	1524088	2673385	28.20%	3.286%
13	12.151	1550	1558	1564	rBV2	26457	46150	0.49%	0.057%
14	13.821	1832	1842	1854	rBV	3250997	4528010	47.76%	5.566%
15	14.098	1882	1889	1905	rBV	3570733	5407978	57.04%	6.648%
16	14.410	1934	1942	1957	rBV2	2038927	3120790	32.92%	3.836%
17	14.615	1970	1977	1999	rBV	1155044	1872308	19.75%	2.301%
18	15.204	2071	2077	2082	rVB	17706	24929	0.26%	0.031%
19	15.404	2104	2111	2120	rBV	5008586	6977569	73.60%	8.577%
20	15.527	2126	2132	2145	rBV	1224357	1699527	17.93%	2.089%
21	15.645	2147	2152	2158	rVB2	55611	82762	0.87%	0.102%
22	16.186	2240	2244	2249	rVB5	11275	15597	0.16%	0.019%
23	16.945	2368	2373	2378	rBV3	10595	15217	0.16%	0.019%
24	17.156	2402	2409	2416	rBV	2853896	4076673	43.00%	5.011%
25	17.256	2419	2426	2438	rBV	5706311	7930747	83.65%	9.749%
26	19.109	2738	2741	2744	rBV5	6639	11033	0.12%	0.014%
27	19.180	2750	2753	2760	rVB	67297	88064	0.93%	0.108%
28	19.433	2793	2796	2801	rBV	42109	57342	0.60%	0.070%
29	19.550	2809	2816	2826	rBV	7104024	9480790	100.00%	11.654%
30	21.339	3114	3120	3126	rBV	3398896	4466301	47.11%	5.490%
31	23.462	3474	3481	3491	rBV	4168448	8057030	84.98%	9.904%
32	23.609	3499	3506	3517	rVB	2007218	3828755	40.38%	4.706%

LSC Area Percent Report

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM062519\
Data File : BM021181.D
Acq On : 26 Jun 2019 03:05
Operator : HP/JU
Sample : PB120883BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK83

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0

Filtering: 5
Min Area: 0.1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
Title : SVOA CALIBRATION


Sum of corrected areas: 81353038

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM062519\
Data File : BM021181.D
Acq On : 26 Jun 2019 03:05
Operator : HP/JU
Sample : PB120883BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK83

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

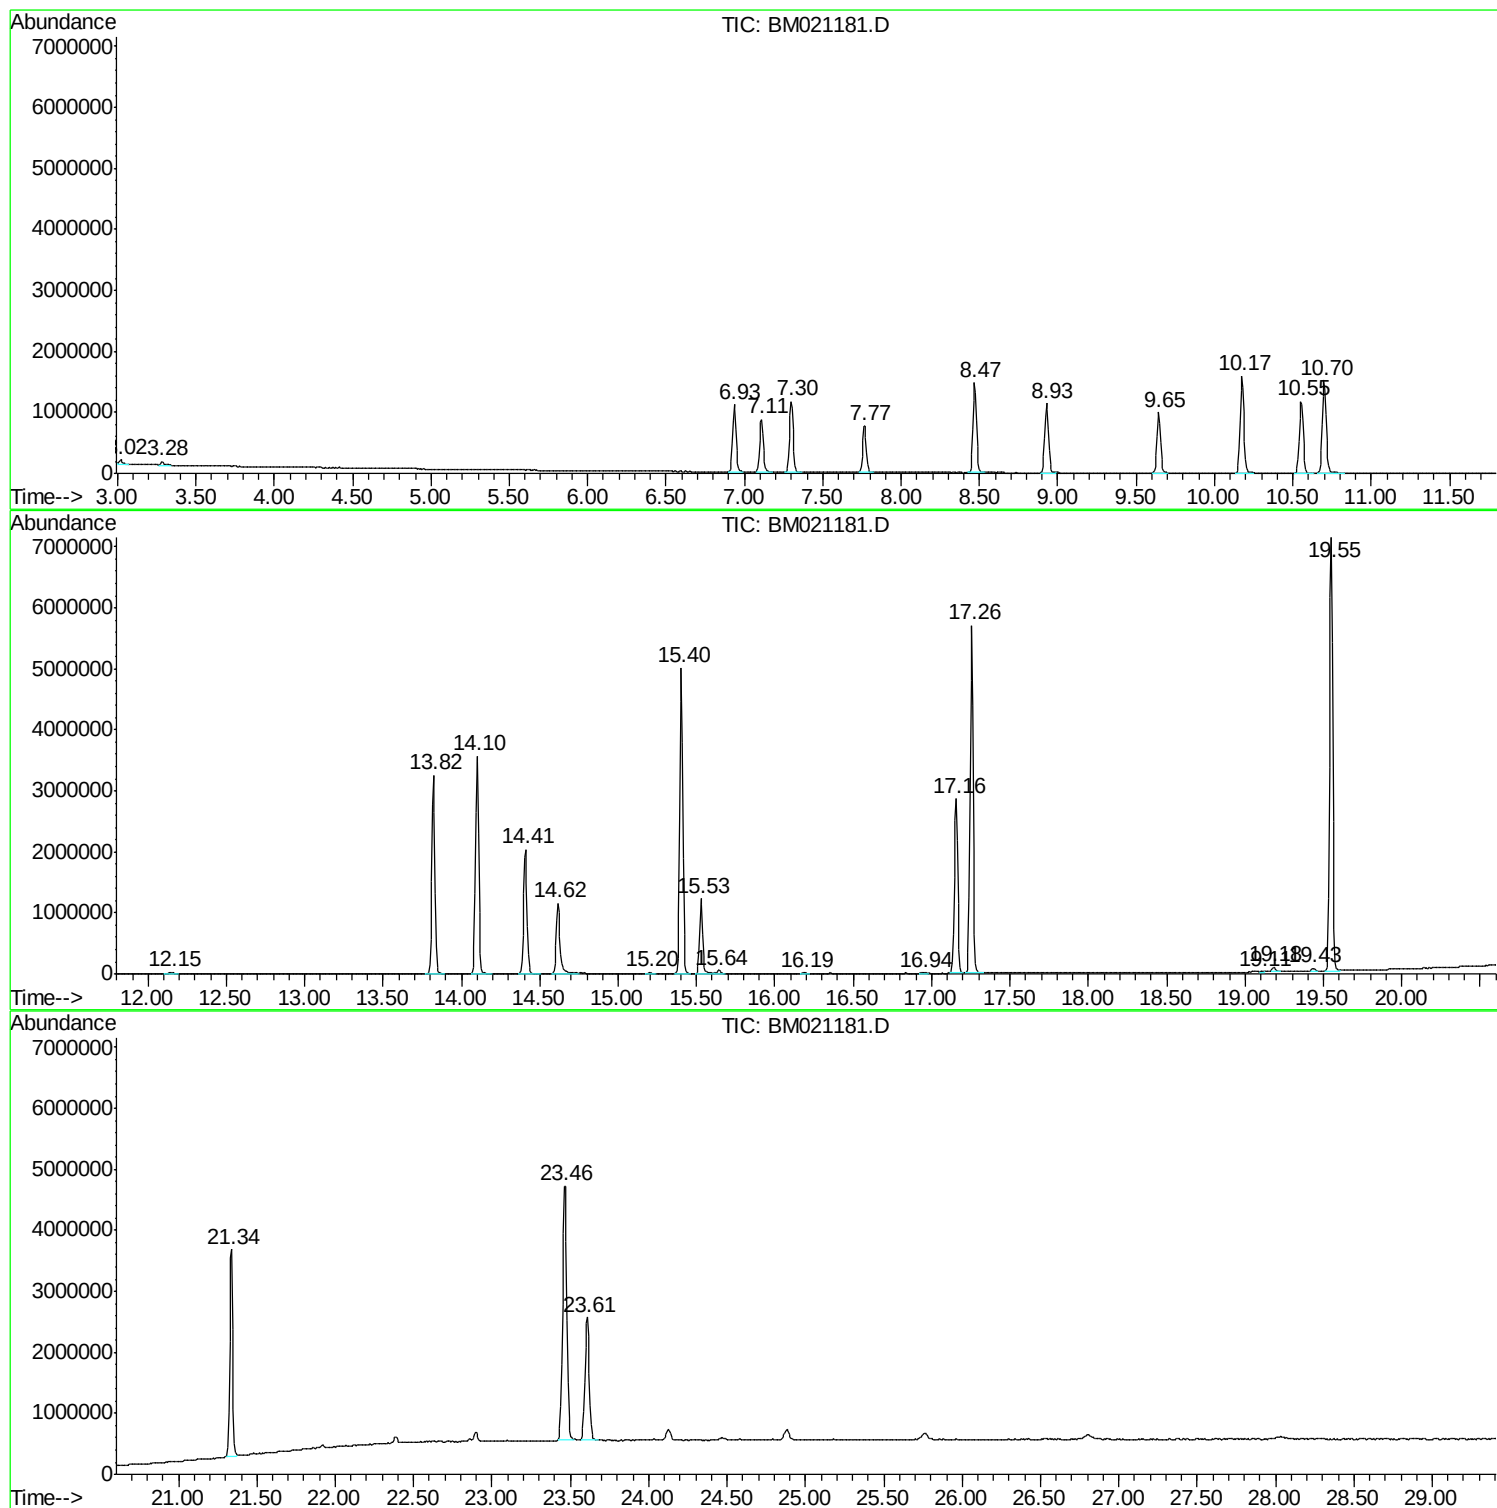

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM062519\
Data File : BM021181.D
Acq On : 26 Jun 2019 03:05
Operator : HP/JU
Sample : PB120883BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK83

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM062519\
Data File : BM021181.D
Acq On : 26 Jun 2019 03:05
Operator : HP/JU
Sample : PB120883BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK83

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc