

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062623\
 Data File : BM040404.D
 Acq On : 26 Jun 2023 16:41
 Operator : MA/JU
 Sample : PB153416BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK416

Quant Time: Jun 27 04:26:21 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 23 00:44:24 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.949	152	7003	0.400	ng/ul	0.00
4) Naphthalene-d8	10.756	136	23103	0.400	ng/ul #	0.00
9) Acenaphthene-d10	14.586	164	9889	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.332	188	17309	0.400	ng/ul	0.00
17) Chrysene-d12	21.515	240	12304	0.400	ng/ul	0.00
23) Perylene-d12	23.929	264	14960	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.333	96	64722	5.884	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.345	152	10544	0.326	ng/ul	0.00
18) Fluoranthene-d10	19.361	212	13357	0.339	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.581	166	3139	0.079	ng/ul#	16
20) Pyrene	19.723	202	2216	0.040	ng/ul#	1
26) Benzo(a)pyrene	23.771	252	4893	0.094	ng/ul#	52


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062623\
Data File : BM040404.D
Acq On : 26 Jun 2023 16:41
Operator : MA/JU
Sample : PB153416BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK416

Quant Time: Jun 27 04:26:21 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 23 00:44:24 2023
Response via : Initial Calibration




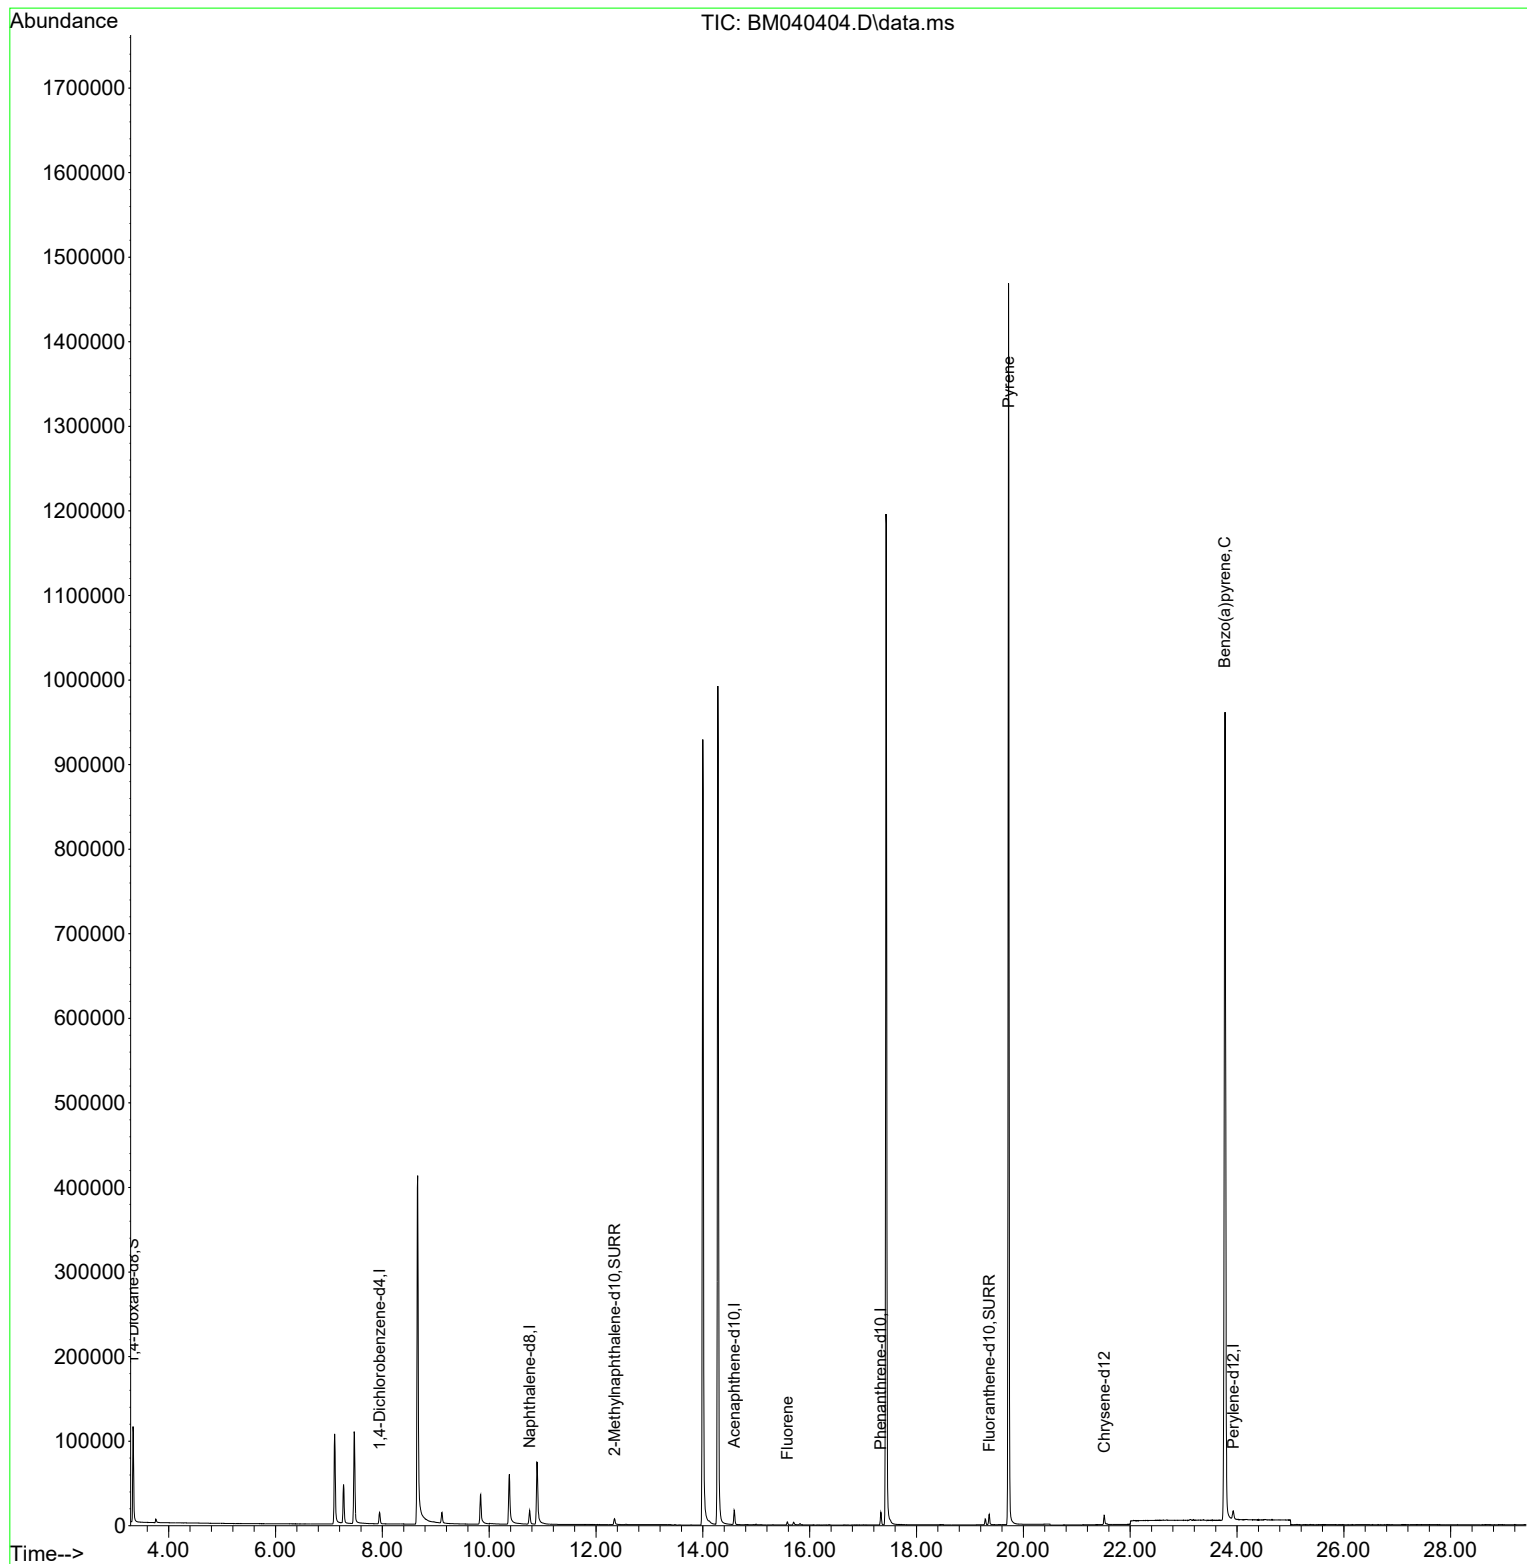


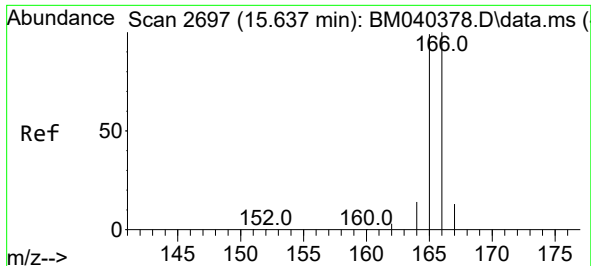

#12
Fluorene
Concen: 0.079 ng/ul
RT: 15.581 min Scan# 20
Delta R.T. -0.060 min
Lab File: BM040404.D
Acq: 26 Jun 2023 16:41




Instrument :
BNA_M
ClientSampleId :
SBLK416


Tgt Ion:166 Resp: 3139
Ion Ratio Lower Upper
166 100
165 10.3 79.6 119.4#
167 33.7 11.4 17.0#

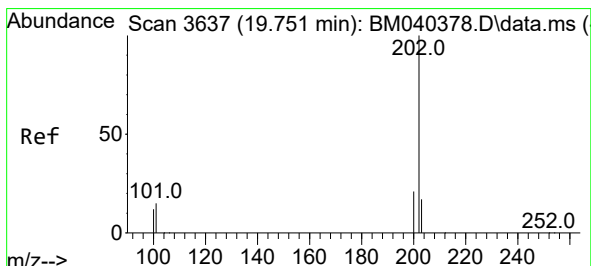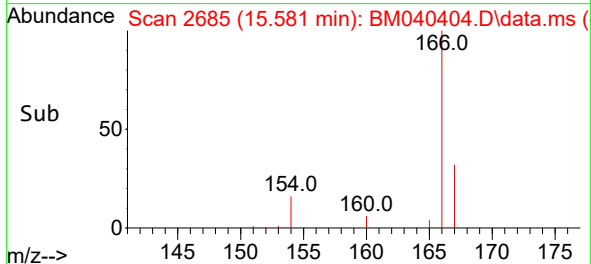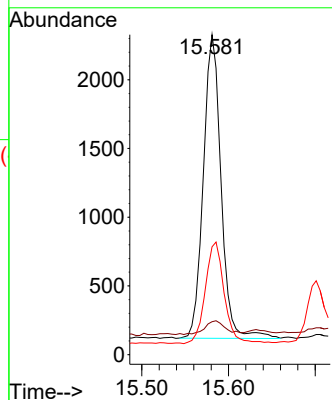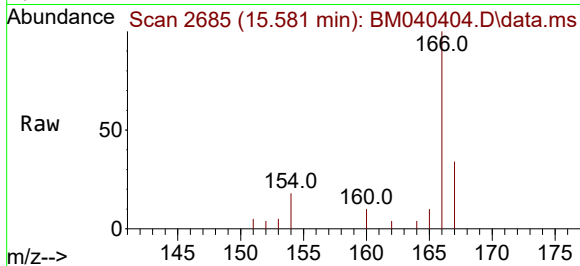

#20
Pyrene
Concen: 0.040 ng/ul
RT: 19.723 min Scan# 3631
Delta R.T. -0.033 min
Lab File: BM040404.D
Acq: 26 Jun 2023 16:41


Tgt Ion:202 Resp: 2216
Ion Ratio Lower Upper
202 100
101 169.9 12.6 18.8#
100 1266.9 9.8 14.6#

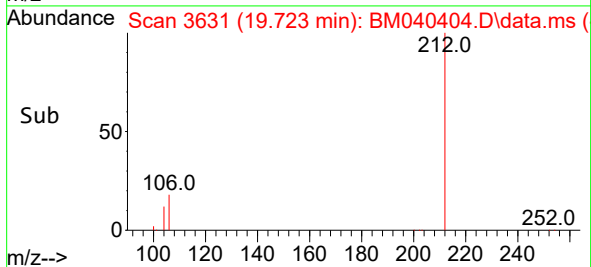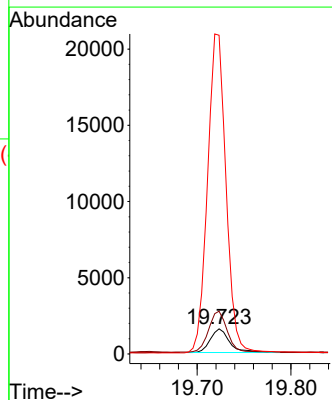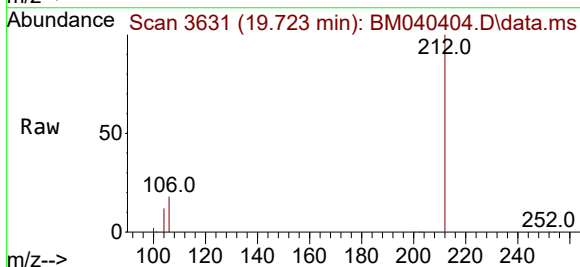

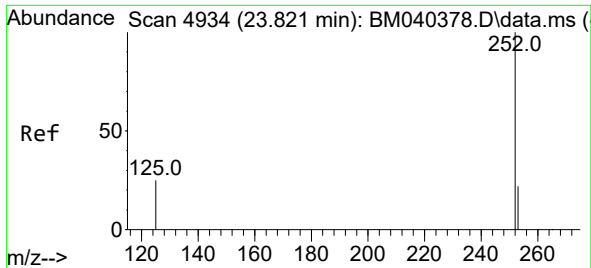

#26
Benzo(a)pyrene
Concen: 0.094 ng/ul
RT: 23.771 min Scan# 4917
Delta R.T. -0.053 min
Lab File: BM040404.D
Acq: 26 Jun 2023 16:41

Instrument :
BNA_M
ClientSampleId :
SBLK416

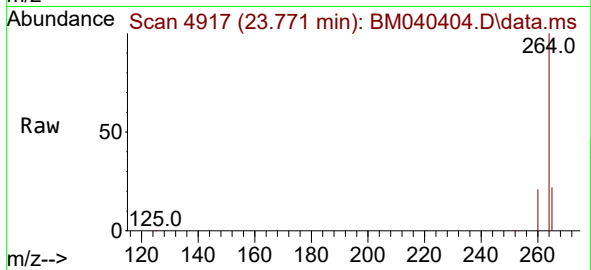

Tgt Ion:252 Resp: 4893
Ion Ratio Lower Upper
252 100
253 51.8 22.9 34.3#
125 53.3 21.0 31.4#

