

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM062719\
 Data File : BM021219.D
 Acq On : 27 Jun 2019 16:32
 Operator : HP/JU
 Sample : K3502-09
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C5AD9

Quant Time: Jun 27 18:39:41 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jun 27 15:09:50 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.76	152	230158	20.00	ng/ul	0.00
18) Naphthalene-d8	10.55	136	1035792	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.40	164	680829	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.15	188	1584078	20.00	ng/ul	0.00
77) Chrysene-d12	21.33	240	1194578	20.00	ng/ul	0.00
85) Perylene-d12	23.61	264	1208309	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.28	96	16787	3.46	ng/uL	0.00
5) Phenol-d5	6.93	99	342690	17.11	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.10	67	221150	18.53	ng/ul	0.00
9) 2-Chlorophenol-d4	7.29	132	292010	17.94	ng/ul	0.00
13) 4-Methylphenol-d8	8.46	113	268567	16.06	ng/ul	0.00
19) Nitrobenzene-d5	8.93	128	163760	19.47	ng/ul	0.00
22) 2-Nitrophenol-d4	9.64	143	184990	19.81	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.17	165	361238	19.03	ng/ul	0.00
29) 4-Chloroaniline-d4	10.70	131	384582	19.42	ng/ul	0.00
43) Dimethylphthalate-d6	13.82	166	1364057	22.17	ng/ul	0.00
46) Acenaphthylene-d8	14.10	160	1520366	20.19	ng/ul	0.00
51) 4-Nitrophenol-d4	14.62	143	146418	14.63	ng/ul	0.00
57) Fluorene-d10	15.40	176	1183703	22.12	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.53	200	153939	15.81	ng/ul	0.00
70) Anthracene-d10	17.25	188	1840339	22.36	ng/ul	0.00
78) Pyrene-d10	19.54	212	1854549	25.87	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.46	264	1573646	22.07	ng/ul	0.00


Target Compounds					Ovalue	
44) Dimethylphthalate	13.86	163	266372	4.757	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM062719\
Data File : BM021219.D
Acq On : 27 Jun 2019 16:32
Operator : HP/JU
Sample : K3502-09
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C5AD9

Quant Time: Jun 27 18:39:41 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jun 27 15:09:50 2019
Response via : Initial Calibration

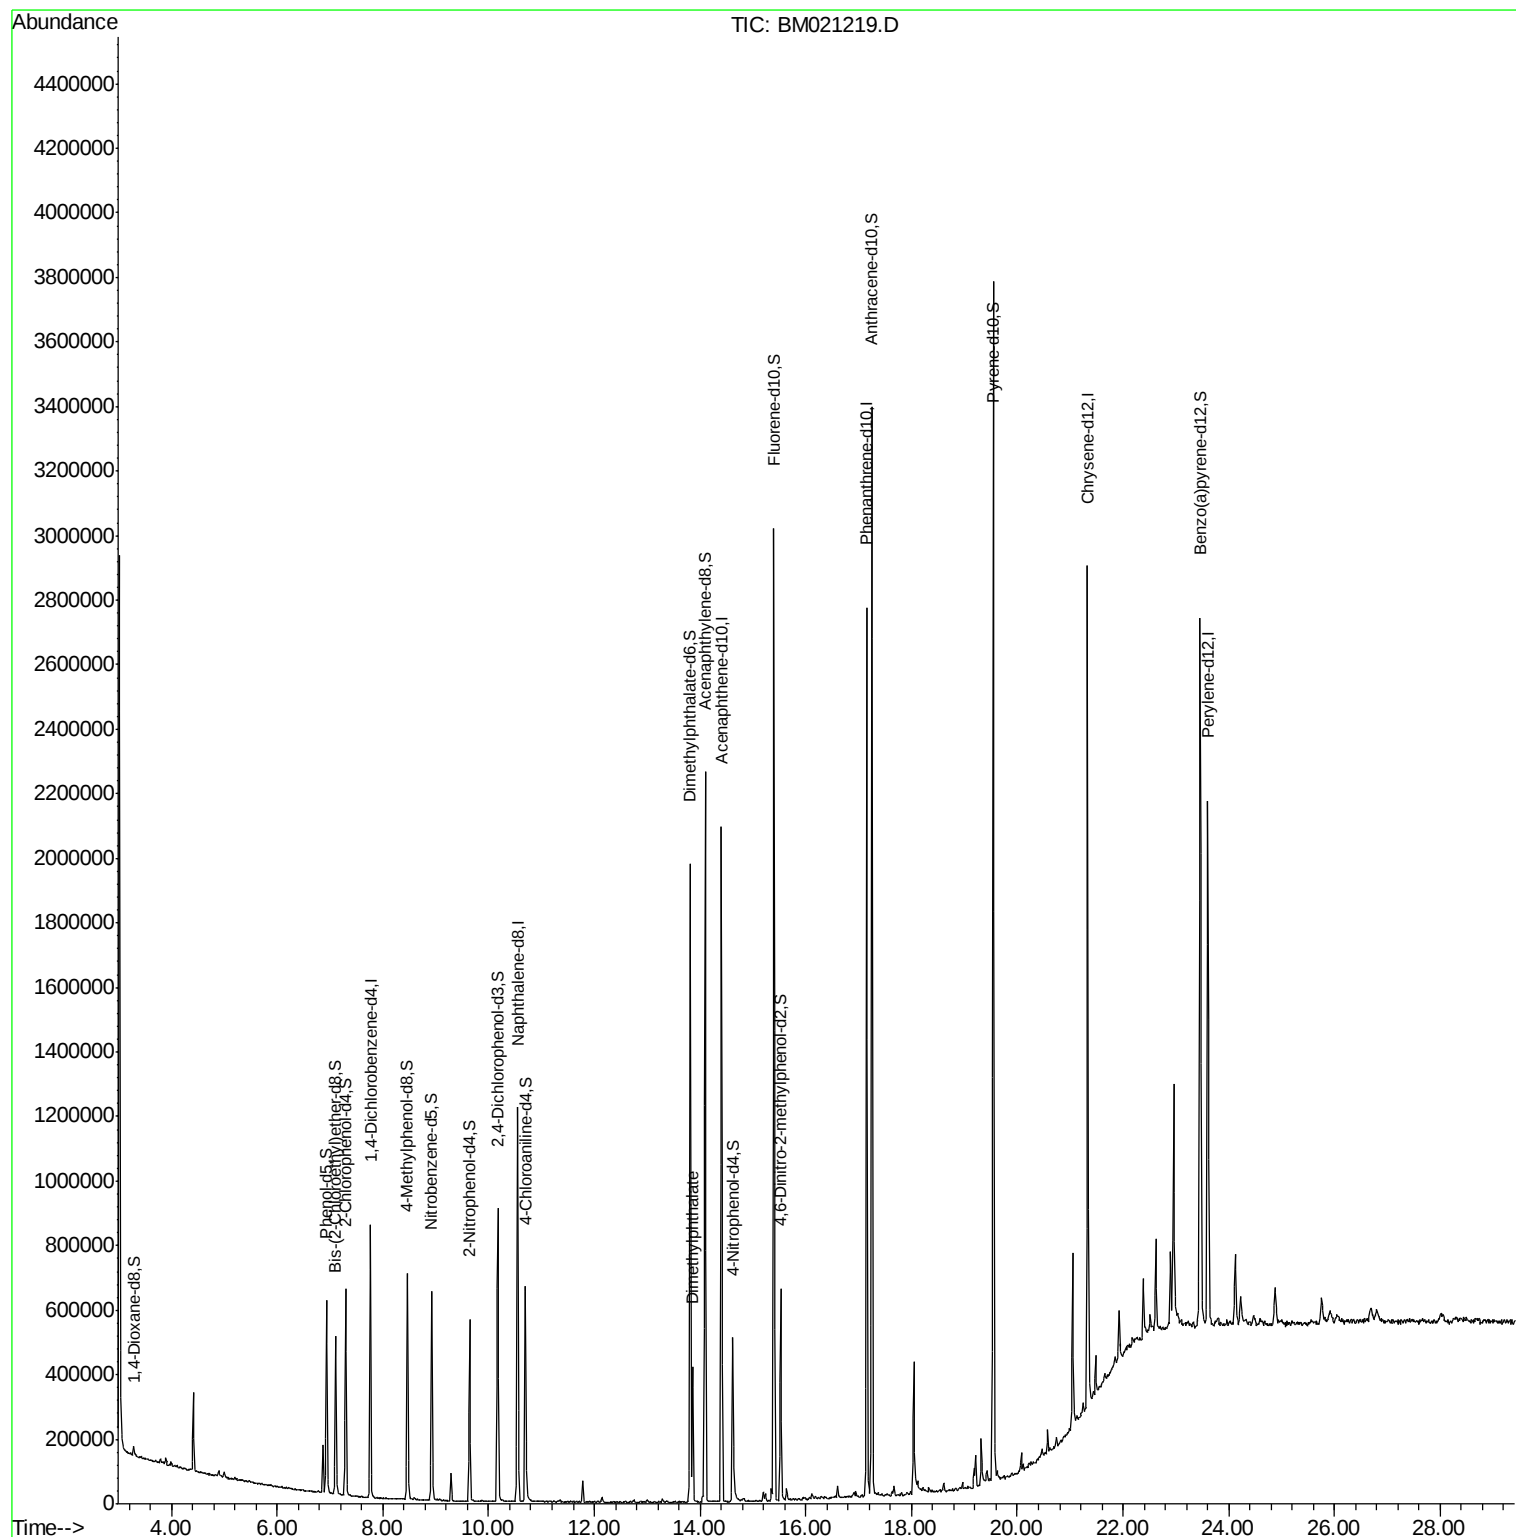

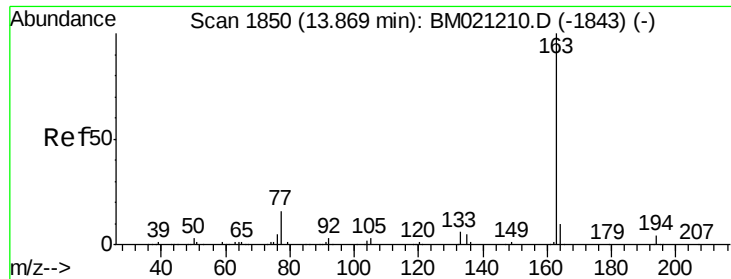

#44

Dimethylphthalate

Concen: 4.757 ng/ul

RT: 13.86 min Scan# 1849

Delta R.T. -0.01 min

Lab File: BM021219.D

Acq: 27 Jun 2019 16:32

Instrument :

BNA_M

ClientSampleId :

C5AD9


Tot Ion:163 Resp: 266372

Ion Ratio Lower Upper

163 100

194 4.5 3.4 5.2

164 10.4 7.7 11.5

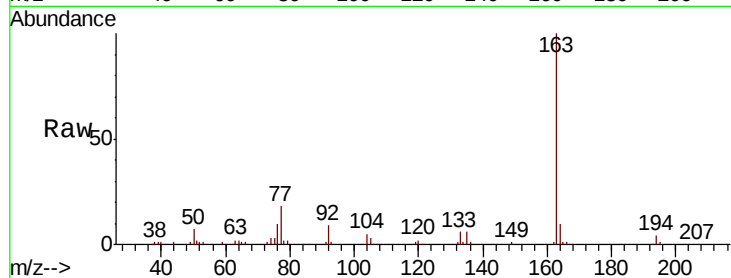

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

