

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062824\
 Data File : BM046349.D
 Acq On : 28 Jun 2024 12:46
 Operator : MA/JU
 Sample : P3076-10
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 7-S-1

Quant Time: Jun 28 13:29:57 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM062724.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 28 03:23:08 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.369	152	119708	20.000	ng	0.00
21) Naphthalene-d8	10.139	136	470683	20.000	ng	0.01
39) Acenaphthene-d10	14.022	164	282811	20.000	ng	0.00
64) Phenanthrene-d10	16.774	188	561315	20.000	ng	0.00
76) Chrysene-d12	20.992	240	457522	20.000	ng	0.00
86) Perylene-d12	23.662	264	470744	20.000	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.046	112	678446	91.101	ng	0.00
7) Phenol-d6	6.628	99	875974	82.799	ng	0.00
23) Nitrobenzene-d5	8.540	82	598120	52.680	ng	0.00
42) 2,4,6-Tribromophenol	15.527	330	289670	84.223	ng	0.00
45) 2-Fluorobiphenyl	12.639	172	972484	46.607	ng	0.00
79) Terphenyl-d14	19.421	244	1468078	53.089	ng	-0.01
Target Compounds						
						Qvalue
56) 4-Nitrophenol	14.451	139	842	3.855	ng	# 1
75) Fluoranthene	18.845	202	90889	2.575	ng	97
78) Pyrene	19.209	202	87255	2.746	ng	99
84) Bis(2-ethylhexyl)phtha...	20.927	149	7381	2.712	ng	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062824\
Data File : BM046349.D
Acq On : 28 Jun 2024 12:46
Operator : MA/JU
Sample : P3076-10
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
7-S-1

Quant Time: Jun 28 13:29:57 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM062724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 28 03:23:08 2024
Response via : Initial Calibration




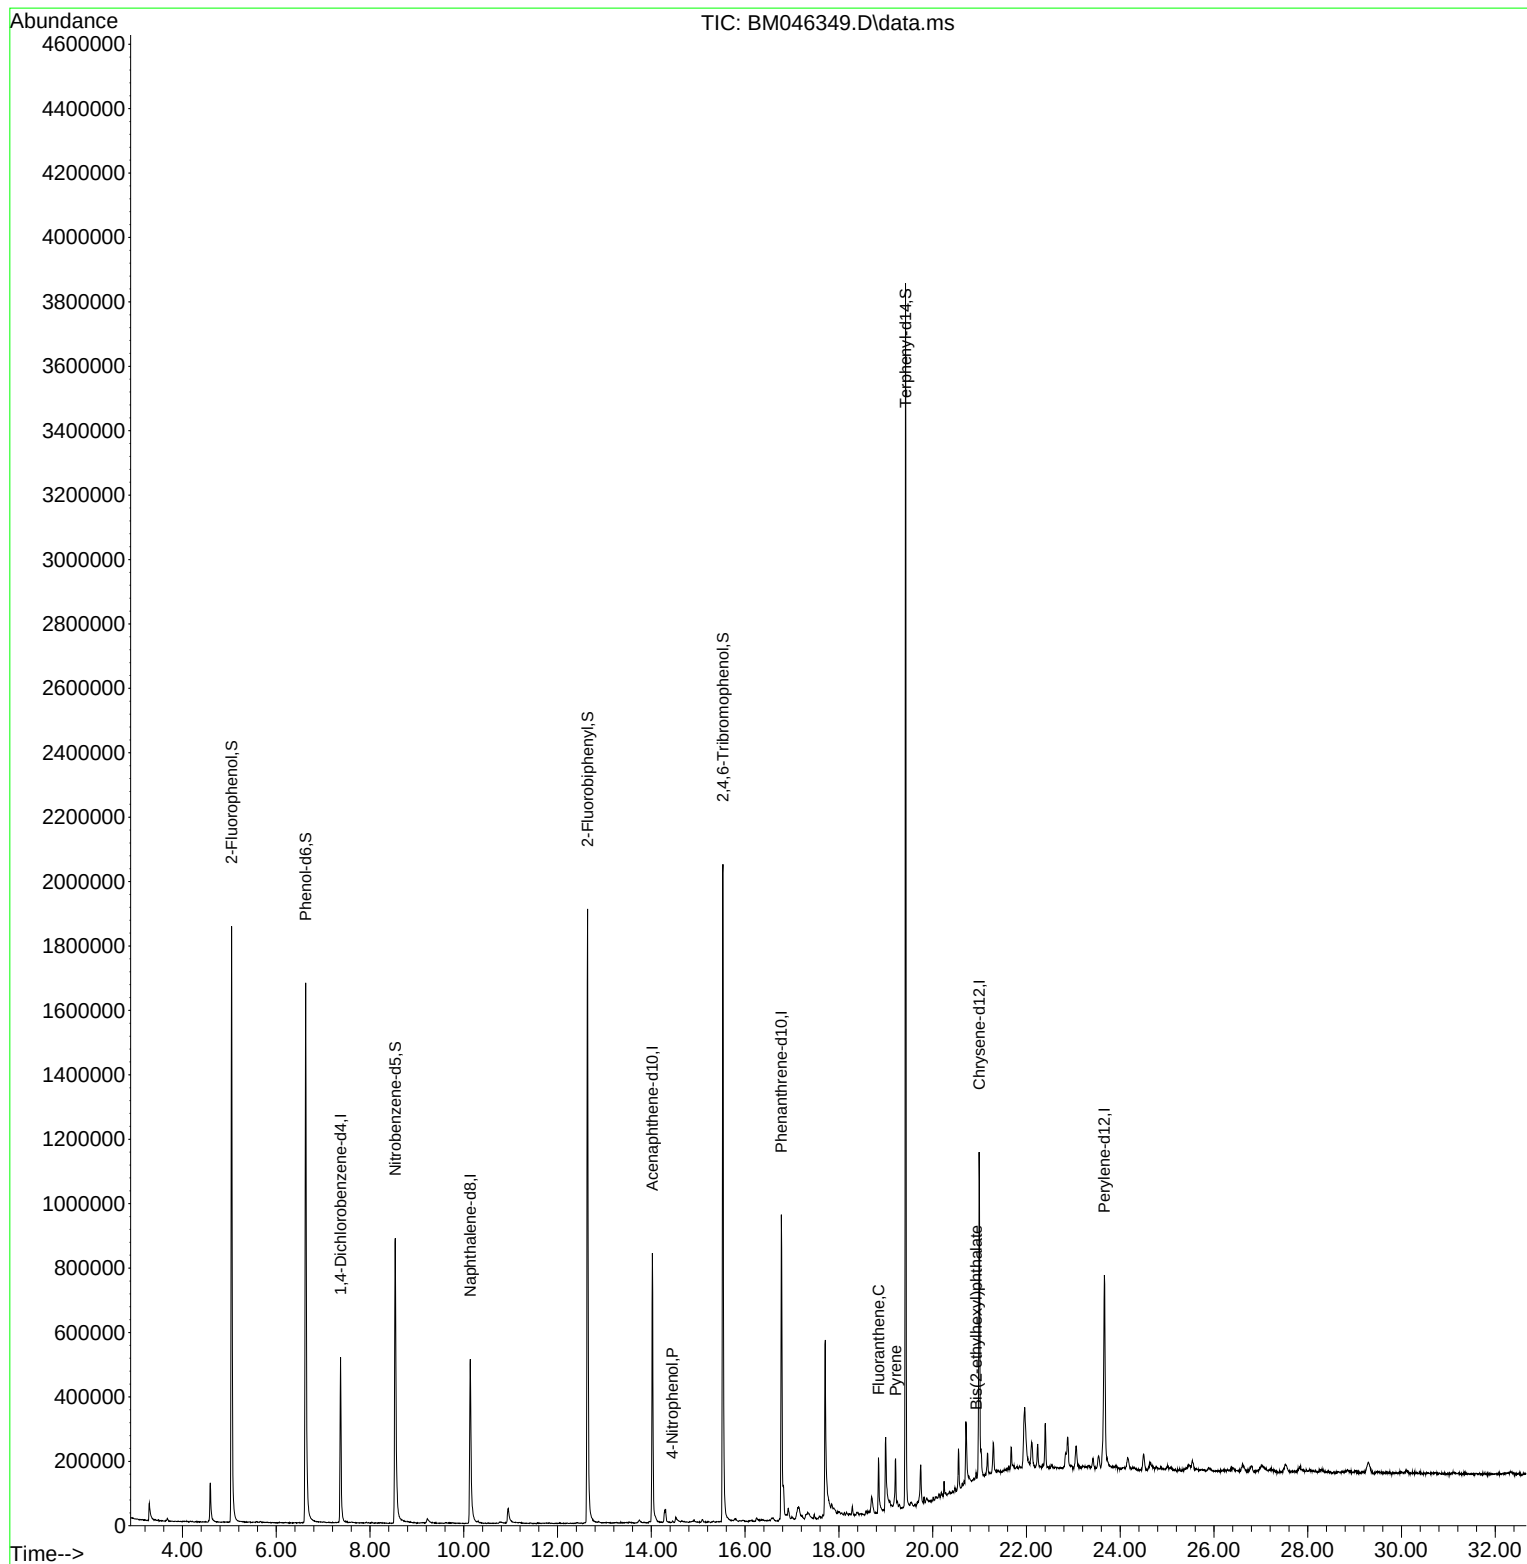


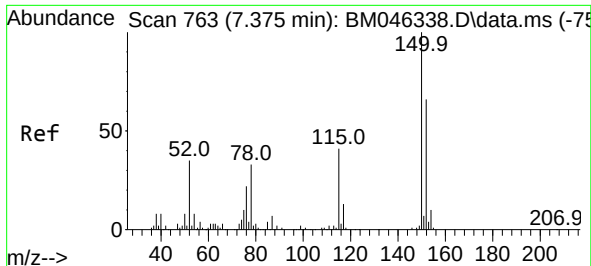

#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.369 min Scan# 70
Delta R.T. -0.006 min
Lab File: BM046349.D
Acq: 28 Jun 2024 12:46




Instrument :
BNA_M
ClientSampleId :
7-S-1


Tgt Ion:152 Resp: 119708
Ion Ratio Lower Upper
152 100
150 155.4 122.1 183.1
115 63.8 50.2 75.4

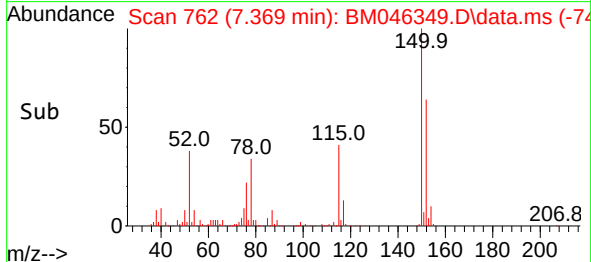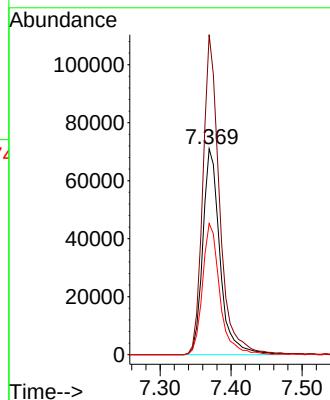

#5
2-Fluorophenol
Concen: 91.101 ng
RT: 5.046 min Scan# 367
Delta R.T. -0.006 min
Lab File: BM046349.D
Acq: 28 Jun 2024 12:46

Tgt Ion:112 Resp: 678446
Ion Ratio Lower Upper
112 100
64 67.3 52.8 79.2
63 42.0 32.9 49.3


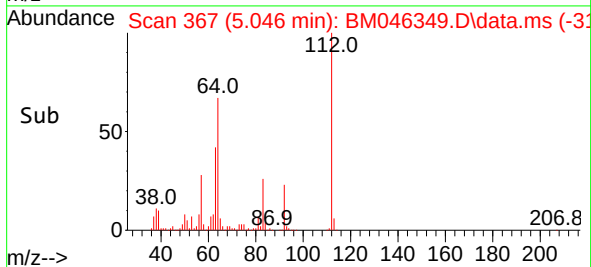
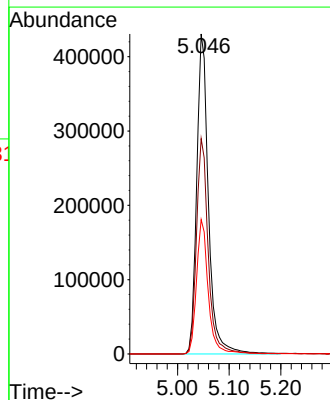
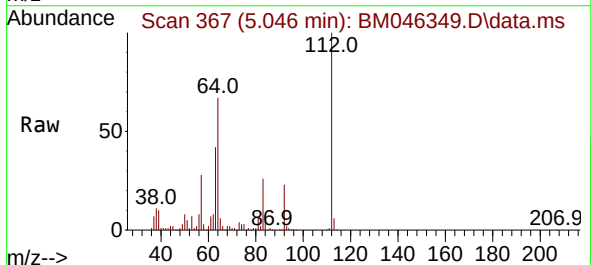


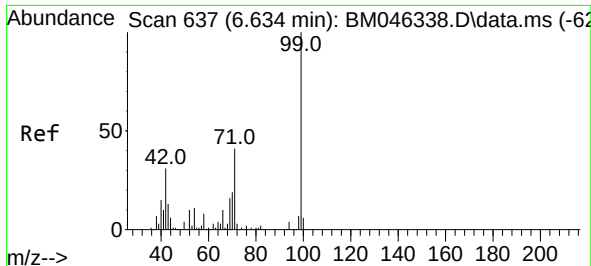

#7
Phenol-d6
Concen: 82.799 ng
RT: 6.628 min Scan# 61
Delta R.T. -0.006 min
Lab File: BM046349.D
Acq: 28 Jun 2024 12:46




Instrument :
BNA_M
ClientSampleId :
7-S-1


Tgt Ion: 99 Resp: 875974
Ion Ratio Lower Upper
99 100
42 31.3 24.8 37.2
71 42.1 33.1 49.7

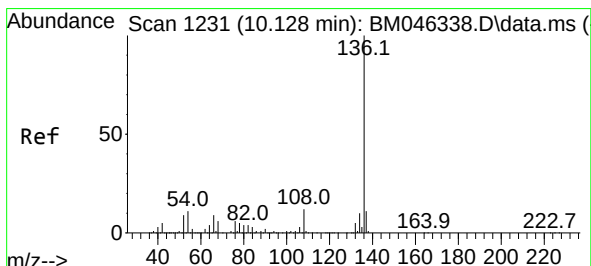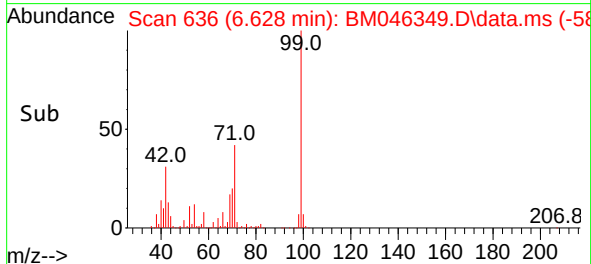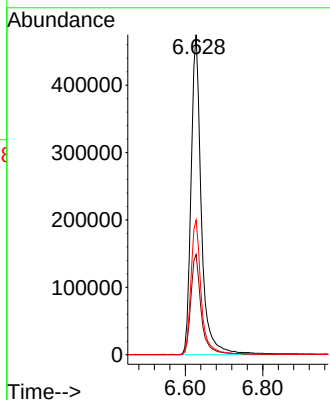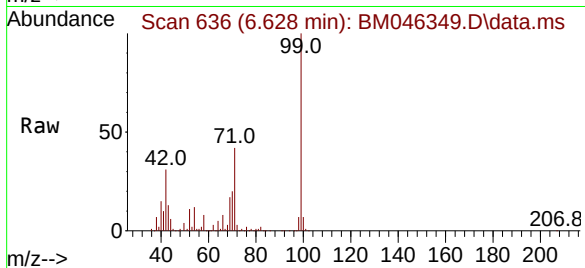

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.139 min Scan# 1233
Delta R.T. 0.011 min
Lab File: BM046349.D
Acq: 28 Jun 2024 12:46

Tgt Ion: 136 Resp: 470683
Ion Ratio Lower Upper
136 100
137 11.3 8.6 13.0
54 10.6 9.0 13.4
68 6.3 5.1 7.7


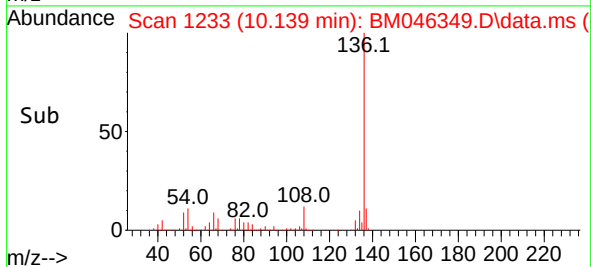
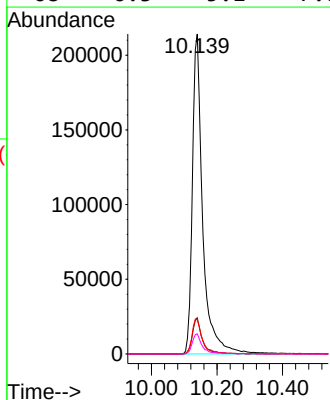
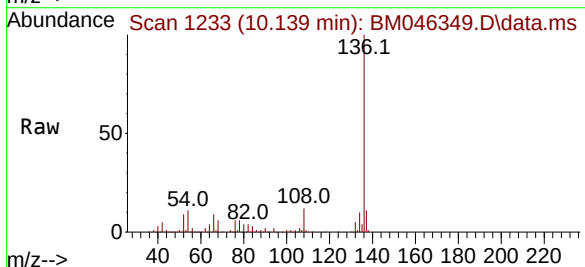


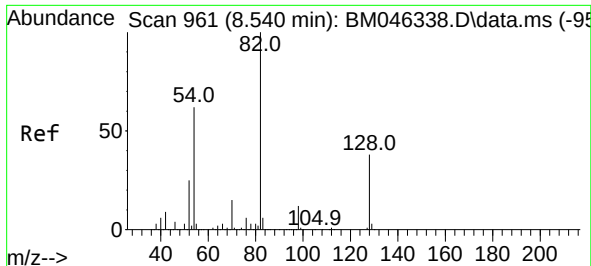

#23
Nitrobenzene-d5
Concen: 52.680 ng
RT: 8.540 min Scan# 961
Delta R.T. 0.000 min
Lab File: BM046349.D
Acq: 28 Jun 2024 12:46




Instrument :
BNA_M
ClientSampleId :
7-S-1


Tgt Ion: 82 Resp: 598120
Ion Ratio Lower Upper
82 100
128 37.4 30.6 46.0
54 62.2 49.6 74.4

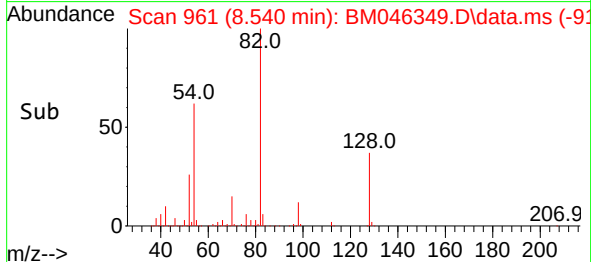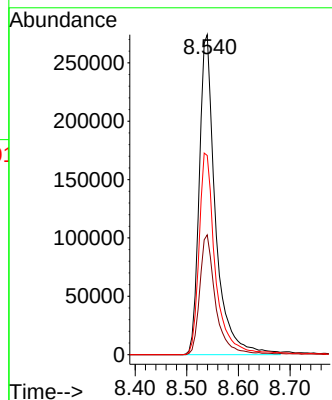

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.022 min Scan# 1893
Delta R.T. -0.000 min
Lab File: BM046349.D
Acq: 28 Jun 2024 12:46

Tgt Ion: 164 Resp: 282811
Ion Ratio Lower Upper
164 100
162 100.5 80.5 120.7
160 46.3 37.0 55.6


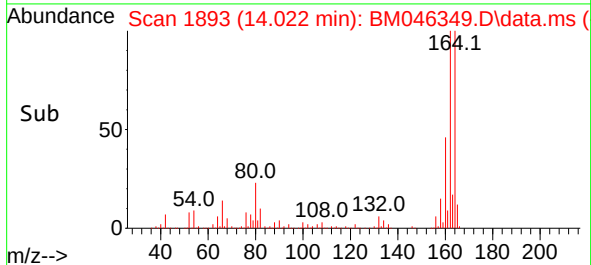
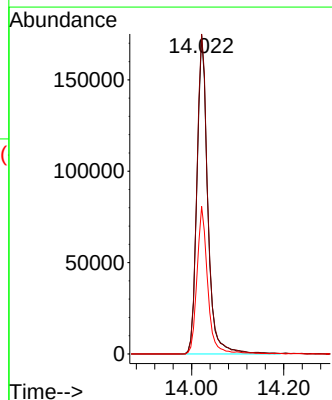
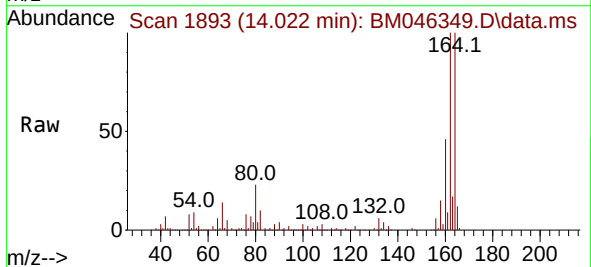


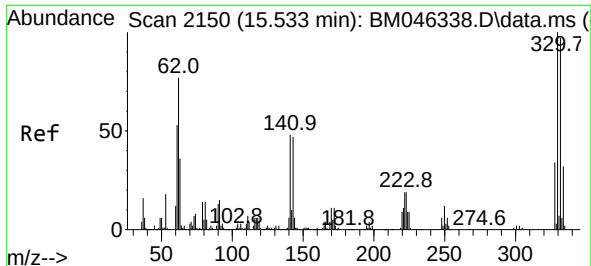

#42
2,4,6-Tribromophenol
Concen: 84.223 ng
RT: 15.527 min Scan# 2150
Delta R.T. -0.006 min
Lab File: BM046349.D
Acq: 28 Jun 2024 12:46




Instrument :
BNA_M
ClientSampleId :
7-S-1


Tgt Ion:330 Resp: 289670
Ion Ratio Lower Upper
330 100
332 96.9 77.8 116.6
141 55.5 43.2 64.8

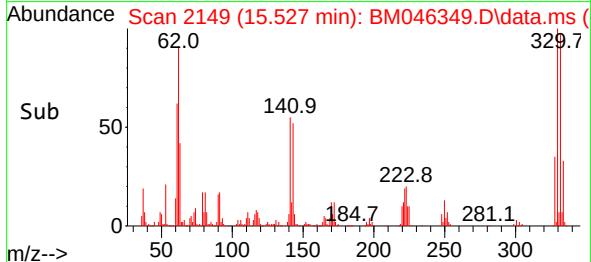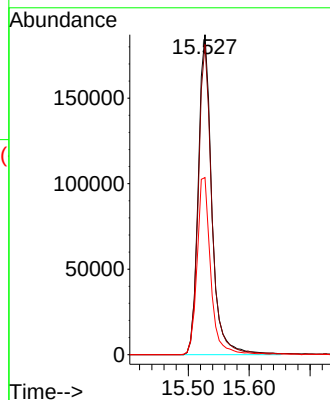

#45
2-Fluorobiphenyl
Concen: 46.607 ng
RT: 12.639 min Scan# 1658
Delta R.T. 0.006 min
Lab File: BM046349.D
Acq: 28 Jun 2024 12:46

Tgt Ion:172 Resp: 972484
Ion Ratio Lower Upper
172 100
171 34.4 28.1 42.1
170 24.4 19.4 29.0


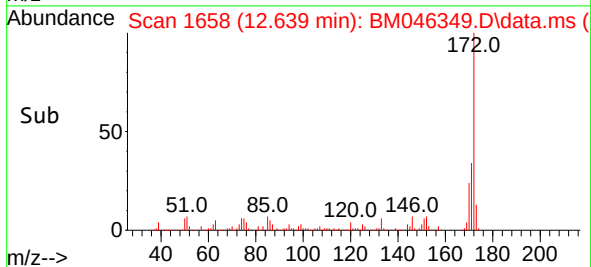
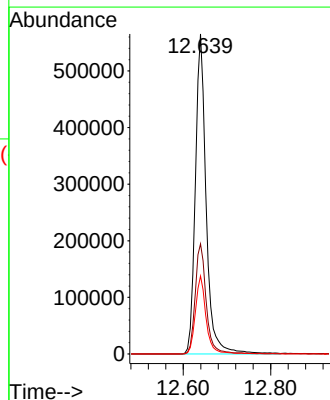
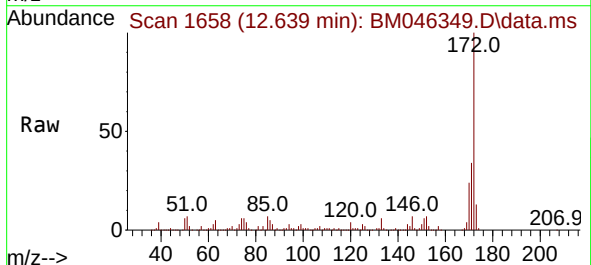


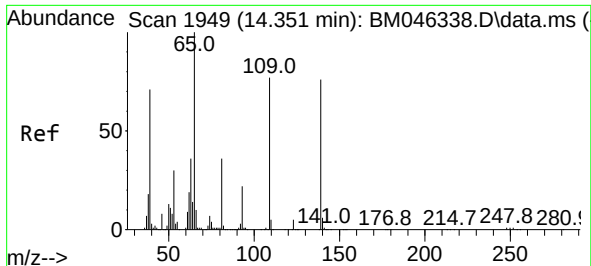

#56
4-Nitrophenol
Concen: 3.855 ng
RT: 14.451 min Scan# 1949
Delta R.T. 0.100 min
Lab File: BM046349.D
Acq: 28 Jun 2024 12:46




Instrument :
BNA_M
ClientSampleId :
7-S-1


Tgt Ion:139 Resp: 842
Ion Ratio Lower Upper
139 100
109 0.0 82.0 122.0#
65 0.0 112.0 152.0#

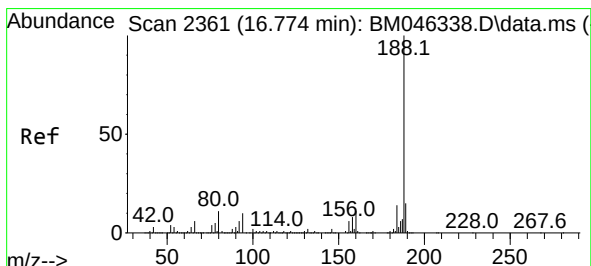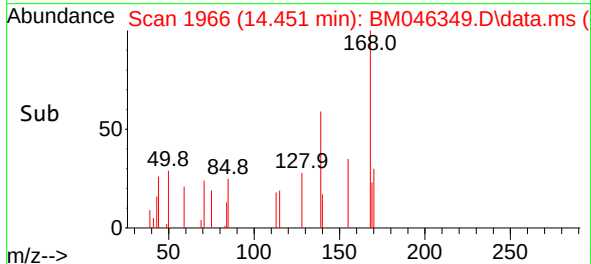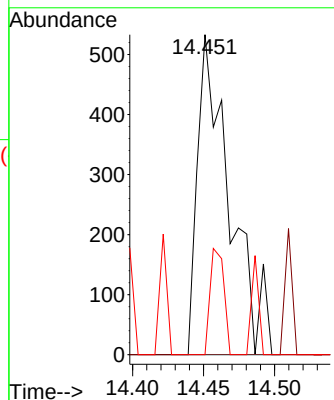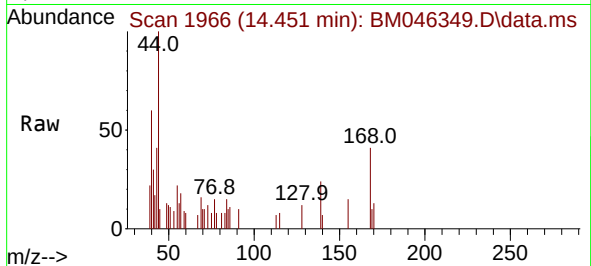

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 16.774 min Scan# 2361
Delta R.T. 0.000 min
Lab File: BM046349.D
Acq: 28 Jun 2024 12:46

Tgt Ion:188 Resp: 561315
Ion Ratio Lower Upper
188 100
94 9.4 7.9 11.9
80 11.6 9.0 13.6

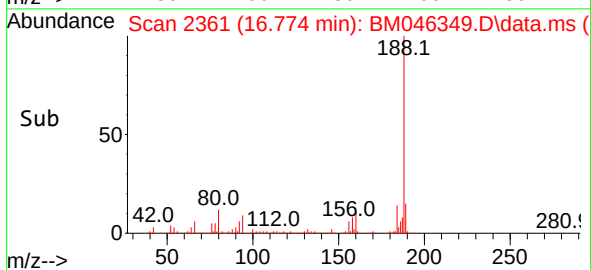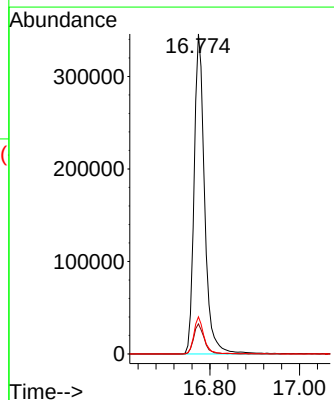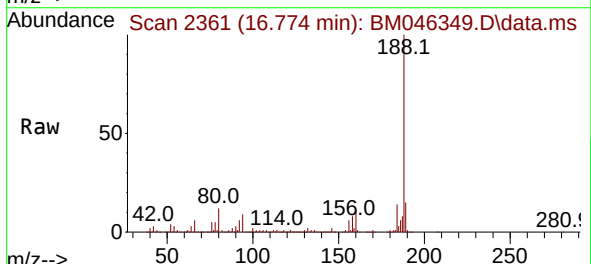



#75

Fluoranthene

Concen: 2.575 ng

RT: 18.845 min Scan# 21

Delta R.T. 0.000 min

Lab File: BM046349.D

Acq: 28 Jun 2024 12:46

Instrument :

BNA_M

ClientSampleId :

7-S-1





Tgt Ion:202 Resp: 90889

Ion Ratio Lower Upper

202 100

101 10.4 0.0 31.4

203 15.8 0.0 37.2

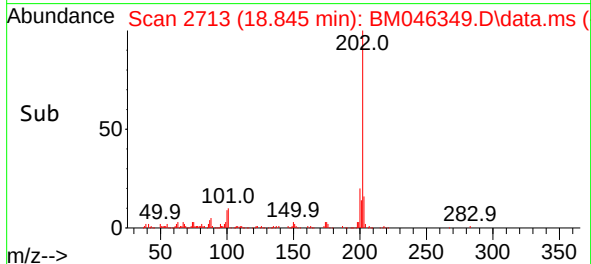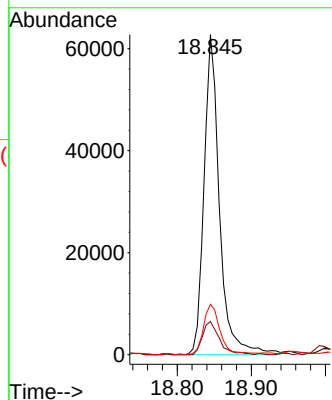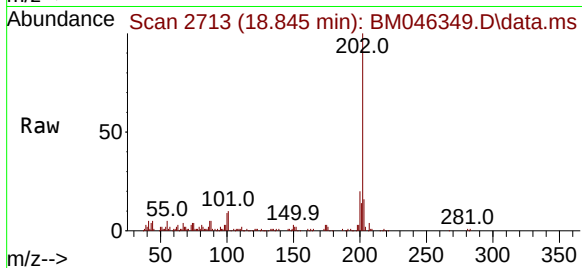

#76

Chrysene-d12

Concen: 20.000 ng

RT: 20.992 min Scan# 3078

Delta R.T. -0.006 min

Lab File: BM046349.D

Acq: 28 Jun 2024 12:46




Tgt Ion:240 Resp: 457522


Ion Ratio Lower Upper

240 100

120 11.8 9.3 13.9

236 26.1 20.5 30.7


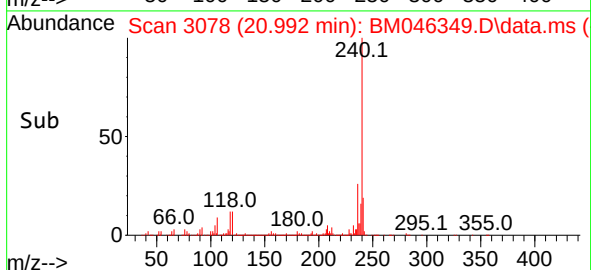
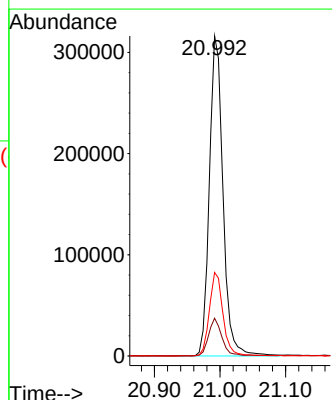
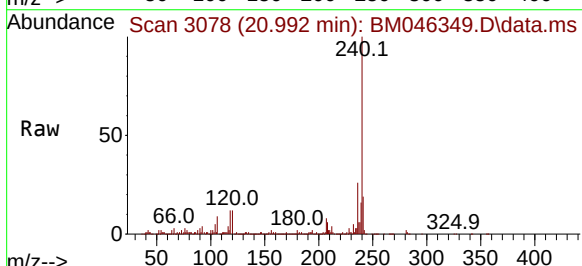




#78
Pyrene
Concen: 2.746 ng
RT: 19.209 min Scan# 21
Delta R.T. 0.000 min
Lab File: BM046349.D
Acq: 28 Jun 2024 12:46




Instrument :
BNA_M
ClientSampleId :
7-S-1


Tgt Ion:202 Resp: 87255
Ion Ratio Lower Upper
202 100
200 22.2 17.3 25.9
203 17.4 14.3 21.5

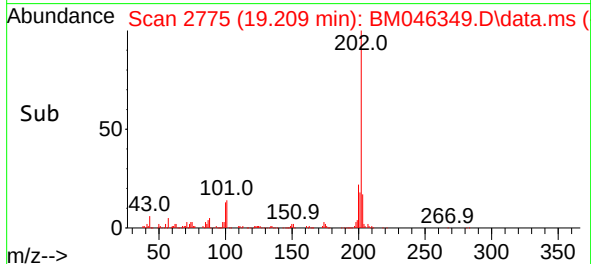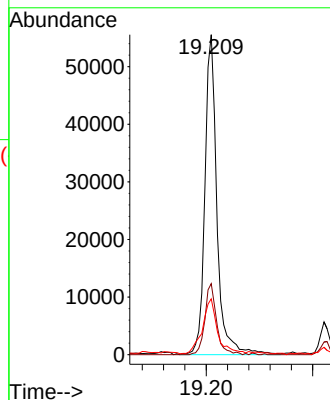

#79
Terphenyl-d14
Concen: 53.089 ng
RT: 19.421 min Scan# 2811
Delta R.T. -0.012 min
Lab File: BM046349.D
Acq: 28 Jun 2024 12:46

Tgt Ion:244 Resp: 1468078
Ion Ratio Lower Upper
244 100
212 8.0 6.5 9.7
122 12.3 9.4 14.0


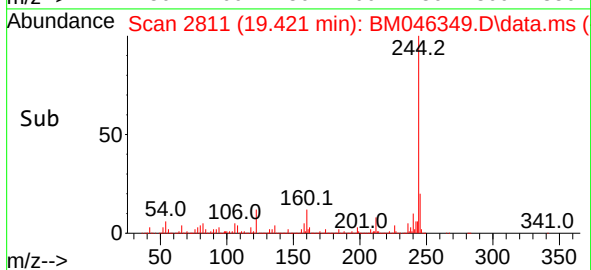
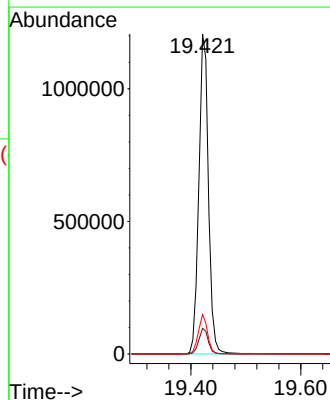
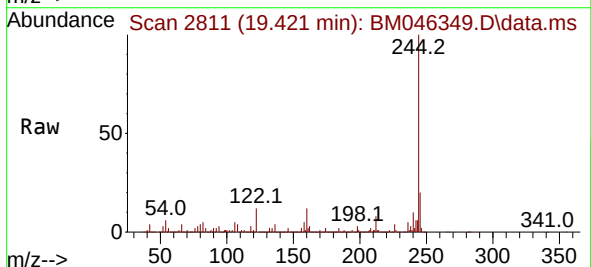




#84
 Bis(2-ethylhexyl)phthalate
 Concen: 2.712 ng
 RT: 20.927 min Scan# 3067
 Delta R.T. 0.000 min
 Lab File: BM046349.D
 Acq: 28 Jun 2024 12:46

Instrument :
 BNA_M
 ClientSampleId :
 7-S-1

Tgt Ion:149 Resp: 7381
 Ion Ratio Lower Upper
 149 100
 167 26.6 19.6 29.4
 279 3.6 2.6 4.0

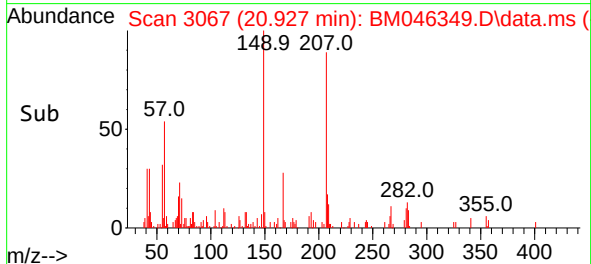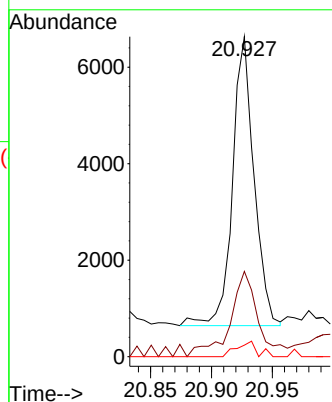

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 23.662 min Scan# 3532
 Delta R.T. -0.012 min
 Lab File: BM046349.D
 Acq: 28 Jun 2024 12:46

Tgt Ion:264 Resp: 470744
 Ion Ratio Lower Upper
 264 100
 260 23.6 18.5 27.7
 265 21.8 17.7 26.5

