
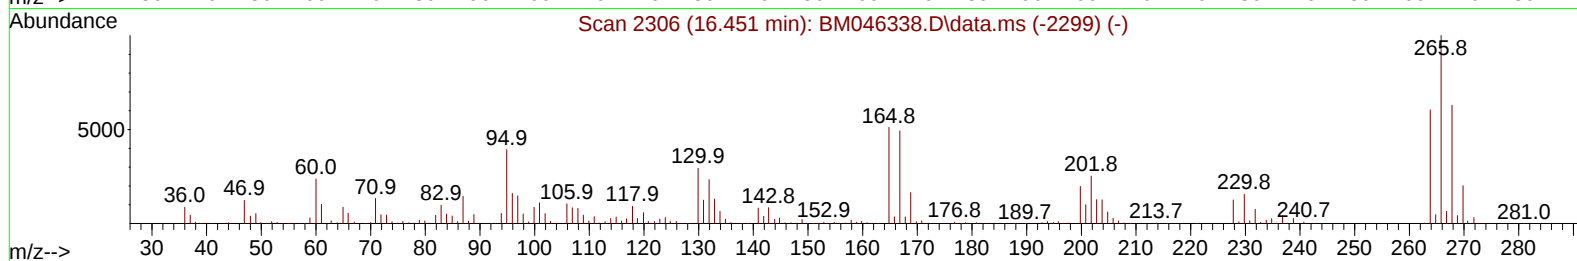
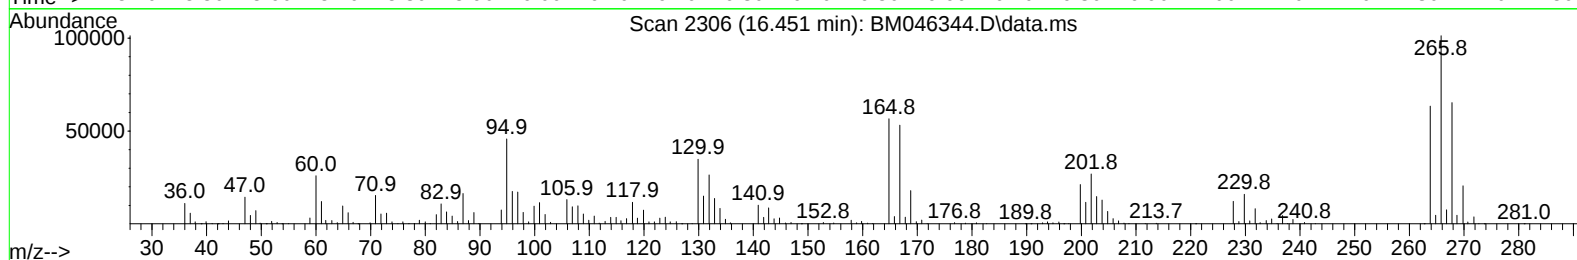


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062824\
Data File : BM046344.D
Acq On : 28 Jun 2024 08:56
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 28 11:47:42 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM062724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 28 03:23:08 2024
Response via : Initial Calibration

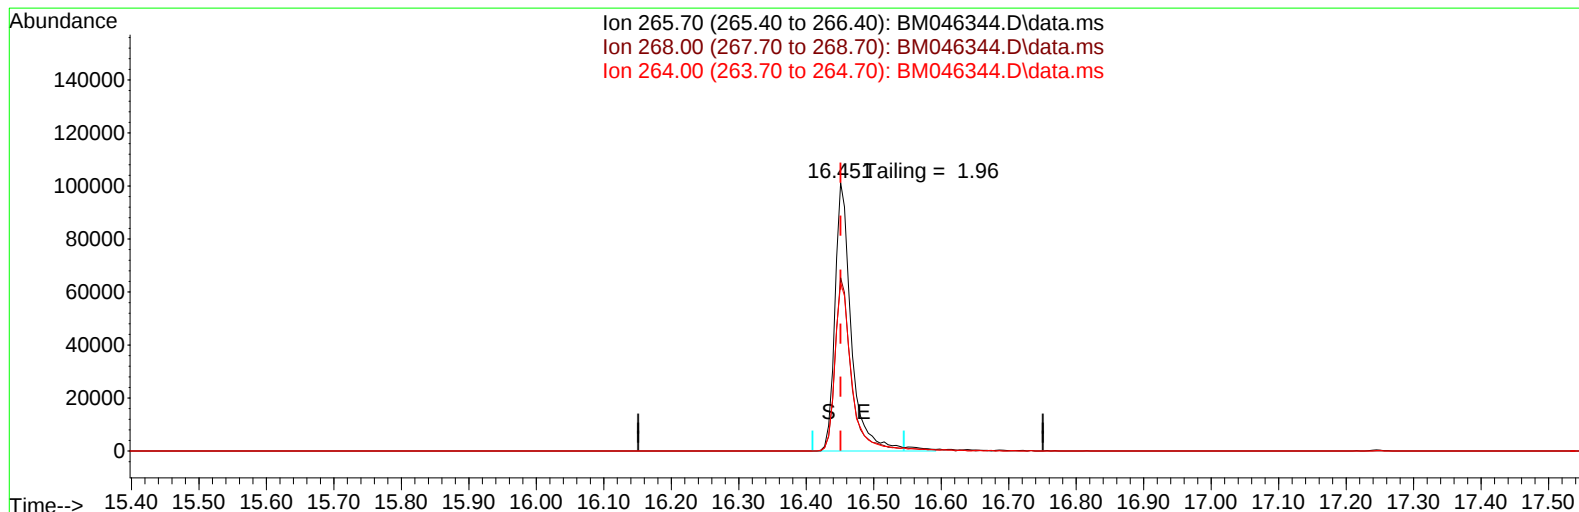

TIC: BM046344.D\data.ms




(70) Pentachlorophenol (C)

16.451min (-0.000) 55344.62 ng

response 170379

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.90	69.16
264.00	60.50	62.58
0.00	0.00	0.00

Quant Time: Jun 28 11:47:42 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM062724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 28 03:23:08 2024
Response via : Initial Calibration

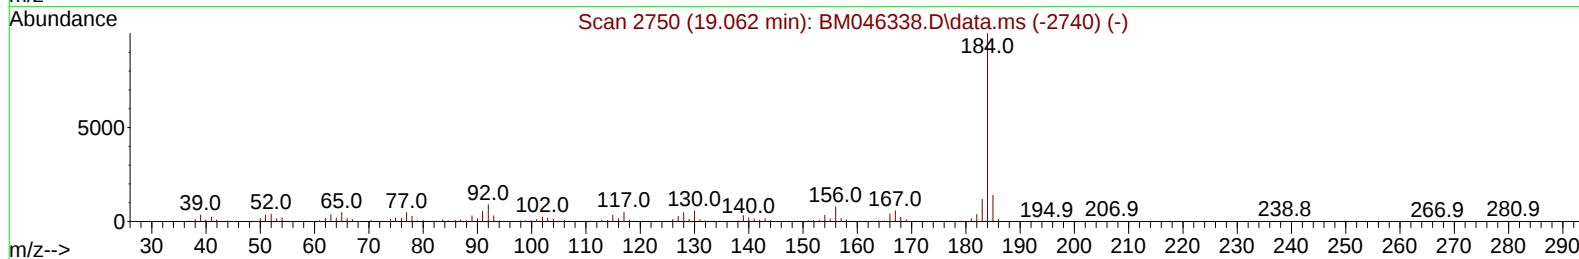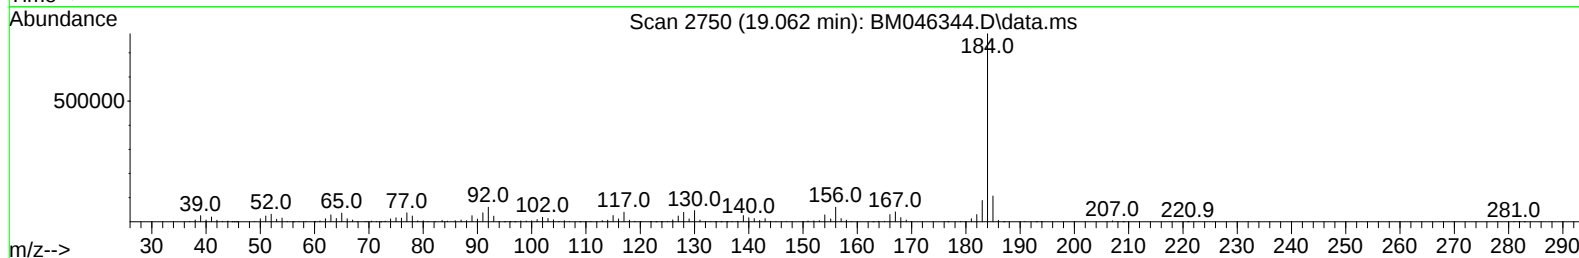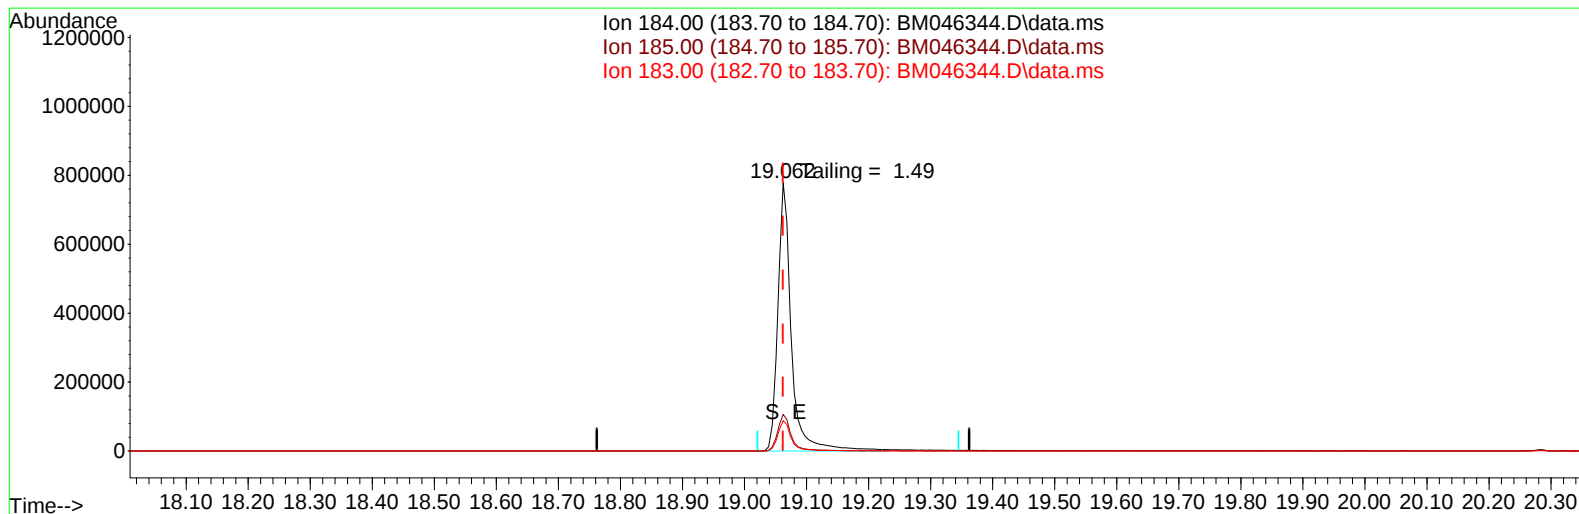

TIC: BM046344.D\data.ms

(77) Benzidine

19.062min (+ 0.000) 26773.17 ng

response **1201165**

Ion	Exp%	Act%
-----	------	------

184.00	100.00	100.00
--------	--------	--------

185.00	13.90	13.69
--------	-------	-------

183.00	11.80	11.38
--------	-------	-------

0.00 0.00 0.00