

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062824\
 Data File : BM046346.D
 Acq On : 28 Jun 2024 10:18
 Operator : MA/JU
 Sample : PB161765BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB161765BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM062724.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM046346.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.598	286	291	303	rBV	110499	184272	3.13%	0.710%
2	5.051	362	368	395	rBV	1755135	2842307	48.28%	10.946%
3	6.634	630	637	666	rBV	1443474	2946874	50.06%	11.349%
4	7.375	757	763	782	rBV	281481	518599	8.81%	1.997%
5	8.545	953	962	983	rBV	697935	1763692	29.96%	6.792%
6	10.151	1228	1235	1264	rBV	213825	666102	11.31%	2.565%
7	12.645	1652	1659	1687	rBV	1803241	3564390	60.55%	13.727%
8	14.033	1888	1895	1914	rBV	427269	895835	15.22%	3.450%
9	15.527	2143	2149	2182	rBV	1811295	3262816	55.42%	12.566%
10	16.786	2355	2363	2387	rBV	473686	1070174	18.18%	4.121%
11	19.427	2806	2812	2827	rBV	4748231	5886959	100.00%	22.672%
12	21.003	3074	3080	3093	rBV	621740	1156952	19.65%	4.456%
13	23.674	3526	3534	3553	rBV2	425993	1207214	20.51%	4.649%




Sum of corrected areas: 25966186

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062824\
Data File : BM046346.D
Acq On : 28 Jun 2024 10:18
Operator : MA/JU
Sample : PB161765BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB161765BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM062724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

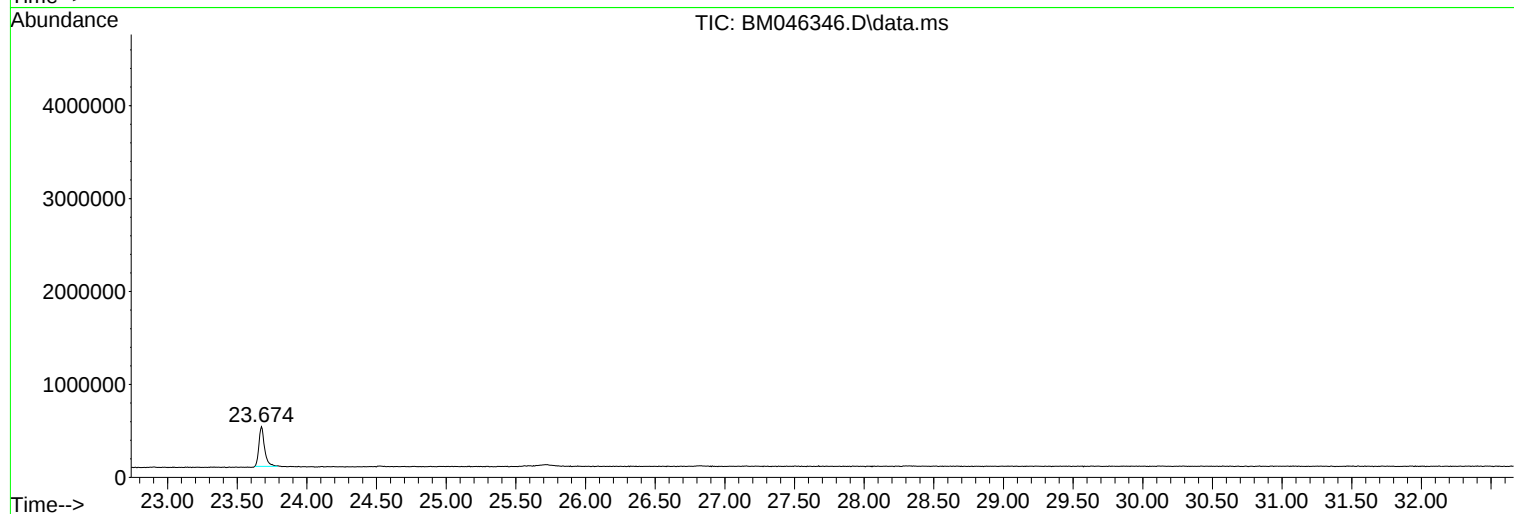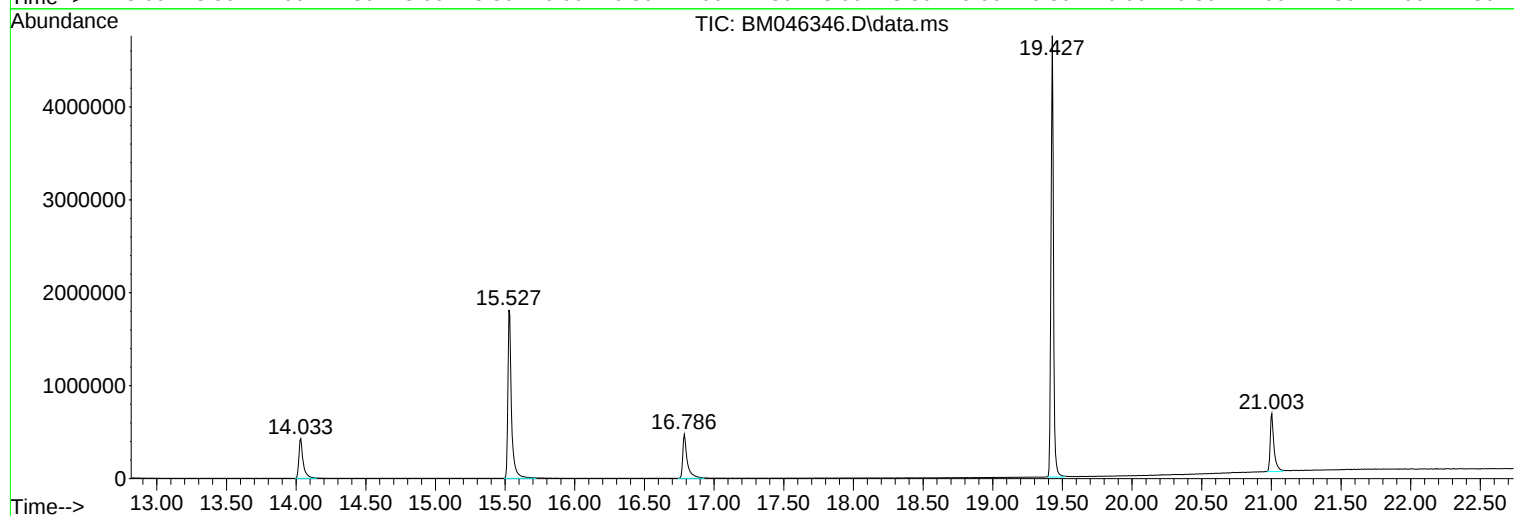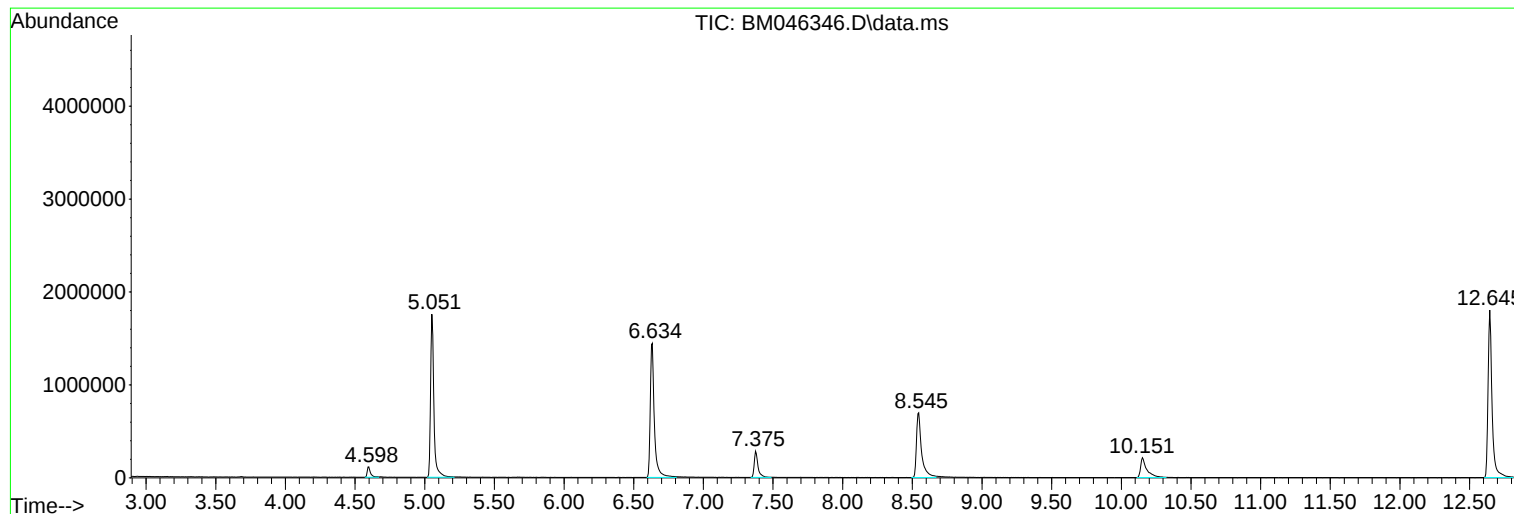

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062824\
Data File : BM046346.D
Acq On : 28 Jun 2024 10:18
Operator : MA/JU
Sample : PB161765BL
Misc :
ALS Vial : 3 Sample Multiplier: 1










Instrument :
BNA_M
ClientSampleId :
PB161765BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM062724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.	
4.598	7.11 ng	184272	1,4-Dichlorobenzene-d4	7.375	
Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	50
2	Propylamine	59	C3H9N	000107-10-8	40
3	Acetic acid, 1,1-dimethylethyl e...	116	C6H12O2	000540-88-5	38
4	2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	16
5	1-Propen-2-ol, acetate	100	C5H8O2	000108-22-5	12

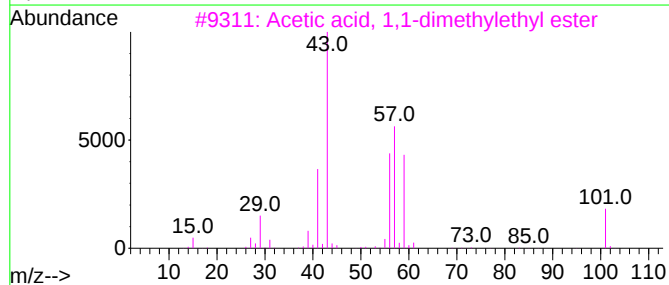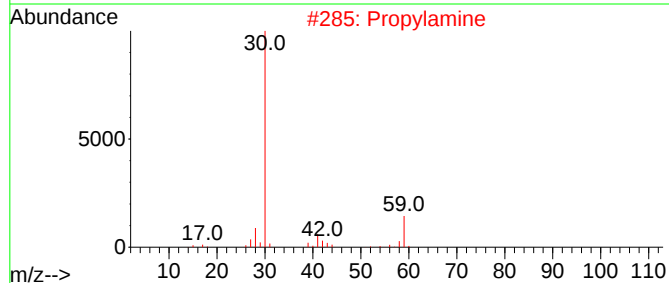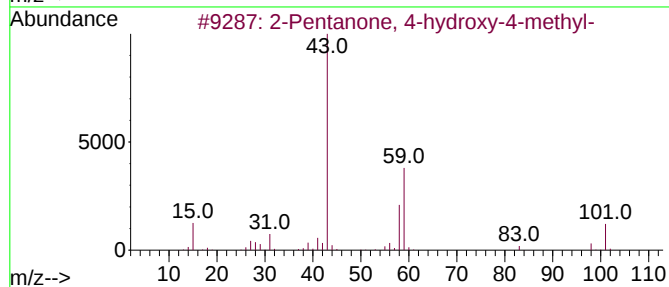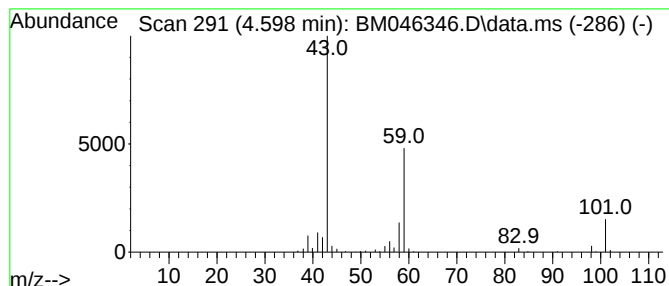

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062824\
Data File : BM046346.D
Acq On : 28 Jun 2024 10:18
Operator : MA/JU
Sample : PB161765BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB161765BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM062724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	4.598	7.1	ng	184272	1	7.375	518599	20.0