


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062824\
Data File : BM046344.D
Acq On : 28 Jun 2024 08:56
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270E-Tune.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Oct 07 11:38:17 2020

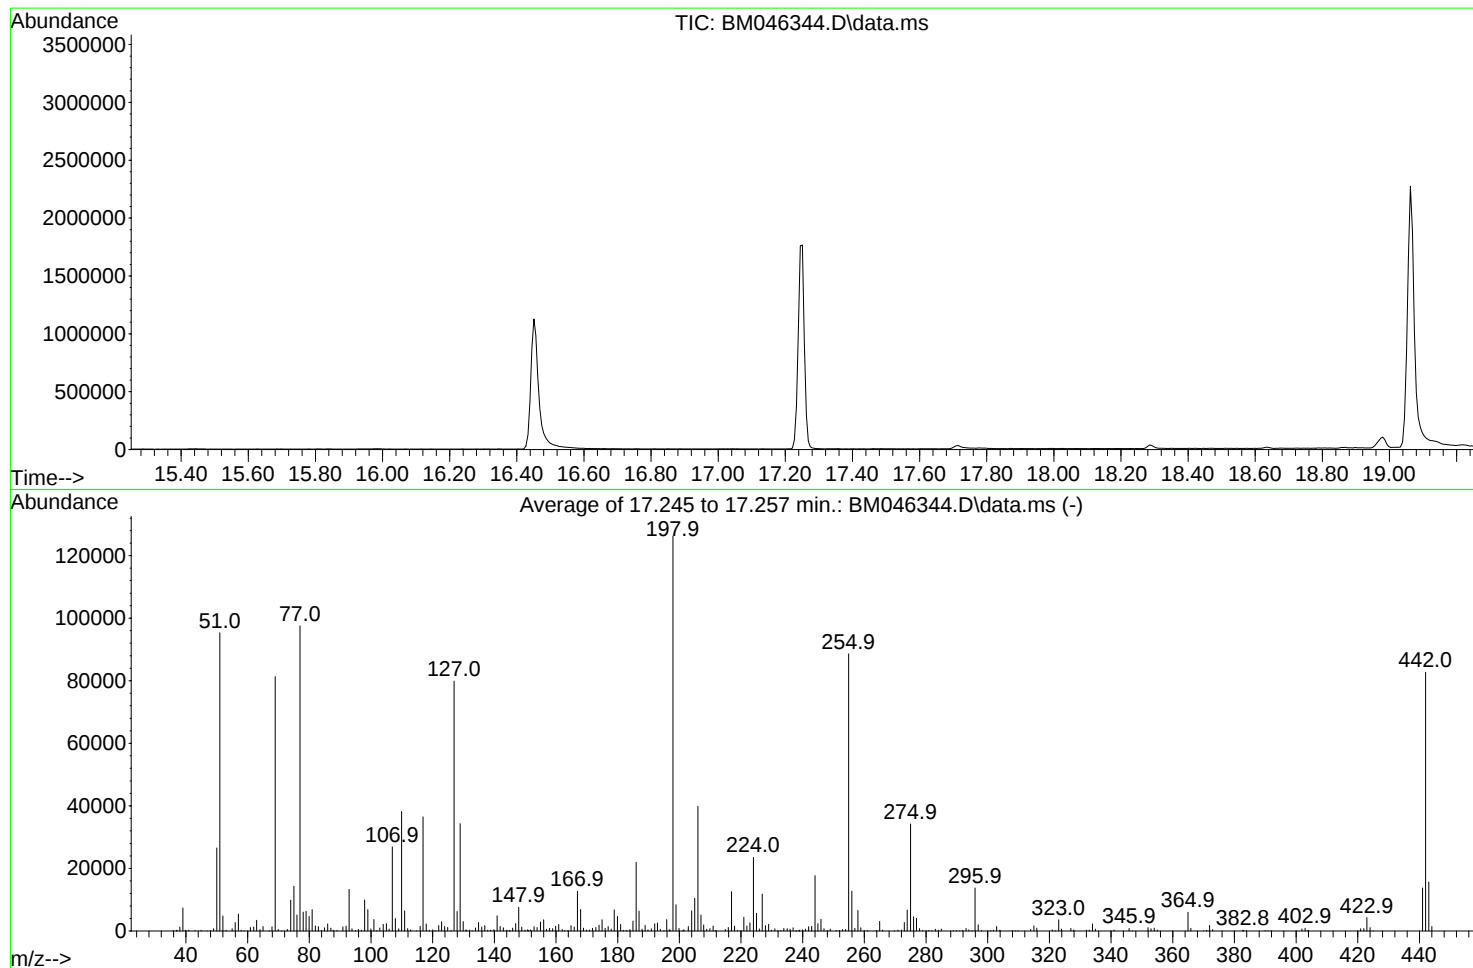

AutoFind: Scans 2441, 2442, 2443; Background Corrected with Scan 2434

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.7	1354	PASS
69	69	100	100	100.0	81352	PASS
70	69	0.00	2	0.6	505	PASS
197	198	0.00	2	0.3	437	PASS
198	198	100	100	100.0	126227	PASS
199	198	5	9	6.6	8394	PASS
365	198	1	100	4.7	5980	PASS
441	443	0.01	150	87.9	13772	PASS
442	442	100	100	100.0	82701	PASS
443	442	15	24	18.9	15669	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
6/28/2024	BNA_M	<u>BM046344.D</u>
Compound Name	Response	Retention Time
DDT	623477	20.286
DDD	5886	19.898
DDE	119	19.345
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6005	629482	0.95

Instrument :
BNA_M
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062824\
Data File : BM046344.D
Acq On : 28 Jun 2024 08:56
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Jun 28 11:47:42 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM062724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 28 03:23:08 2024
Response via : Initial Calibration

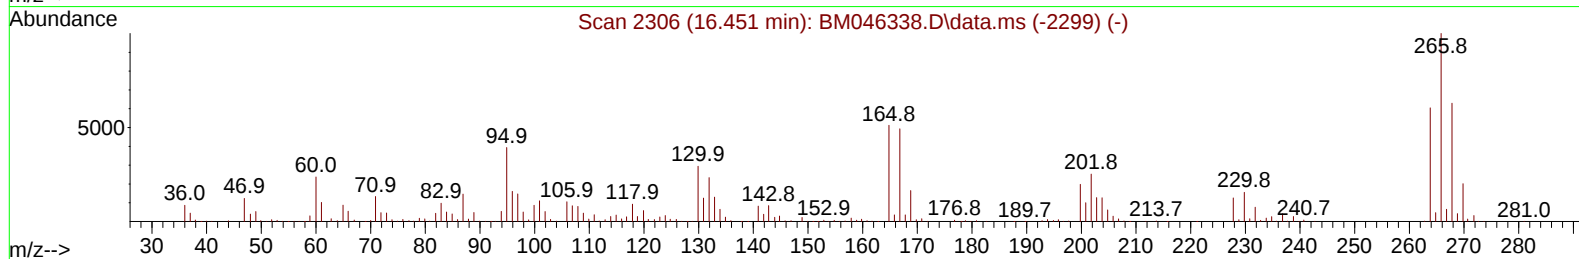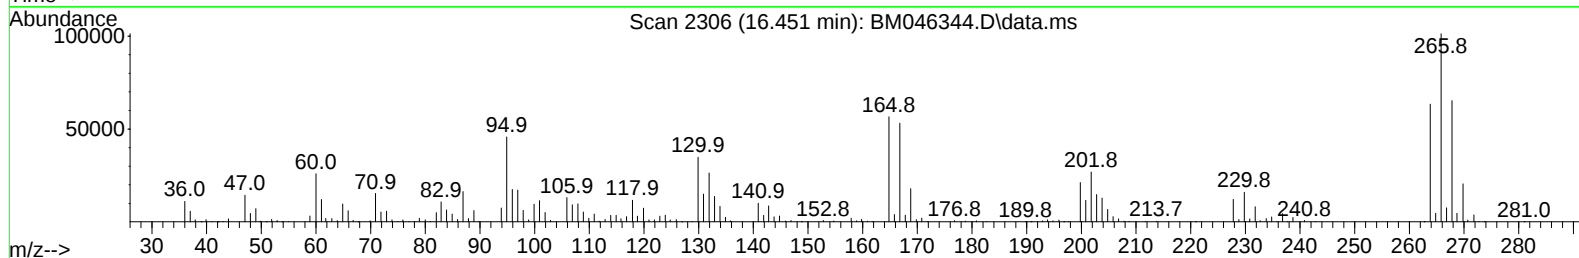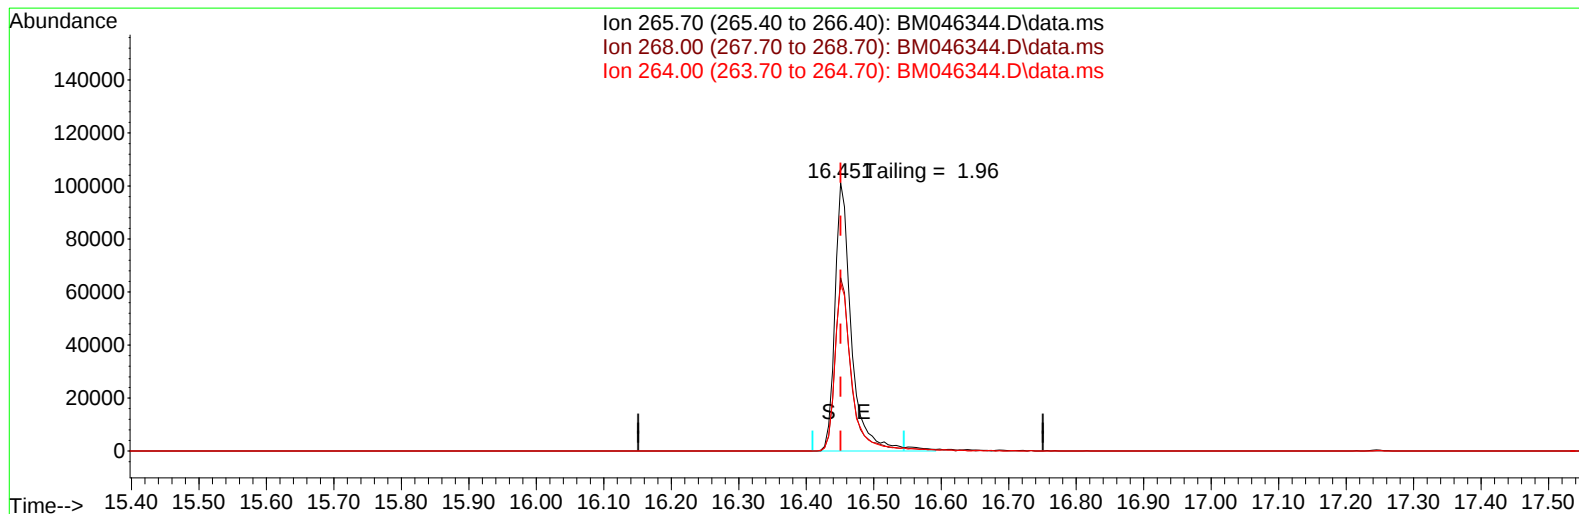

TIC: BM046344.D\data.ms

(70) Pentachlorophenol (C)

16.451min (-0.000) 55344.62 ng




response 170379

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.90	69.16
264.00	60.50	62.58
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062824\  
Data File : BM046344.D  
Acq On    : 28 Jun 2024  08:56  
Operator  : MA/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Jun 28 11:47:42 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM062724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 28 03:23:08 2024
Response via : Initial Calibration

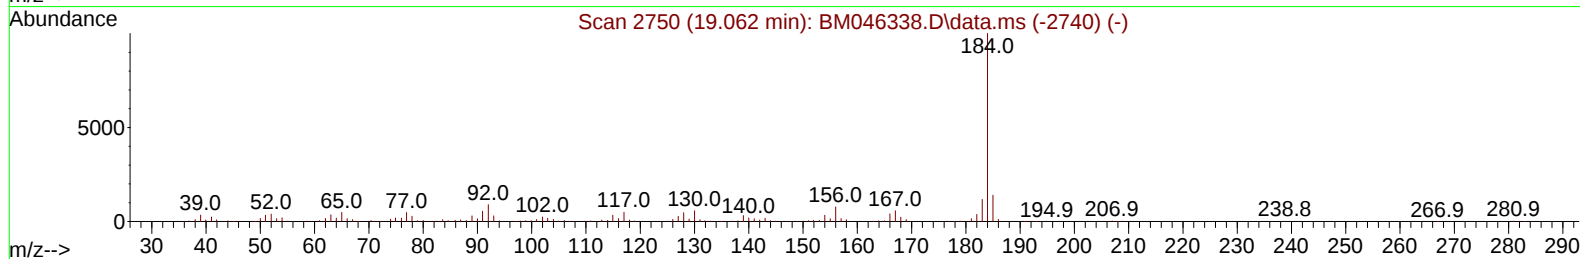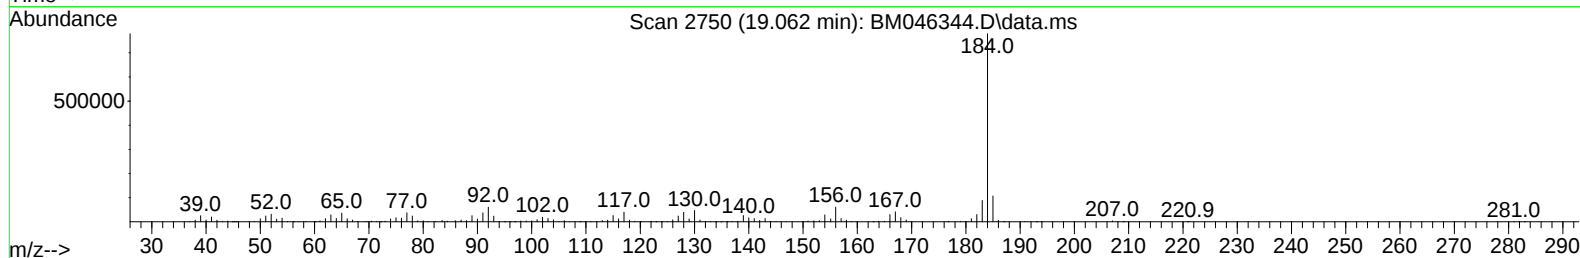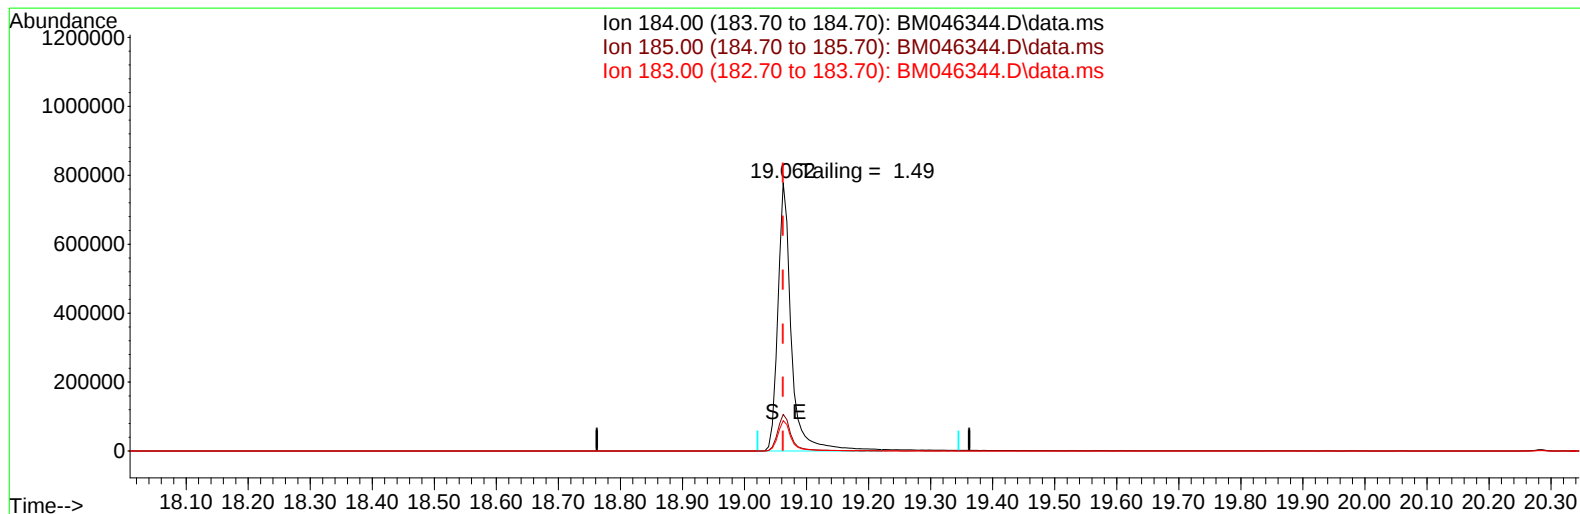

TIC: BM046344.D\data.ms

(77) Benzidine

19.062min (+ 0.000) 26773.17 ng

response 1201165

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	13.69
183.00	11.80	11.38
0.00	0.00	0.00