

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062923\
 Data File : BM040428.D
 Acq On : 29 Jun 2023 09:16
 Operator : MA/JU
 Sample : PB153628BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK628

Quant Time: Jun 30 03:04:19 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 23 00:44:24 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.940	152	6037	0.400	ng/ul	-0.01
4) Naphthalene-d8	10.751	136	20979	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.582	164	9915	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.328	188	18306	0.400	ng/ul	0.00
17) Chrysene-d12	21.512	240	10862	0.400	ng/ul	0.00
23) Perylene-d12	23.923	264	12383	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.325	96	47288	4.987	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.340	152	8371	0.285	ng/ul	-0.01
18) Fluoranthene-d10	19.356	212	10965	0.315	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.576	166	2785	0.070	ng/ul#	16
20) Pyrene	19.719	202	1859	0.038	ng/ul#	1
26) Benzo(a)pyrene	23.768	252	3432	0.080	ng/ul#	43


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062923\
Data File : BM040428.D
Acq On : 29 Jun 2023 09:16
Operator : MA/JU
Sample : PB153628BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK628

Quant Time: Jun 30 03:04:19 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 23 00:44:24 2023
Response via : Initial Calibration




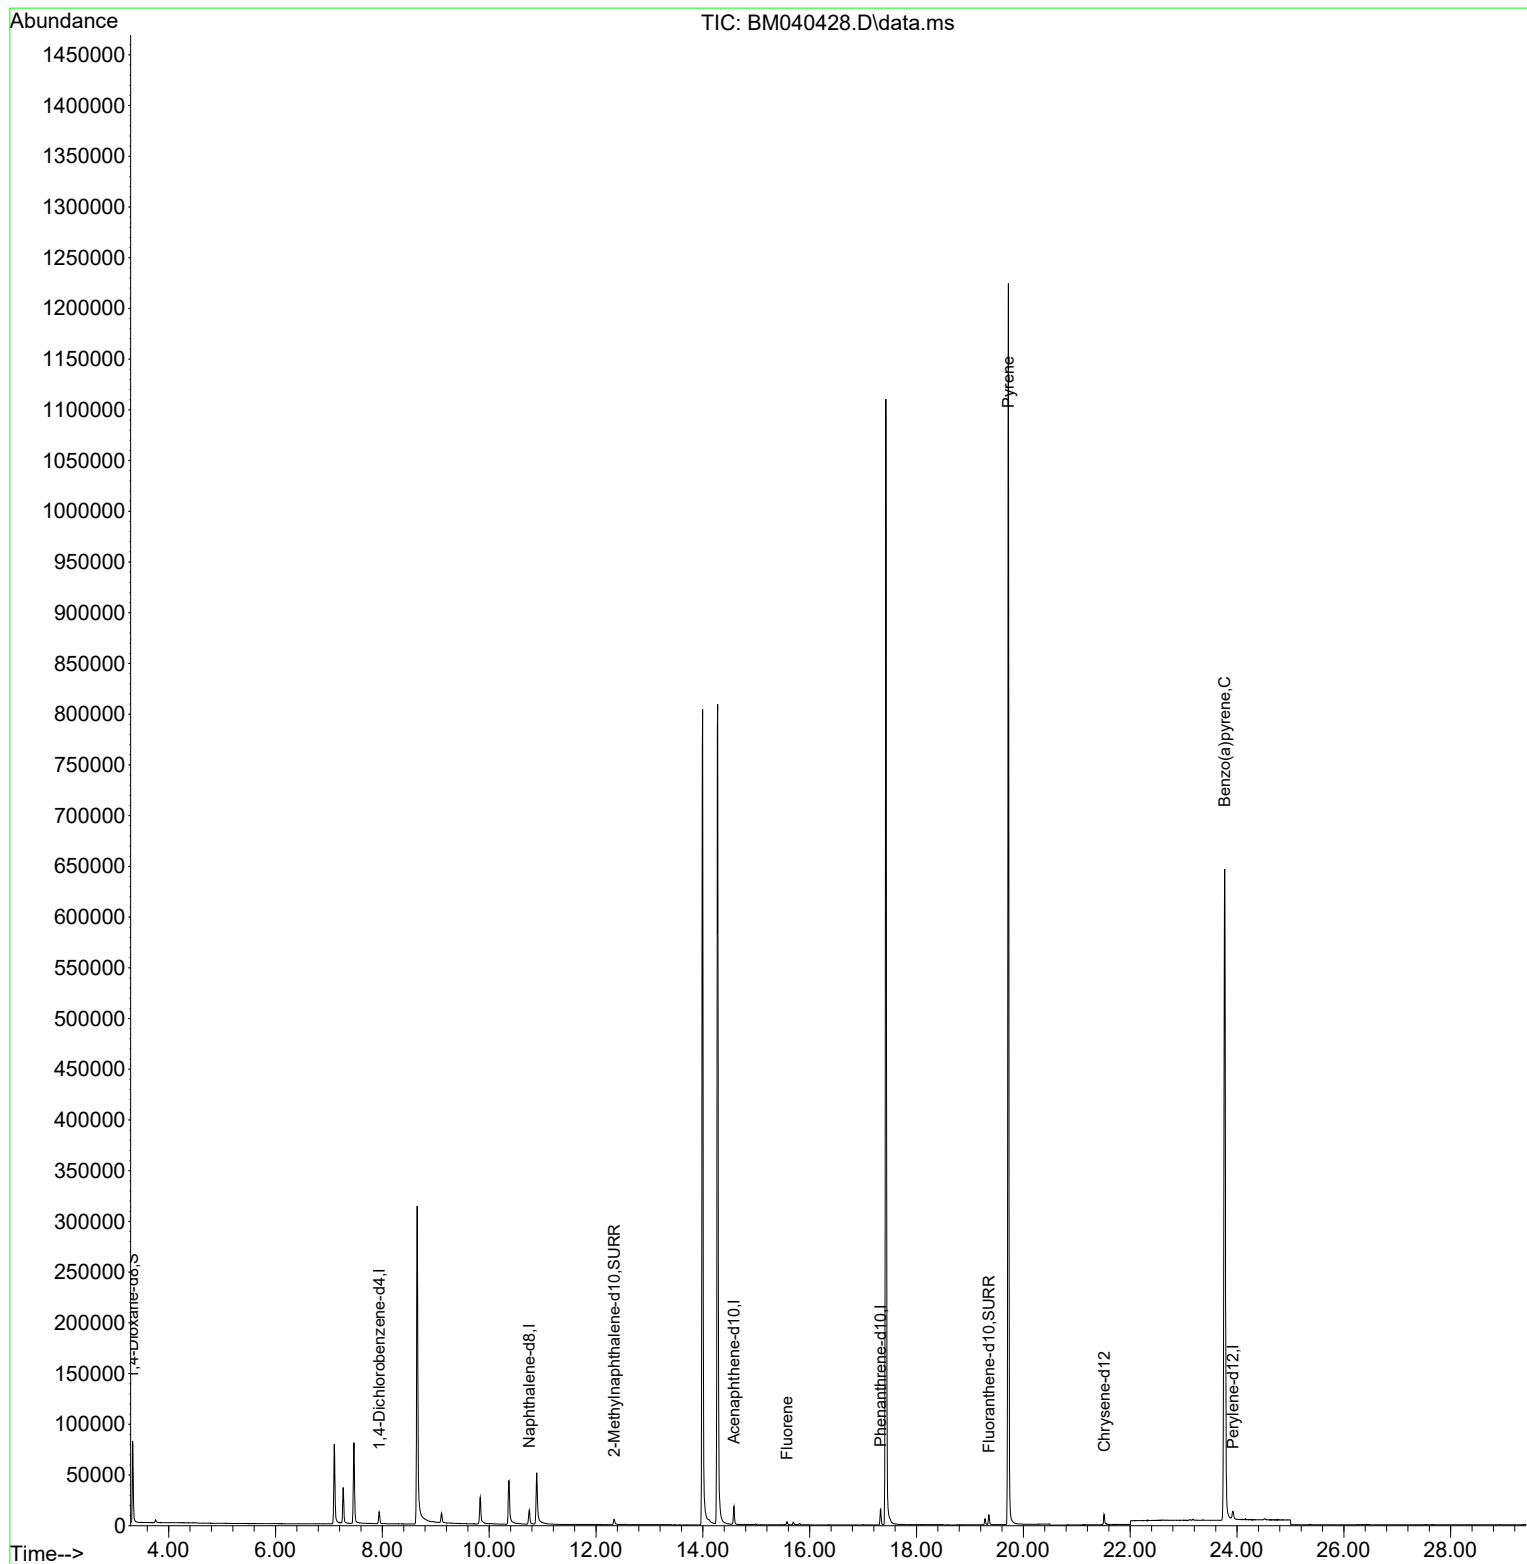


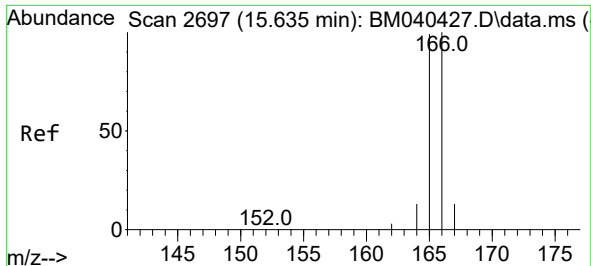

#12
Fluorene
Concen: 0.070 ng/ul
RT: 15.576 min Scan# 21
Delta R.T. -0.065 min
Lab File: BM040428.D
Acq: 29 Jun 2023 09:16




Instrument :
BNA_M
ClientSampleId :
SBLK628


Tgt Ion:166 Resp: 2785
Ion Ratio Lower Upper
166 100
165 11.6 79.6 119.4#
167 36.4 11.4 17.0#

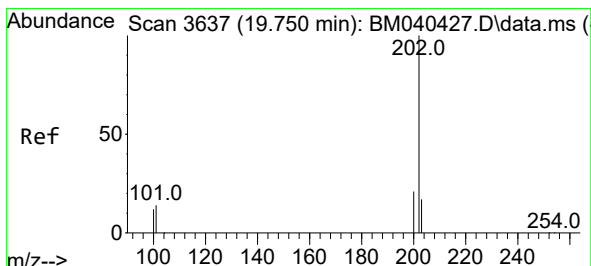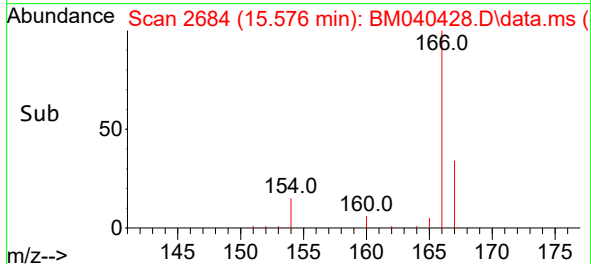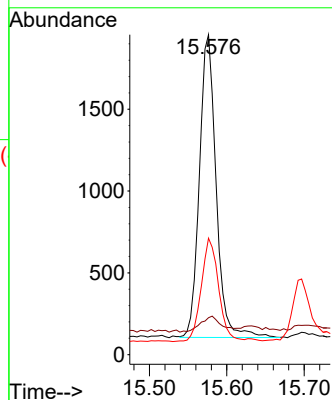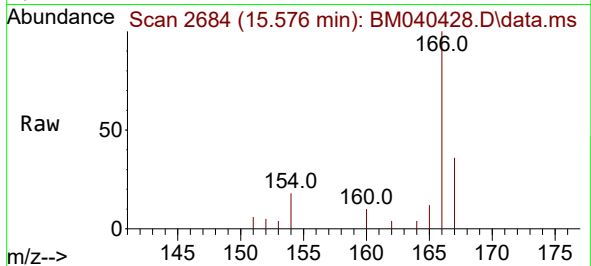

#20
Pyrene
Concen: 0.038 ng/ul
RT: 19.719 min Scan# 3630
Delta R.T. -0.037 min
Lab File: BM040428.D
Acq: 29 Jun 2023 09:16


Tgt Ion:202 Resp: 1859
Ion Ratio Lower Upper
202 100
101 169.0 12.6 18.8#
100 1243.3 9.8 14.6#

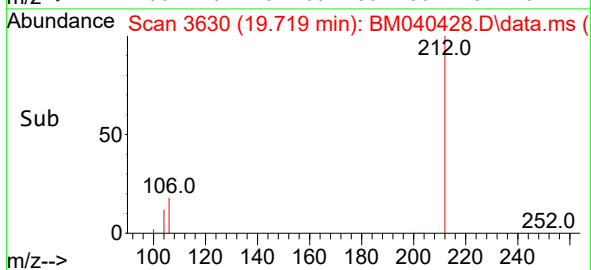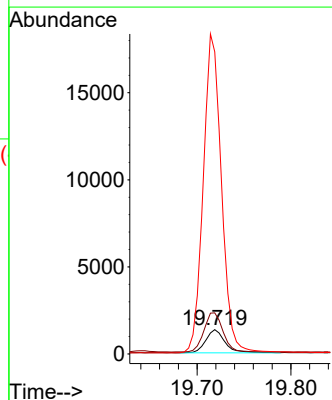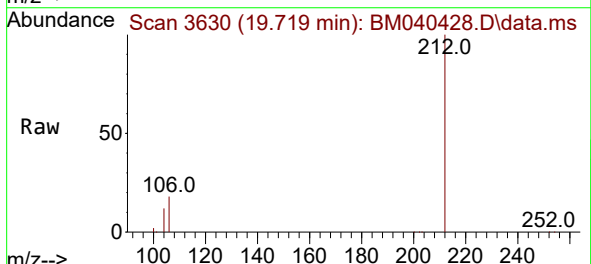

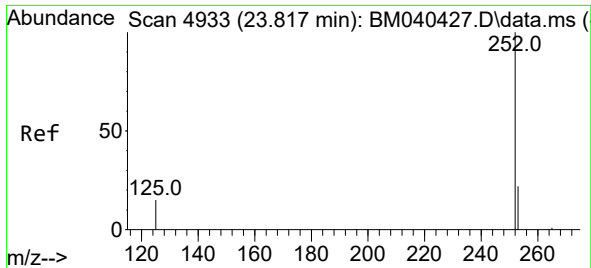

#26
Benzo(a)pyrene
Concen: 0.080 ng/ul
RT: 23.768 min Scan# 4916
Delta R.T. -0.056 min
Lab File: BM040428.D
Acq: 29 Jun 2023 09:16

Instrument :
BNA_M
ClientSampleId :
SBLK628

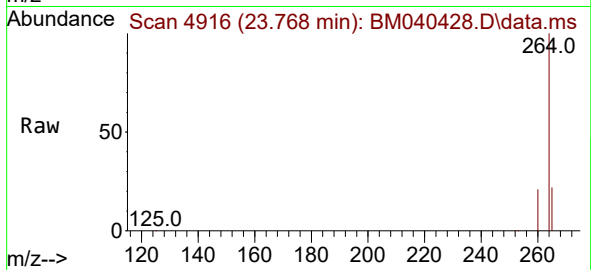

Tgt Ion:252 Resp: 3432
Ion Ratio Lower Upper
252 100
253 54.2 22.9 34.3#
125 60.3 21.0 31.4#

