

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062923\
 Data File : BM040441.D
 Acq On : 29 Jun 2023 17:19
 Operator : MA/JU
 Sample : PB153636BL
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK636

Quant Time: Jun 30 03:06:29 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 23 00:44:24 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.945	152	7720	0.400	ng/ul	0.00
4) Naphthalene-d8	10.751	136	28302	0.400	ng/ul	#-0.01
9) Acenaphthene-d10	14.586	164	14502	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.332	188	27327	0.400	ng/ul	0.00
17) Chrysene-d12	21.512	240	15507	0.400	ng/ul	0.00
23) Perylene-d12	23.923	264	16947	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.329	96	57289	4.724	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.340	152	11637	0.293	ng/ul	-0.01
18) Fluoranthene-d10	19.356	212	16938	0.341	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.576	166	3841	0.066	ng/ul#	16
20) Pyrene	19.723	202	2737	0.039	ng/ul#	1
26) Benzo(a)pyrene	23.771	252	4415	0.075	ng/ul#	33


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062923\
Data File : BM040441.D
Acq On : 29 Jun 2023 17:19
Operator : MA/JU
Sample : PB153636BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK636

Quant Time: Jun 30 03:06:29 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 23 00:44:24 2023
Response via : Initial Calibration




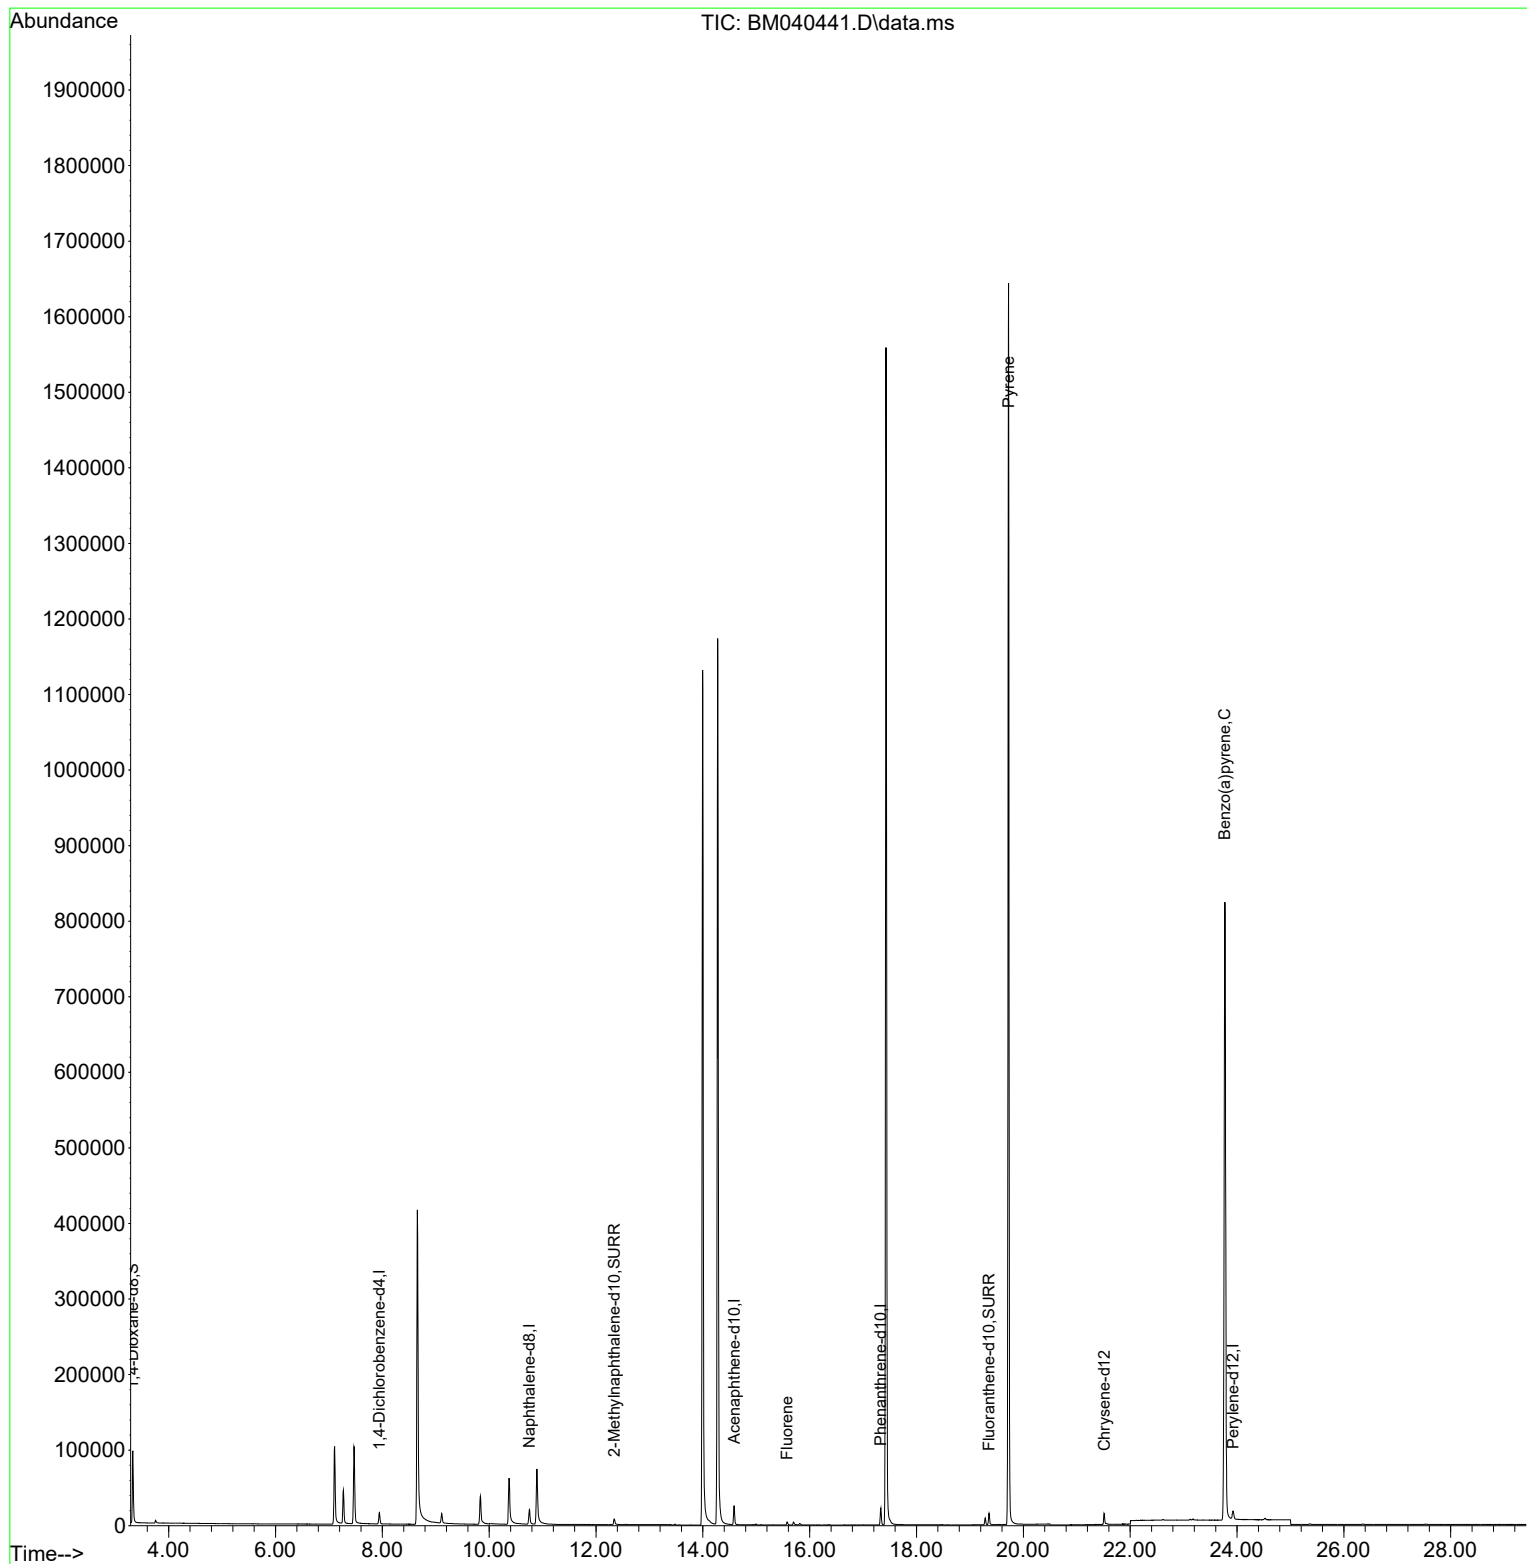


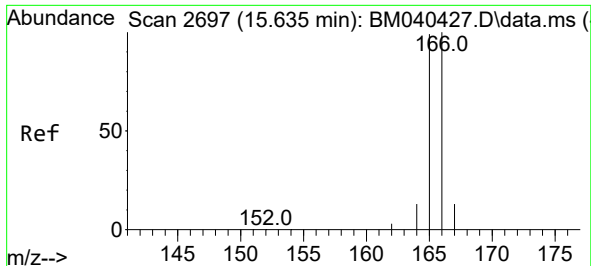

#12
Fluorene
Concen: 0.066 ng/ul
RT: 15.576 min Scan# 2684
Delta R.T. -0.065 min
Lab File: BM040441.D
Acq: 29 Jun 2023 17:19




Instrument :
BNA_M
ClientSampleId :
SBLK636


Tgt Ion:166 Resp: 3841
Ion Ratio Lower Upper
166 100
165 10.2 79.6 119.4#
167 32.5 11.4 17.0#

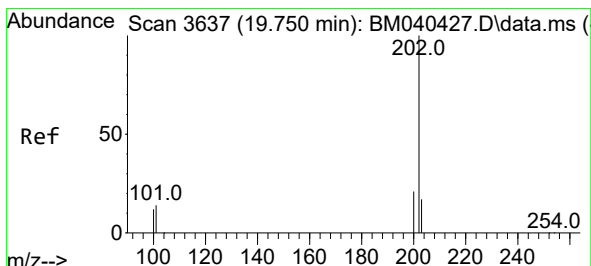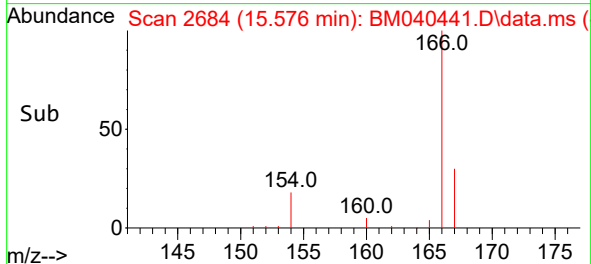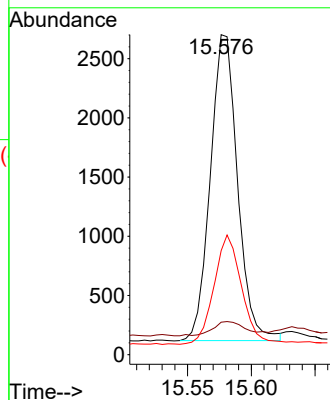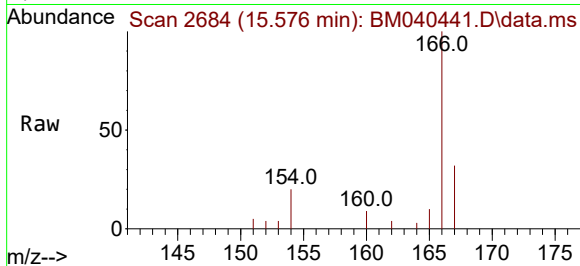

#20
Pyrene
Concen: 0.039 ng/ul
RT: 19.723 min Scan# 3631
Delta R.T. -0.033 min
Lab File: BM040441.D
Acq: 29 Jun 2023 17:19


Tgt Ion:202 Resp: 2737
Ion Ratio Lower Upper
202 100
101 165.9 12.6 18.8#
100 1180.3 9.8 14.6#

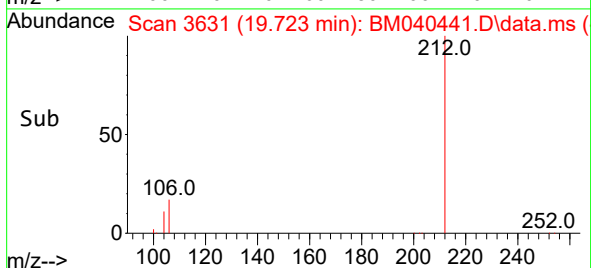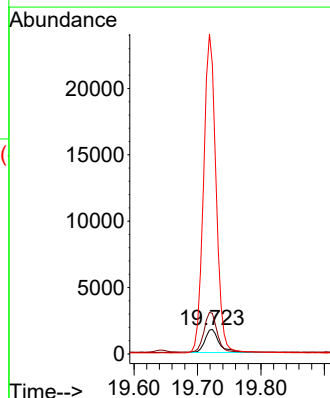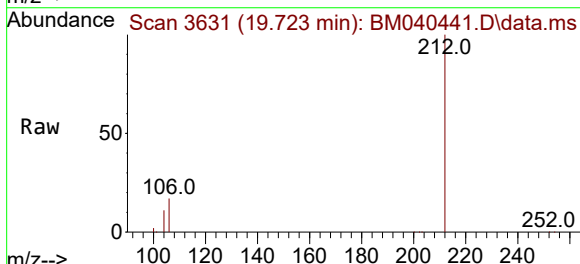

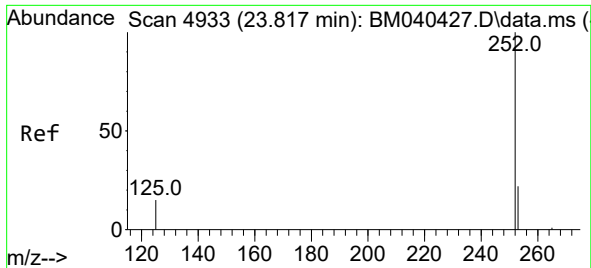

#26
 Benzo(a)pyrene
 Concen: 0.075 ng/ul
 RT: 23.771 min Scan# 4917
 Delta R.T. -0.053 min
 Lab File: BM040441.D
 Acq: 29 Jun 2023 17:19

Instrument :
 BNA_M
 ClientSampleId :
 SBLK636

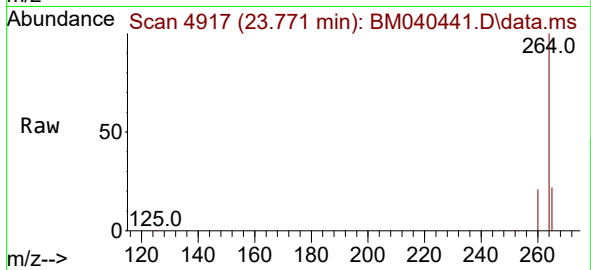

Tgt Ion:252 Resp: 4415
 Ion Ratio Lower Upper
 252 100
 253 58.4 22.9 34.3#
 125 67.0 21.0 31.4#

