

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063023\
 Data File : BM040461.D
 Acq On : 30 Jun 2023 08:26
 Operator : MA/JU
 Sample : PB153575BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK575

Quant Time: Jul 01 03:02:03 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Jul 01 03:00:05 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.936	152	7520	0.400	ng/ul	0.00
4) Naphthalene-d8	10.745	136	27362	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.577	164	13308	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.324	188	24380	0.400	ng/ul	0.00
17) Chrysene-d12	21.509	240	14534	0.400	ng/ul	0.00
23) Perylene-d12	23.918	264	16009	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.325	96	53875	4.561	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.334	152	10179	0.265	ng/ul	0.00
18) Fluoranthene-d10	19.352	212	13538	0.291	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.719	202	2339	0.035	ng/ul#	1
26) Benzo(a)pyrene	23.766	252	4372	0.078	ng/ul#	48


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063023\
Data File : BM040461.D
Acq On : 30 Jun 2023 08:26
Operator : MA/JU
Sample : PB153575BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK575

Quant Time: Jul 01 03:02:03 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jul 01 03:00:05 2023
Response via : Initial Calibration




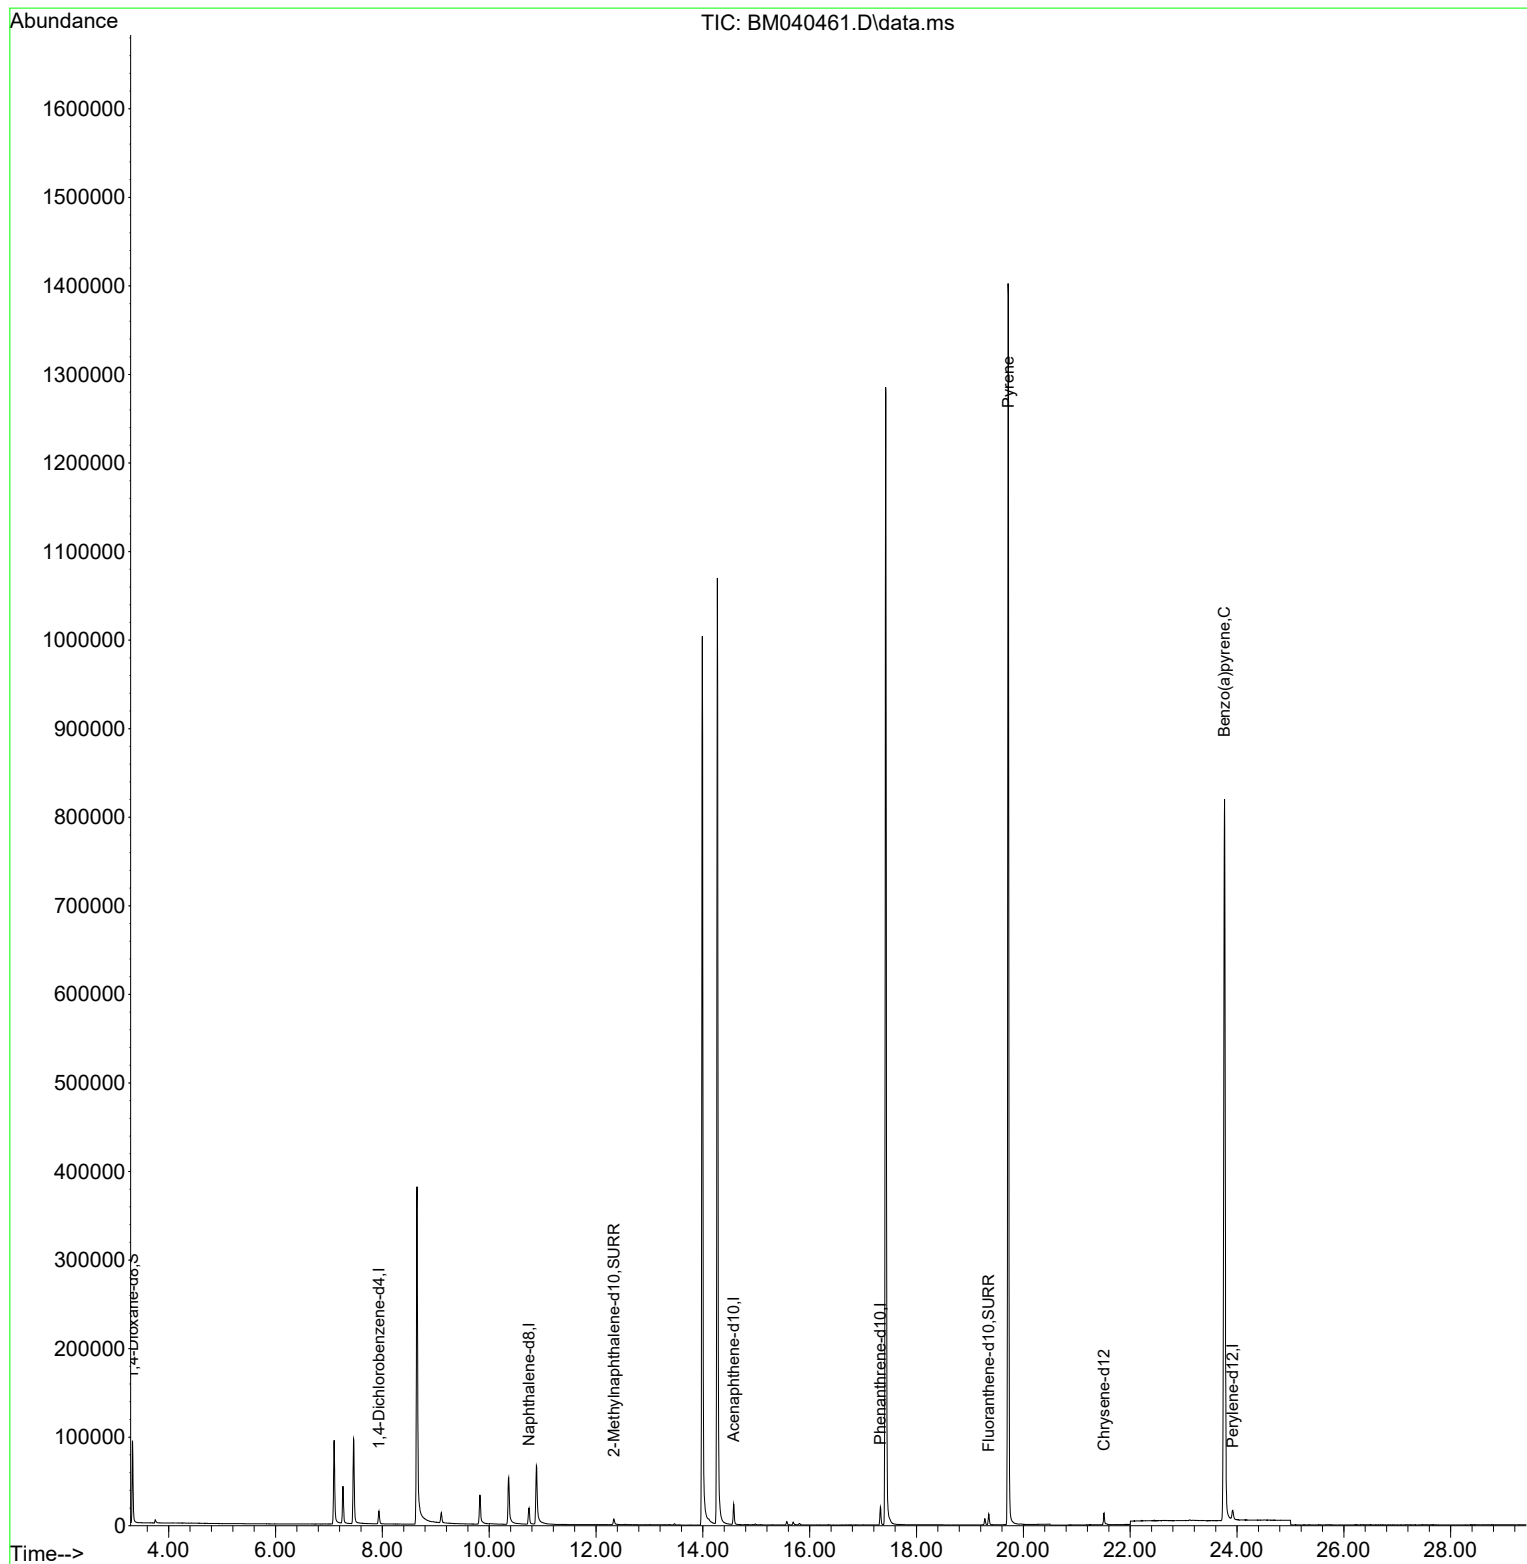


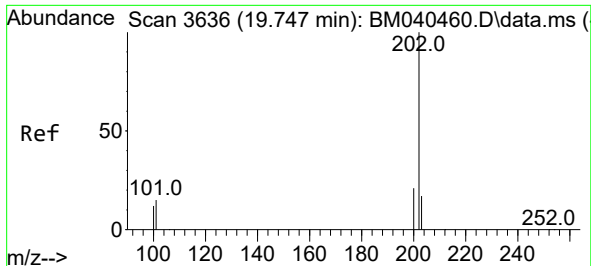

#20
Pyrene
Concen: 0.035 ng/ul
RT: 19.719 min Scan# 3630
Delta R.T. -0.028 min
Lab File: BM040461.D
Acq: 30 Jun 2023 08:26

Instrument :
BNA_M
ClientSampleId :
SBLK575

Tgt Ion:202 Resp: 2339
Ion Ratio Lower Upper
202 100
101 169.1 12.6 18.8#
100 1225.9 9.8 14.6#

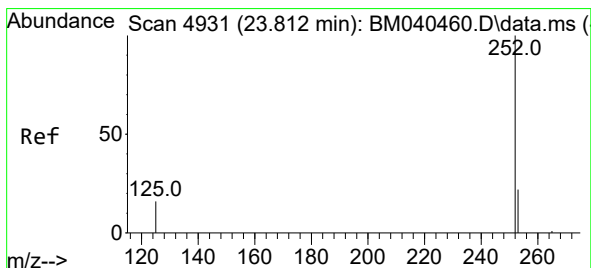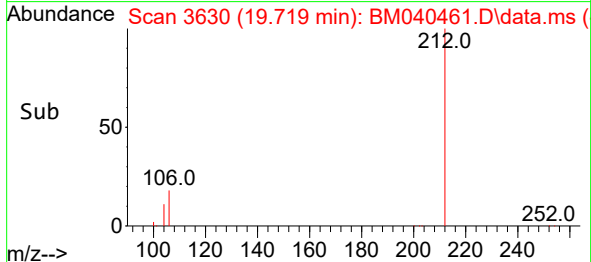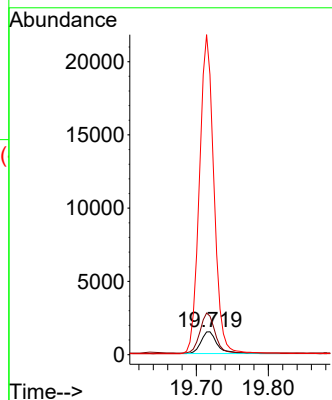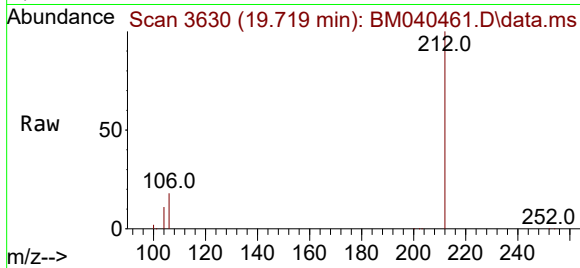

#26
Benzo(a)pyrene
Concen: 0.078 ng/ul
RT: 23.766 min Scan# 4915
Delta R.T. -0.047 min
Lab File: BM040461.D
Acq: 30 Jun 2023 08:26

Tgt Ion:252 Resp: 4372
Ion Ratio Lower Upper
252 100
253 53.8 22.9 34.3#
125 55.8 21.0 31.4#

