

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063023\
 Data File : BM040478.D
 Acq On : 30 Jun 2023 19:00
 Operator : MA/JU
 Sample : PB153575BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK575

Quant Time: Jul 01 03:04:33 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Jul 01 03:00:05 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.936	152	8165	0.400	ng/ul	0.00
4) Naphthalene-d8	10.745	136	31115	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.577	164	16661	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.328	188	32391	0.400	ng/ul	0.00
17) Chrysene-d12	21.509	240	20515	0.400	ng/ul	0.00
23) Perylene-d12	23.917	264	20092	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.325	96	55748	4.347	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.334	152	11996	0.275	ng/ul	0.00
18) Fluoranthene-d10	19.352	212	19820	0.301	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.719	202	3412	0.037	ng/ul#	1
26) Benzo(a)pyrene	23.765	252	5445	0.078	ng/ul#	51


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063023\
Data File : BM040478.D
Acq On : 30 Jun 2023 19:00
Operator : MA/JU
Sample : PB153575BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK575

Quant Time: Jul 01 03:04:33 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jul 01 03:00:05 2023
Response via : Initial Calibration




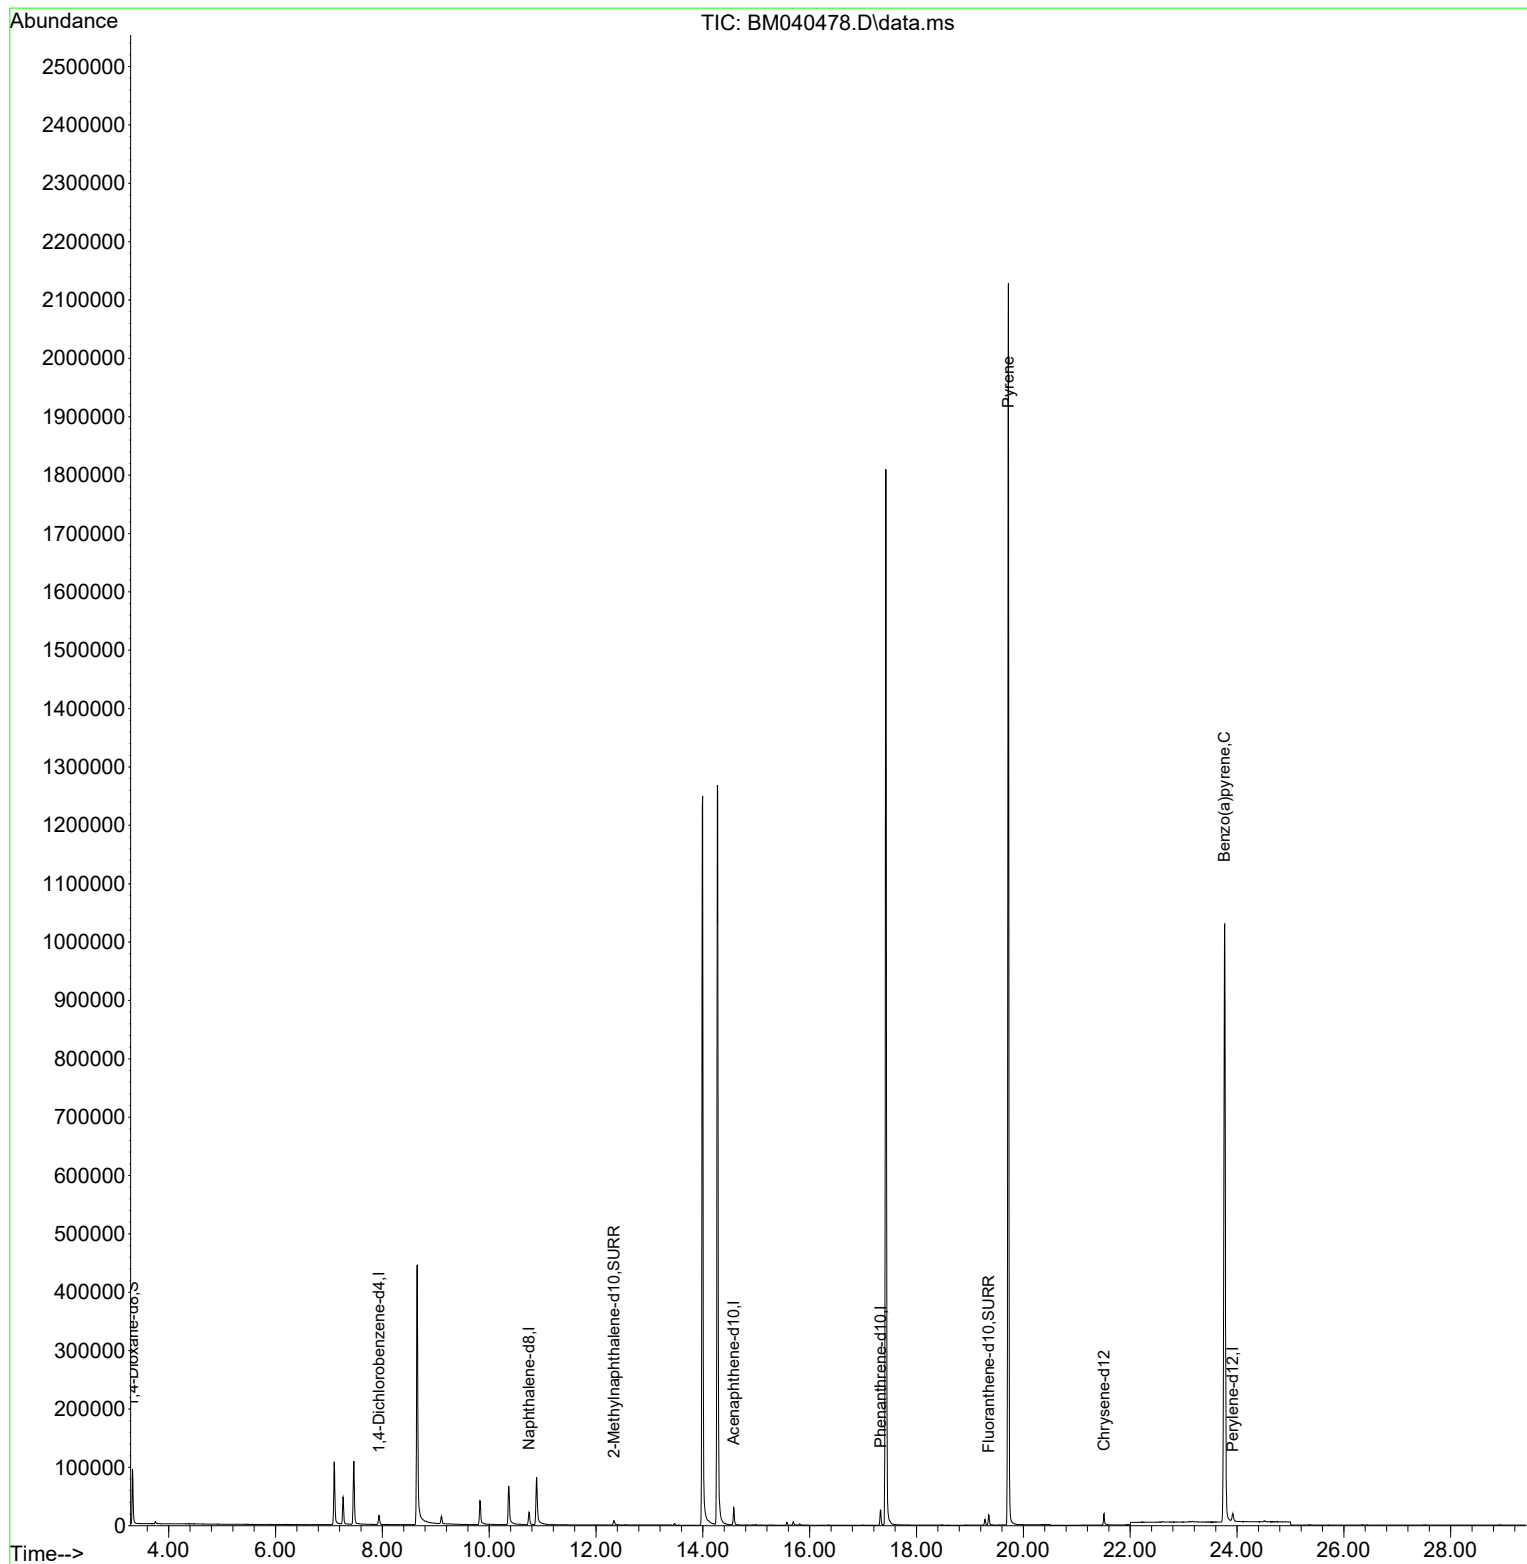


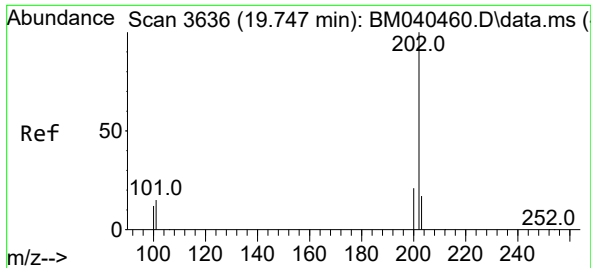

#20
Pyrene
Concen: 0.037 ng/ul
RT: 19.719 min Scan# 3630
Delta R.T. -0.028 min
Lab File: BM040478.D
Acq: 30 Jun 2023 19:00

Instrument :
BNA_M
ClientSampleId :
SBLK575

Tgt Ion:202 Resp: 3412
Ion Ratio Lower Upper
202 100
101 168.1 12.6 18.8#
100 1246.4 9.8 14.6#

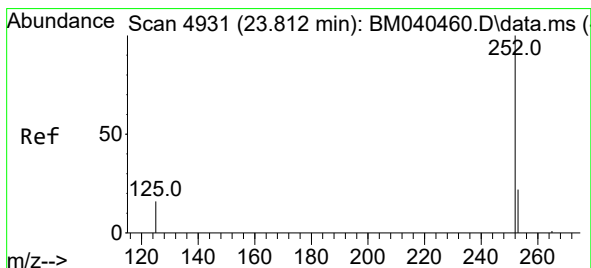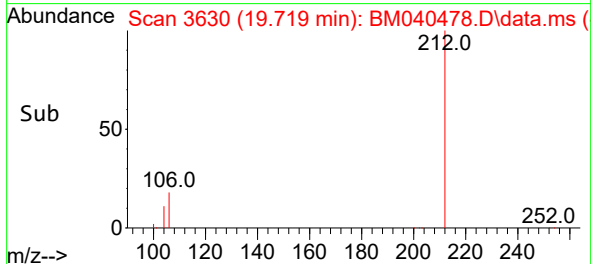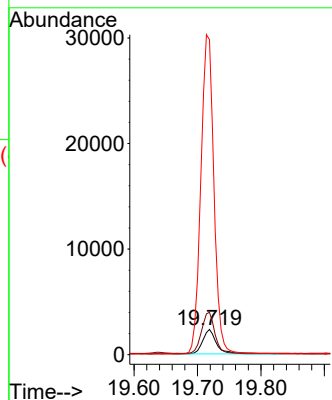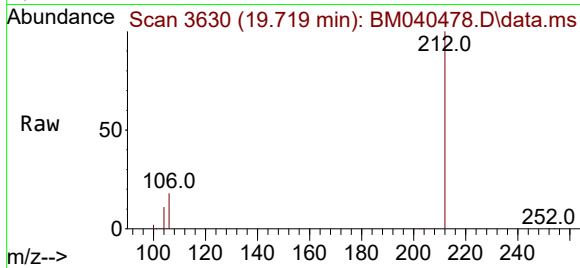

#26
Benzo(a)pyrene
Concen: 0.078 ng/ul
RT: 23.765 min Scan# 4915
Delta R.T. -0.047 min
Lab File: BM040478.D
Acq: 30 Jun 2023 19:00

Tgt Ion:252 Resp: 5445
Ion Ratio Lower Upper
252 100
253 50.3 22.9 34.3#
125 55.4 21.0 31.4#

