




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063023\
Data File : BM040473.D
Acq On : 30 Jun 2023 15:51
Operator : MA/JU
Sample : 03161-04DL 5X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCFWD0DL

Manual IntegrationsAPPROVED

Quant Time: Jul 01 03:03:46 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jul 01 03:00:05 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/01/2023
Supervised By :mohammad ahmed 07/01/2023

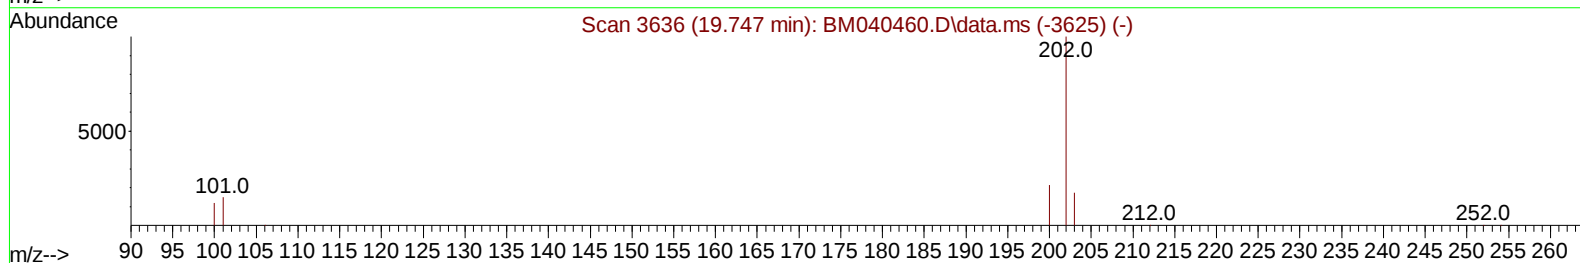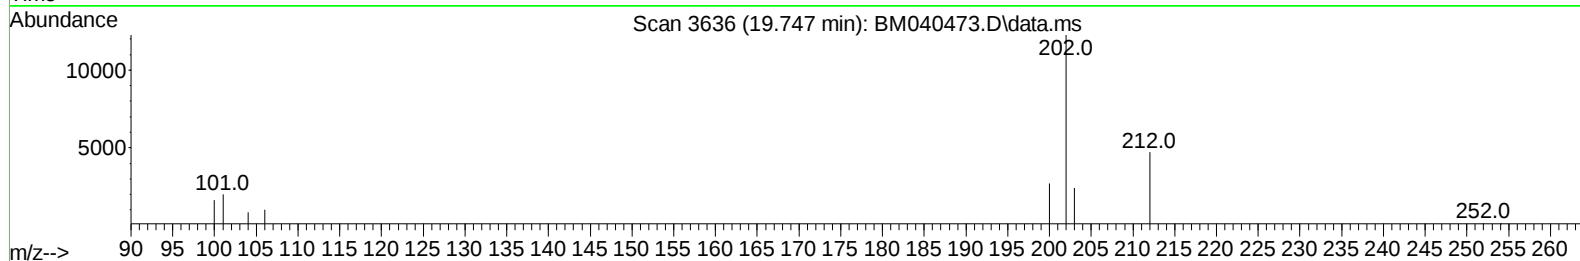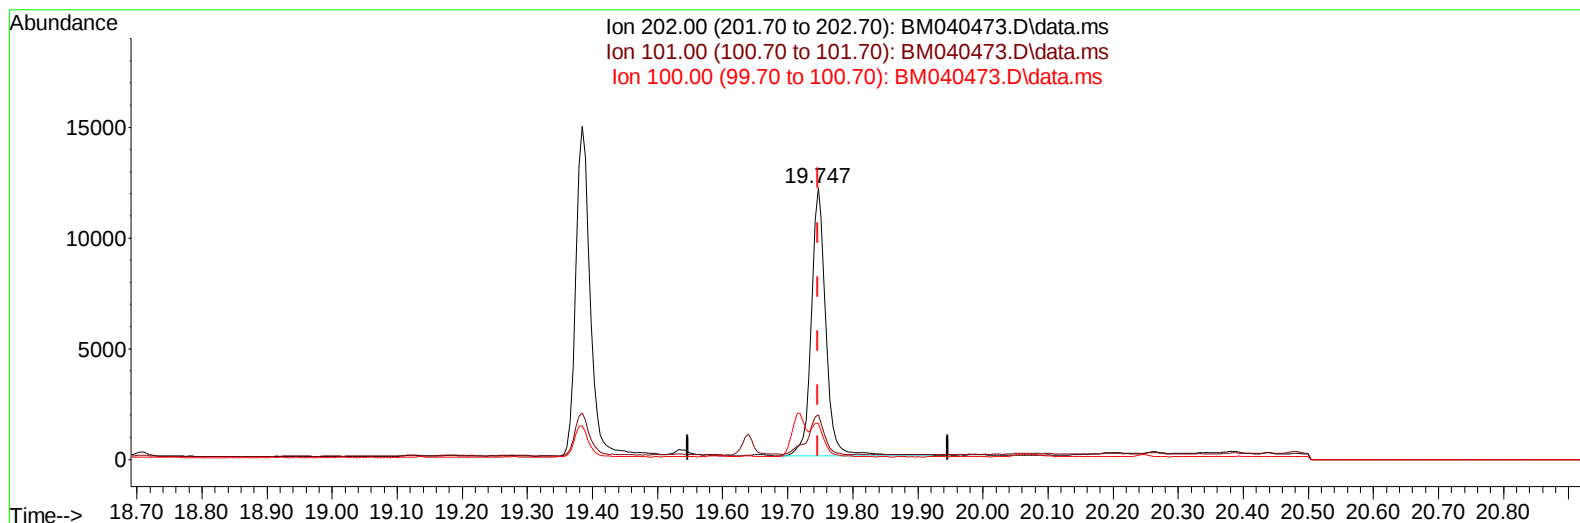

TIC: BM040473.D\data.ms

(20) Pyrene

19.747min (+ 0.000) 0.25 ng/u1

response 18765

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	15.70	16.29
100.00	12.20	13.25
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063023\
Data File : BM040473.D
Acq On : 30 Jun 2023 15:51
Operator : MA/JU
Sample : 03161-04DL 5X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCFWD0DL

Manual IntegrationsAPPROVED

Quant Time: Jul 01 03:03:46 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jul 01 03:00:05 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/01/2023
Supervised By :mohammad ahmed 07/01/2023

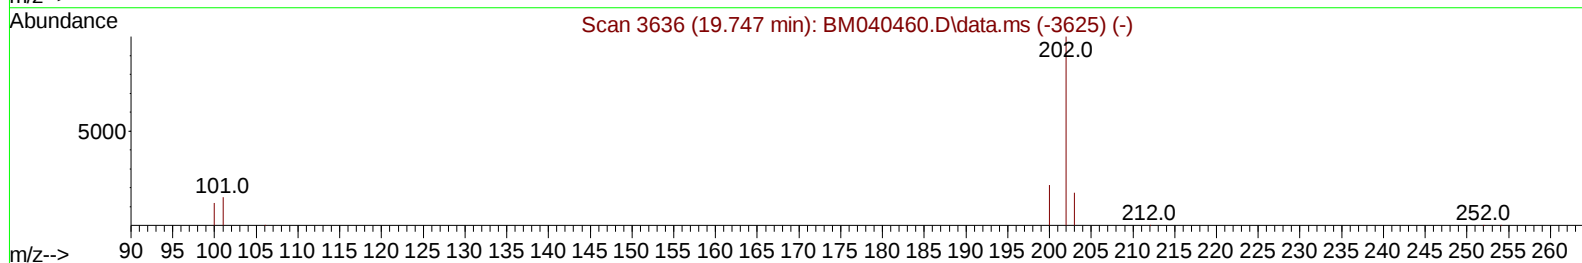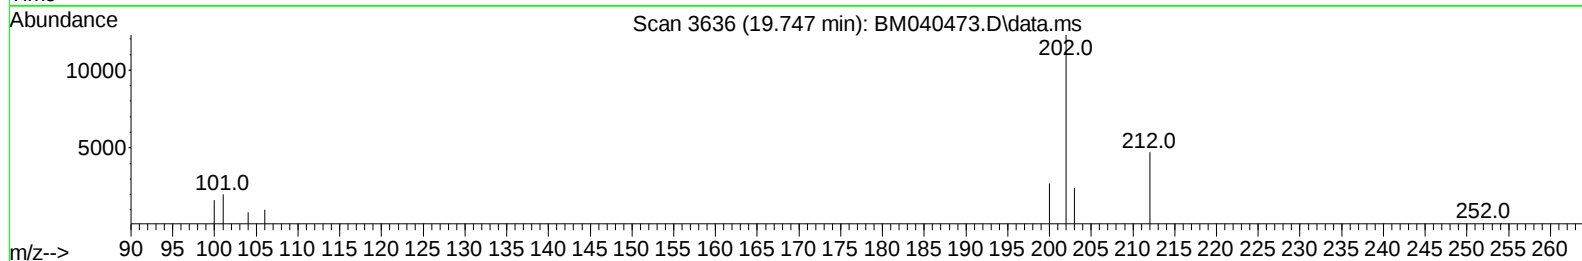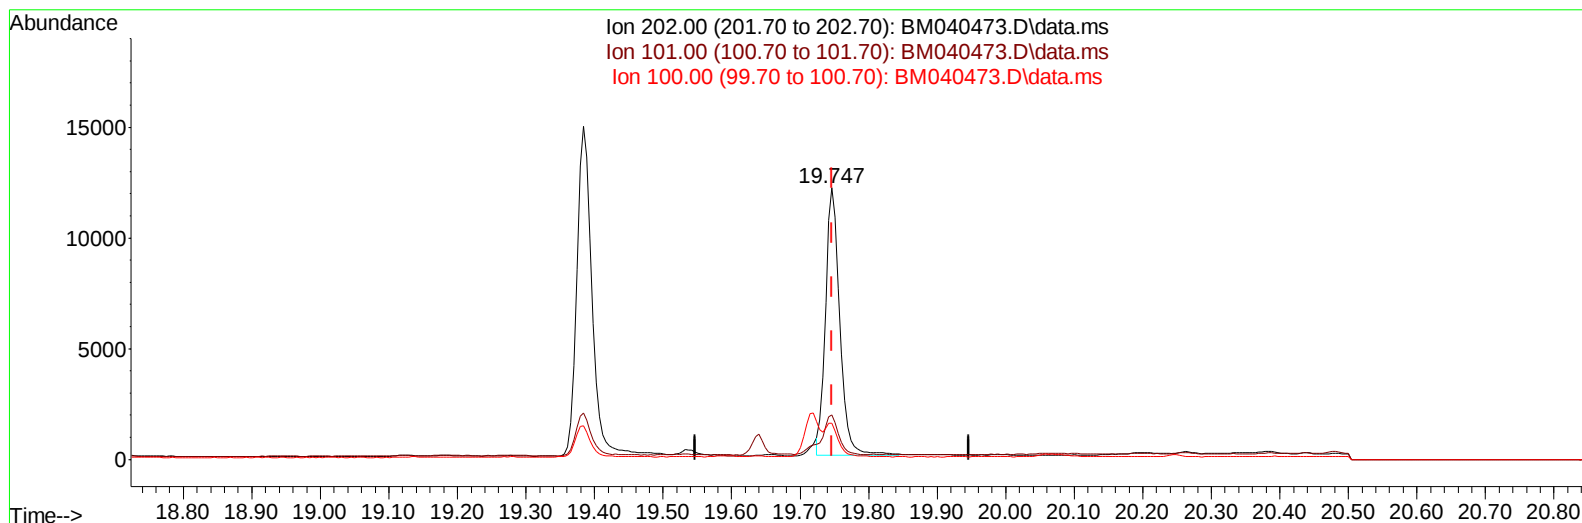

TIC: BM040473.D\data.ms

(20) Pyrene

19.747min (+ 0.000) 0.24 ng/ul m

response 17910

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	15.70	16.29
100.00	12.20	13.25
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063023\
 Data File : BM040473.D
 Acq On : 30 Jun 2023 15:51
 Operator : MA/JU
 Sample : 03161-04DL 5X
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DCFW0DL

Manual IntegrationsAPPROVED

Quant Time: Jul 01 03:03:46 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Jul 01 03:00:05 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/01/2023
 Supervised By :mohammad ahmed 07/01/2023

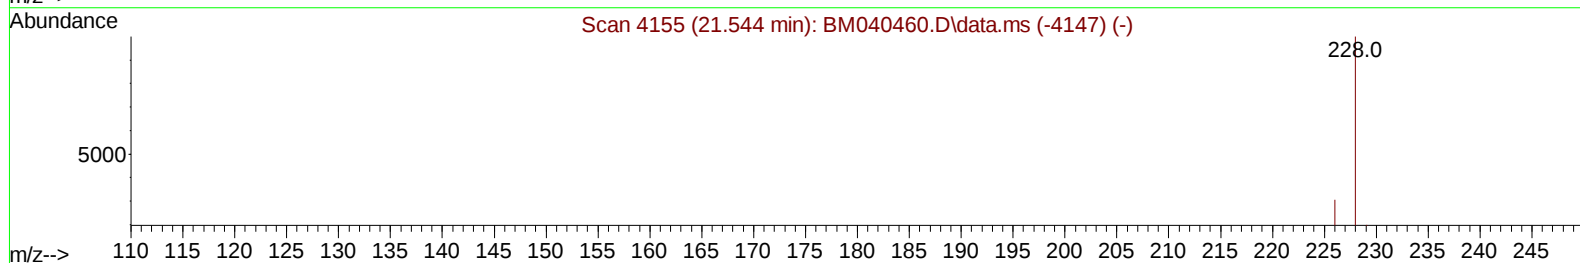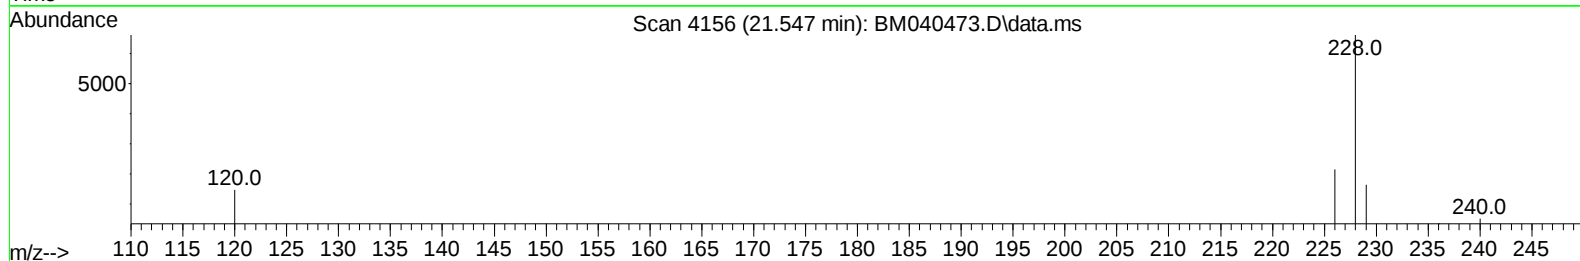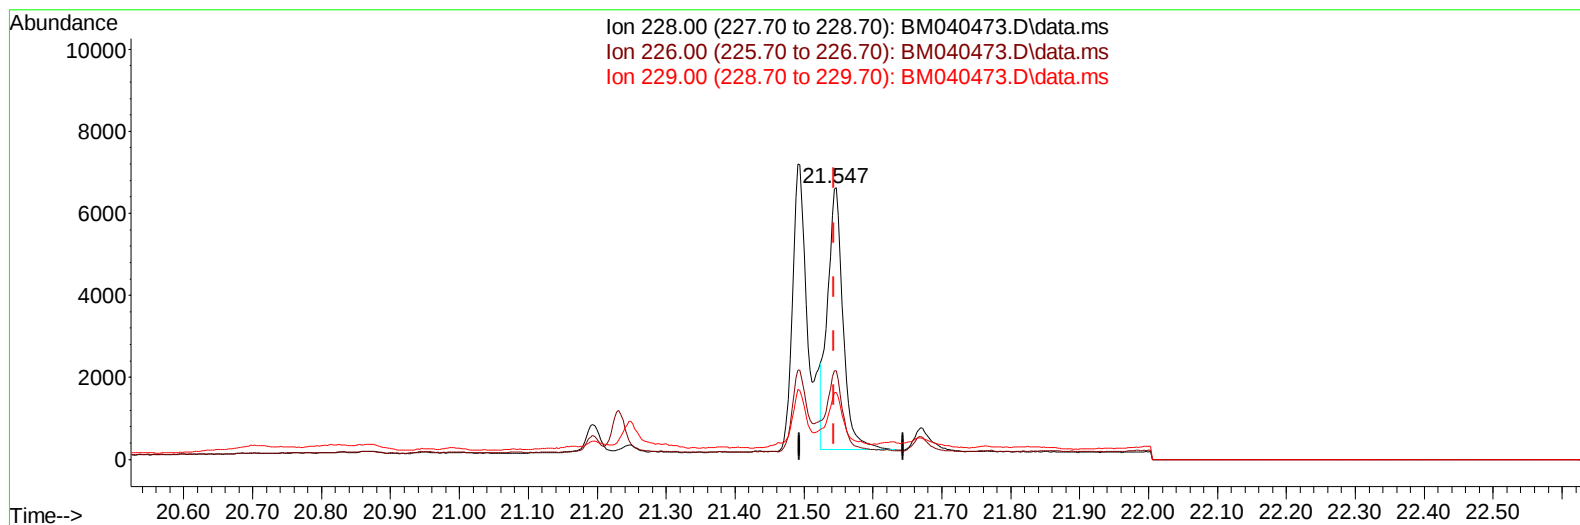

TIC: BM040473.D\data.ms

(22) Chrysene

21.547min (+ 0.003) 0.16 ng/u1

response 10117

Ion	Exp%	Act%
228.00	100.00	100.00
226.00	31.10	32.56
229.00	19.70	24.72#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063023\
 Data File : BM040473.D
 Acq On : 30 Jun 2023 15:51
 Operator : MA/JU
 Sample : 03161-04DL 5X
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DCFW0DL

Manual IntegrationsAPPROVED

Quant Time: Jul 01 03:03:46 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Jul 01 03:00:05 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/01/2023
 Supervised By :mohammad ahmed 07/01/2023

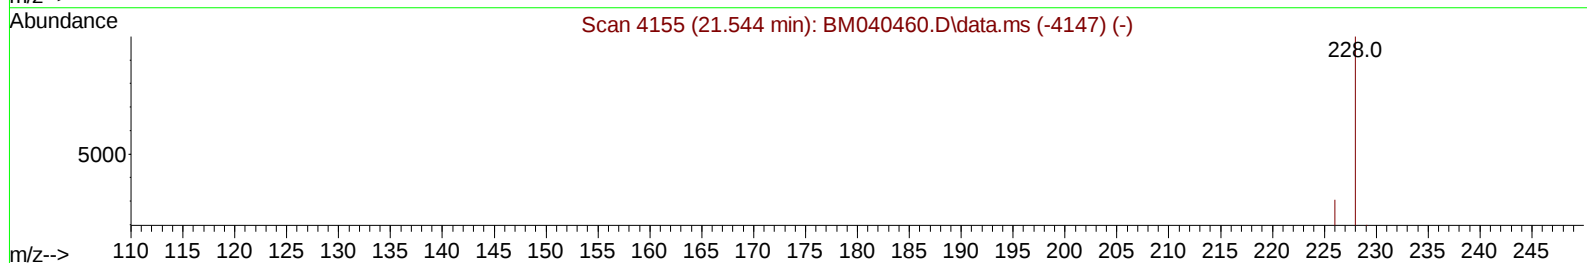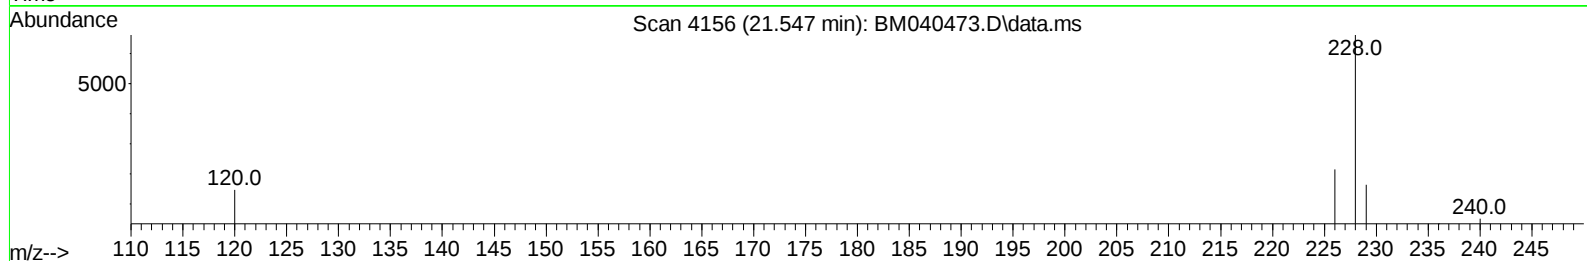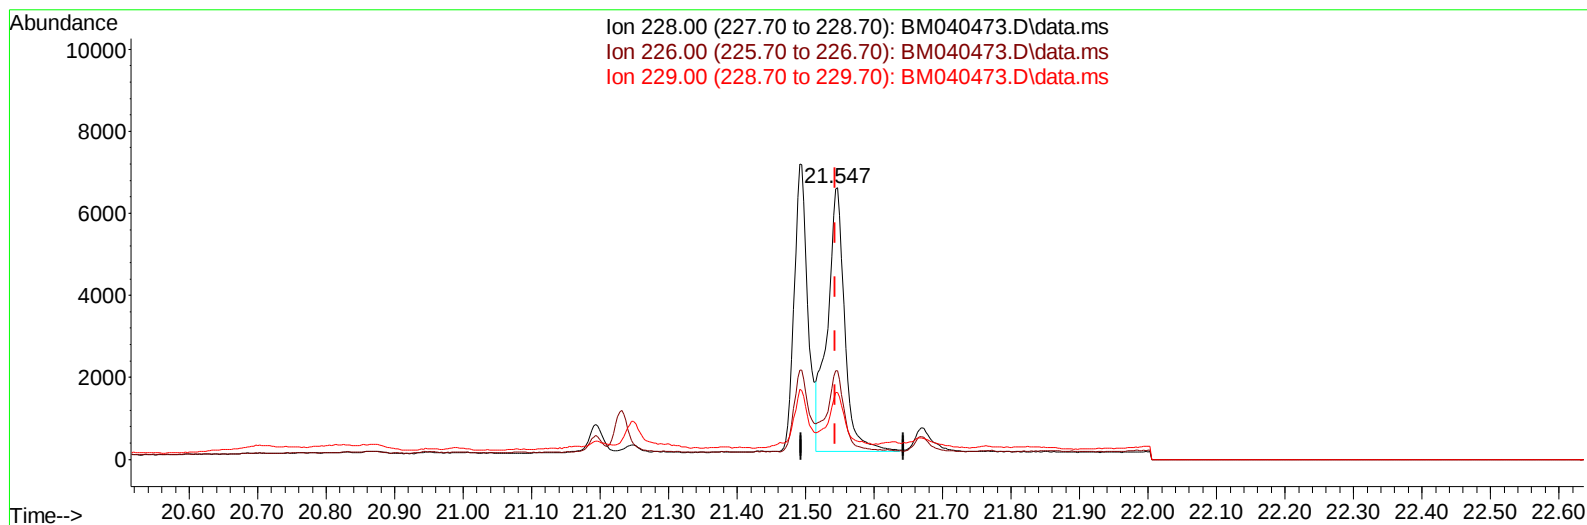

TIC: BM040473.D\data.ms

(22) Chrysene

21.547min (+ 0.003) 0.18 ng/ul m

response 11501

Ion	Exp%	Act%
228.00	100.00	100.00
226.00	31.10	32.56
229.00	19.70	24.72#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063023\
 Data File : BM040473.D
 Acq On : 30 Jun 2023 15:51
 Operator : MA/JU
 Sample : 03161-04DL 5X
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DCFW0DL

Manual IntegrationsAPPROVED

Quant Time: Jul 01 03:03:46 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Jul 01 03:00:05 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/01/2023
 Supervised By :mohammad ahmed 07/01/2023

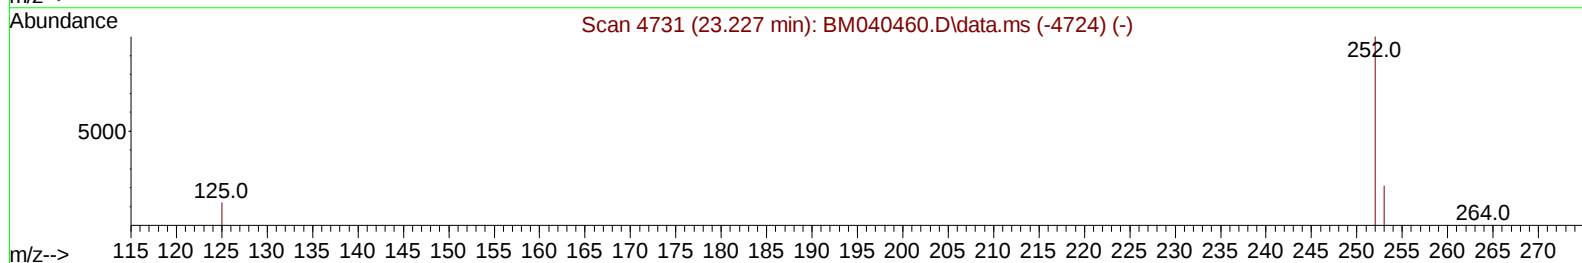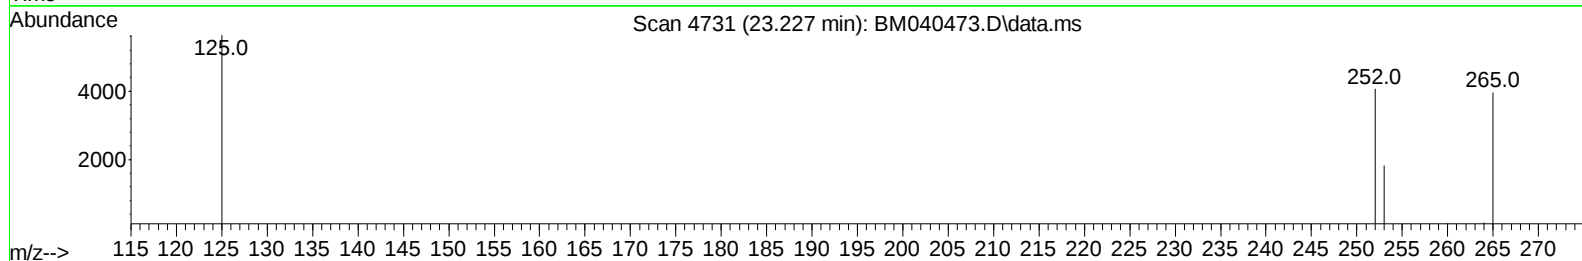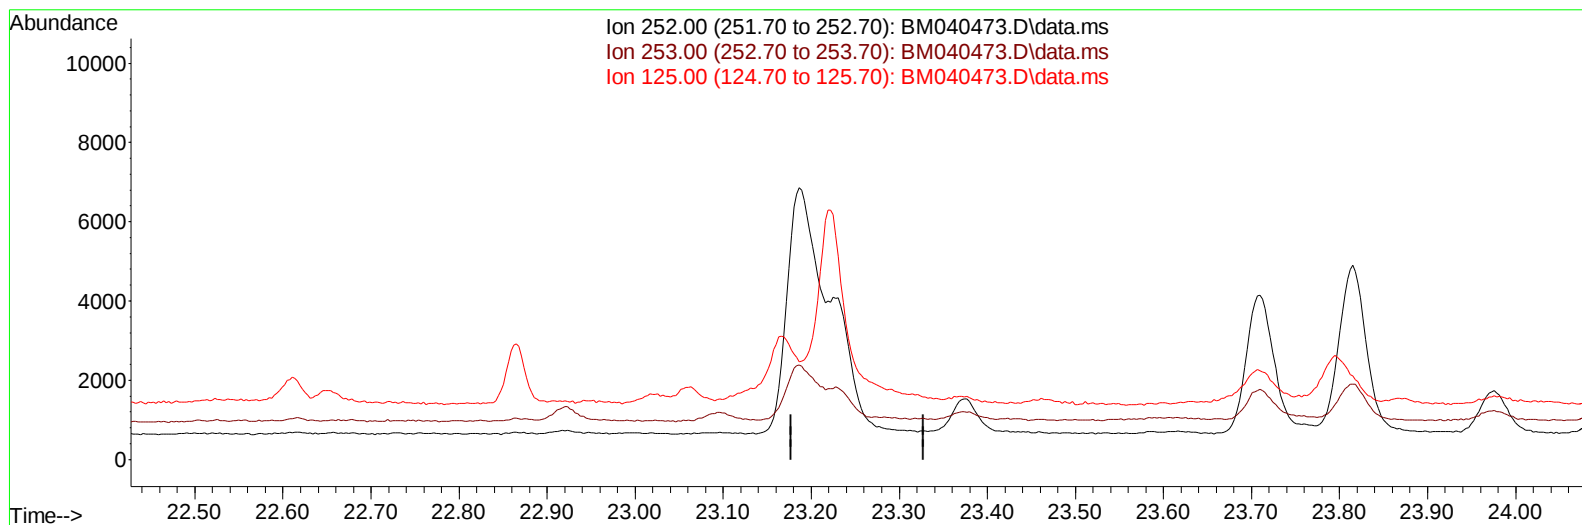

TIC: BM040473.D\data.ms

(25) Benzo(k)fluoranthene

23.227min (-23.227) 0.00 ng/u1

response 0

Ion	Exp%	Act%
252.00	100.00	0.00
253.00	26.50	0.00#
125.00	20.50	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063023\
 Data File : BM040473.D
 Acq On : 30 Jun 2023 15:51
 Operator : MA/JU
 Sample : 03161-04DL 5X
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DCFW0DL

Manual IntegrationsAPPROVED

Quant Time: Jul 01 03:03:46 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Jul 01 03:00:05 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/01/2023
 Supervised By :mohammad ahmed 07/01/2023

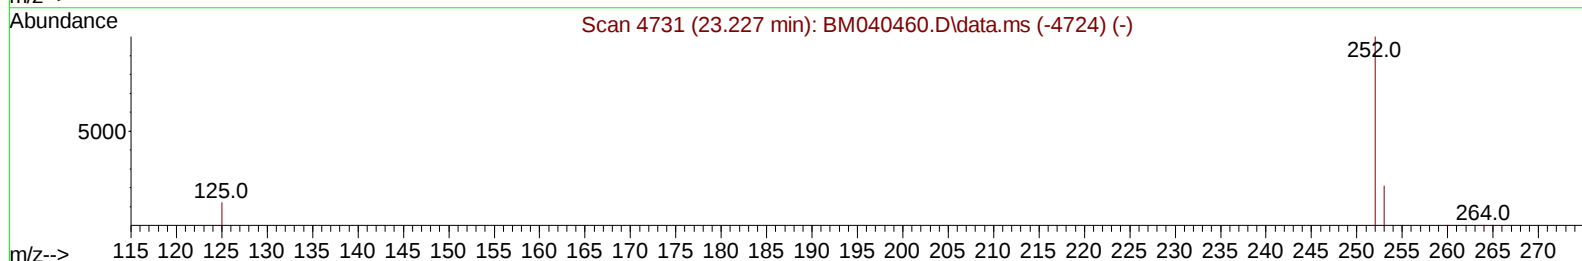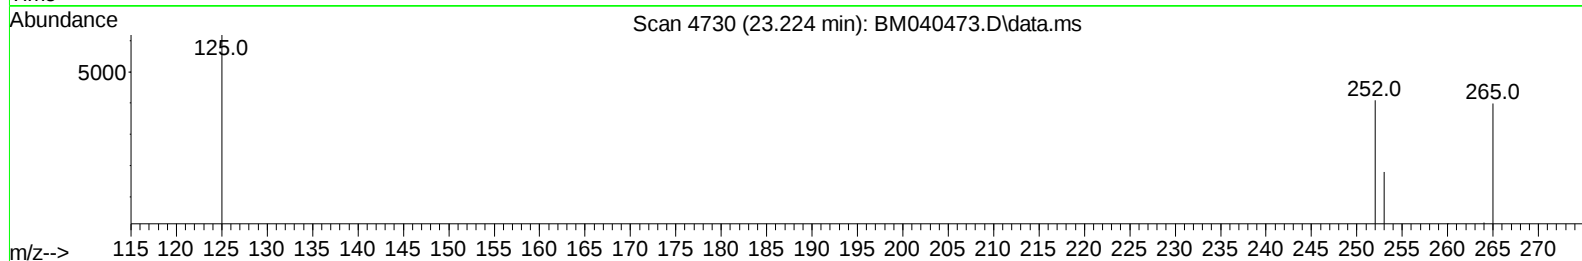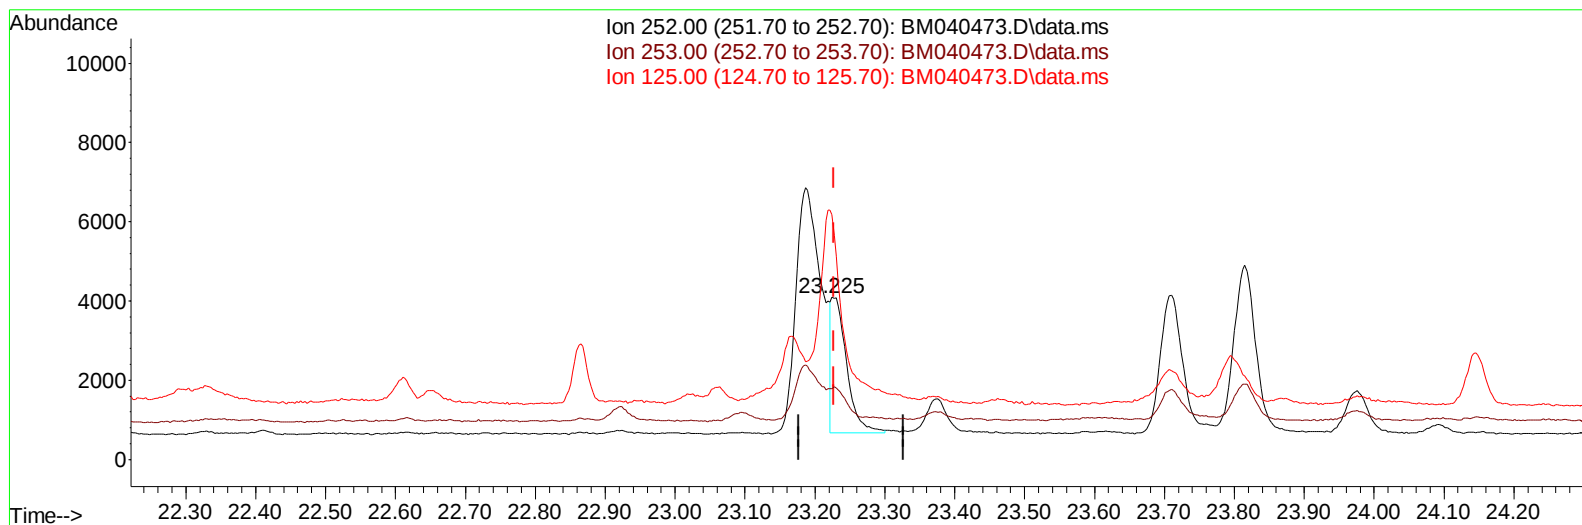

TIC: BM040473.D\data.ms

(25) Benzo(k)fluoranthene

23.224min (-0.003) 0.09 ng/u1 m

response 5122

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	26.50	43.87#
125.00	20.50	151.19#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063023\
 Data File : BM040473.D
 Acq On : 30 Jun 2023 15:51
 Operator : MA/JU
 Sample : 03161-04DL 5X
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DCFW0DL

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 07/01/2023
 Supervised By :mohammad ahmed 07/01/2023

Quant Time: Jul 01 03:03:46 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Jul 01 03:00:05 2023
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.940	152		8431	0.400	ng/ul	0.00
4) Naphthalene-d8	10.750	136		32127	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.582	164		15894	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.328	188		29633	0.400	ng/ul	0.00
17) Chrysene-d12	21.509	240		16615	0.400	ng/ul	0.00
23) Perylene-d12	23.923	264		15426	0.400	ng/ul	0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.329	96		4077	0.308	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.340	152		1025	0.023	ng/ul	0.00
18) Fluoranthene-d10	19.356	212		1455	0.027	ng/ul	0.00
Target Compounds							
						Qvalue	
15) Phenanthrene	17.370	178		6963	0.076	ng/ul#	94
16) Anthracene	17.463	178		1709	0.022	ng/ul#	70
19) Fluoranthene	19.384	202		22766	0.323	ng/ul	99
20) Pyrene	19.747	202		17910m	0.237	ng/ul	
21) Benzo(a)anthracene	21.491	228		9744	0.173	ng/ul	94
22) Chrysene	21.547	228		11501m	0.179	ng/ul	
24) Benzo(b)fluoranthene	23.186	252		15788	0.264	ng/ul	77
25) Benzo(k)fluoranthene	23.224	252		5122m	0.087	ng/ul	
26) Benzo(a)pyrene	23.815	252		9170	0.171	ng/ul#	74
27) Indeno(1,2,3-cd)pyrene	26.424	276		7683	0.103	ng/ul#	87
28) Dibenzo(a,h)anthracene	26.437	278		2014	0.034	ng/ul#	8
29) Benzo(g,h,i)perylene	27.198	276		7459	0.114	ng/ul#	83

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063023\
Data File : BM040473.D
Acq On : 30 Jun 2023 15:51
Operator : MA/JU
Sample : 03161-04DL 5X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCFWD0DL

Manual IntegrationsAPPROVED

Quant Time: Jul 01 03:03:46 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jul 01 03:00:05 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/01/2023
Supervised By :mohammad ahmed 07/01/2023

