

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM070119\
 Data File : BM021306.D
 Acq On : 01 Jul 2019 13:14
 Operator : HP/JU
 Sample : K3559-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C5AE2

Quant Time: Jul 02 00:54:38 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jul 01 01:16:07 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.76	152	209537	20.00	ng/ul	0.00
18) Naphthalene-d8	10.54	136	939736	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.40	164	603432	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.15	188	1320461	20.00	ng/ul	0.00
77) Chrysene-d12	21.34	240	917936	20.00	ng/ul	0.00
85) Perylene-d12	23.61	264	1065751	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.28	96	25185	5.71	ng/uL	0.00
5) Phenol-d5	6.93	99	147057	8.06	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.10	67	314716	28.96	ng/ul	0.00
9) 2-Chlorophenol-d4	7.29	132	397562	26.83	ng/ul	0.00
13) 4-Methylphenol-d8	8.46	113	283588	18.63	ng/ul	0.00
19) Nitrobenzene-d5	8.92	128	255505	33.48	ng/ul	0.00
22) 2-Nitrophenol-d4	9.63	143	299619	35.37	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.16	165	563345	32.71	ng/ul	0.00
29) 4-Chloroaniline-d4	10.69	131	67855	3.78	ng/ul	0.00
43) Dimethylphthalate-d6	13.81	166	1918865	35.19	ng/ul	0.00
46) Acenaphthylene-d8	14.09	160	2251794	33.74	ng/ul	0.00
51) 4-Nitrophenol-d4	14.63	143	48210	5.44	ng/ul	0.00
57) Fluorene-d10	15.39	176	1635590	34.49	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.53	200	234156	28.85	ng/ul	0.00
70) Anthracene-d10	17.24	188	2510115	36.58	ng/ul	0.00
78) Pyrene-d10	19.54	212	2307581	41.89	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.47	264	2320189	36.90	ng/ul	0.00


Target Compounds					Qvalue
44) Dimethylphthalate	13.86	163	134034	2.700	ng/ul 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM070119\
Data File : BM021306.D
Acq On : 01 Jul 2019 13:14
Operator : HP/JU
Sample : K3559-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C5AE2

Quant Time: Jul 02 00:54:38 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jul 01 01:16:07 2019
Response via : Initial Calibration

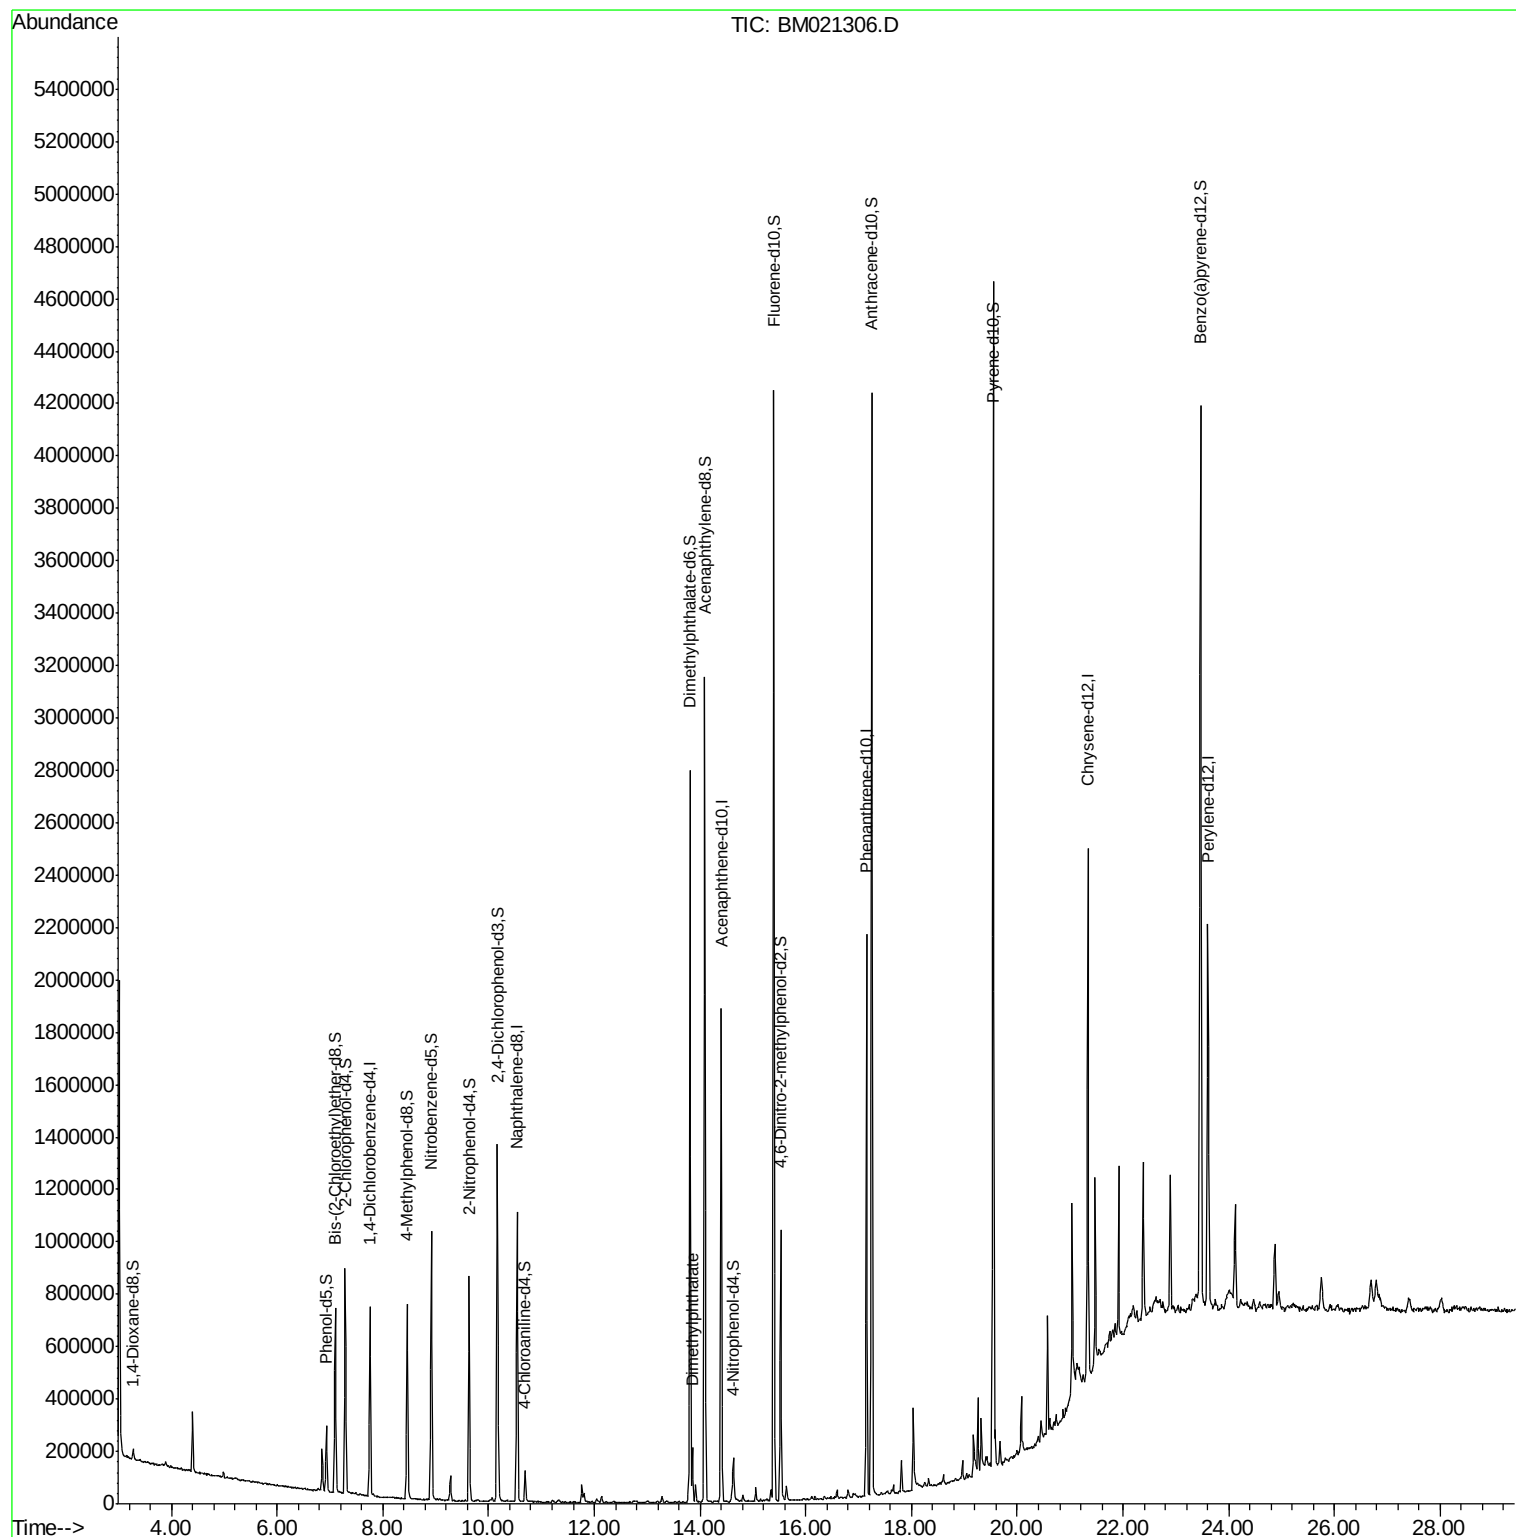

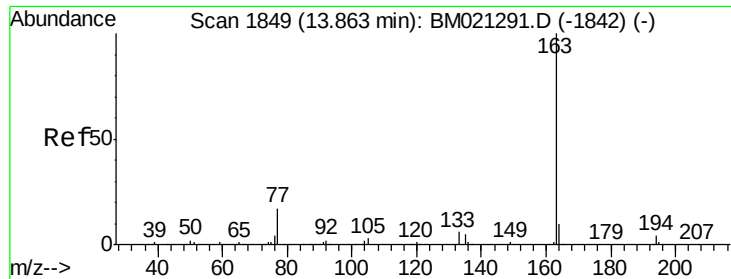

#44

Dimethylphthalate

Concen: 2.700 ng/ul

RT: 13.86 min Scan# 1848

Delta R.T. -0.01 min

Lab File: BM021306.D

Acq: 01 Jul 2019 13:14

Instrument :

BNA_M

ClientSampleId :

C5AE2


Tgt Ion:163 Resp: 134034

Ion Ratio Lower Upper

163 100

194 4.6 3.4 5.2

164 9.2 7.7 11.5

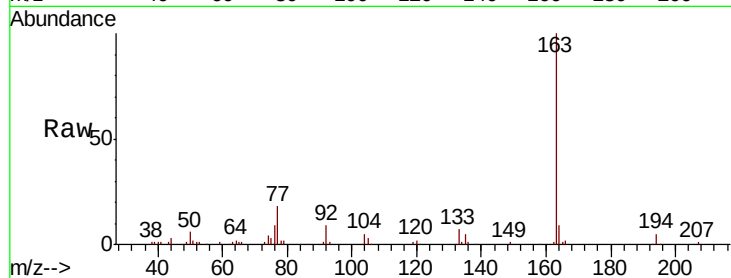

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

